
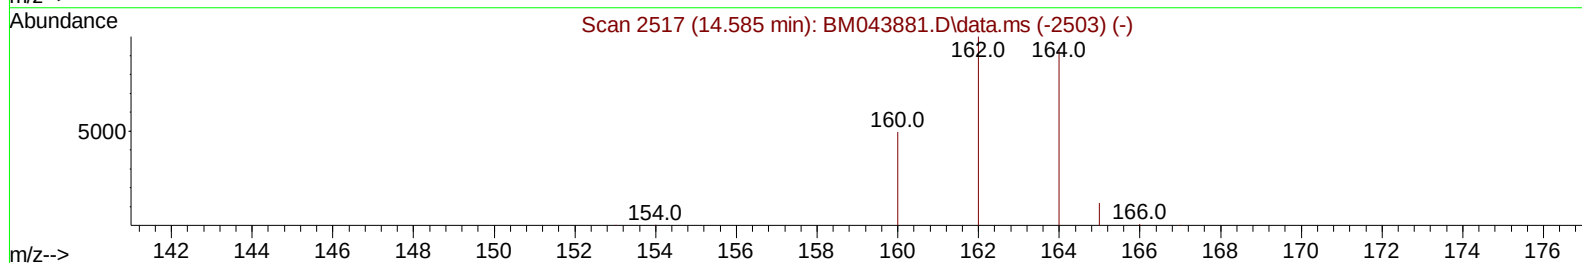
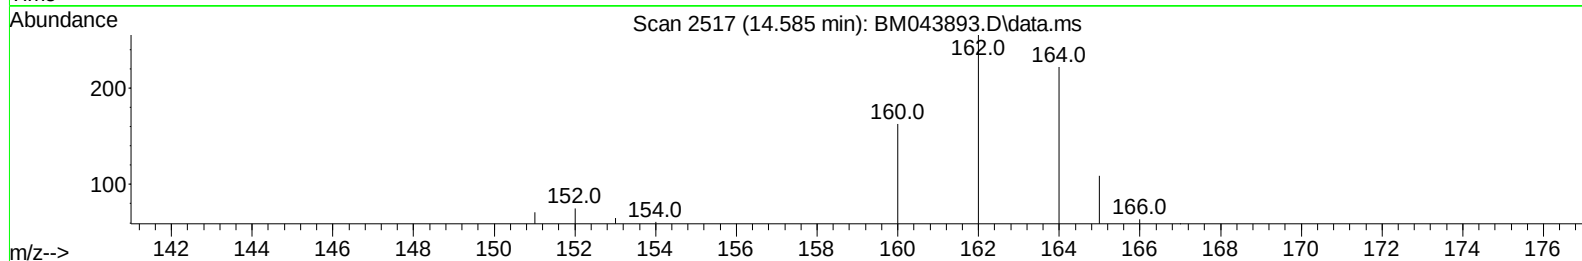


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043893.D
Acq On : 22 Jan 2024 20:19
Operator : MA/JU
Sample : PB158503BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jan 23 00:30:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

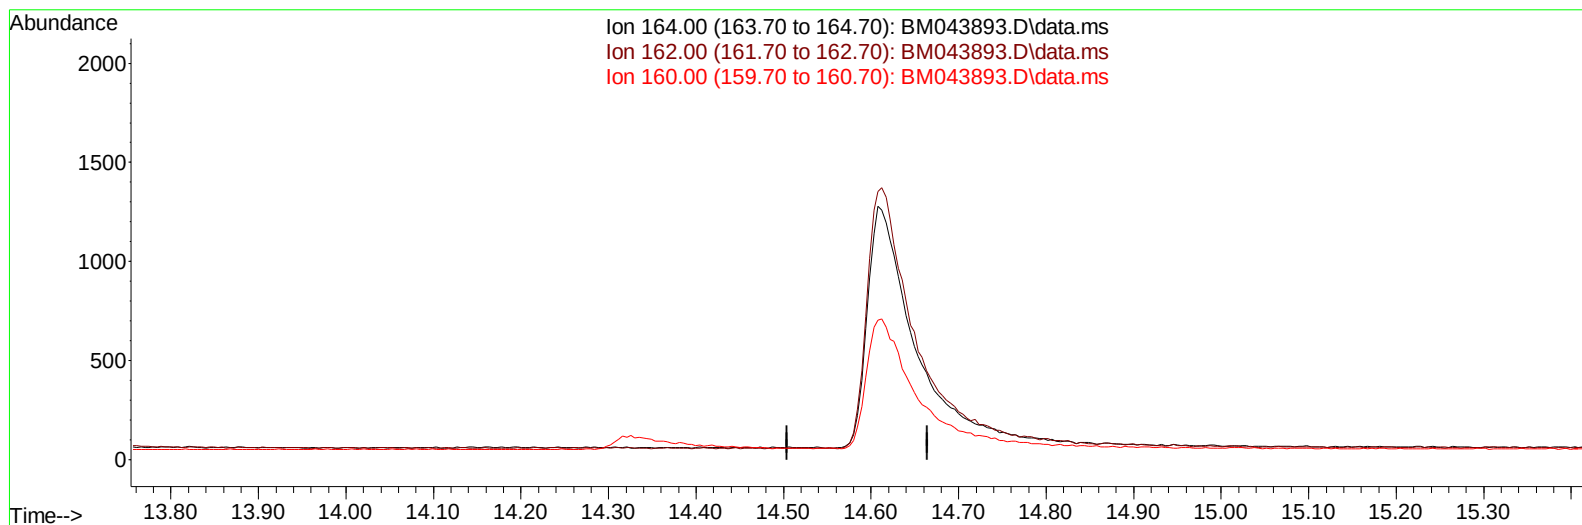

TIC: BM043893.D\data.ms

(9) Acenaphthene-d10 (I)




14.584min (-14.584) 0.00 ng/ul

response 0

Ion	Exp%	Act%
164.00	100.00	0.00
162.00	106.40	0.00#
160.00	52.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043893.D
Acq On : 22 Jan 2024 20:19
Operator : MA/JU
Sample : PB158503BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jan 23 00:30:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

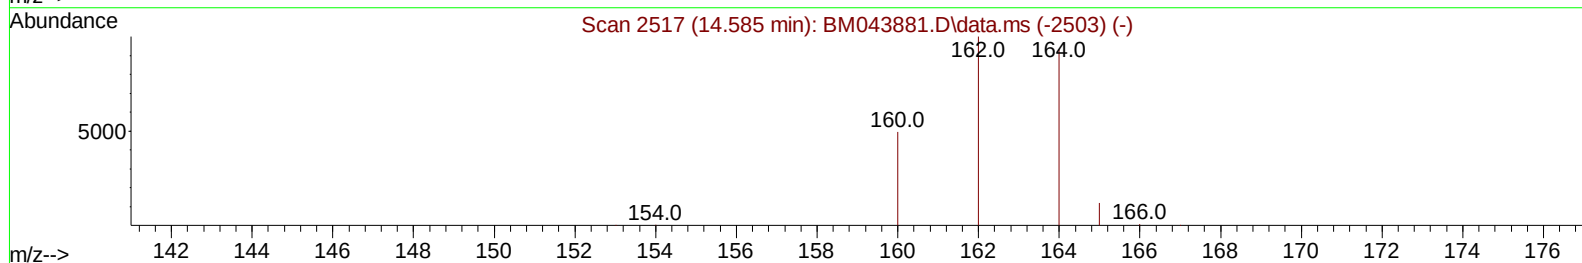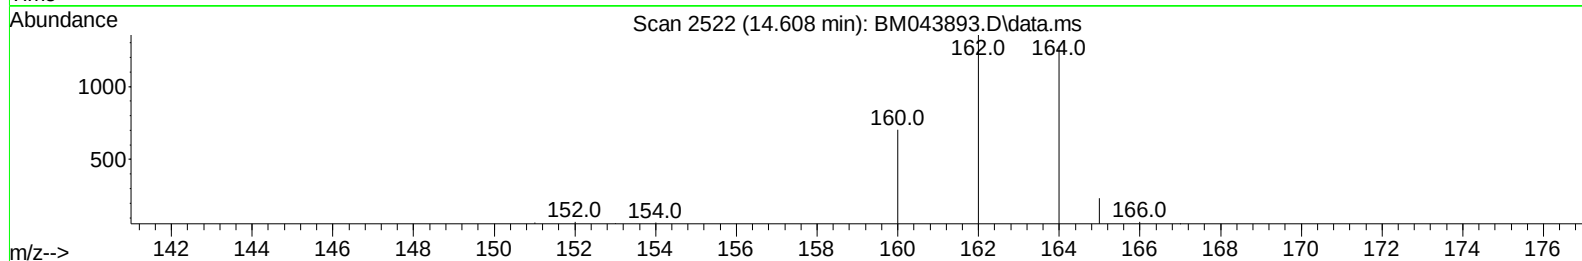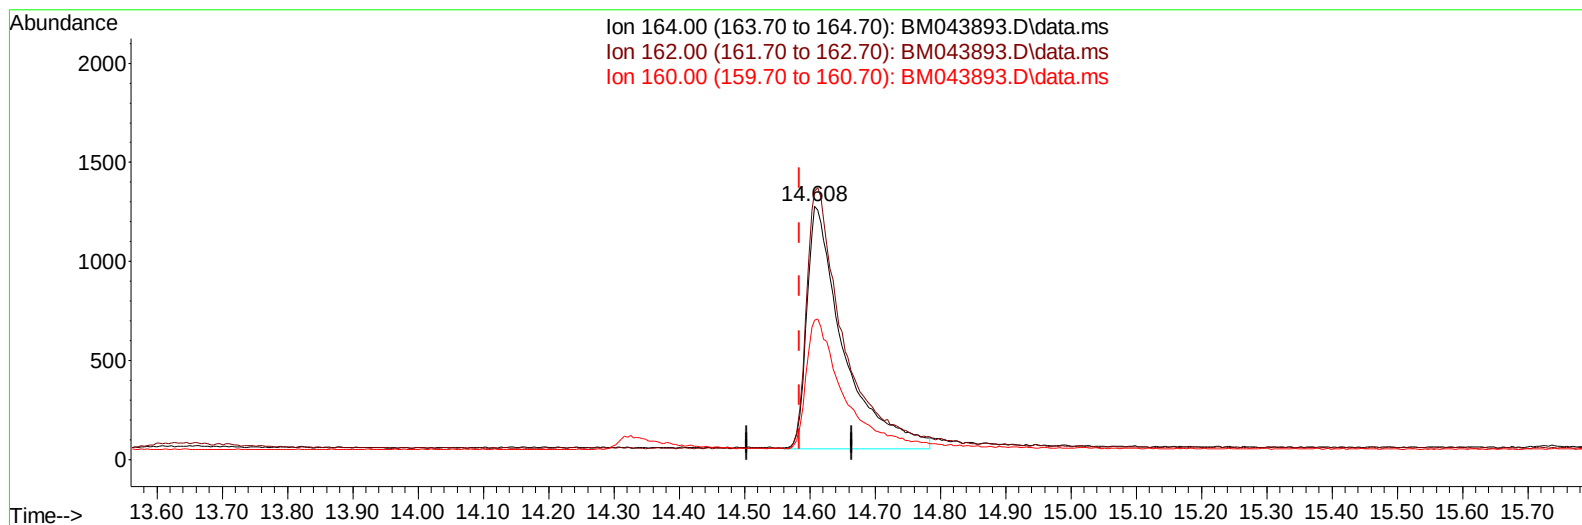

TIC: BM043893.D\data.ms

(9) Acenaphthene-d10 (I)

14.608min (+ 0.023) 0.40 ng/ul m

response 4778

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	105.79
160.00	52.70	55.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
 Data File : BM043893.D
 Acq On : 22 Jan 2024 20:19
 Operator : MA/JU
 Sample : PB158503BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jan 23 00:30:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 19 22:45:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	3204	0.400	ng/ul	# 0.03
4) Naphthalene-d8	10.837	136	9029	0.400	ng/ul	# 0.07
9) Acenaphthene-d10	14.608	164	4778m	0.400	ng/ul	0.02
13) Phenanthrene-d10	17.385	188	8129	0.400	ng/ul	0.03
17) Chrysene-d12	21.550	240	6045	0.400	ng/ul	# 0.01
23) Perylene-d12	23.961	264	7665	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	3475	0.796	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.448	152	3093	0.270	ng/ul	0.08
18) Fluoranthene-d10	19.387	212	5826	0.292	ng/ul	0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012224\
Data File : BM043893.D
Acq On : 22 Jan 2024 20:19
Operator : MA/JU
Sample : PB158503BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jan 23 00:30:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 22:45:24 2024
Response via : Initial Calibration

