

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049374.D
 Acq On : 21 Jan 2025 20:58
 Operator : RC/JU
 Sample : PB166157BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS157

Quant Time: Jan 22 00:23:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 13 16:56:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.522	152	217104	20.000	ng/u1	0.00
20) Naphthalene-d8	10.280	136	844130	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.163	164	593710	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.909	188	1217543	20.000	ng/u1	0.00
79) Chrysene-d12	21.144	240	1169996	20.000	ng/u1	0.00
88) Perylene-d12	23.921	264	1051564	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.122	96	33576	6.399	ng/uL	0.00
4) Pyridine-d5	3.510	84	490747	29.378	ng/u1	0.00
7) Phenol-d5	6.716	99	545277	29.919	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67	375791	30.967	ng/u1	0.00
11) 2-Chlorophenol-d4	7.063	132	427056	30.632	ng/u1	0.00
15) 4-Methylphenol-d8	8.233	113	405238	28.674	ng/u1	0.00
21) Nitrobenzene-d5	8.663	128	197933	30.749	ng/u1	0.00
24) 2-Nitrophenol-d4	9.380	143	212839	29.577	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.916	165	459935	31.322	ng/u1	0.00
31) 4-Chloroaniline-d4	10.427	131	513040	26.552	ng/u1	0.00
46) Dimethylphthalate-d6	13.586	166	1372986	31.071	ng/u1	0.00
49) Acenaphthylene-d8	13.851	160	1607971	31.875	ng/u1	0.00
54) 4-Nitrophenol-d4	14.386	143	210189	28.724	ng/u1	0.00
60) Fluorene-d10	15.162	176	1278395	33.489	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.292	200	223496	28.803	ng/u1	0.00
73) Anthracene-d10	17.009	188	1968653	32.708	ng/u1	0.00
81) Pyrene-d10	19.315	212	2286367	32.110	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.738	264	1882886	33.355	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.151	88	67766	11.788	ng/uL	93
5) Pyridine	3.528	79	495572	29.348	ng/u1	96
6) Benzaldehyde	6.675	77	213178	21.697	ng/u1	99
8) Phenol	6.739	94	559241	29.514	ng/u1	98
10) Bis(2-Chloroethyl)ether	6.963	93	455564	29.524	ng/u1	99
12) 2-Chlorophenol	7.092	128	433041	29.882	ng/u1	98
13) 2-Methylphenol	7.969	108	387947	28.023	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.045	45	715641	30.946	ng/u1	99
16) Acetophenone	8.333	105	683336	29.605	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.333	70	373925	29.993	ng/u1	97
18) 4-Methylphenol	8.298	108	427059	28.156	ng/u1	99
19) Hexachloroethane	8.581	117	188985	30.351	ng/u1	97
22) Nitrobenzene	8.704	77	515884	30.935	ng/u1	99
23) Isophorone	9.233	82	939399	28.991	ng/u1	99
25) 2-Nitrophenol	9.410	139	233524	29.527	ng/u1	98
26) 2,4-Dimethylphenol	9.480	107	362430	24.486	ng/u1	97
27) Bis(2-Chloroethoxy)met...	9.716	93	602647	30.260	ng/u1	99
29) 2,4-Dichlorophenol	9.939	162	447151	30.565	ng/u1	99
30) Naphthalene	10.333	128	1367612	30.528	ng/u1	100
32) 4-Chloroaniline	10.451	127	415878	22.571	ng/u1	99
33) Hexachlorobutadiene	10.622	225	324137	31.031	ng/u1	99
34) Caprolactam	11.227	113	66436	15.254	ng/u1	96
35) 4-Chloro-3-methylphenol	11.586	107	412892	30.185	ng/u1	100
36) 2-Methylnaphthalene	11.951	142	983107	30.667	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049374.D
 Acq On : 21 Jan 2025 20:58
 Operator : RC/JU
 Sample : PB166157BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS157

Quant Time: Jan 22 00:23:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 13 16:56:06 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.174	142	982356	30.798	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.327	216	629168	30.615	ng/ul	99
40) Hexachlorocyclopentadiene	12.310	237	295284	23.949	ng/ul	99
41) 2,4,6-Trichlorophenol	12.580	196	345409	27.322	ng/ul	97
42) 2,4,5-Trichlorophenol	12.651	196	392238	28.948	ng/ul	98
43) 1,1'-Biphenyl	12.986	154	1340843	30.846	ng/ul	98
44) 2-Chloronaphthalene	13.021	162	1083677	31.173	ng/ul	98
45) 2-Nitroaniline	13.239	65	290646	31.685	ng/ul	99
47) Dimethylphthalate	13.633	163	1328040	30.381	ng/ul	100
48) 2,6-Dinitrotoluene	13.745	165	251143	30.795	ng/ul	95
50) Acenaphthylene	13.880	152	1651328	31.930	ng/ul	99
51) 3-Nitroaniline	14.074	138	231372	28.916	ng/ul	97
52) Acenaphthene	14.227	153	1159216	31.372	ng/ul	99
53) 2,4-Dinitrophenol	14.286	184	121271	23.743	ng/ul	96
55) 4-Nitrophenol	14.404	109	154436	28.620	ng/ul	98
56) Dibenzofuran	14.563	168	1677786	31.975	ng/ul	99
57) 2,4-Dinitrotoluene	14.539	165	385472	31.852	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	14.798	232	297611	26.001	ng/ul	97
59) Diethylphthalate	15.010	149	1349940	31.687	ng/ul	98
61) Fluorene	15.215	166	1461045	34.080	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.221	204	778894	33.337	ng/ul	97
63) 4-Nitroaniline	15.245	138	247635	34.397	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.304	198	243536	28.785	ng/ul	97
67) N-Nitrosodiphenylamine	15.433	169	1146955	31.749	ng/ul	99
68) 4-Bromophenyl-phenylether	16.115	248	435326	31.444	ng/ul	99
69) Hexachlorobenzene	16.221	284	494687	30.723	ng/ul	98
70) Atrazine	16.398	200	136095	9.215	ng/ul	95
71) Pentachlorophenol	16.568	266	235613	22.088	ng/ul	99
72) Phenanthrene	16.956	178	2226977	32.901	ng/ul	100
74) Anthracene	17.045	178	2200039	32.382	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	12.945	216	607935	29.876	ng/ul	99
76) Pentachlorobenzene	14.486	250	577347	28.426	ng/ul	98
77) Carbazole	17.321	167	1903995	31.586	ng/ul	99
78) Di-n-butylphthalate	17.903	149	2369275	32.078	ng/ul	99
80) Fluoranthene	18.980	202	2573024	31.447	ng/ul	98
82) Pyrene	19.345	202	2747000	31.540	ng/ul	96
83) Butylbenzylphthalate	20.274	149	955333	30.982	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.062	252	653126	29.811	ng/ul	100
85) Benzo(a)anthracene	21.127	228	2592619	31.797	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.080	149	1453390	31.693	ng/ul	99
87) Chrysene	21.186	228	2403137	32.285	ng/ul	99
89) Di-n-octyl phthalate	22.138	149	2196850	28.677	ng/ul	100
90) Benzo(b)fluoranthene	23.056	252	2325818	33.045	ng/ul	99
91) Benzo(k)fluoranthene	23.109	252	2394539	34.121	ng/ul	100
93) Benzo(a)pyrene	23.797	252	1992129	31.335	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	27.009	276	2251686	30.875	ng/ul	99
95) Dibenzo(a,h)anthracene	27.056	278	1876693	31.595	ng/ul	99
96) Benzo(g,h,i)perylene	27.968	276	1715597	31.513	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049374.D
 Acq On : 21 Jan 2025 20:58
 Operator : RC/JU
 Sample : PB166157BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS157

Quant Time: Jan 22 00:23:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 13 16:56:06 2025
 Response via : Initial Calibration




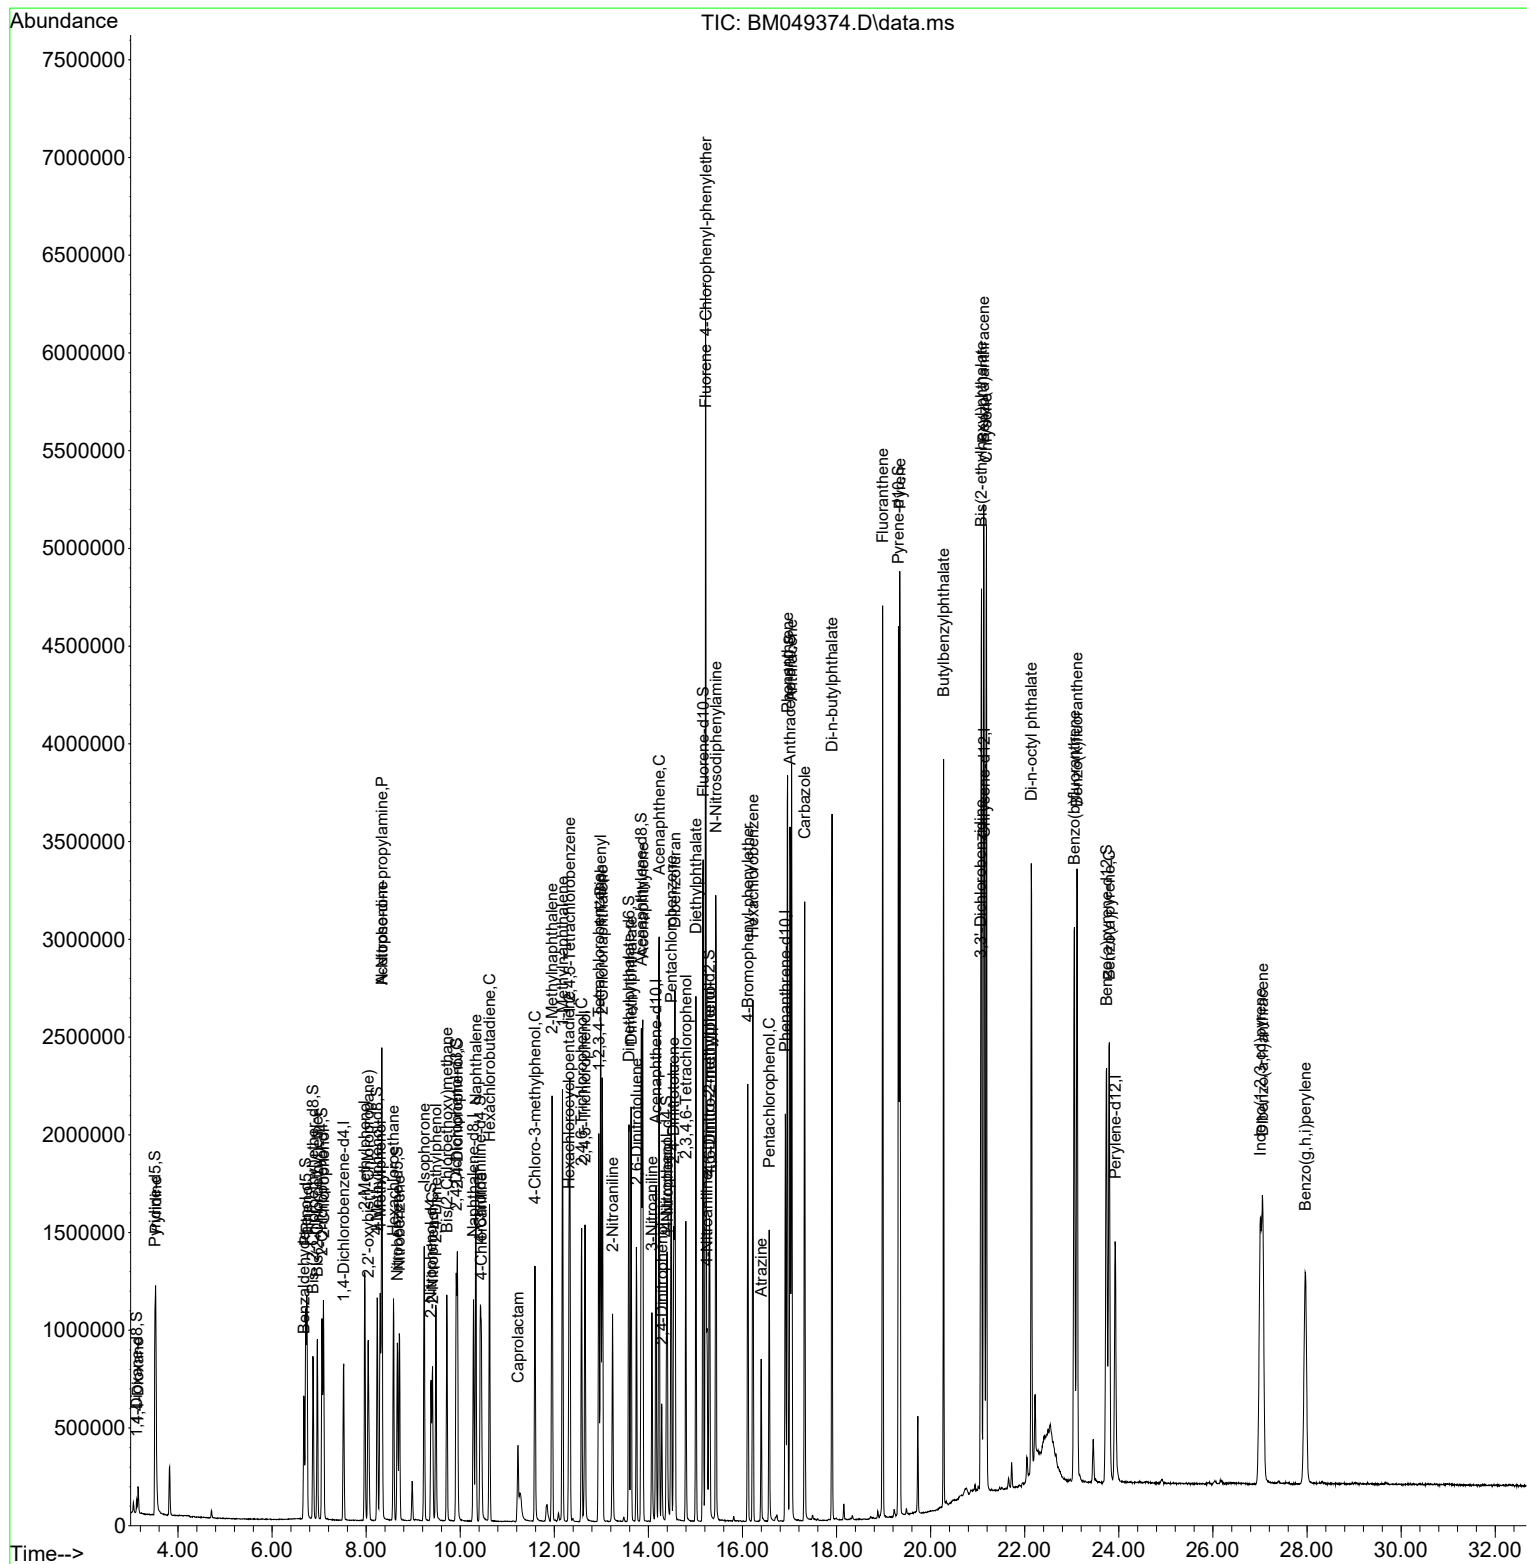




#2
1,4-Dioxane
Concen: 11.788 ng/uL
RT: 3.151 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion: 88 Resp: 67766
Ion Ratio Lower Upper
88 100
43 33.3 22.7 34.1
58 81.4 61.3 91.9

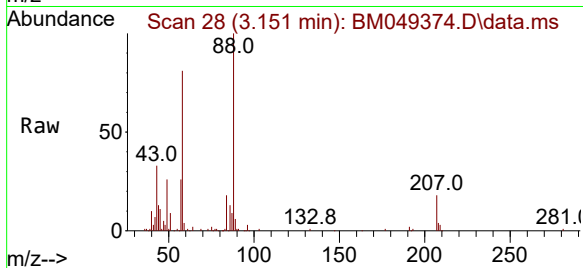

#5
Pyridine
Concen: 29.348 ng/uL
RT: 3.528 min Scan# 92
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 79 Resp: 495572
Ion Ratio Lower Upper
79 100
52 80.9 61.2 91.8
51 36.7 28.2 42.4



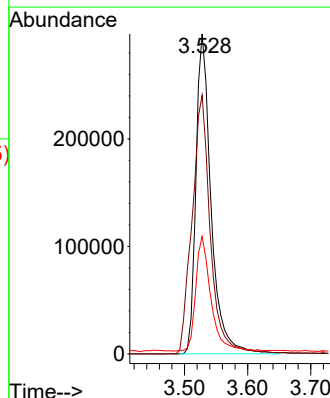
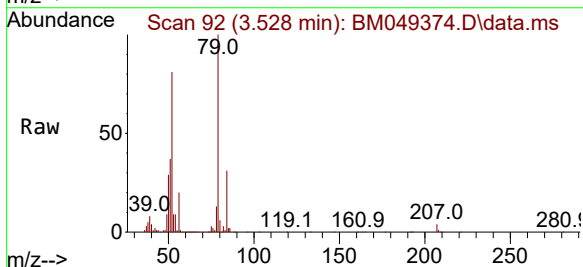




#6
Benzaldehyde
Concen: 21.697 ng/ul
RT: 6.675 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion: 77 Resp: 213178
Ion Ratio Lower Upper
77 100
105 90.9 73.4 110.0
106 87.6 71.3 106.9



#8
Phenol
Concen: 29.514 ng/ul
RT: 6.739 min Scan# 638
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 94 Resp: 559241
Ion Ratio Lower Upper
94 100
65 29.6 22.8 34.2
66 35.1 27.5 41.3









#10
Bis(2-Chloroethyl)ether
Concen: 29.524 ng/ul
RT: 6.963 min Scan# 610
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion: 93 Resp: 455564
Ion Ratio Lower Upper
93 100
63 80.8 63.9 95.9
95 32.5 25.9 38.9

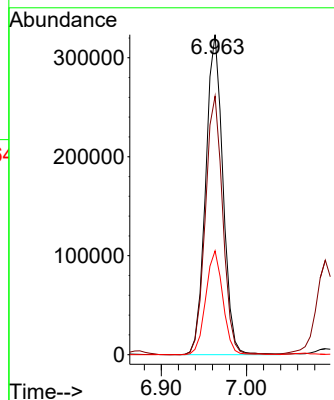

#12
2-Chlorophenol
Concen: 29.882 ng/ul
RT: 7.092 min Scan# 698
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 128 Resp: 433041
Ion Ratio Lower Upper
128 100
64 51.2 39.4 59.0
130 31.8 26.0 39.0



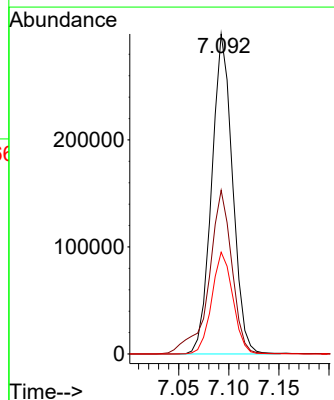





#13
2-Methylphenol
Concen: 28.023 ng/ul
RT: 7.969 min Scan# 847
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:108 Resp: 387947
Ion Ratio Lower Upper
108 100
107 86.9 72.0 108.0



#14
2,2'-oxybis(1-Chloropropane)
Concen: 30.946 ng/ul
RT: 8.045 min Scan# 860
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 45 Resp: 715641
Ion Ratio Lower Upper
45 100
77 14.0 10.9 16.3
79 9.9 8.2 12.2









#16
Acetophenone
Concen: 29.605 ng/ul
RT: 8.333 min Scan# 909
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:105 Resp: 683336
Ion Ratio Lower Upper
105 100
77 81.9 63.2 94.8
51 29.0 20.9 31.3



#17
N-Nitroso-di-n-propylamine
Concen: 29.993 ng/ul
RT: 8.333 min Scan# 909
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 70 Resp: 373925
Ion Ratio Lower Upper
70 100
42 57.3 43.8 65.6
101 8.8 7.0 10.6
130 18.6 15.4 23.0









#18
4-Methylphenol
Concen: 28.156 ng/ul
RT: 8.298 min Scan# 903
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:108 Resp: 427059
Ion Ratio Lower Upper
108 100
107 110.6 88.0 132.0



#19
Hexachloroethane
Concen: 30.351 ng/ul
RT: 8.581 min Scan# 951
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:117 Resp: 188985
Ion Ratio Lower Upper
117 100
201 115.5 95.9 143.9
199 71.6 57.9 86.9









#22
Nitrobenzene
Concen: 30.935 ng/ul
RT: 8.704 min Scan# 91
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion: 77 Resp: 515884
Ion Ratio Lower Upper
77 100
123 42.0 34.2 51.4
65 12.4 10.6 15.8

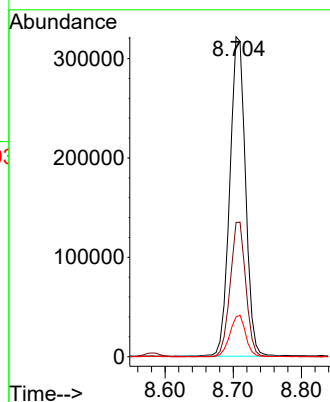

#23
Isophorone
Concen: 28.991 ng/ul
RT: 9.233 min Scan# 1062
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 82 Resp: 939399
Ion Ratio Lower Upper
82 100
95 6.4 5.0 7.6
138 17.0 13.4 20.0







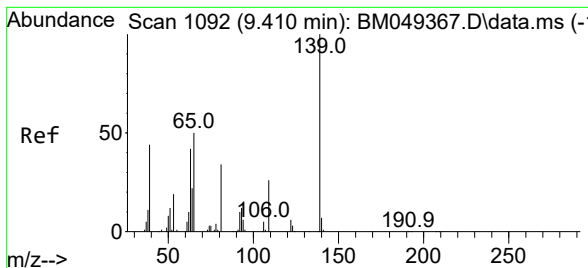

#25
2-Nitrophenol
Concen: 29.527 ng/ul
RT: 9.410 min Scan# 1092
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:139 Resp: 233524
Ion Ratio Lower Upper
139 100
65 53.0 40.7 61.1
109 26.5 21.4 32.0

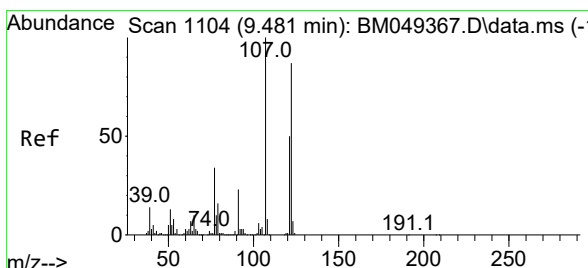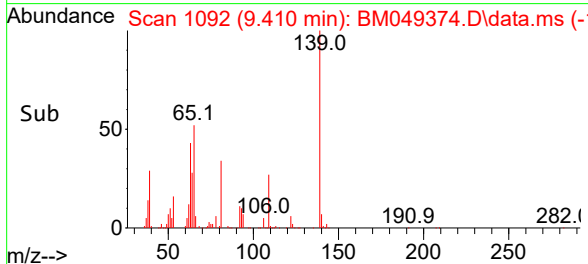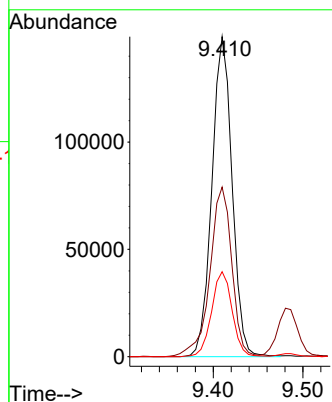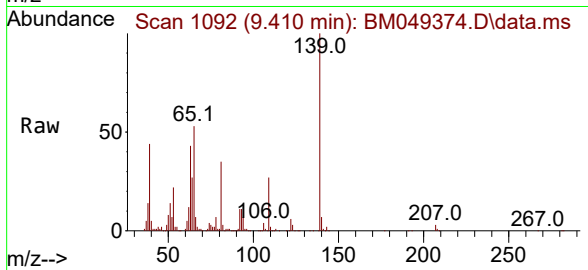

#26
2,4-Dimethylphenol
Concen: 24.486 ng/ul
RT: 9.480 min Scan# 1104
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:107 Resp: 362430
Ion Ratio Lower Upper
107 100
121 50.0 40.4 60.6
122 85.1 70.8 106.2


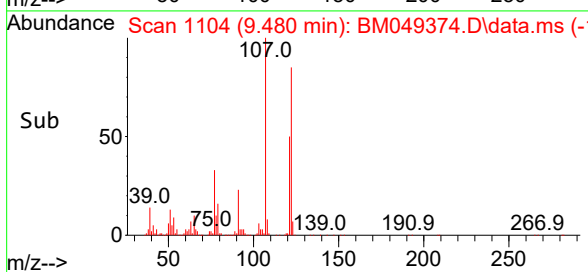
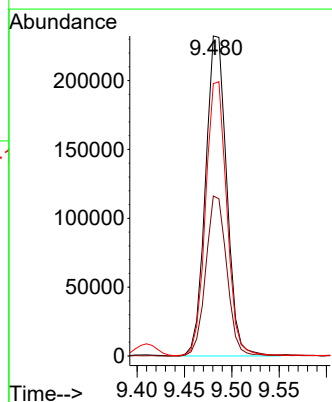
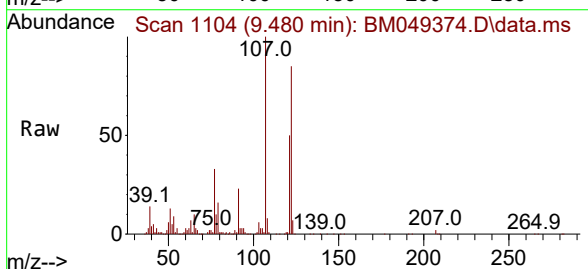


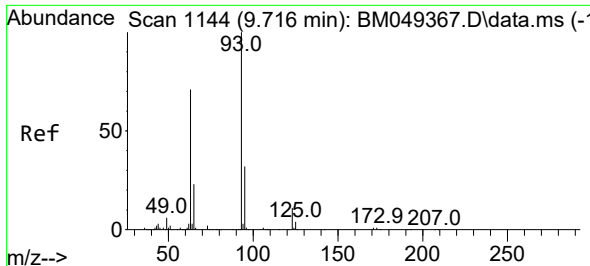

#27
 Bis(2-Chloroethoxy)methane
 Concen: 30.260 ng/ul
 RT: 9.716 min Scan# 1144
 Delta R.T. -0.006 min
 Lab File: BM049374.D
 Acq: 21 Jan 2025 20:58




Instrument :
 BNA_M
 ClientSampleId :
 SLCS157


Tgt Ion: 93 Resp: 602647
 Ion Ratio Lower Upper
 93 100
 95 32.4 25.1 37.7
 123 10.8 8.7 13.1

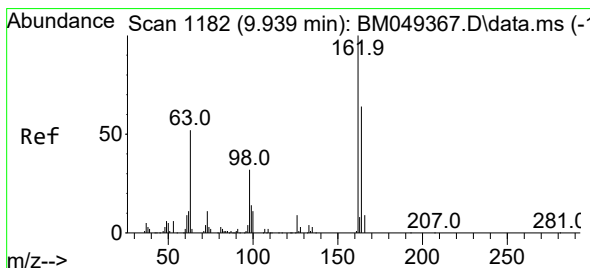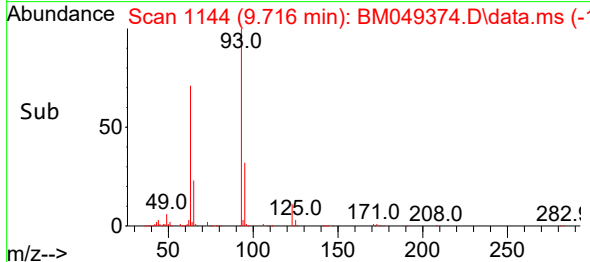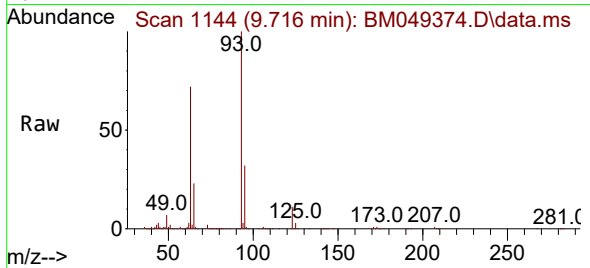

#29
 2,4-Dichlorophenol
 Concen: 30.565 ng/ul
 RT: 9.939 min Scan# 1182
 Delta R.T. -0.006 min
 Lab File: BM049374.D
 Acq: 21 Jan 2025 20:58

Tgt Ion: 162 Resp: 447151
 Ion Ratio Lower Upper
 162 100
 164 65.8 51.8 77.8
 98 33.3 26.5 39.7


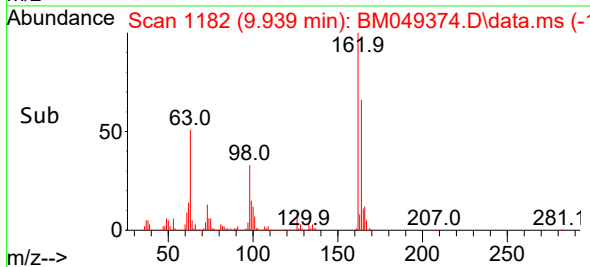

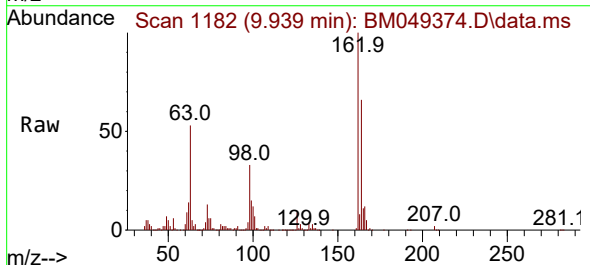




#30
Naphthalene
Concen: 30.528 ng/ul
RT: 10.333 min Scan# 1249
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:128 Resp: 1367612
Ion Ratio Lower Upper
128 100
129 10.6 8.5 12.7
127 12.8 10.2 15.2

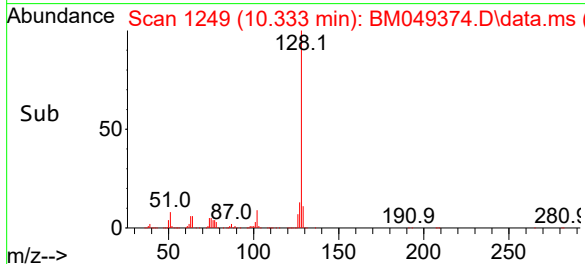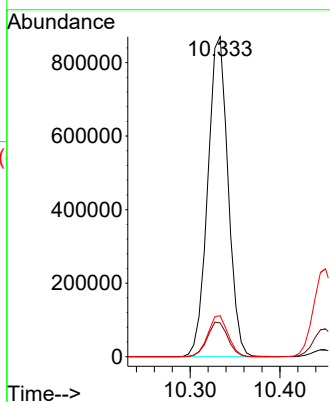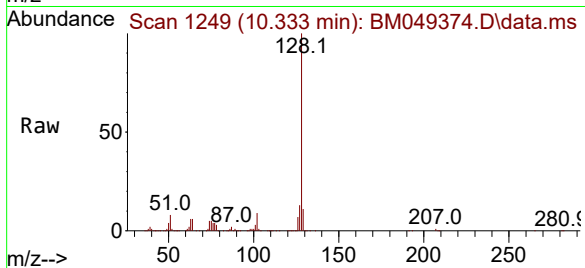

#32
4-Chloroaniline
Concen: 22.571 ng/ul
RT: 10.451 min Scan# 1269
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:127 Resp: 415878
Ion Ratio Lower Upper
127 100
129 31.5 25.7 38.5


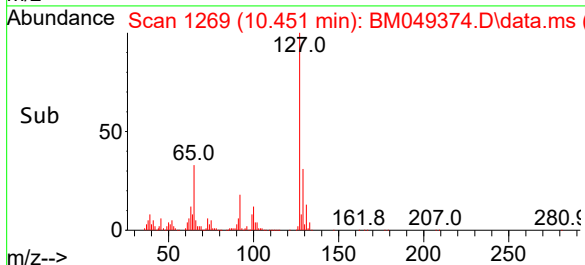

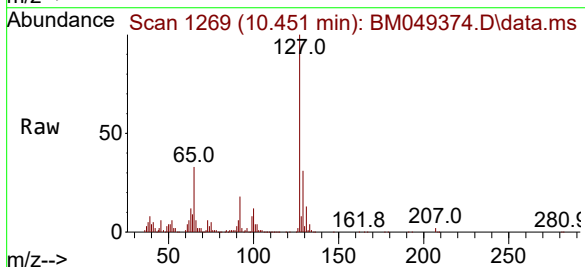




#33
Hexachlorobutadiene
Concen: 31.031 ng/ul
RT: 10.622 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:225 Resp: 324137
Ion Ratio Lower Upper
225 100
223 64.1 50.4 75.6
227 65.0 52.0 78.0



#34
Caprolactam
Concen: 15.254 ng/ul
RT: 11.227 min Scan# 1401
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:113 Resp: 66436
Ion Ratio Lower Upper
113 100
55 187.3 155.1 232.7
56 140.0 114.8 172.2









#35
4-Chloro-3-methylphenol
Concen: 30.185 ng/ul
RT: 11.586 min Scan# 1462
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:107 Resp: 412892
Ion Ratio Lower Upper
107 100
144 27.4 21.8 32.8
142 83.6 67.3 100.9

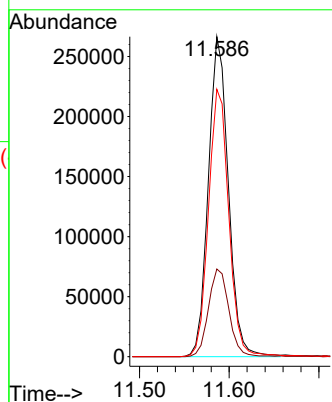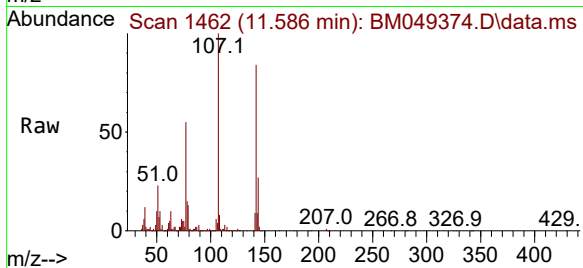

#36
2-Methylnaphthalene
Concen: 30.667 ng/ul
RT: 11.951 min Scan# 1524
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:142 Resp: 983107
Ion Ratio Lower Upper
142 100
141 88.9 69.6 104.4

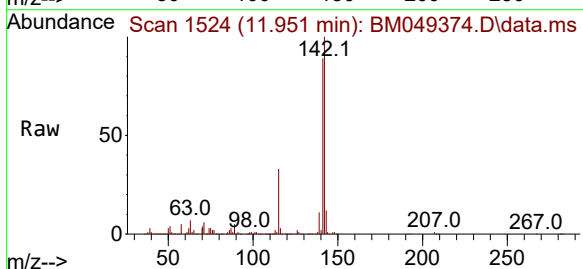



#37

1-Methylnaphthalene

Concen: 30.798 ng/ul

RT: 12.174 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:142 Resp: 982356

Ion Ratio Lower Upper

142 100

141 92.7 71.9 107.9

116 3.7 2.8 4.2

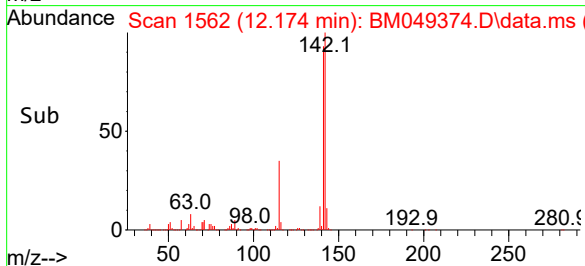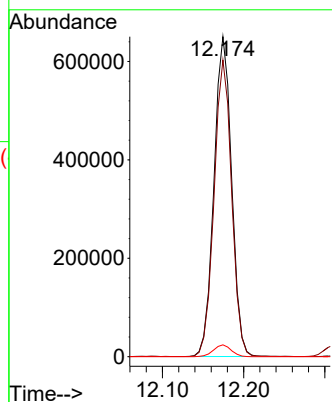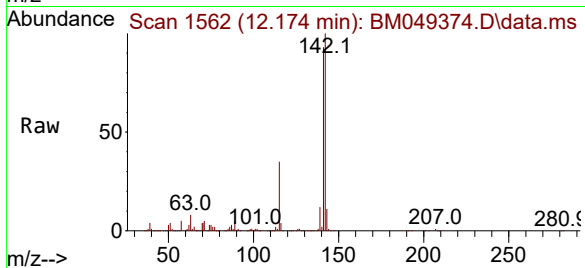

#39

1,2,4,5-Tetrachlorobenzene

Concen: 30.615 ng/ul

RT: 12.327 min Scan# 1588

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Tgt Ion:216 Resp: 629168




Ion Ratio Lower Upper


216 100

214 78.0 63.4 95.2

179 19.9 15.7 23.5

108 14.7 11.4 17.2


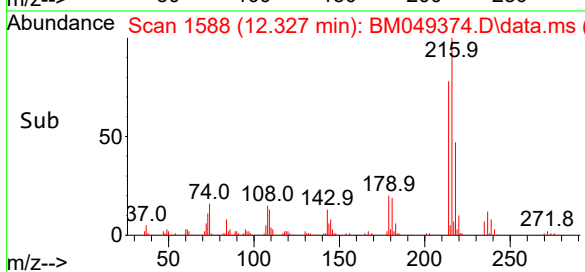

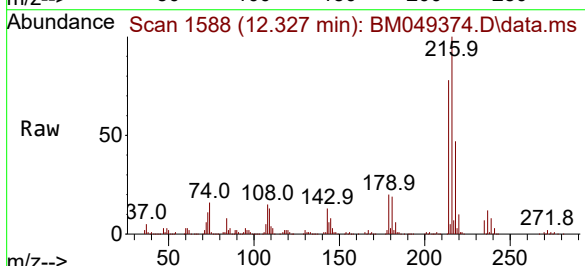




#40
Hexachlorocyclopentadiene
Concen: 23.949 ng/ul
RT: 12.310 min Scan# 1585
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:237 Resp: 295284
Ion Ratio Lower Upper
237 100
235 62.9 49.9 74.9
272 12.6 11.2 16.8



#41
2,4,6-Trichlorophenol
Concen: 27.322 ng/ul
RT: 12.580 min Scan# 1631
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:196 Resp: 345409
Ion Ratio Lower Upper
196 100
198 98.3 76.4 114.6
200 32.2 24.2 36.4





#42

2,4,5-Trichlorophenol

Concen: 28.948 ng/ul

RT: 12.651 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:196 Resp: 392238

Ion Ratio Lower Upper

196 100

198 95.5 78.2 117.4

200 30.8 24.9 37.3



#43

1,1'-Biphenyl

Concen: 30.846 ng/ul

RT: 12.986 min Scan# 1700

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:154 Resp: 1340843


Ion Ratio Lower Upper

154 100

153 39.6 31.0 46.4

76 12.9 9.1 13.7







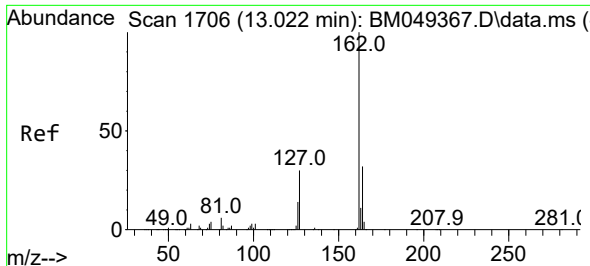

#44
2-Chloronaphthalene
Concen: 31.173 ng/ul
RT: 13.021 min Scan# 1706
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:162 Resp: 1083677
Ion Ratio Lower Upper
162 100
164 33.1 26.8 40.2
127 33.1 27.8 41.8

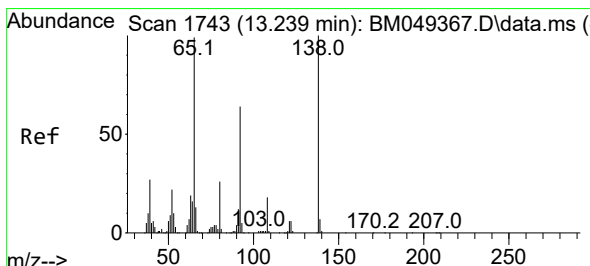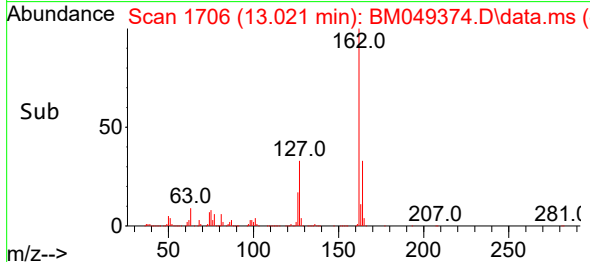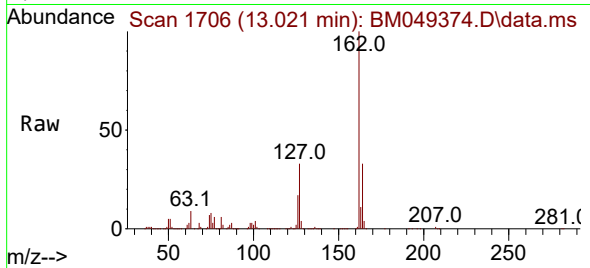

#45
2-Nitroaniline
Concen: 31.685 ng/ul
RT: 13.239 min Scan# 1743
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion: 65 Resp: 290646
Ion Ratio Lower Upper
65 100
92 66.5 52.5 78.7
138 99.9 80.4 120.6


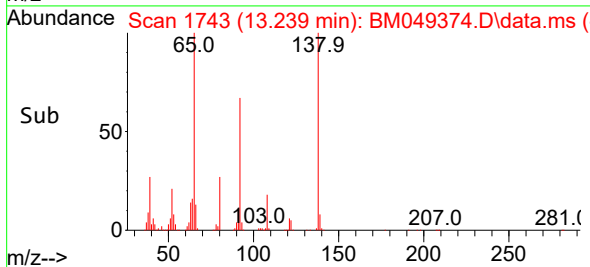

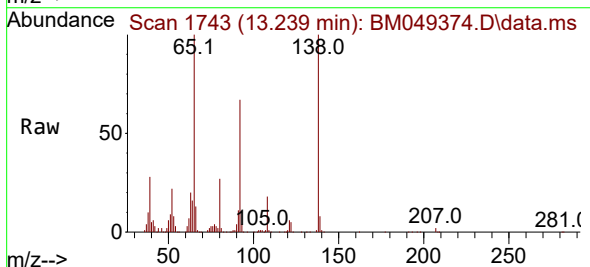




#47
Dimethylphthalate
Concen: 30.381 ng/ul
RT: 13.633 min Scan# 1810
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:163 Resp: 1328040
Ion Ratio Lower Upper
163 100
194 4.3 3.3 4.9
164 10.3 8.2 12.4

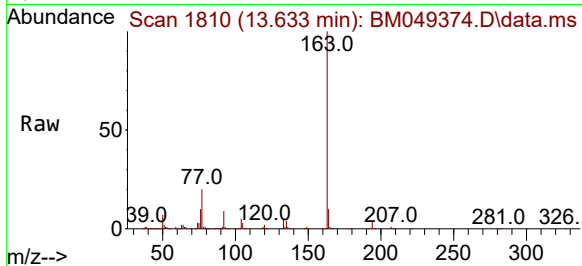

#48
2,6-Dinitrotoluene
Concen: 30.795 ng/ul
RT: 13.745 min Scan# 1829
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:165 Resp: 251143
Ion Ratio Lower Upper
165 100
89 58.9 43.2 64.8
121 20.1 16.2 24.2

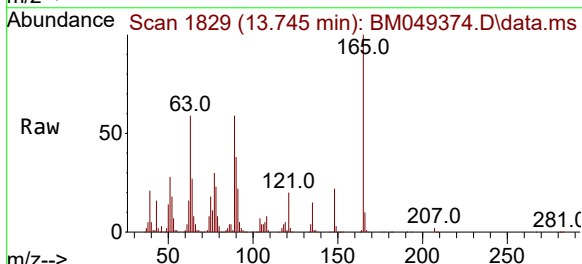

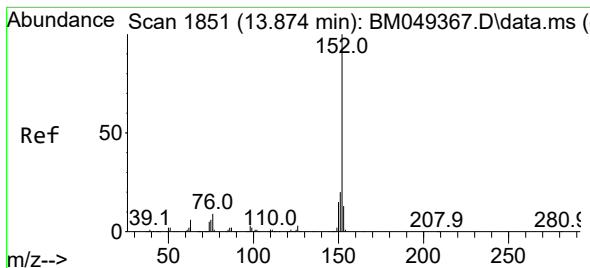

#50

Acenaphthylene

Concen: 31.930 ng/ul

RT: 13.880 min Scan# 1852

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:152 Resp: 1651328

Ion Ratio Lower Upper

152 100

151 19.6 15.8 23.8

153 13.0 10.6 15.8

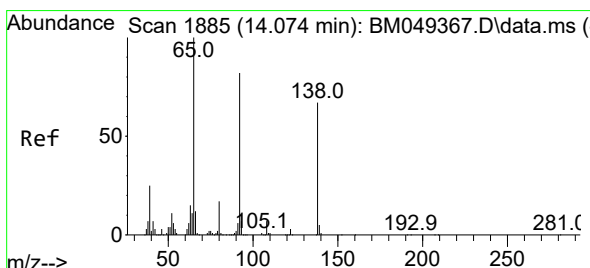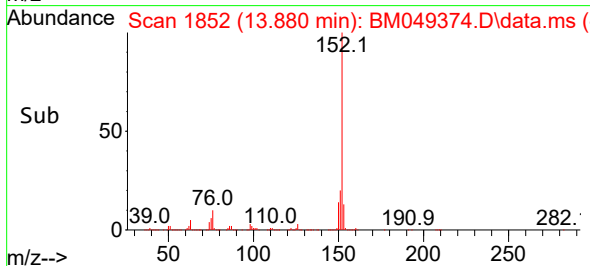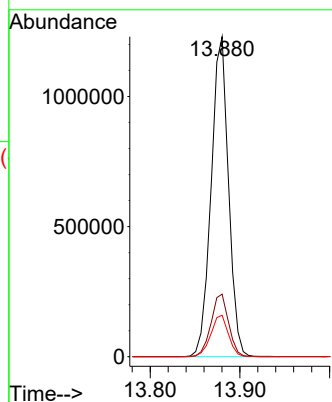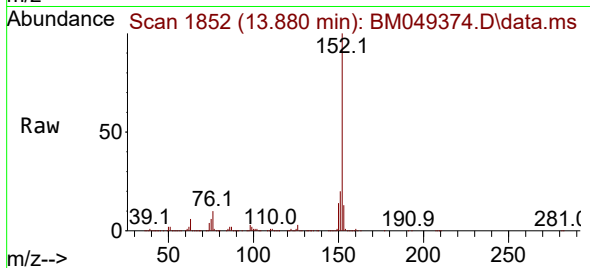

#51

3-Nitroaniline

Concen: 28.916 ng/ul

RT: 14.074 min Scan# 1885

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:138 Resp: 231372


Ion Ratio Lower Upper

138 100

108 9.7 8.0 12.0

92 117.6 91.8 137.6


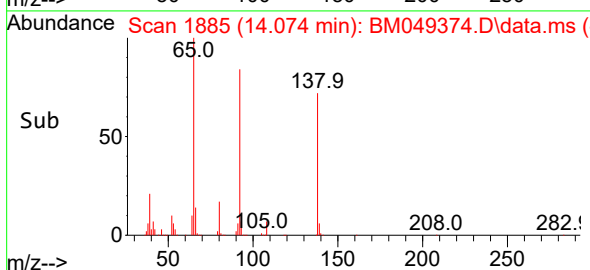

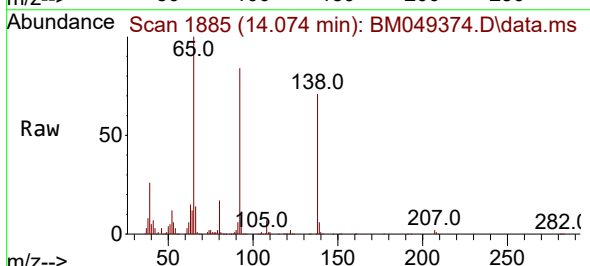


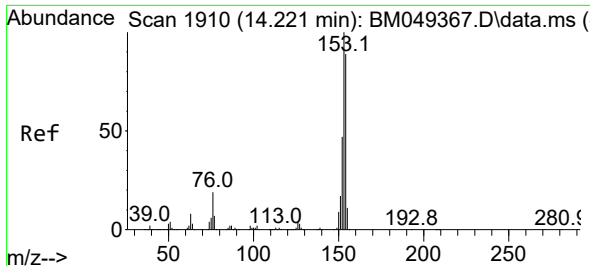

#52
Acenaphthene
Concen: 31.372 ng/ul
RT: 14.227 min Scan# 1910
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:153 Resp: 1159216
Ion Ratio Lower Upper
153 100
152 48.2 39.0 58.6
154 89.1 71.6 107.4

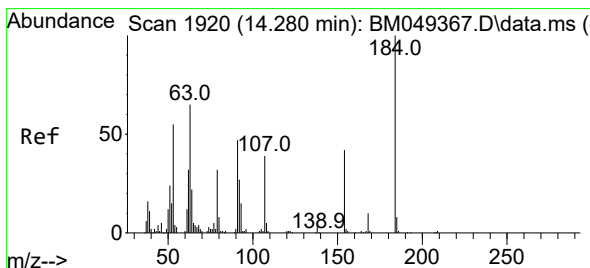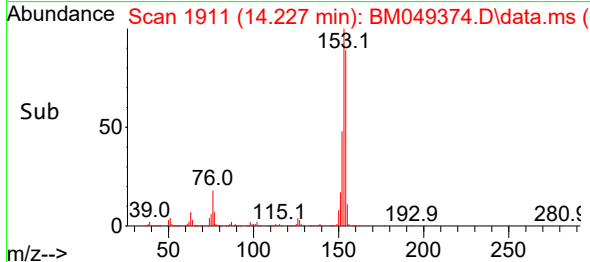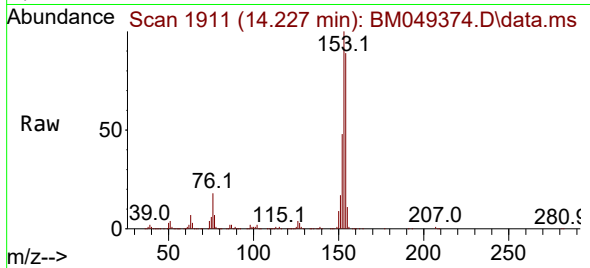

#53
2,4-Dinitrophenol
Concen: 23.743 ng/ul
RT: 14.286 min Scan# 1921
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:184 Resp: 121271
Ion Ratio Lower Upper
184 100
63 60.4 49.5 74.3
154 53.8 47.2 70.8


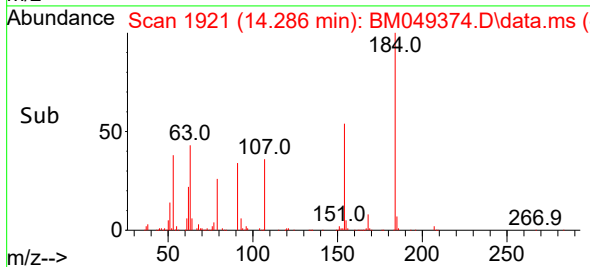

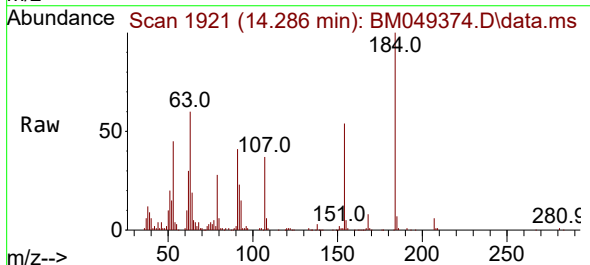




#55
4-Nitrophenol
Concen: 28.620 ng/ul
RT: 14.404 min Scan# 1940
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:109 Resp: 154436
Ion Ratio Lower Upper
109 100
139 149.2 115.7 173.5
65 148.4 119.0 178.6



#56
Dibenzofuran
Concen: 31.975 ng/ul
RT: 14.563 min Scan# 1968
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:168 Resp: 1677786
Ion Ratio Lower Upper
168 100
139 34.3 27.0 40.4





#57

2,4-Dinitrotoluene

Concen: 31.852 ng/ul

RT: 14.539 min Scan# 1964

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:165 Resp: 385472

Ion Ratio Lower Upper

165 100

63 43.7 35.0 52.4

182 2.4 1.9 2.9



#58

2,3,4,6-Tetrachlorophenol

Concen: 26.001 ng/ul

RT: 14.798 min Scan# 2008

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Tgt Ion:232 Resp: 297611




Ion Ratio Lower Upper


232 100

131 38.7 32.3 48.5

130 2.0 1.8 2.6

166 28.5 24.3 36.5



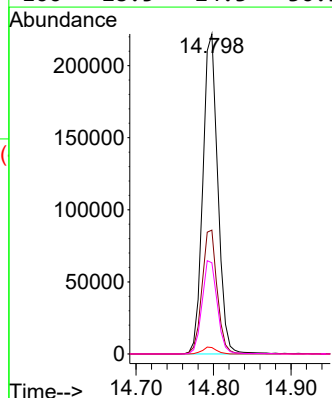





#59
Diethylphthalate
Concen: 31.687 ng/ul
RT: 15.010 min Scan# 2044
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:149 Resp: 1349940
Ion Ratio Lower Upper
149 100
177 22.6 18.9 28.3
150 12.2 9.4 14.2



#61
Fluorene
Concen: 34.080 ng/ul
RT: 15.215 min Scan# 2079
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:166 Resp: 1461045
Ion Ratio Lower Upper
166 100
165 98.3 77.7 116.5
167 13.8 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 33.337 ng/ul
RT: 15.221 min Scan# 2080
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:204 Resp: 778894
Ion Ratio Lower Upper
204 100
206 33.4 25.9 38.9
141 48.1 40.6 61.0



#63
4-Nitroaniline
Concen: 34.397 ng/ul
RT: 15.245 min Scan# 2084
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:138 Resp: 247635
Ion Ratio Lower Upper
138 100
92 50.8 42.0 63.0
108 71.1 60.3 90.5









#66
 4,6-Dinitro-2-methylphenol
 Concen: 28.785 ng/ul
 RT: 15.304 min Scan# 2094
 Delta R.T. -0.006 min
 Lab File: BM049374.D
 Acq: 21 Jan 2025 20:58




Instrument :
 BNA_M
 ClientSampleId :
 SLCS157


Tgt Ion:198 Resp: 243536
 Ion Ratio Lower Upper
 198 100
 182 4.3 3.5 5.3
 77 23.2 17.0 25.6



#67
 N-Nitrosodiphenylamine
 Concen: 31.749 ng/ul
 RT: 15.433 min Scan# 2116
 Delta R.T. -0.006 min
 Lab File: BM049374.D
 Acq: 21 Jan 2025 20:58

Tgt Ion:169 Resp: 1146955
 Ion Ratio Lower Upper
 169 100
 168 67.9 53.8 80.8
 167 37.2 29.7 44.5









#68
4-Bromophenyl-phenylether
Concen: 31.444 ng/ul
RT: 16.115 min Scan# 2111
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:248 Resp: 435326
Ion Ratio Lower Upper
248 100
250 97.7 78.1 117.1
141 60.9 49.8 74.6



#69
Hexachlorobenzene
Concen: 30.723 ng/ul
RT: 16.221 min Scan# 2250
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:284 Resp: 494687
Ion Ratio Lower Upper
284 100
142 32.0 24.3 36.5
249 30.6 24.6 37.0

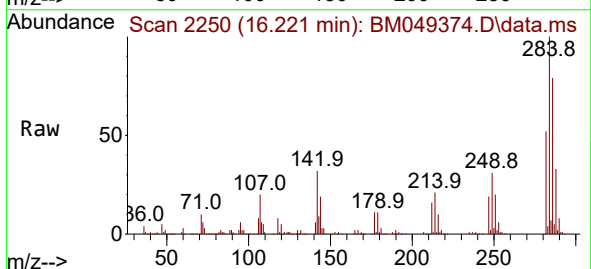



#70

Atrazine

Concen: 9.215 ng/ul

RT: 16.398 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:200 Resp: 136095

Ion Ratio Lower Upper

200 100

173 24.2 20.2 30.2

215 46.6 40.6 61.0

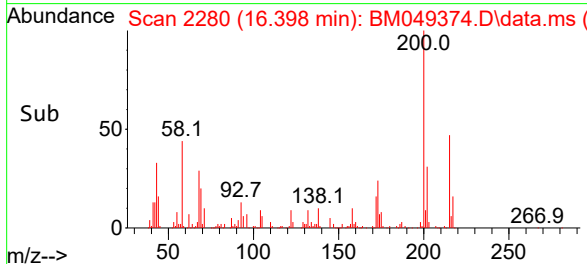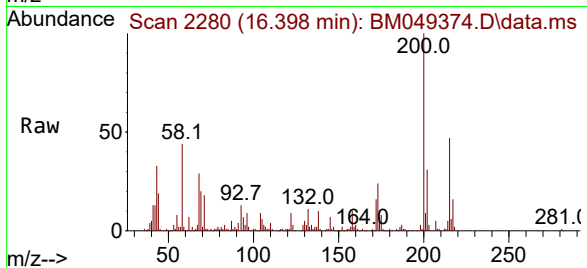

#71

Pentachlorophenol

Concen: 22.088 ng/ul

RT: 16.568 min Scan# 2309

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:266 Resp: 235613


Ion Ratio Lower Upper

266 100

264 61.1 48.6 72.8

268 63.2 49.4 74.0


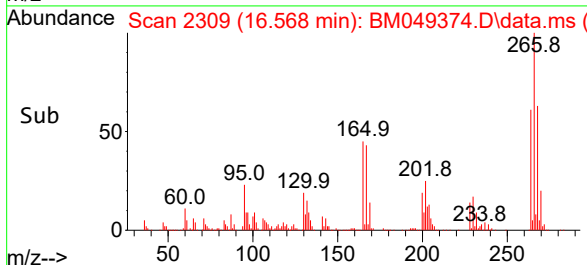

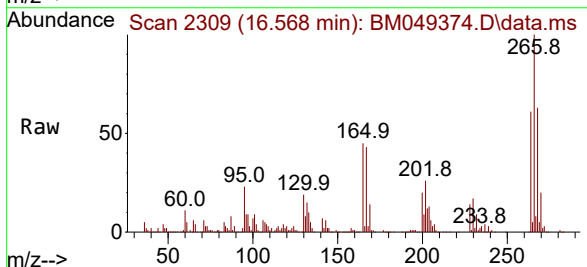




#72
Phenanthrene
Concen: 32.901 ng/uI
RT: 16.956 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:178 Resp: 2226977
Ion Ratio Lower Upper
178 100
179 15.4 12.6 19.0
176 19.3 15.4 23.2

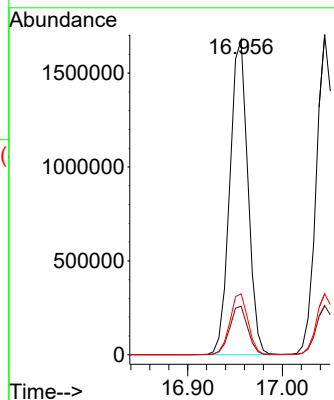

#74
Anthracene
Concen: 32.382 ng/uI
RT: 17.045 min Scan# 2390
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:178 Resp: 2200039
Ion Ratio Lower Upper
178 100
179 15.4 12.5 18.7
176 19.1 15.1 22.7

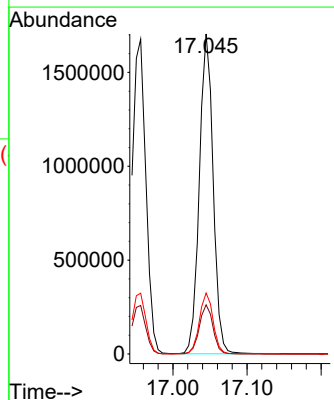



#75

1,2,3,4-Tetrachlorobenzene

Concen: 29.876 ng/uL

RT: 12.945 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:216 Resp: 607935

Ion Ratio Lower Upper

216 100

214 79.6 63.0 94.6

218 48.8 39.0 58.6

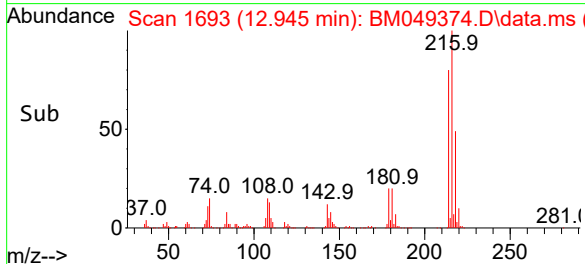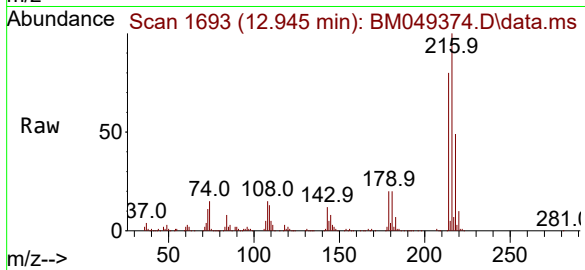

#76

Pentachlorobenzene

Concen: 28.426 ng/uL

RT: 14.486 min Scan# 1955

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:250 Resp: 577347


Ion Ratio Lower Upper

250 100

248 61.5 50.5 75.7

252 63.9 50.5 75.7


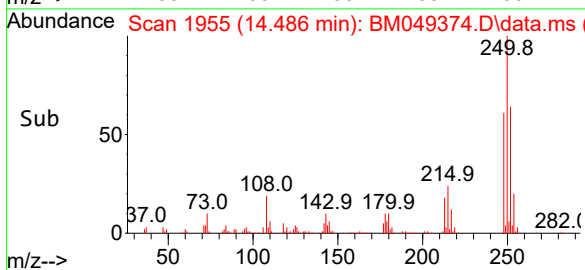

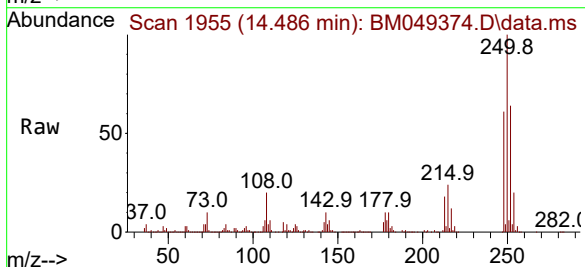


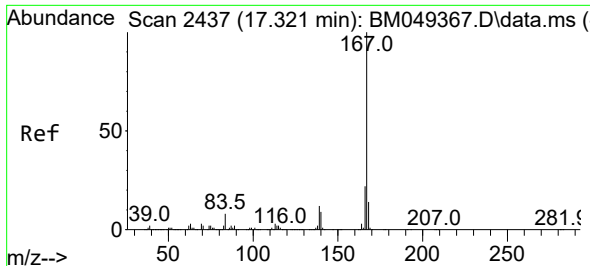

#77
 Carbazole
 Concen: 31.586 ng/ul
 RT: 17.321 min Scan# 2437
 Delta R.T. -0.006 min
 Lab File: BM049374.D
 Acq: 21 Jan 2025 20:58




Instrument :
 BNA_M
 ClientSampleId :
 SLCS157


Tgt Ion:167 Resp: 1903995
 Ion Ratio Lower Upper
 167 100
 166 21.6 16.7 25.1
 139 11.7 9.5 14.3

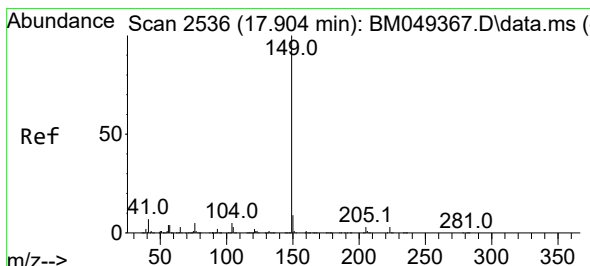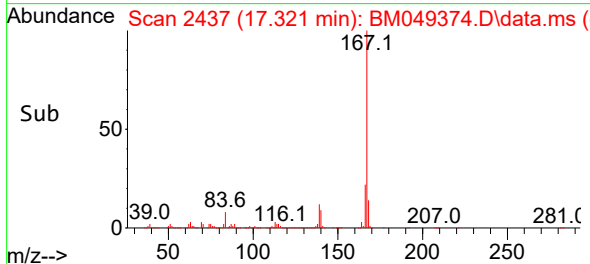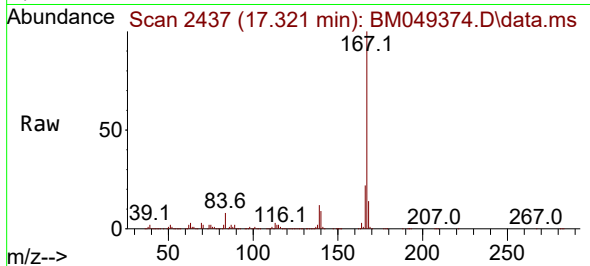

#78
 Di-n-butylphthalate
 Concen: 32.078 ng/ul
 RT: 17.903 min Scan# 2536
 Delta R.T. -0.006 min
 Lab File: BM049374.D
 Acq: 21 Jan 2025 20:58

Tgt Ion:149 Resp: 2369275
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.1 10.7
 104 4.8 3.7 5.5

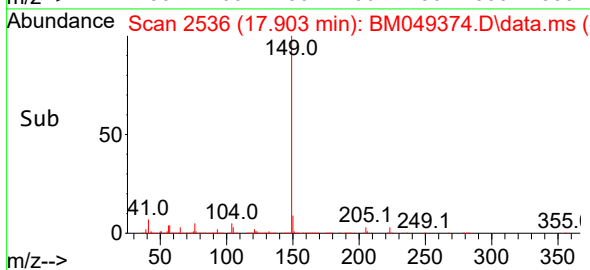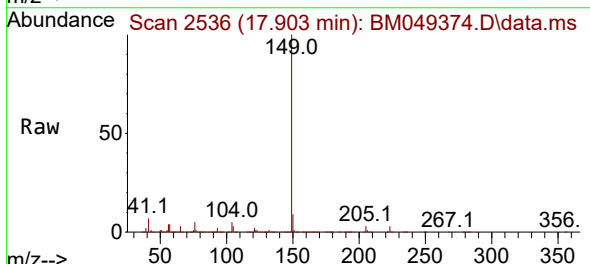



#80

Fluoranthene

Concen: 31.447 ng/ul

RT: 18.980 min Scan# 2719

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:202 Resp: 2573024

Ion Ratio Lower Upper

202 100

101 9.2 7.0 10.4

100 7.3 5.0 7.6

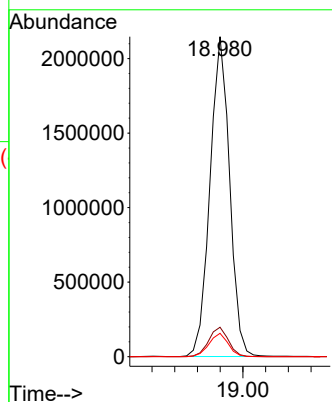

#82

Pyrene

Concen: 31.540 ng/ul

RT: 19.345 min Scan# 2781

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:202 Resp: 2747000


Ion Ratio Lower Upper

202 100

101 11.4 7.8 11.8

100 9.2 6.6 10.0

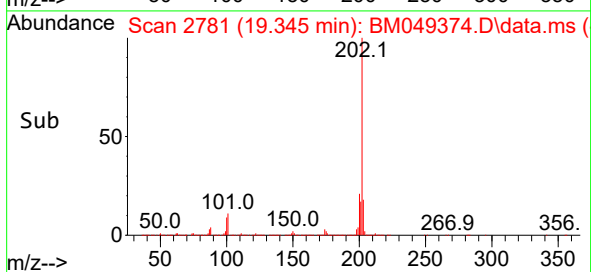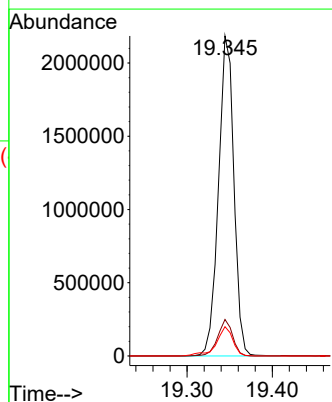



#83

Butylbenzylphthalate

Concen: 30.982 ng/ul

RT: 20.274 min Scan# 2939

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:149 Resp: 955333

Ion Ratio Lower Upper

149 100

91 70.0 57.0 85.4

206 21.5 17.0 25.6

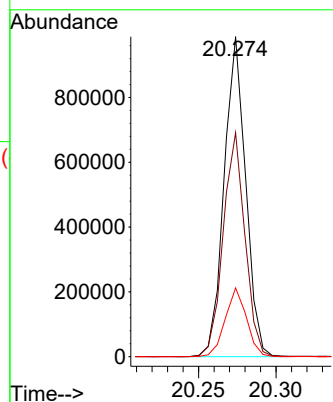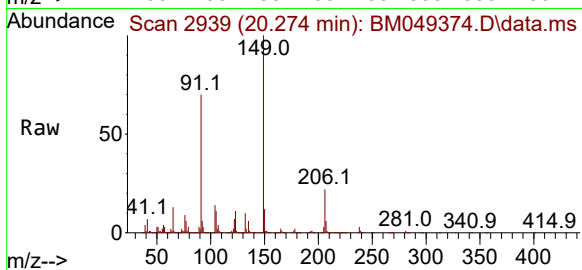

#84

3,3'-Dichlorobenzidine

Concen: 29.811 ng/ul

RT: 21.062 min Scan# 3073

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:252 Resp: 653126


Ion Ratio Lower Upper

252 100

254 65.1 52.1 78.1

126 9.8 7.0 10.6

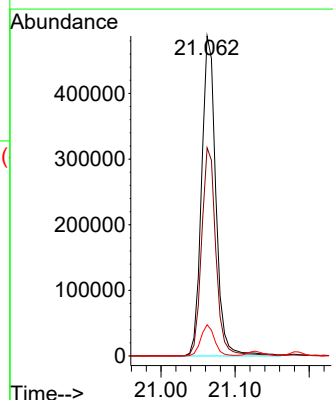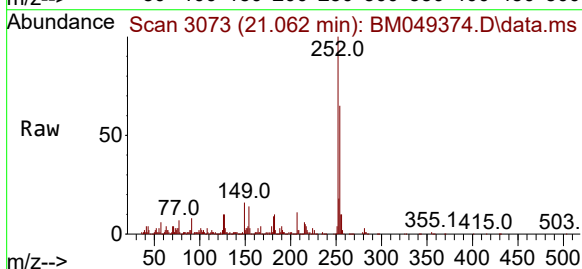



#85

Benzo(a)anthracene

Concen: 31.797 ng/ul

RT: 21.127 min Scan# 3084

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:228 Resp: 2592619

Ion Ratio Lower Upper

228 100

229 19.8 15.8 23.6

226 27.7 22.1 33.1

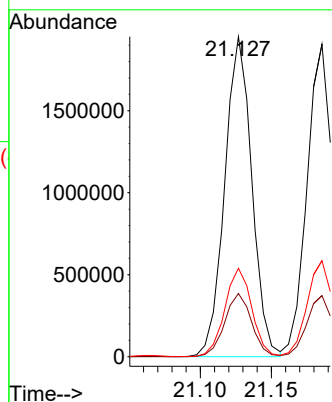

#86

Bis(2-ethylhexyl)phthalate

Concen: 31.693 ng/ul

RT: 21.080 min Scan# 3076

Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:149 Resp: 1453390


Ion Ratio Lower Upper

149 100

167 28.1 23.0 34.4

279 3.9 3.7 5.5





#87

Chrysene

Concen: 32.285 ng/ul

RT: 21.186 min Scan# 3094

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:228 Resp: 2403137

Ion Ratio Lower Upper

228 100

226 30.7 24.3 36.5

229 19.6 16.0 24.0

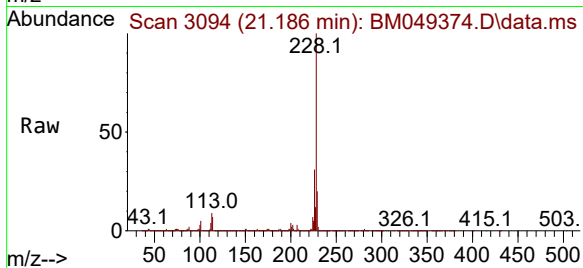

#89

Di-n-octyl phthalate

Concen: 28.677 ng/ul




RT: 22.138 min Scan# 3256


Delta R.T. -0.006 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Tgt Ion:149 Resp: 2196850




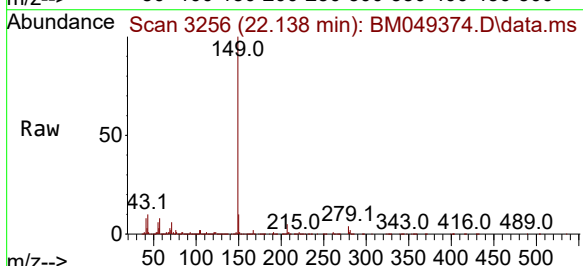




#90
Benzo(b)fluoranthene
Concen: 33.045 ng/ul
RT: 23.056 min Scan# 3411
Delta R.T. -0.000 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58




Instrument :
BNA_M
ClientSampleId :
SLCS157


Tgt Ion:252 Resp: 2325818
Ion Ratio Lower Upper
252 100
253 21.6 17.4 26.2
125 7.9 6.6 9.8



#91
Benzo(k)fluoranthene
Concen: 34.121 ng/ul
RT: 23.109 min Scan# 3421
Delta R.T. -0.006 min
Lab File: BM049374.D
Acq: 21 Jan 2025 20:58

Tgt Ion:252 Resp: 2394539
Ion Ratio Lower Upper
252 100
253 22.2 17.6 26.4
125 8.3 6.5 9.7





#93

Benzo(a)pyrene

Concen: 31.335 ng/ul

RT: 23.797 min Scan# 3

Delta R.T. -0.000 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:252 Resp: 1992129

Ion Ratio Lower Upper

252 100

253 21.7 17.4 26.2

125 8.5 6.9 10.3

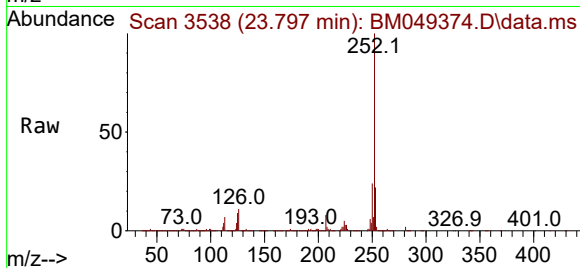

#94

Indeno(1,2,3-cd)pyrene

Concen: 30.875 ng/ul

RT: 27.009 min Scan# 4084

Delta R.T. -0.012 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58




Tgt Ion:276 Resp: 2251686


Ion Ratio Lower Upper

276 100

138 16.8 13.4 20.0

277 24.3 19.1 28.7

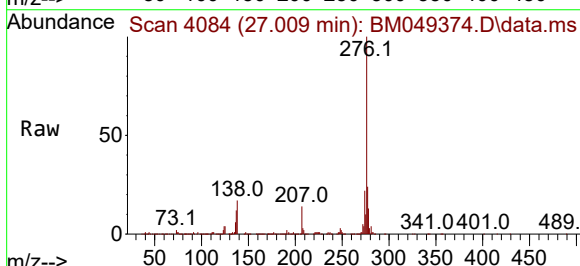



#95

Dibenzo(a,h)anthracene

Concen: 31.595 ng/ul

RT: 27.056 min Scan# 4093

Delta R.T. -0.018 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Instrument :

BNA_M

ClientSampleId :

SLCS157





Tgt Ion:278 Resp: 1876693

Ion Ratio Lower Upper

278 100

139 12.9 9.9 14.9

279 23.9 19.4 29.0

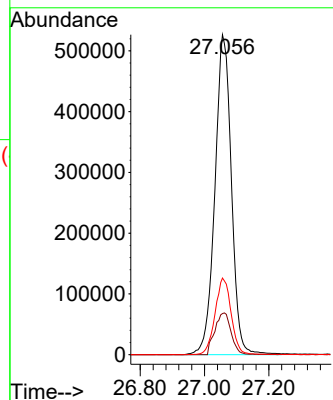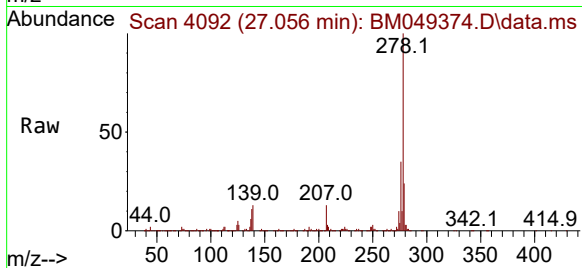

#96

Benzo(g,h,i)perylene

Concen: 31.513 ng/ul

RT: 27.968 min Scan# 4247

Delta R.T. -0.012 min

Lab File: BM049374.D

Acq: 21 Jan 2025 20:58

Tgt Ion:276 Resp: 1715597

Ion Ratio Lower Upper

276 100

138 17.8 14.1 21.1

277 23.9 19.4 29.0

