




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

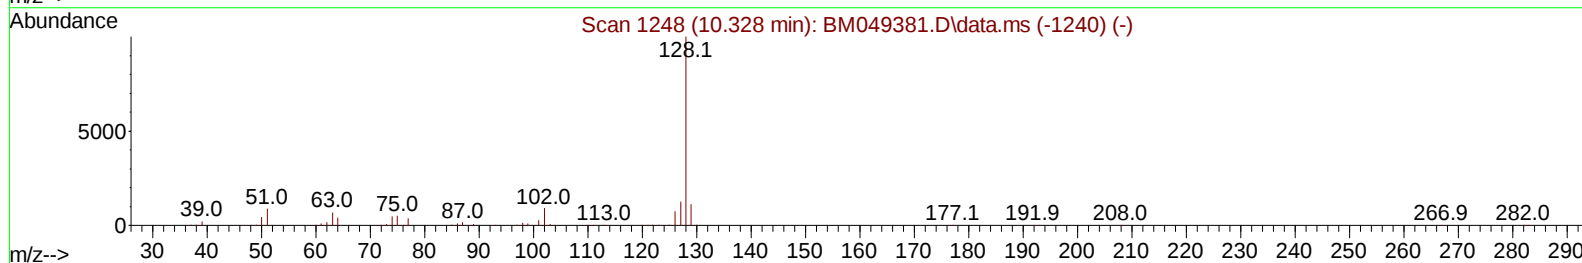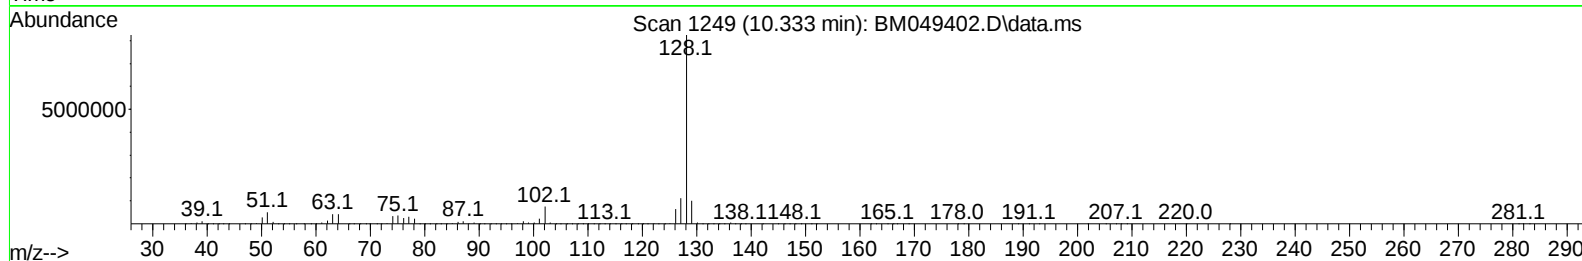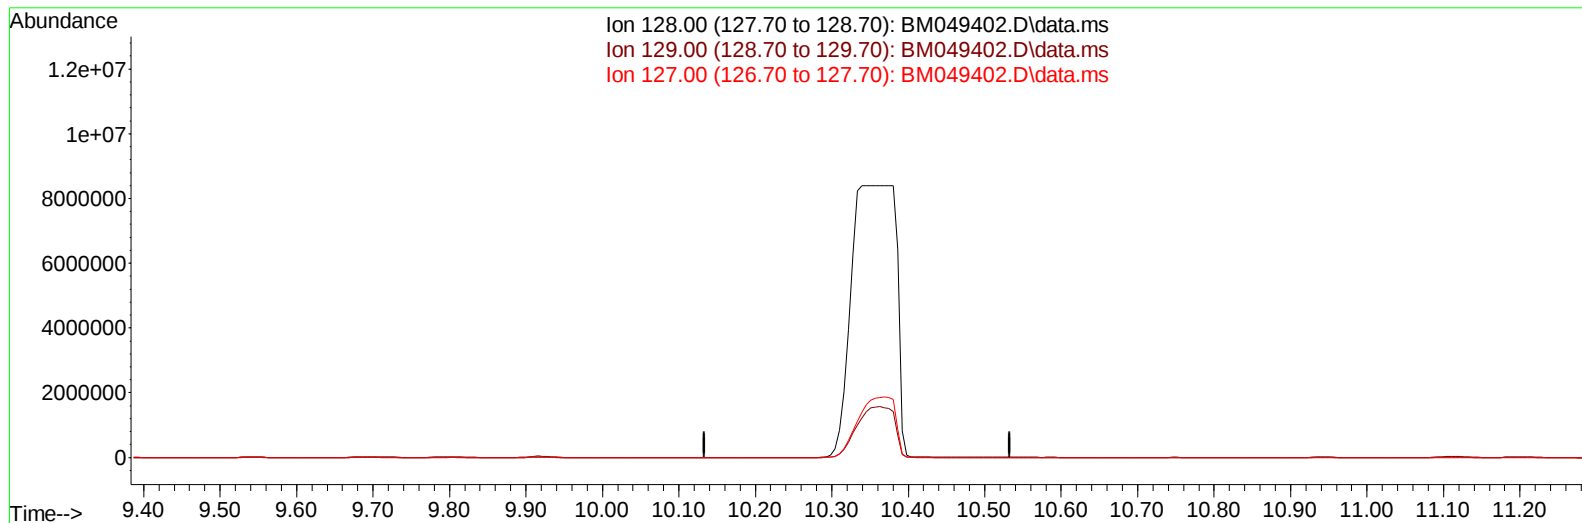

TIC: BM049402.D\data.ms

(30) Naphthalene

10.333min (-10.333) 0.00 ng/u1

response 0

Ion	Exp%	Act%
128.00	100.00	0.00
129.00	10.60	0.00#
127.00	12.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

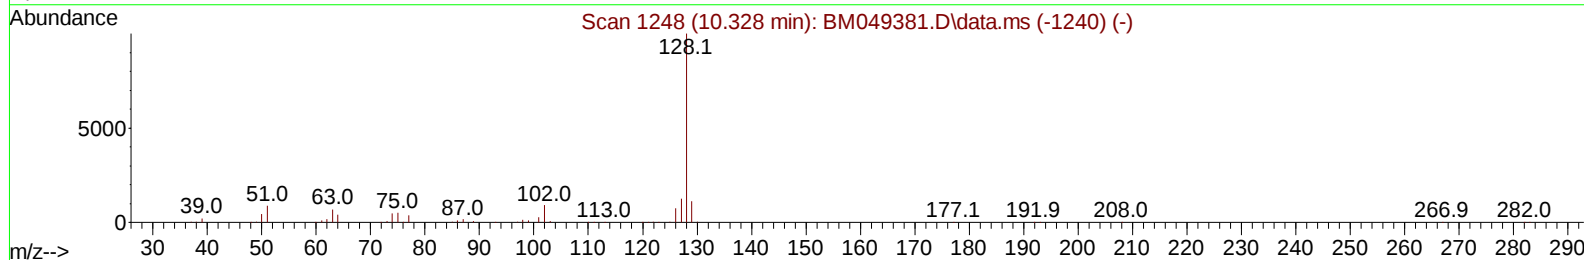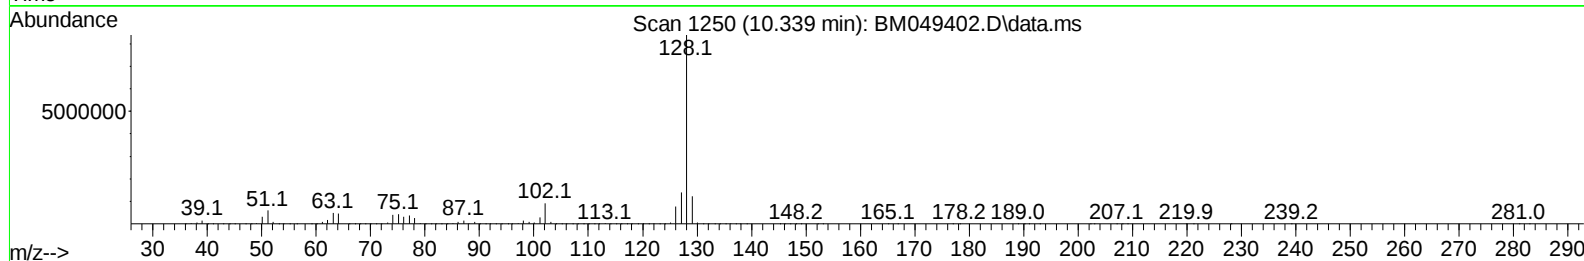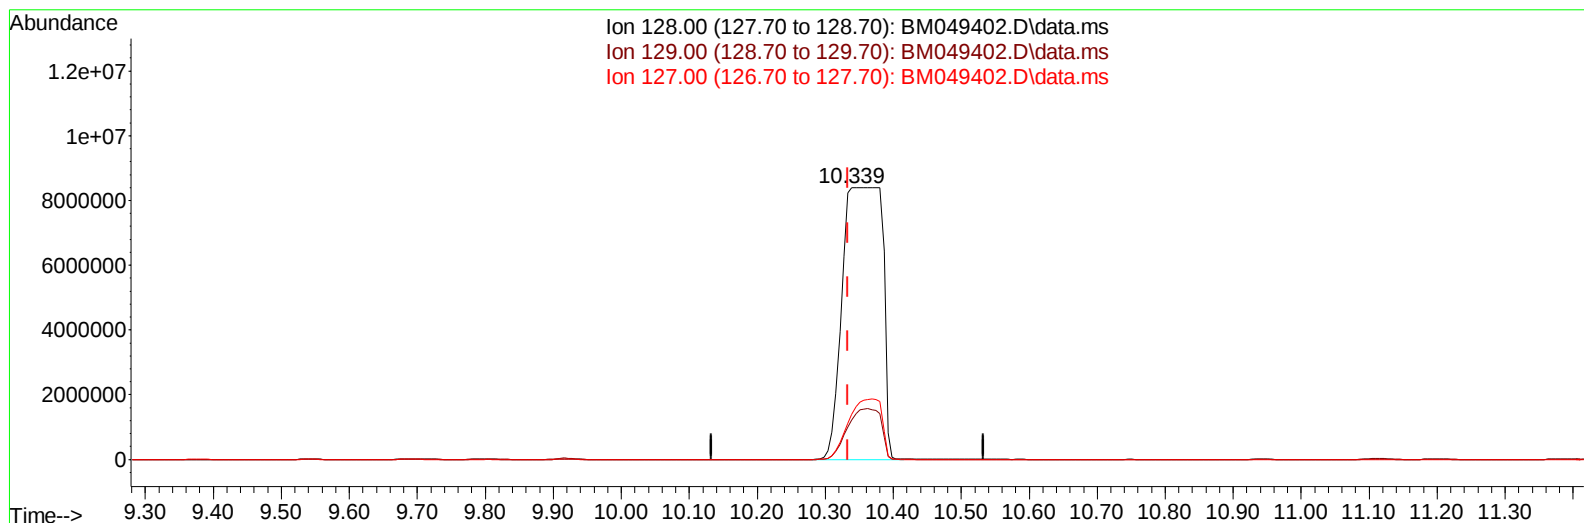

TIC: BM049402.D\data.ms

(30) Naphthalene

10.339min (+ 0.006) 350.69 ng/u1 m

response 33938977

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	10.60	14.57#
127.00	12.70	16.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

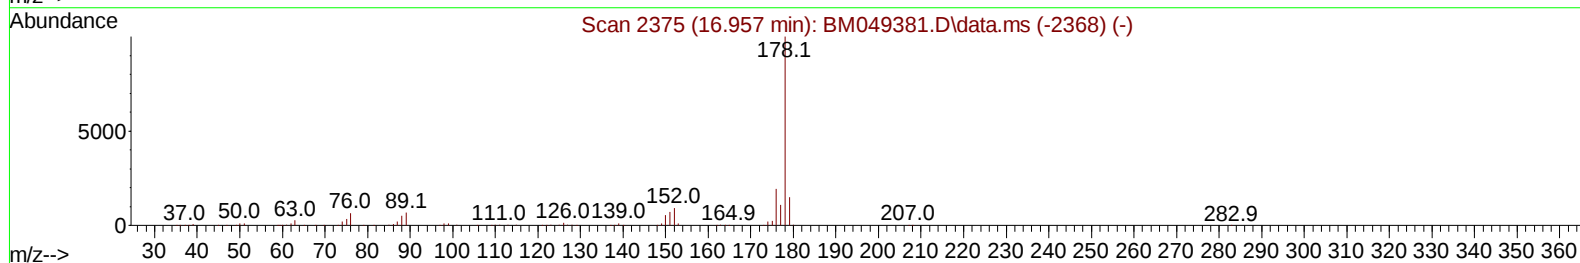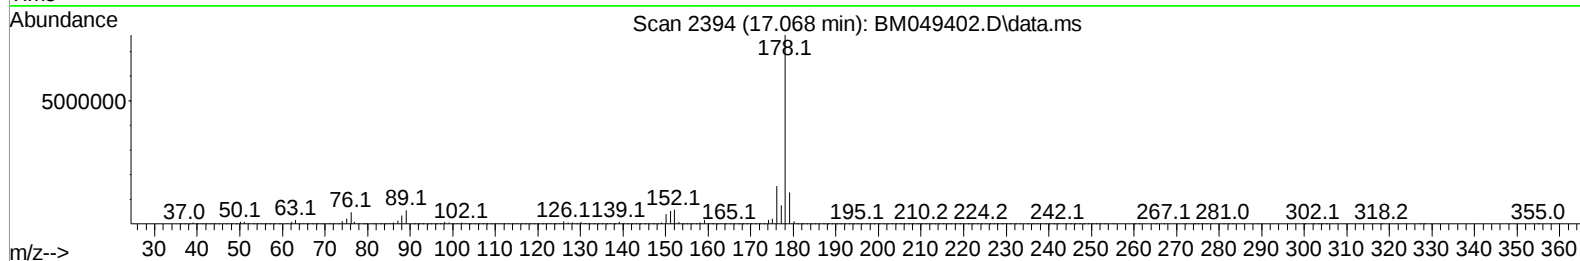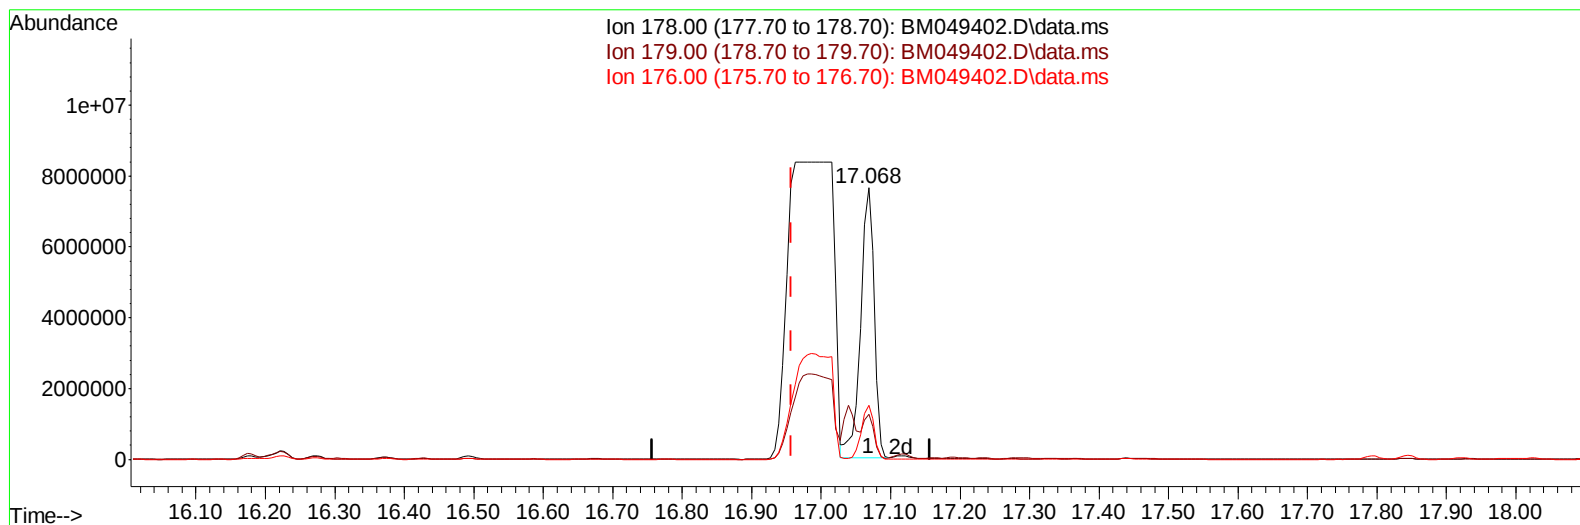

TIC: BM049402.D\data.ms

(72) Phenanthrene

17.068min (+ 0.112) 104.92 ng/u1

response 10307236

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	16.62
176.00	19.30	19.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049402.D
 Acq On : 23 Jan 2025 03:52
 Operator : RC/JU
 Sample : Q1139-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 13 16:56:06 2025
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
 Supervised By :mohammad ahmed 01/24/2025

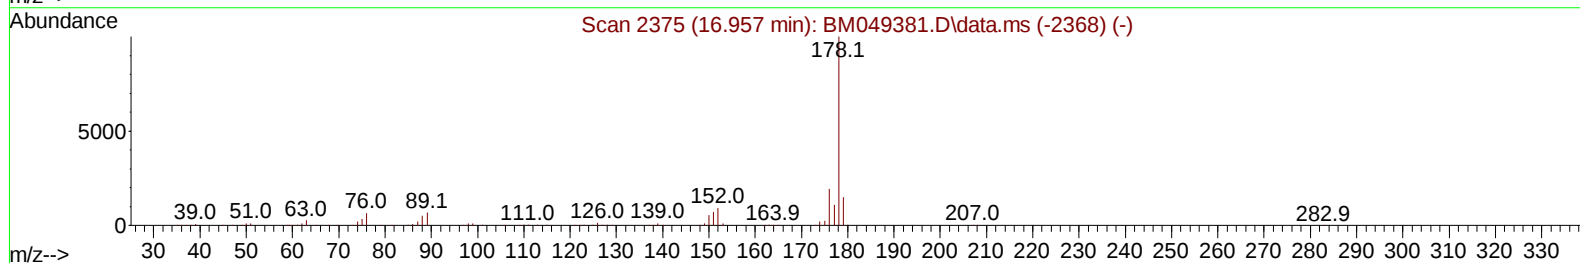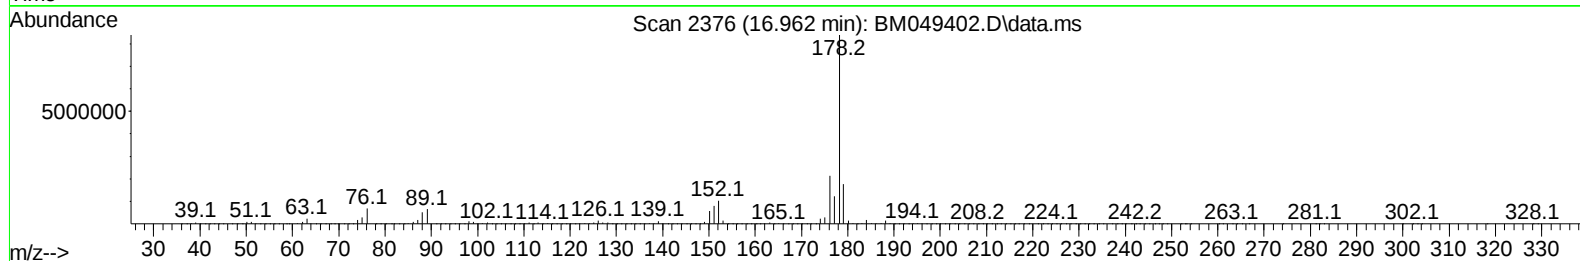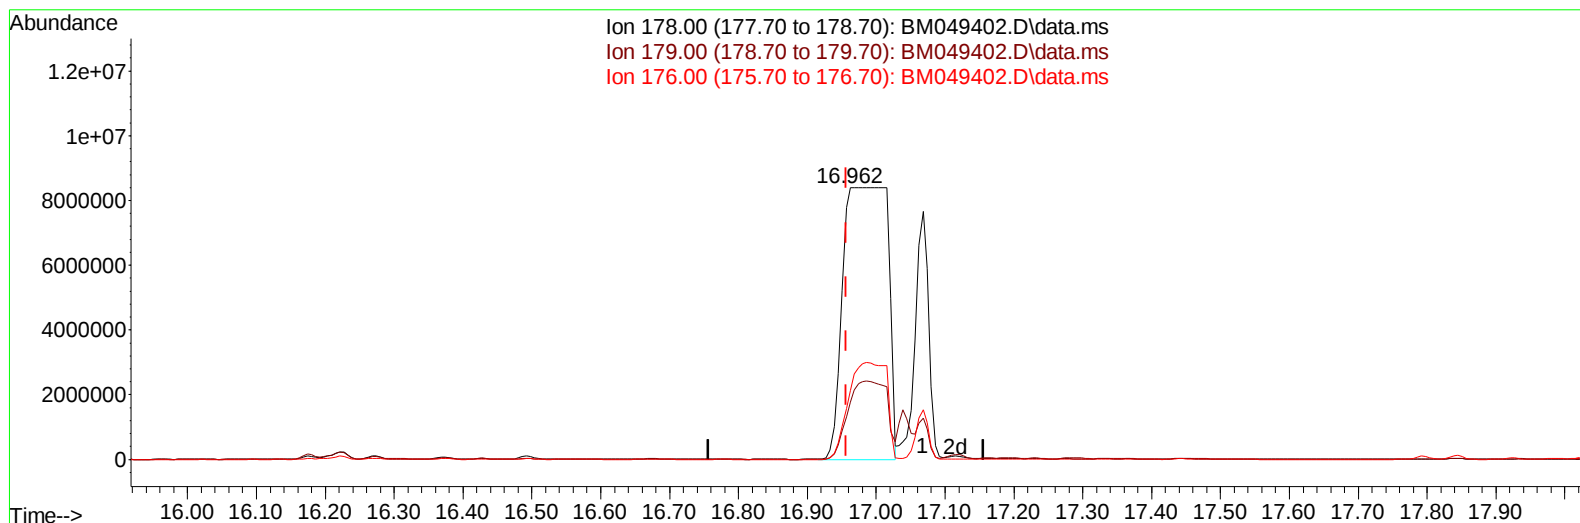

TIC: BM049402.D\data.ms

(72) Phenanthrene

16.962min (+ 0.006) 381.62 ng/u1 m

response 37490925

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	21.08#
176.00	19.30	25.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

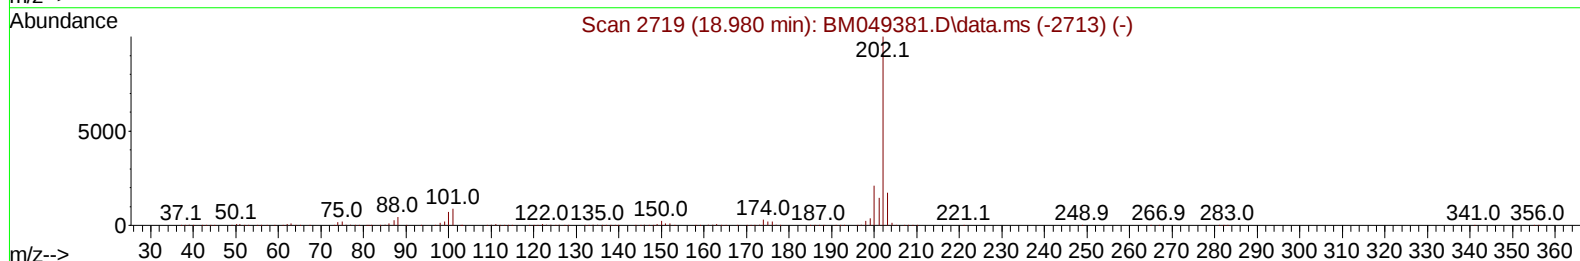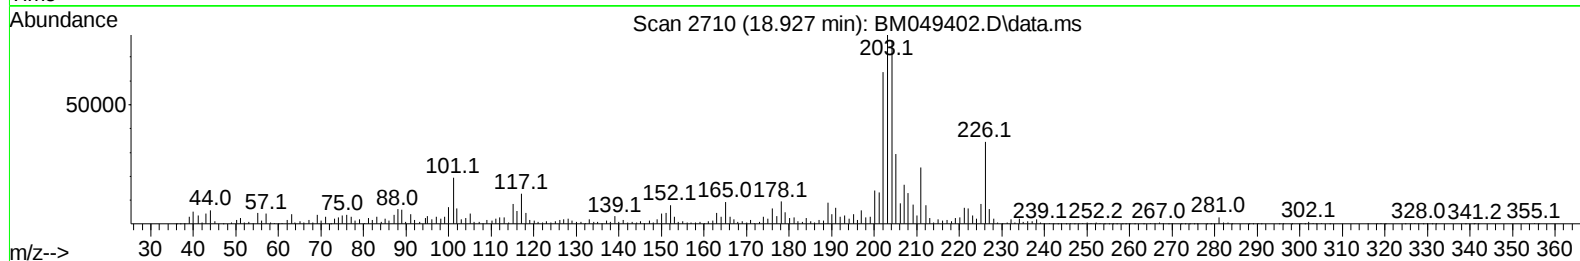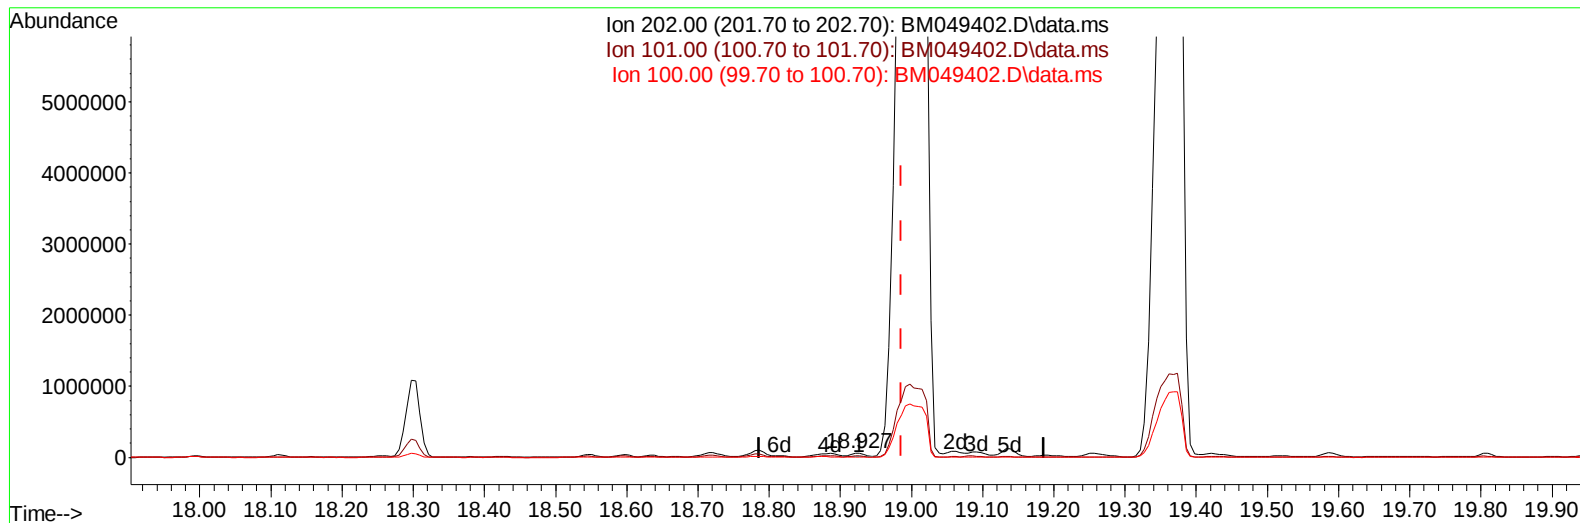

TIC: BM049402.D\data.ms

(80) Fluoranthene

18.927min (-0.059) 0.60 ng/u1

response 68196

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	8.70	30.49#
100.00	6.30	11.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

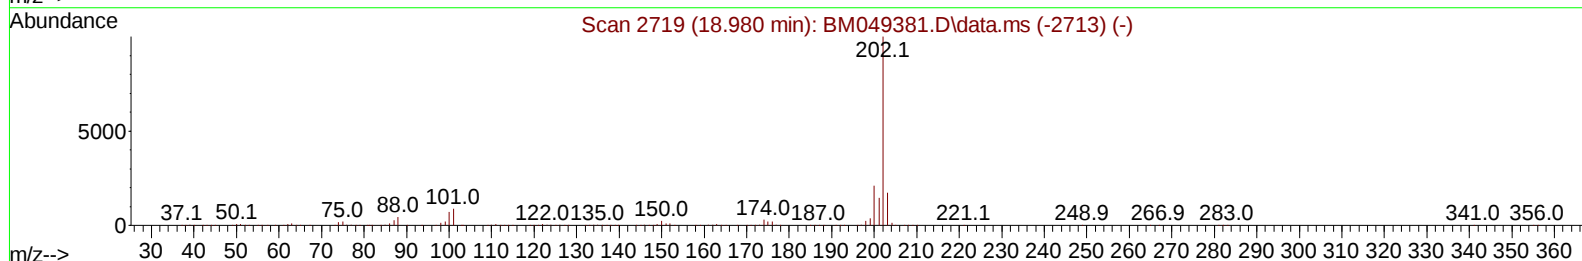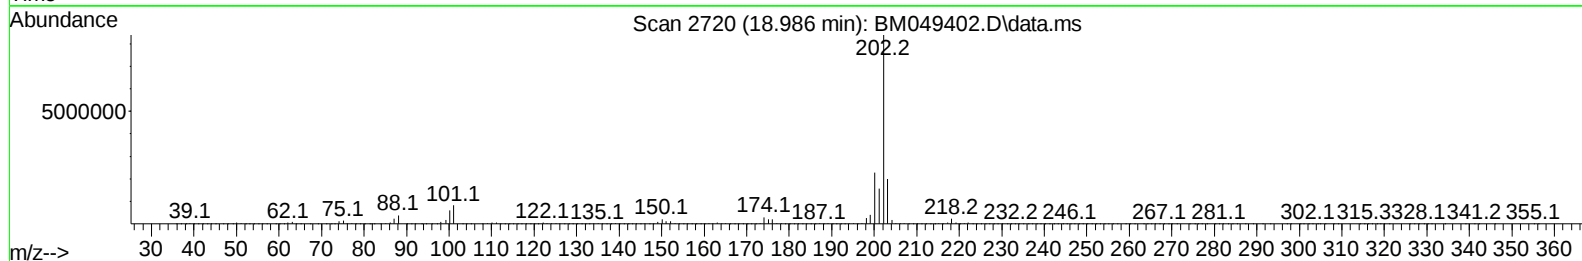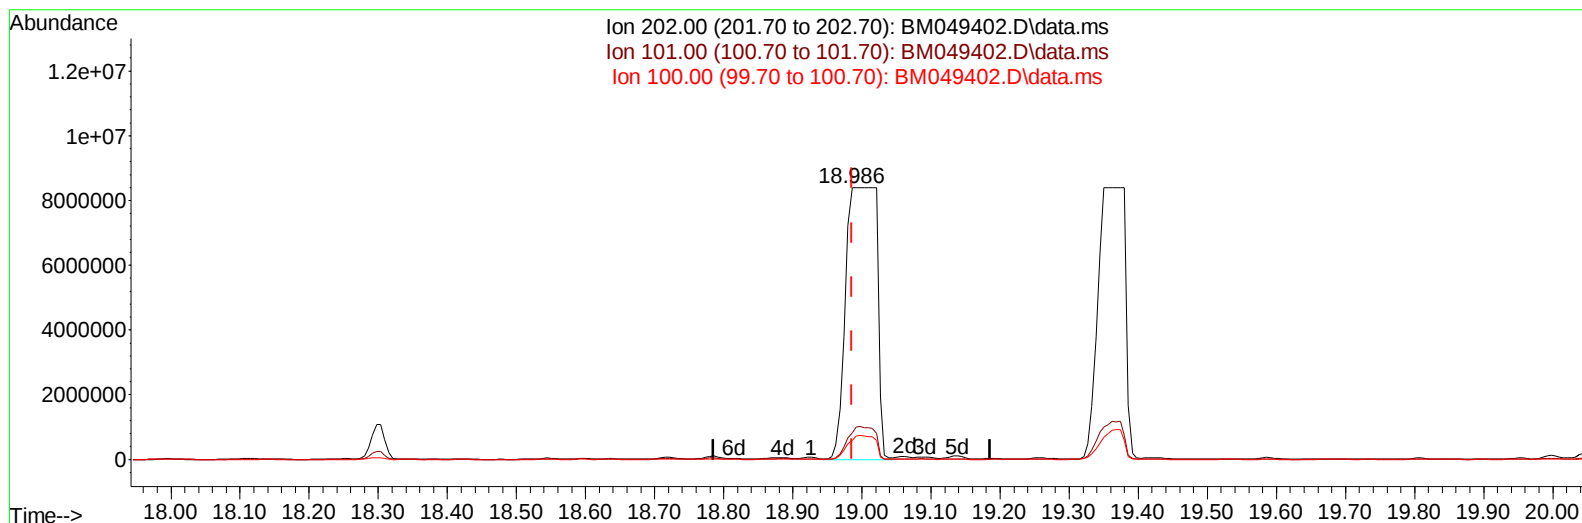

TIC: BM049402.D\data.ms

(80) Fluoranthene

18.986min (-0.000) 231.63 ng/ul m

response 26125298

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	8.70	9.74
100.00	6.30	7.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

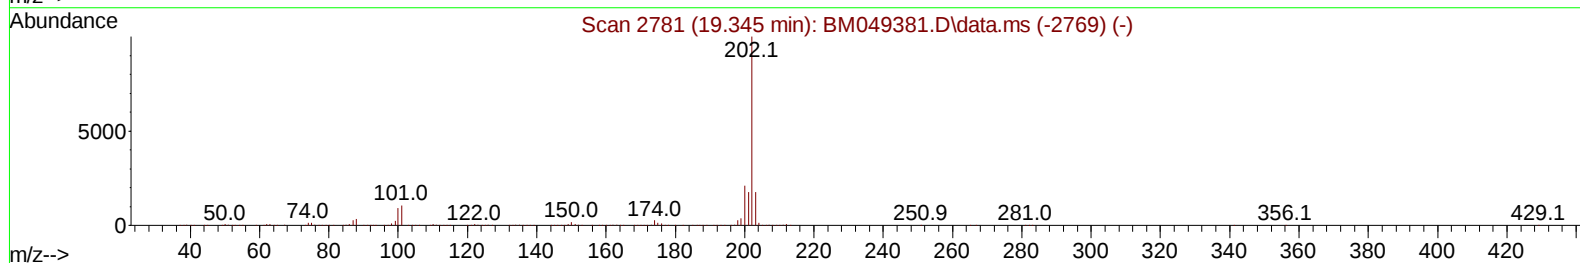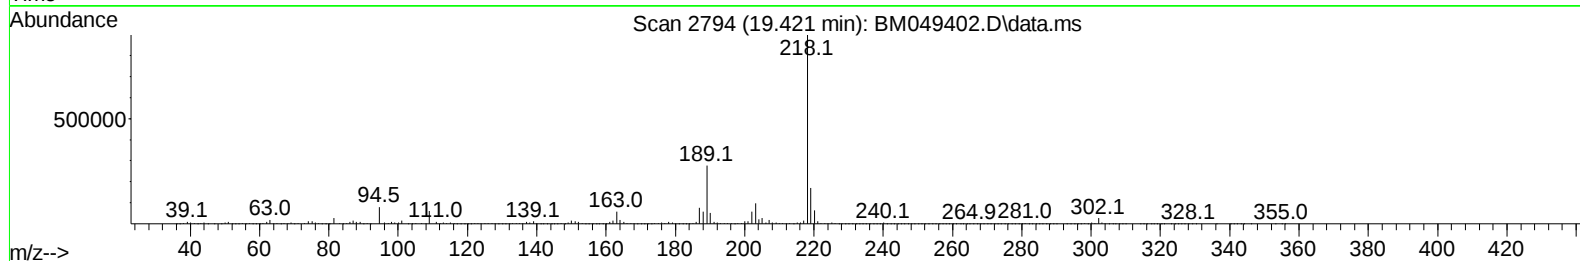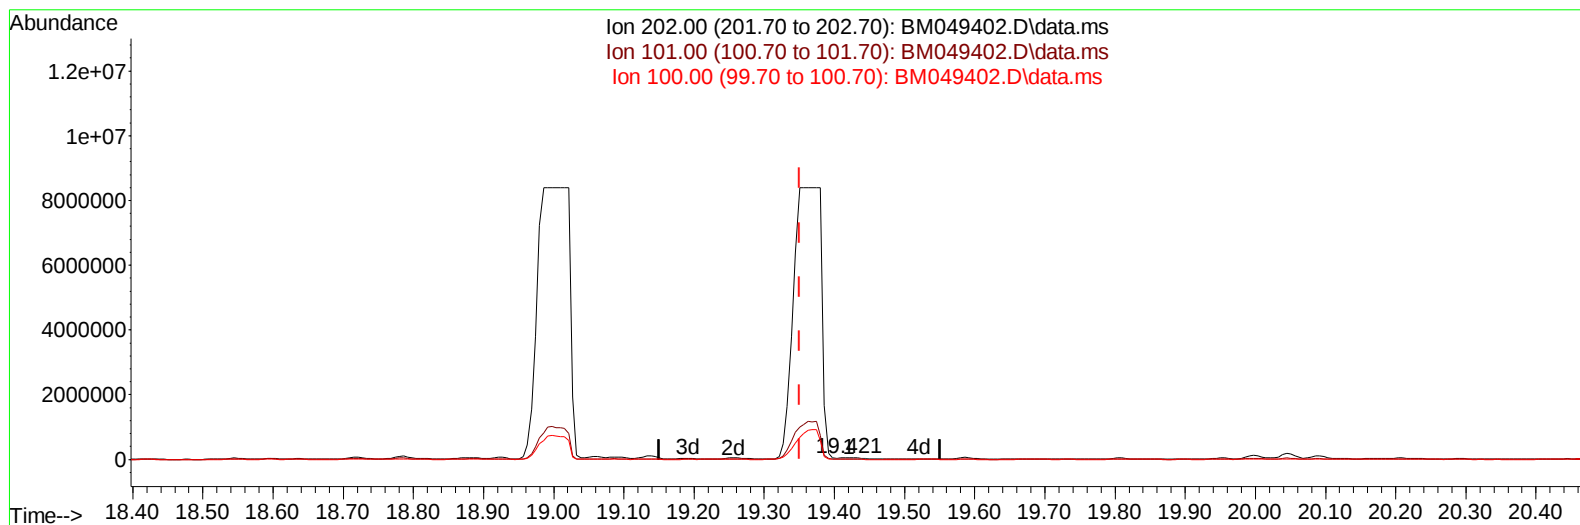

TIC: BM049402.D\data.ms

(82) Pyrene

19.421min (+ 0.071) 0.78 ng/u1

response 94246

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.80	27.34#
100.00	8.30	11.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:23:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

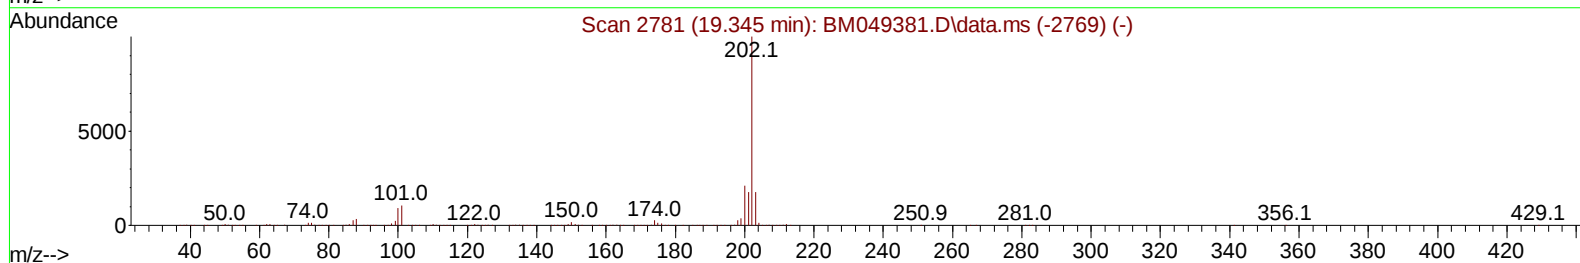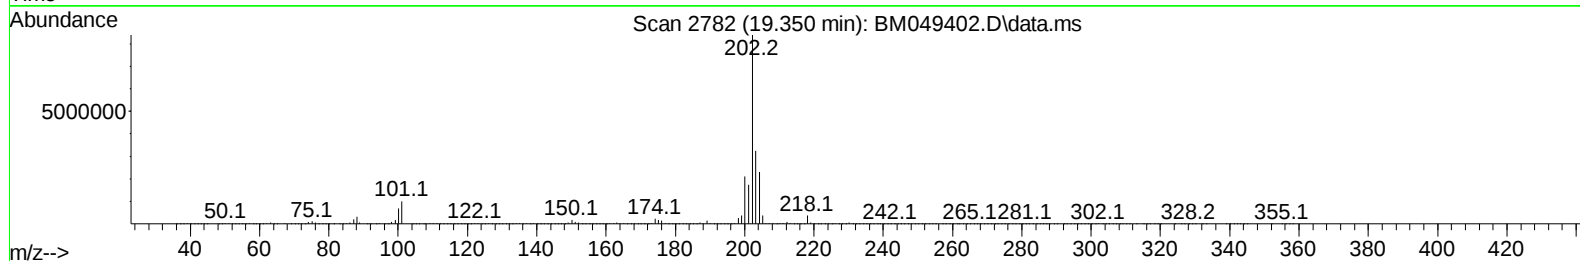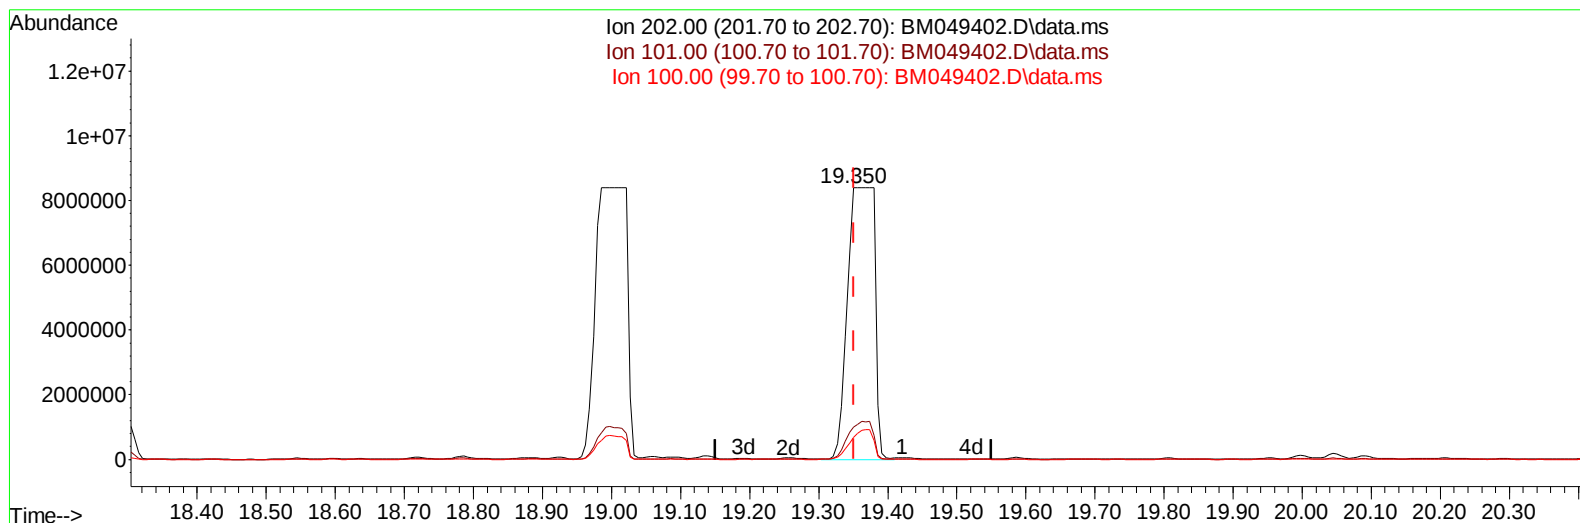

TIC: BM049402.D\data.ms

(82) Pyrene

19.350min (-0.000) 190.16 ng/ul m

response 22830545

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.80	11.92#
100.00	8.30	8.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:25:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

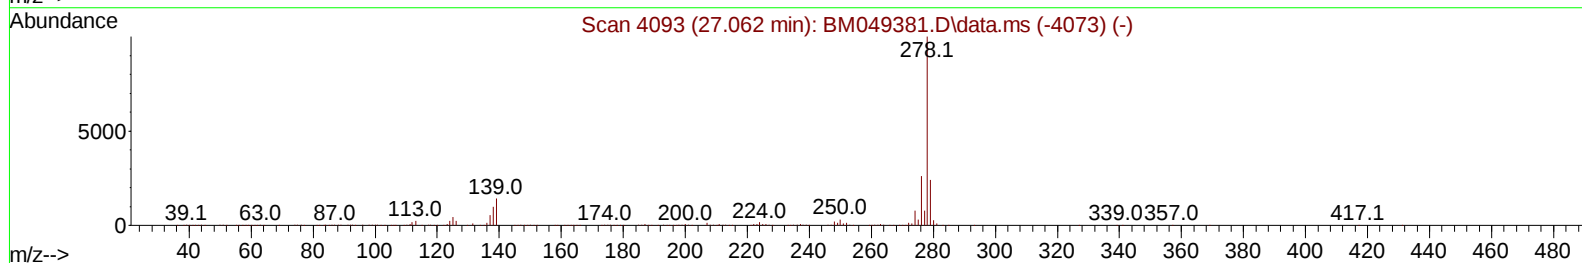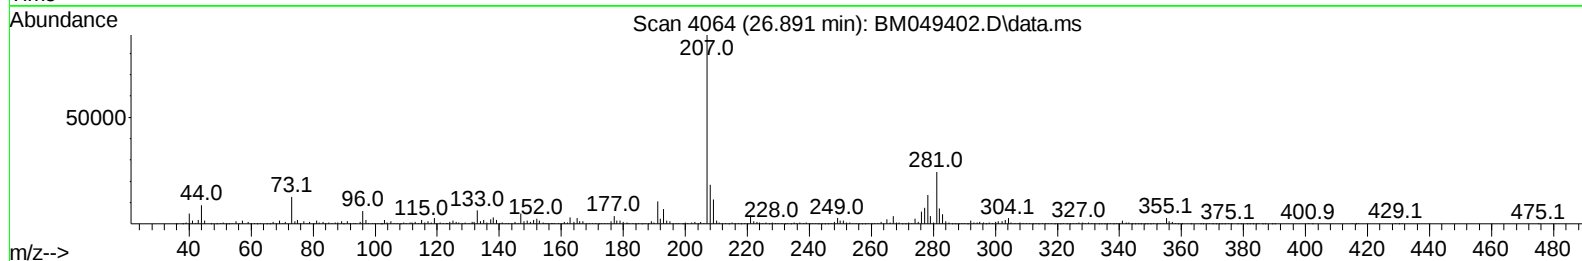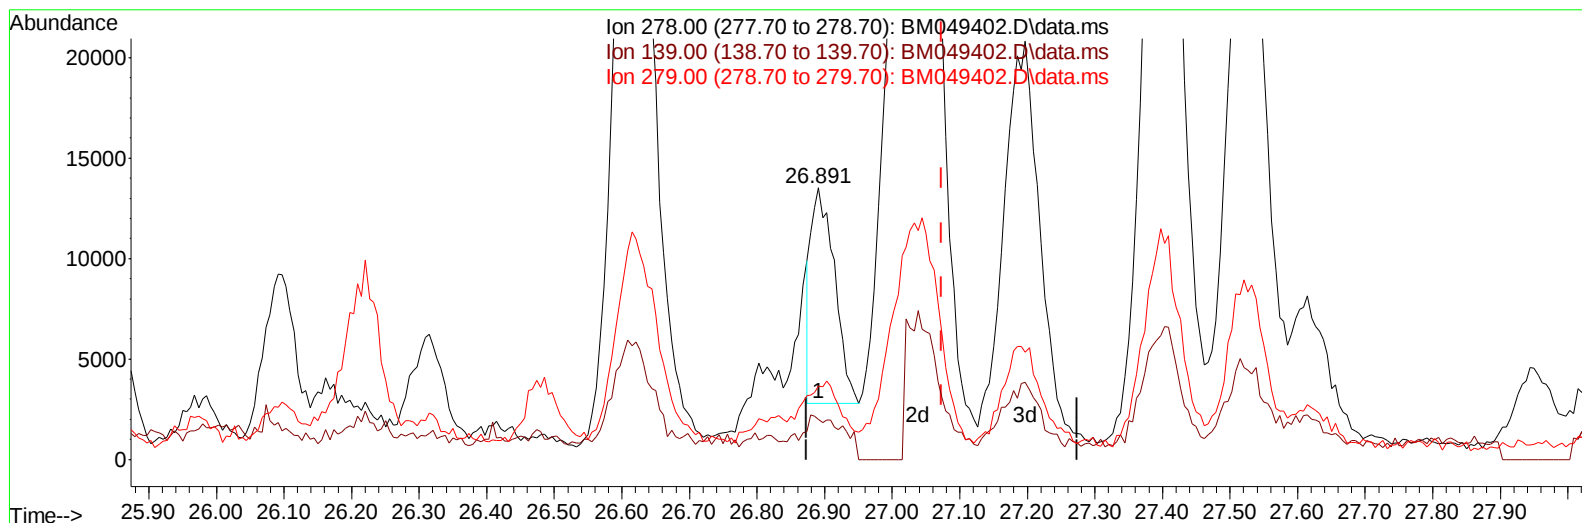

TIC: BM049402.D\data.ms

(95) Dibenzo(a,h)anthracene

26.891min (-0.182) 0.27 ng/u1

response 25910

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	12.40	14.74
279.00	24.20	26.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:25:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

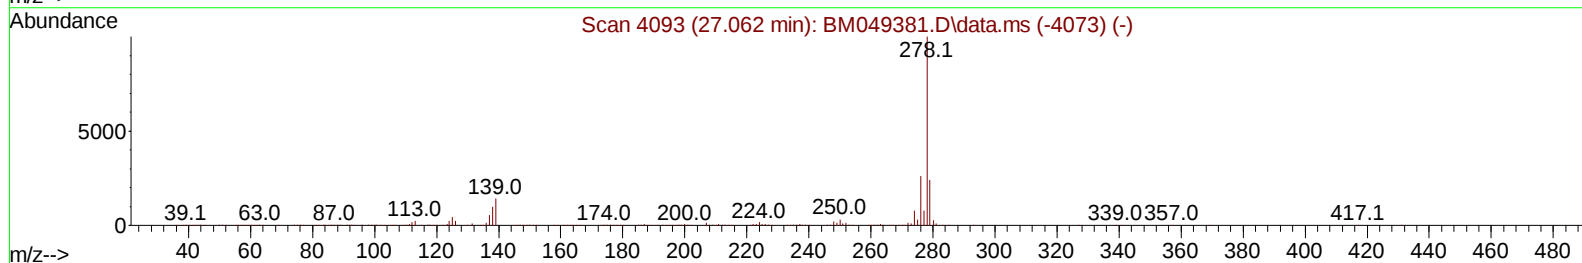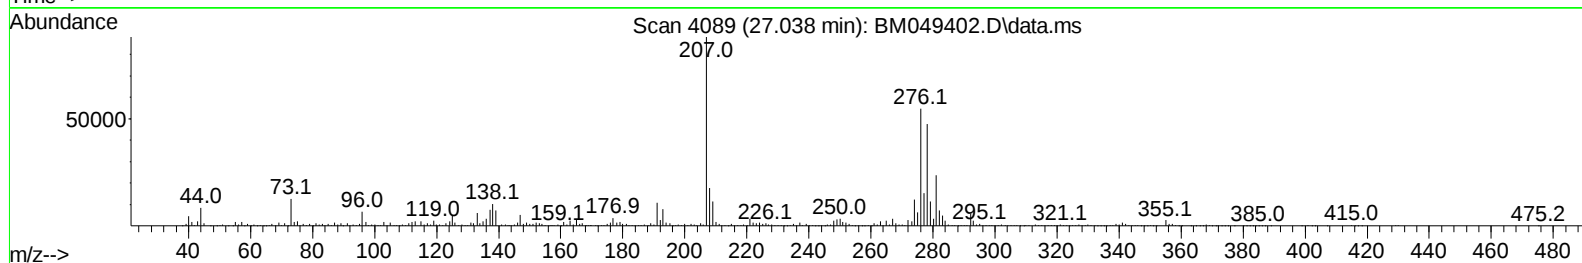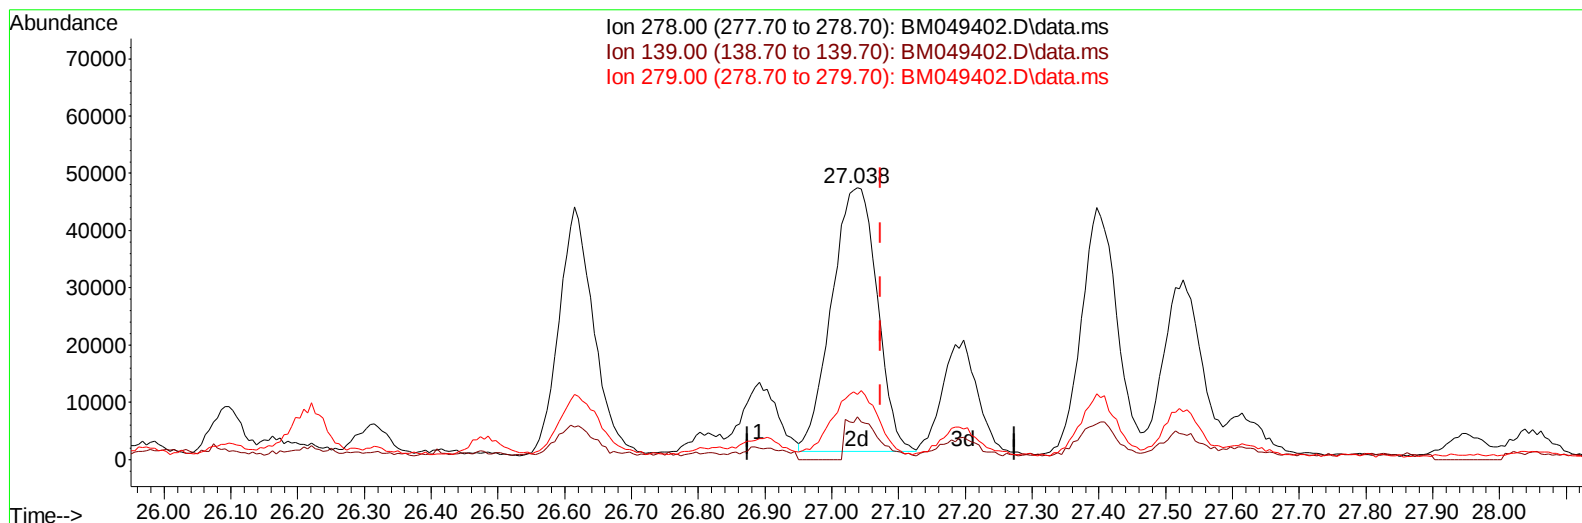

TIC: BM049402.D\data.ms

(95) Dibenzo(a,h)anthracene

27.038min (-0.035) 2.27 ng/u1 m

response 217915

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	12.40	15.65#
279.00	24.20	24.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049402.D
 Acq On : 23 Jan 2025 03:52
 Operator : RC/JU
 Sample : Q1139-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCZH7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/24/2025
 Supervised By :mohammad ahmed 01/24/2025

Quant Time: Jan 23 04:25:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 13 16:56:06 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.516	152		492495	20.000	ng/ul	0.00
20) Naphthalene-d8	10.292	136		1823555	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.163	164		1131053	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.927	188		1767116	20.000	ng/ul	0.01
79) Chrysene-d12	21.150	240		1612825	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264		1696223	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.122	96		41450	3.482	ng/uL	0.00
4) Pyridine-d5	3.510	84		583816	15.407	ng/ul	0.00
7) Phenol-d5	6.710	99		766822	18.548	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67		505393	18.359	ng/ul	0.00
11) 2-Chlorophenol-d4	7.057	132		621200	19.642	ng/ul	0.00
15) 4-Methylphenol-d8	8.228	113		596656	18.611	ng/ul	-0.01
21) Nitrobenzene-d5	8.663	128		291671	20.975	ng/ul	0.00
24) 2-Nitrophenol-d4	9.380	143		322233	20.728	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.916	165		614592	19.375	ng/ul	0.00
31) 4-Chloroaniline-d4	10.427	131		681803	16.334	ng/ul	0.00
46) Dimethylphthalate-d6	13.586	166		1463796	17.388	ng/ul	0.00
49) Acenaphthylene-d8	13.851	160		1467005	15.265	ng/ul	0.00
54) 4-Nitrophenol-d4	14.392	143		191455	13.734	ng/ul	0.00
60) Fluorene-d10	15.162	176		986823	13.569	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.321	200		33557	2.980	ng/ul	0.03
73) Anthracene-d10	17.039	188		1280658	14.660	ng/ul	0.02
81) Pyrene-d10	19.321	212		1368996	13.947	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264		1171814	12.869	ng/ul	-0.01
Target Compounds							
						Qvalue	
30) Naphthalene	10.339	128	33938977m	350.693	ng/ul		
36) 2-Methylnaphthalene	11.974	142	18141037	261.956	ng/ul		100
37) 1-Methylnaphthalene	12.186	142	10162059	147.480	ng/ul		100
50) Acenaphthylene	13.880	152	580941	5.896	ng/ul#		79
52) Acenaphthene	14.239	153	14756202	209.626	ng/ul		98
61) Fluorene	15.233	166	14030674	171.791	ng/ul		98
72) Phenanthrene	16.962	178	37490925m	381.622	ng/ul		
74) Anthracene	17.068	178	10307236	104.527	ng/ul		98
80) Fluoranthene	18.986	202	26125298m	231.633	ng/ul		
82) Pyrene	19.350	202	22830545m	190.160	ng/ul		
85) Benzo(a)anthracene	21.133	228	9847522	87.615	ng/ul		96
87) Chrysene	21.192	228	8467662	82.523	ng/ul		98
90) Benzo(b)fluoranthene	23.056	252	4547596	40.055	ng/ul		98
91) Benzo(k)fluoranthene	23.109	252	1633571	14.431	ng/ul		99
93) Benzo(a)pyrene	23.791	252	2547737	24.844	ng/ul		100
94) Indeno(1,2,3-cd)pyrene	26.997	276	782392	6.651	ng/ul		99
95) Dibenzo(a,h)anthracene	27.038	278	217915m	2.274	ng/ul		
96) Benzo(g,h,i)perylene	27.956	276	585101	6.663	ng/ul		99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049402.D
Acq On : 23 Jan 2025 03:52
Operator : RC/JU
Sample : Q1139-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH7

Manual IntegrationsAPPROVED

Quant Time: Jan 23 04:25:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

