




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

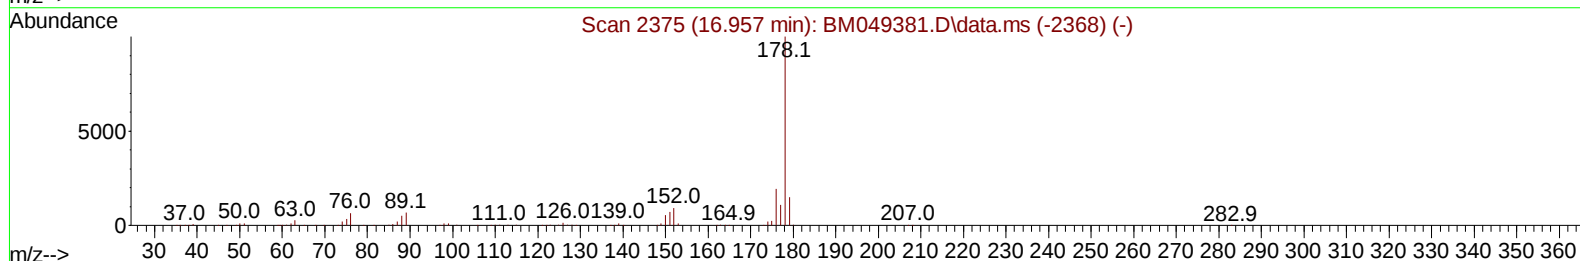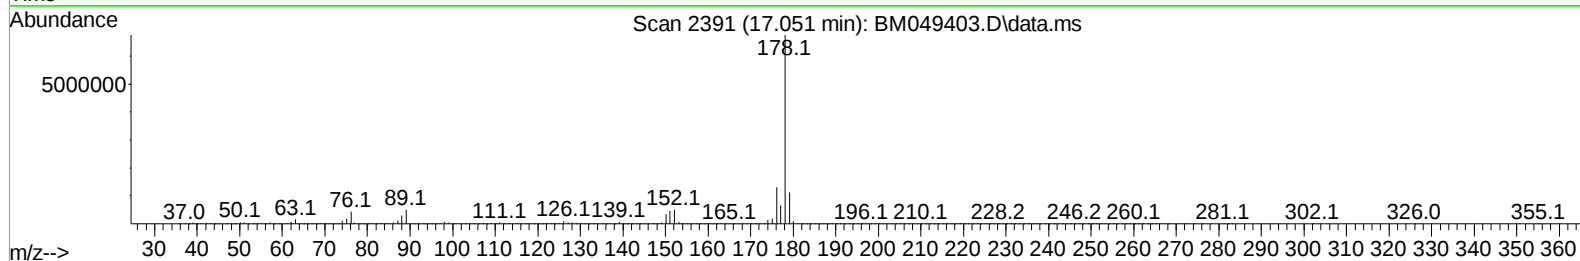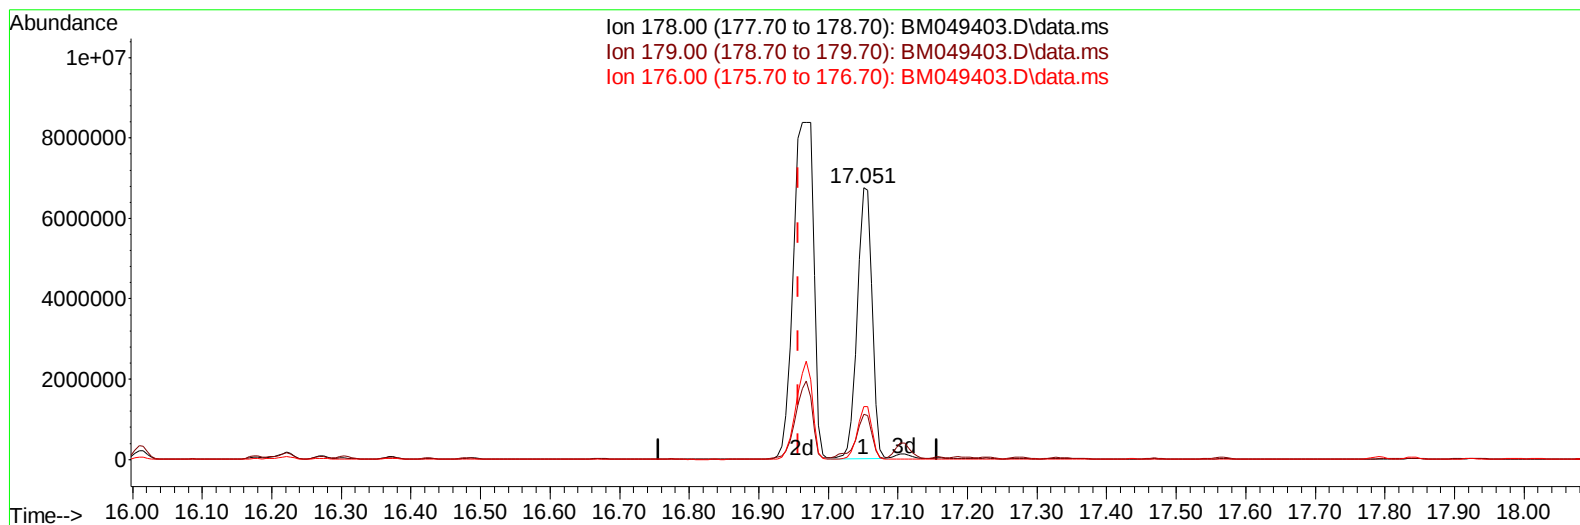

TIC: BM049403.D\data.ms

(72) Phenanthrene

17.051min (+ 0.094) 124.51 ng/u1

response 9996429

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	16.55
176.00	19.30	19.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

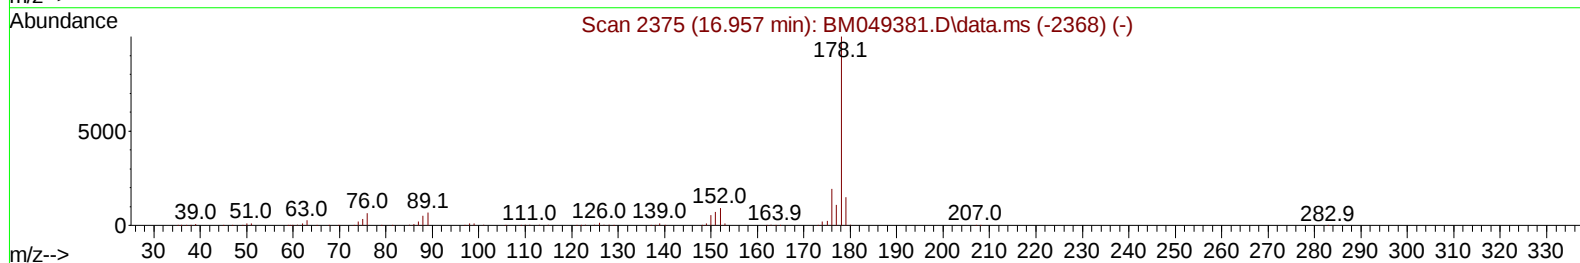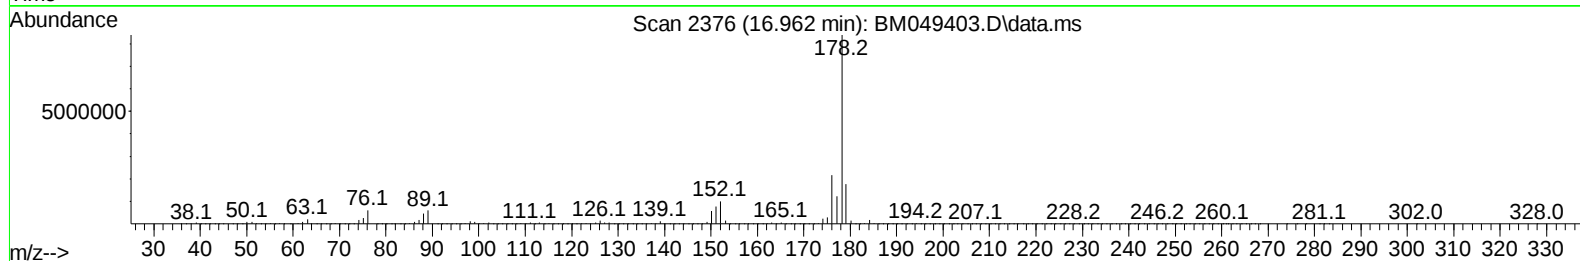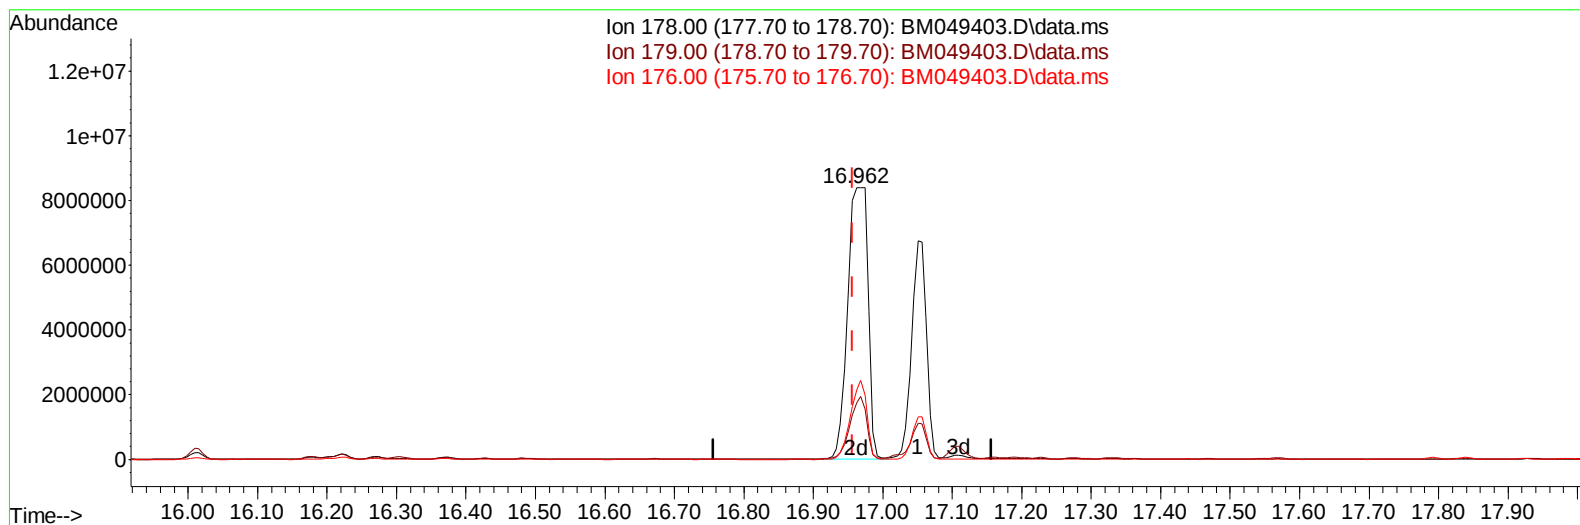

TIC: BM049403.D\data.ms

(72) Phenanthrene

16.962min (+ 0.006) 212.76 ng/u1 m

response 17081212

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	20.99#
176.00	19.30	25.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

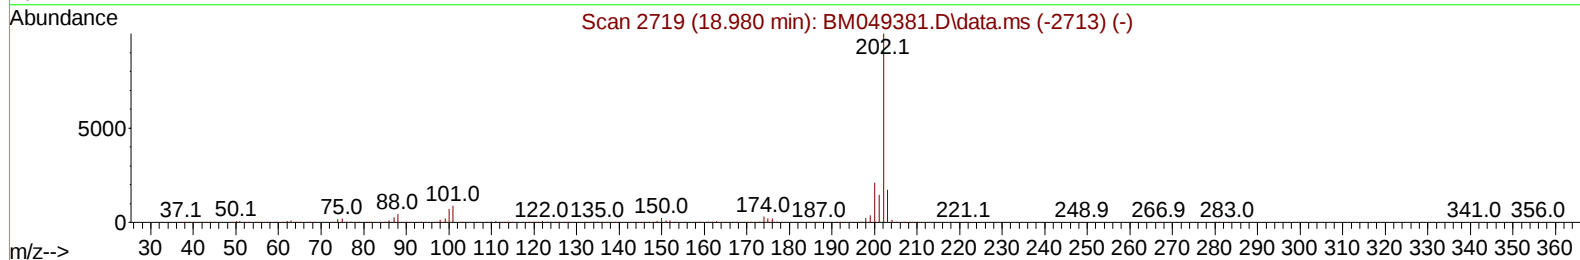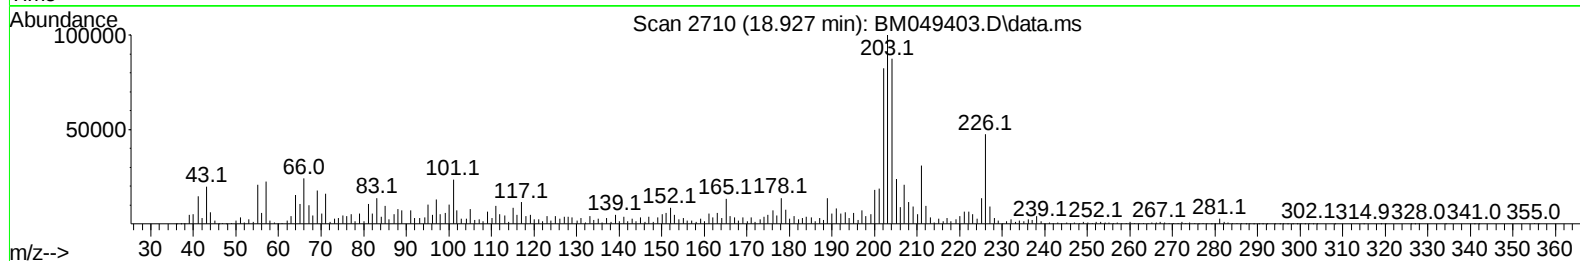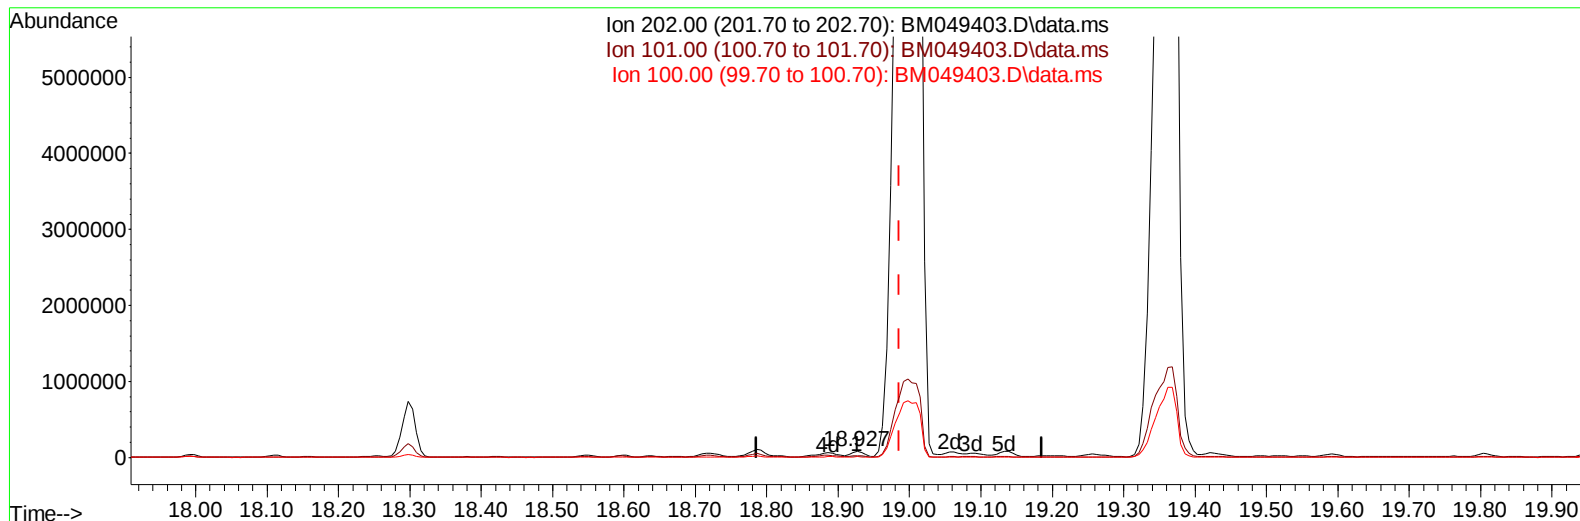

TIC: BM049403.D\data.ms

(80) Fluoranthene

18.927min (-0.059) 0.84 ng/u1

response 76486

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	8.70	28.77#
100.00	6.30	12.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

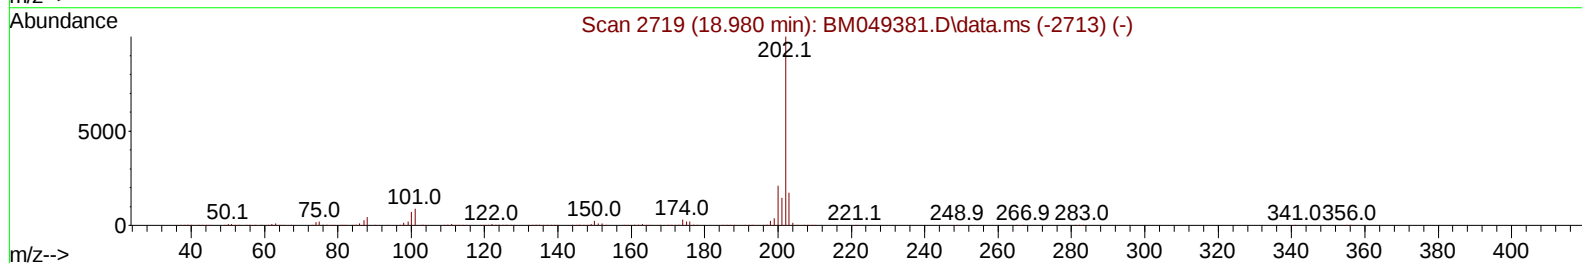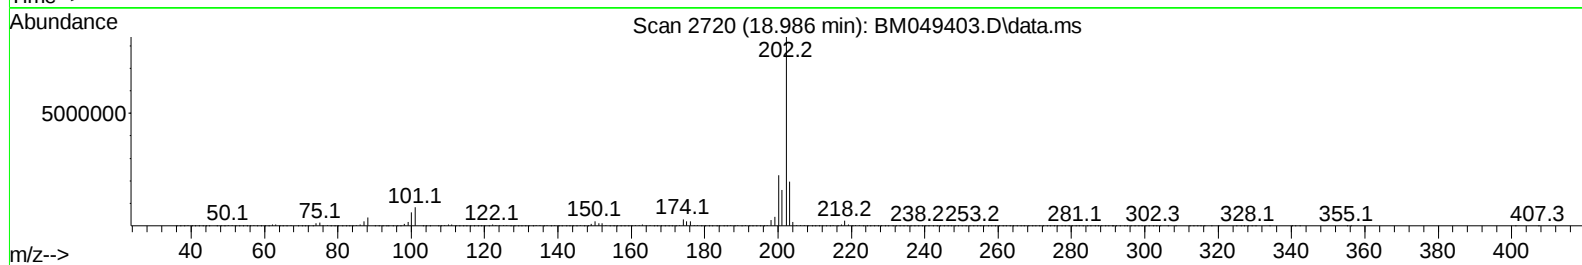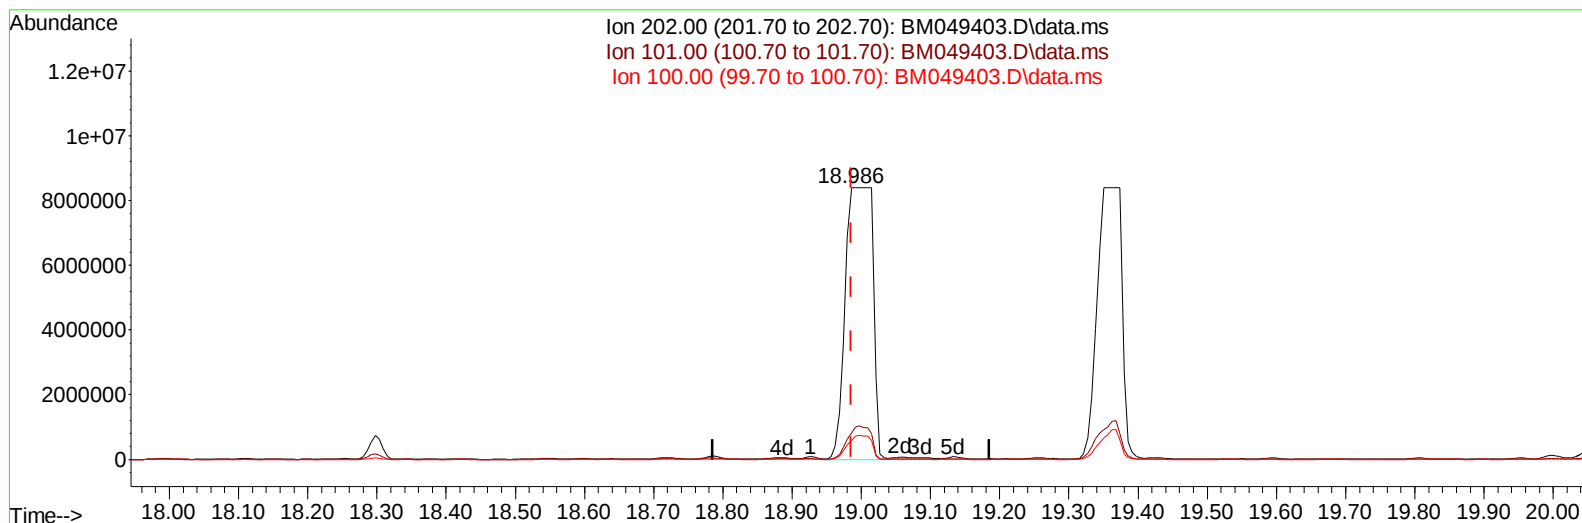

TIC: BM049403.D\data.ms

(80) Fluoranthene

18.986min (-0.000) 255.12 ng/ul m

response 23140615

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	8.70	9.73
100.00	6.30	7.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

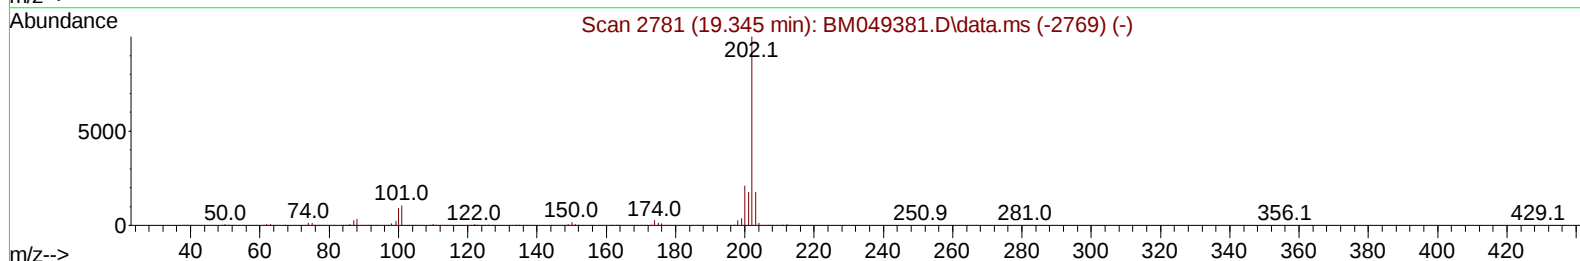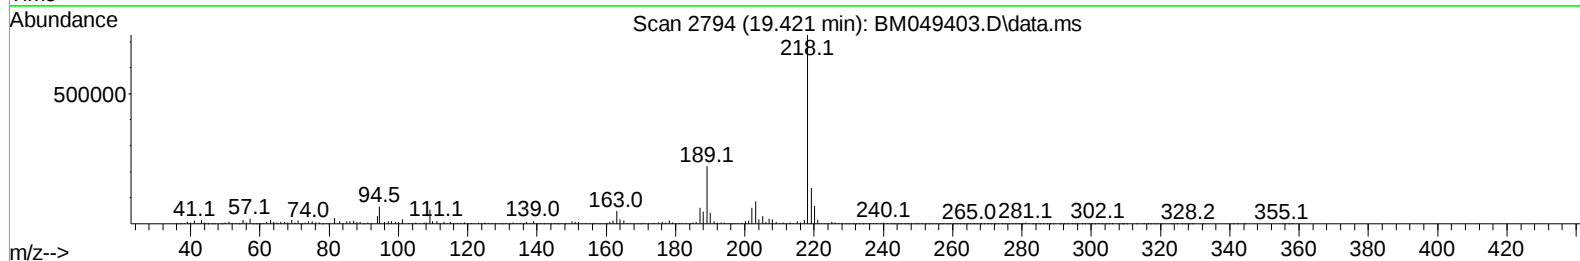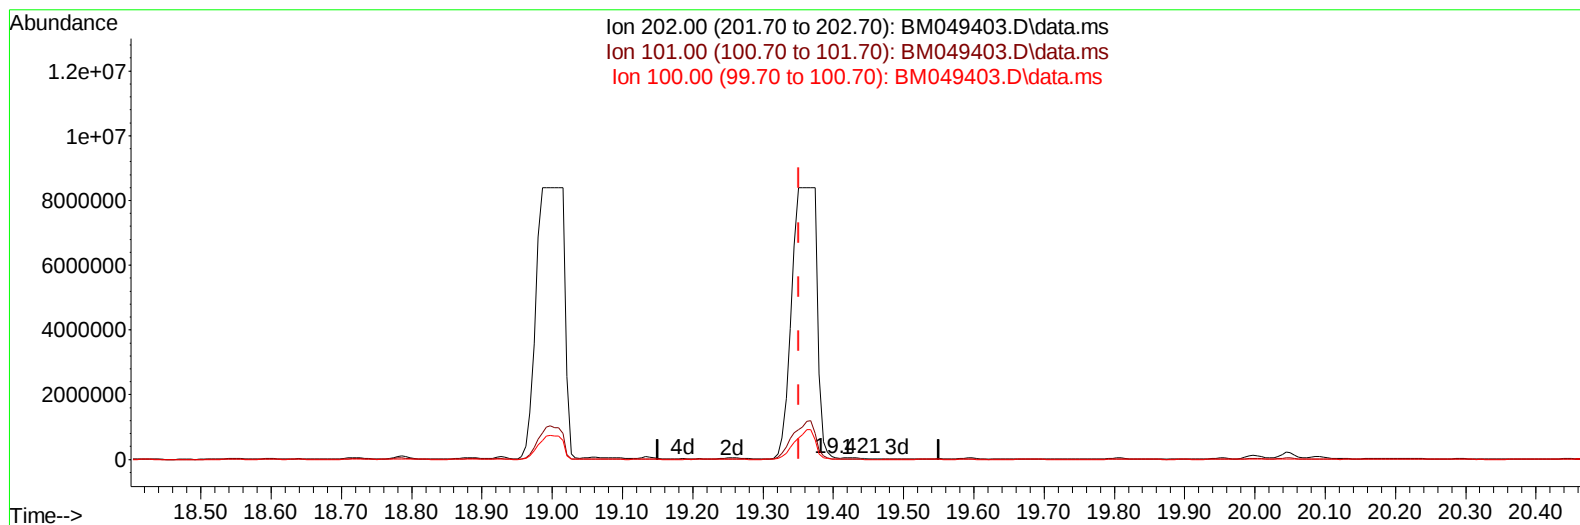

TIC: BM049403.D\data.ms

(82) Pyrene

19.421min (+ 0.071) 0.79 ng/u1

response 75888

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.80	26.83#
100.00	8.30	11.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

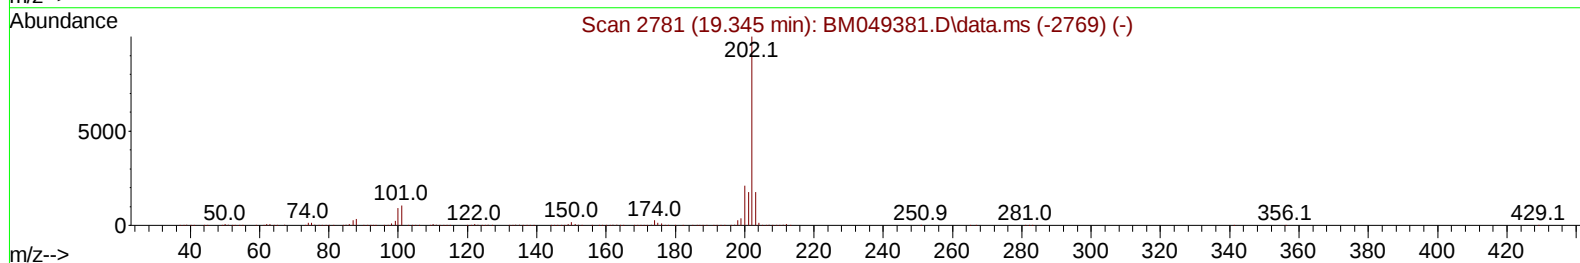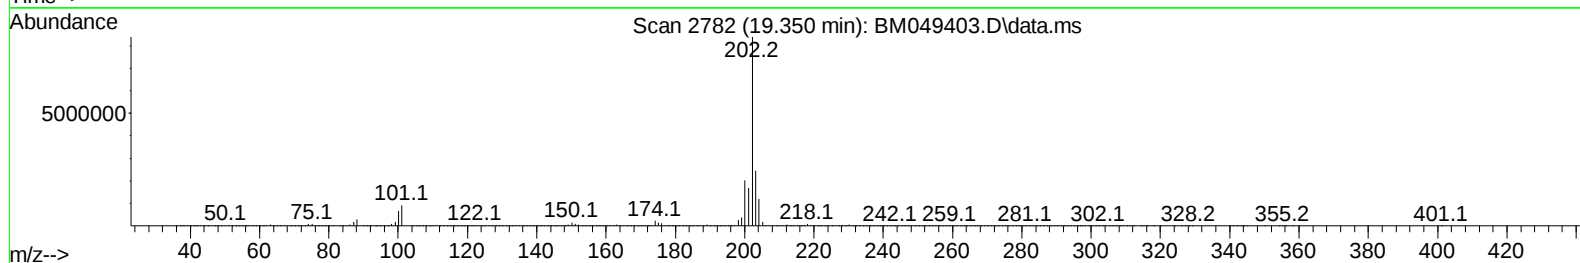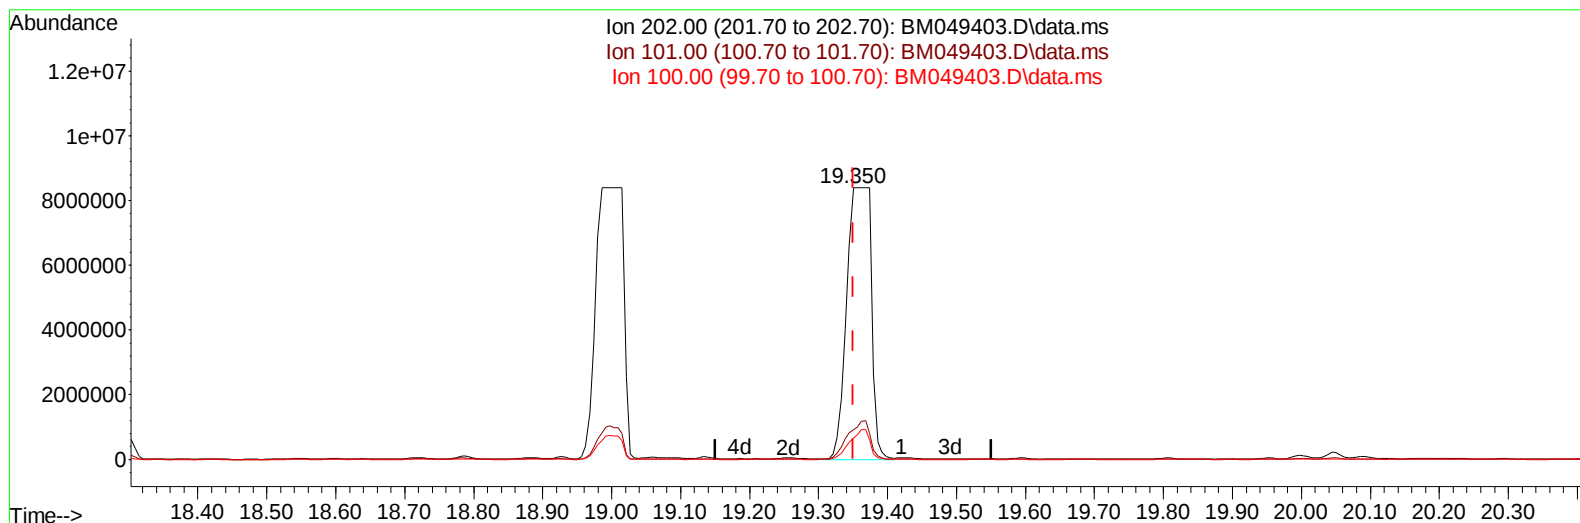

TIC: BM049403.D\data.ms

(82) Pyrene

19.350min (-0.000) 215.31 ng/ul m

response 20788230

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.80	10.88
100.00	8.30	7.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

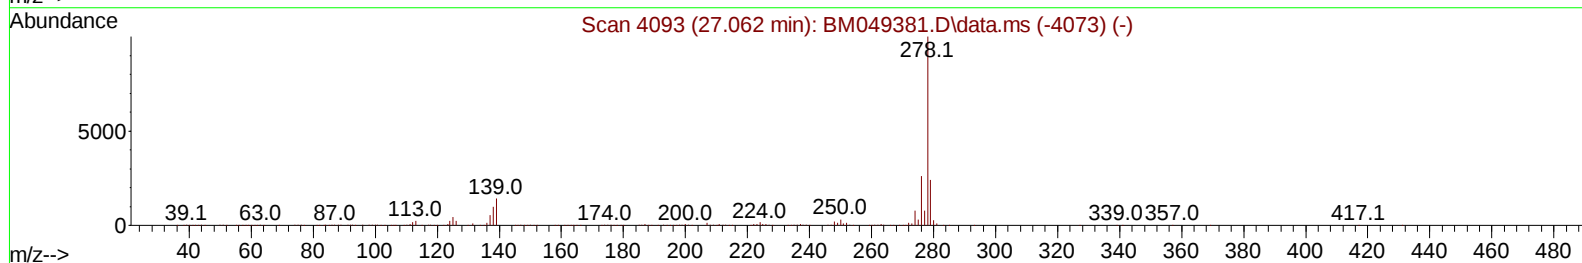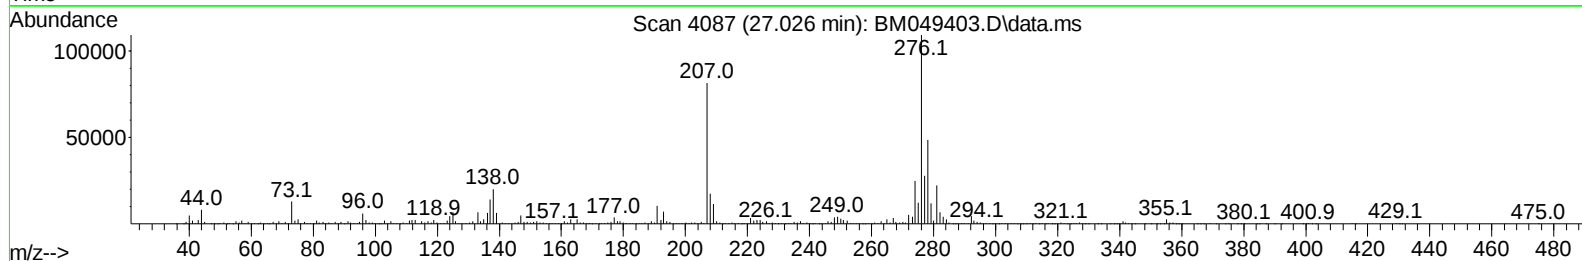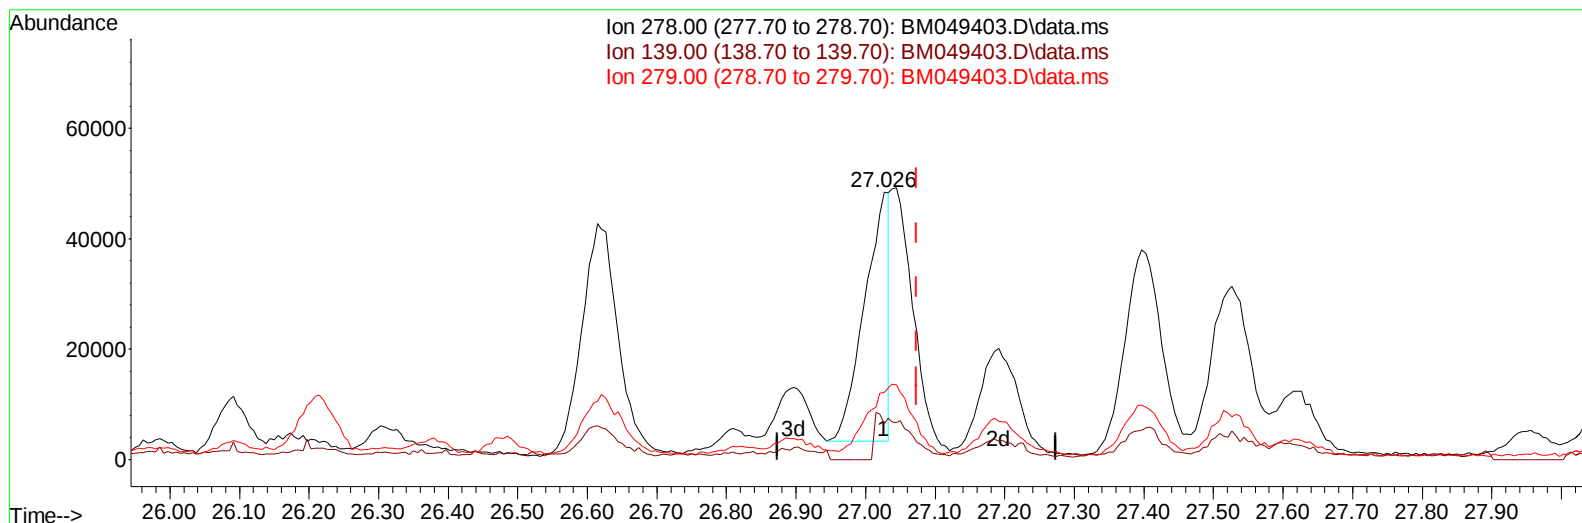

TIC: BM049403.D\data.ms

(95) Dibenzo(a,h)anthracene

27.026min (-0.047) 1.47 ng/u1

response 109681

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	12.40	13.21
279.00	24.20	25.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

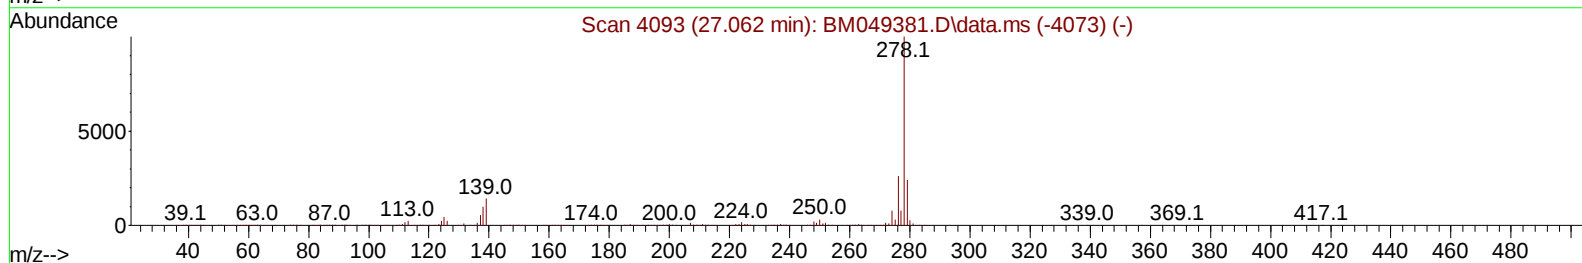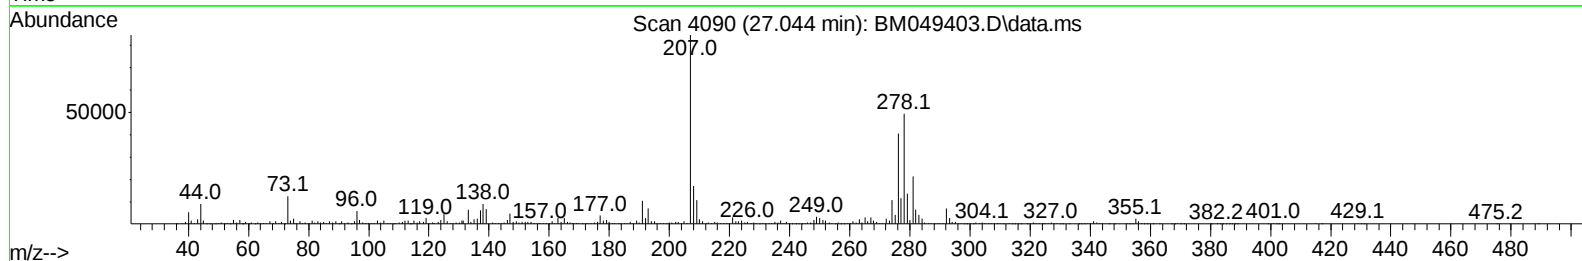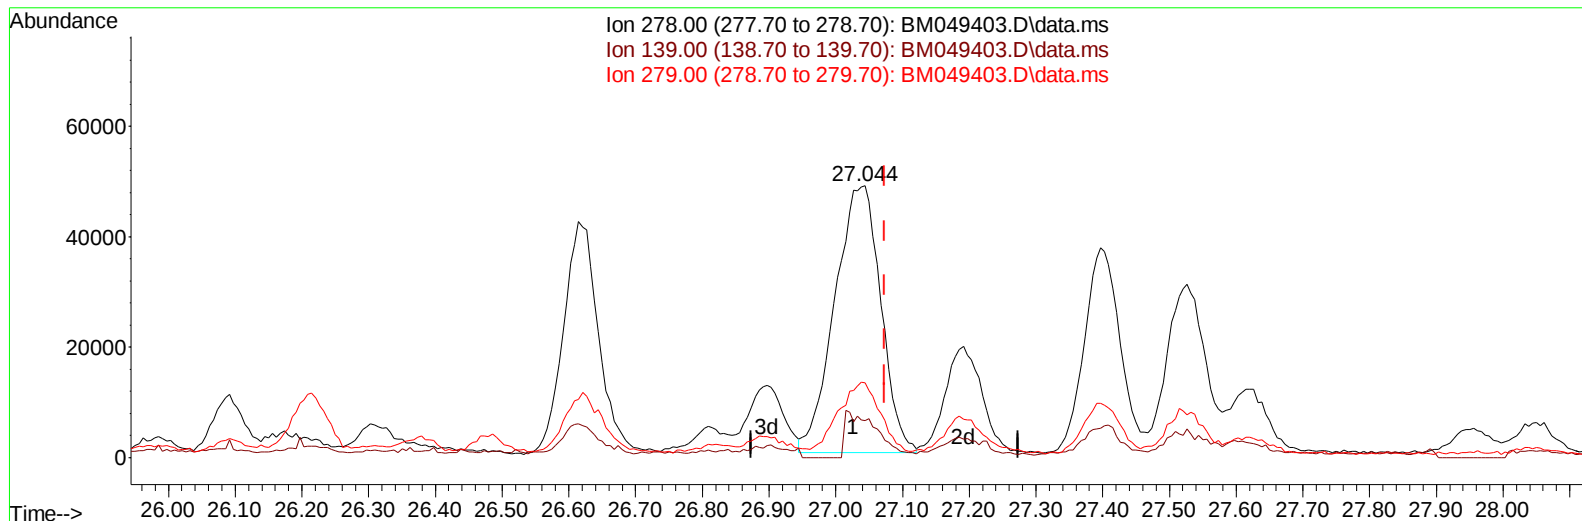

TIC: BM049403.D\data.ms

(95) Dibenzo(a,h)anthracene

27.044min (-0.029) 3.09 ng/u1 m

response 231142

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	12.40	13.49
279.00	24.20	27.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

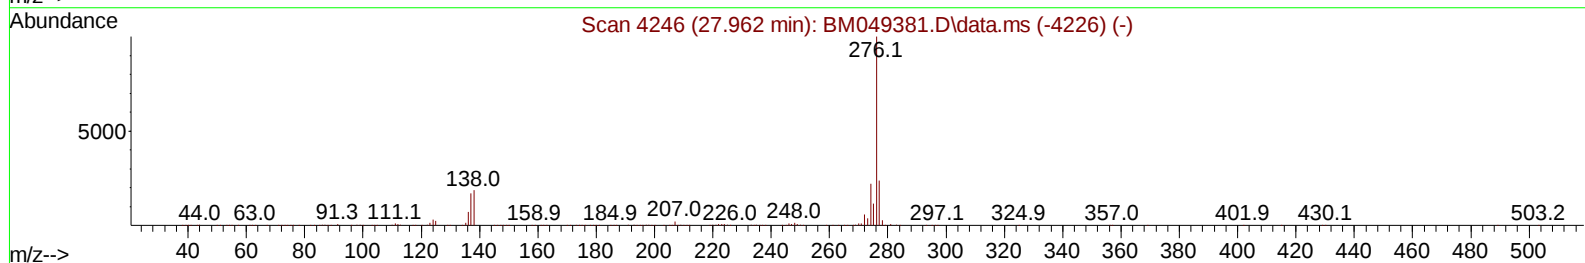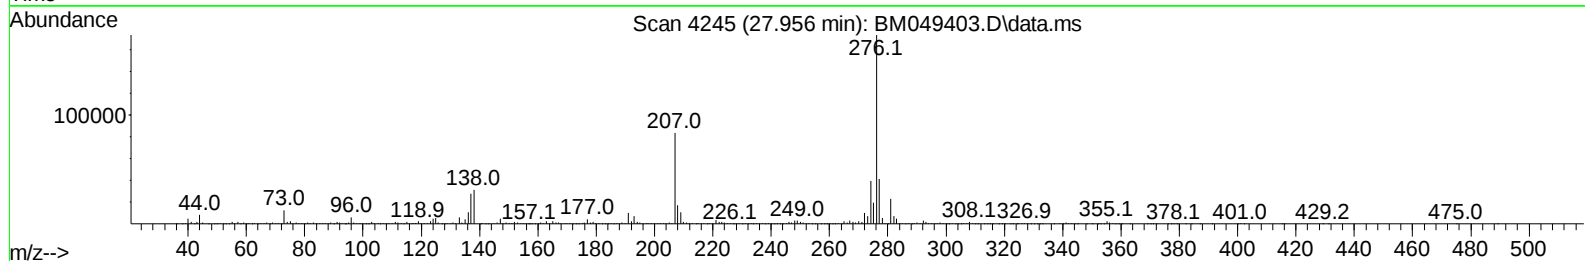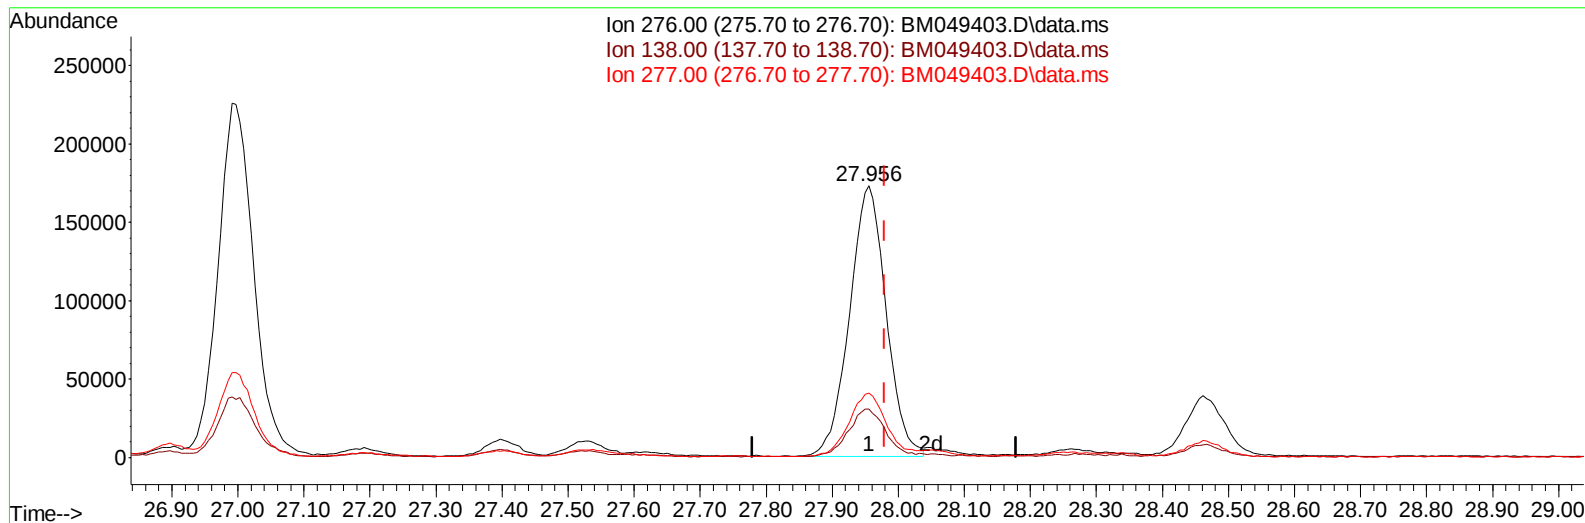

TIC: BM049403.D\data.ms

(96) Benzo(g,h,i)perylene

27.956min (-0.024) 9.72 ng/u1

response 666841

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.60	17.93
277.00	24.20	23.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:02:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

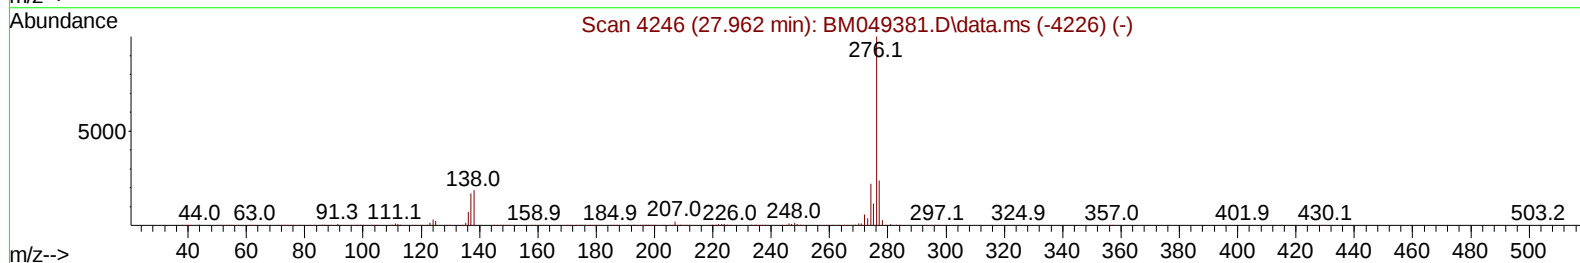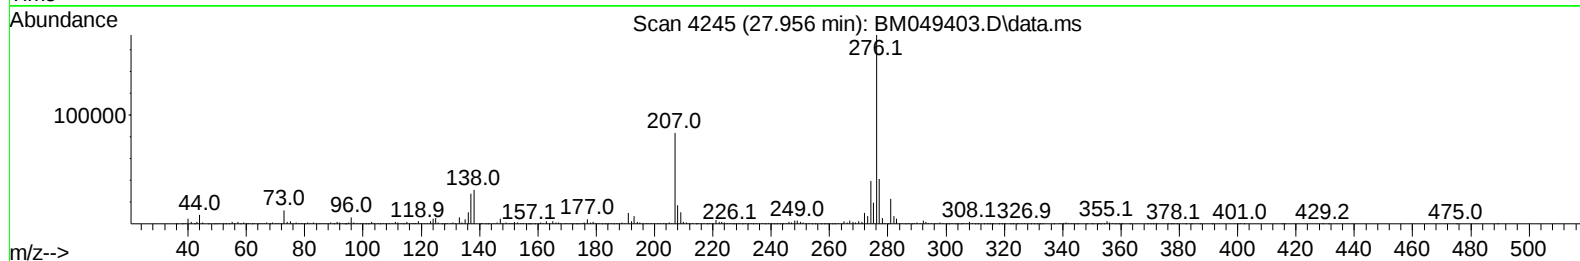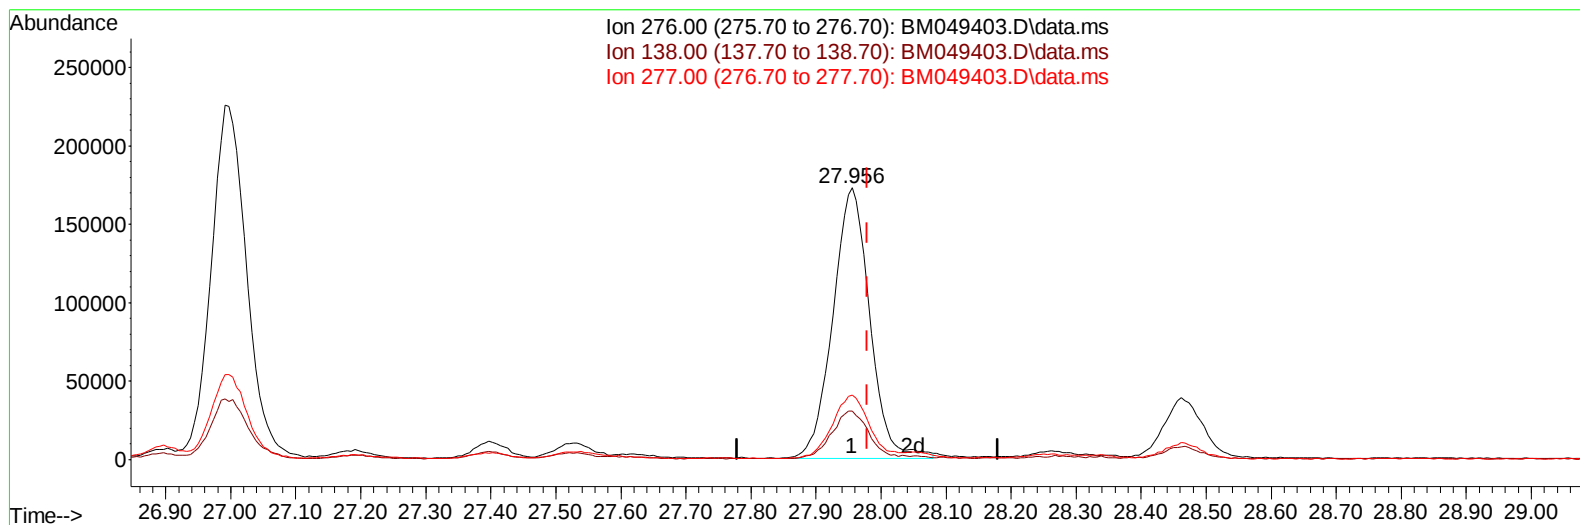

TIC: BM049403.D\data.ms

(96) Benzo(g,h,i)perylene

27.956min (-0.024) 9.92 ng/u1 m

response 680898

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.60	17.93
277.00	24.20	23.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049403.D
 Acq On : 23 Jan 2025 04:31
 Operator : RC/JU
 Sample : Q1139-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:04:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 13 16:56:06 2025
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
 Supervised By :mohammad ahmed 01/24/2025

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.516	152		380279	20.000	ng/ul	0.00
20) Naphthalene-d8	10.280	136		1401990	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.157	164		850826	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.915	188		1444111	20.000	ng/ul	0.00
79) Chrysene-d12	21.144	240		1297024	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264		1325401	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.122	96		42806	4.657	ng/uL	0.00
4) Pyridine-d5	3.510	84		613830	20.979	ng/ul	0.00
7) Phenol-d5	6.716	99		763484	23.917	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67		502040	23.619	ng/ul	0.00
11) 2-Chlorophenol-d4	7.057	132		618767	25.338	ng/ul	0.00
15) 4-Methylphenol-d8	8.234	113		574800	23.220	ng/ul	0.00
21) Nitrobenzene-d5	8.663	128		284961	26.654	ng/ul	0.00
24) 2-Nitrophenol-d4	9.375	143		324711	27.169	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.910	165		592528	24.296	ng/ul	0.00
31) 4-Chloroaniline-d4	10.422	131		654397	20.392	ng/ul	0.00
46) Dimethylphthalate-d6	13.580	166		1545600	24.407	ng/ul	0.00
49) Acenaphthylene-d8	13.845	160		1805632	24.977	ng/ul	0.00
54) 4-Nitrophenol-d4	14.392	143		186522	17.787	ng/ul	0.00
60) Fluorene-d10	15.157	176		1265350	23.130	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200		74921	8.141	ng/ul	0.00
73) Anthracene-d10	17.015	188		1702322	23.846	ng/ul	0.00
81) Pyrene-d10	19.321	212		1848508	23.418	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264		1618922	22.754	ng/ul	-0.01
Target Compounds							
						Qvalue	
30) Naphthalene	10.328	128		1611739	21.662	ng/ul	100
36) 2-Methylnaphthalene	11.951	142		127245	2.390	ng/ul	99
37) 1-Methylnaphthalene	12.174	142		217179	4.100	ng/ul	99
50) Acenaphthylene	13.874	152		324686	4.381	ng/ul#	93
52) Acenaphthene	14.227	153		5401634	102.009	ng/ul	99
61) Fluorene	15.221	166		6270975	102.070	ng/ul	98
72) Phenanthrene	16.962	178		17081212m	212.760	ng/ul	
74) Anthracene	17.051	178		10033368	124.509	ng/ul	98
80) Fluoranthene	18.986	202		23140615m	255.125	ng/ul	
82) Pyrene	19.350	202		20788230m	215.308	ng/ul	
85) Benzo(a)anthracene	21.133	228		7515372	83.146	ng/ul	97
87) Chrysene	21.192	228		7390800	89.566	ng/ul	98
90) Benzo(b)fluoranthene	23.056	252		4409062	49.700	ng/ul	99
91) Benzo(k)fluoranthene	23.109	252		1441080	16.292	ng/ul	100
93) Benzo(a)pyrene	23.791	252		2386518	29.783	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.991	276		842389	9.164	ng/ul	100
95) Dibenzo(a,h)anthracene	27.044	278		231142m	3.087	ng/ul	
96) Benzo(g,h,i)perylene	27.956	276		680898m	9.923	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049403.D
Acq On : 23 Jan 2025 04:31
Operator : RC/JU
Sample : Q1139-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCZH8

Manual IntegrationsAPPROVED

Quant Time: Jan 23 05:04:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 13 16:56:06 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/24/2025
Supervised By :mohammad ahmed 01/24/2025

