

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049368.D
 Acq On : 21 Jan 2025 17:05
 Operator : RC/JU
 Sample : PB166157BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	30	rVB	75930	94464	2.31%	0.207%
2	3.510	85	89	103	rBV	931179	1313648	32.12%	2.884%
3	3.822	138	142	148	rVB	25307	31615	0.77%	0.069%
4	6.710	627	633	647	rBV	916132	1459669	35.69%	3.204%
5	6.869	654	660	672	rVB	802833	1214303	29.69%	2.666%
6	7.063	686	693	705	rVV	929068	1463265	35.78%	3.212%
7	7.522	764	771	780	rBV	820664	1247351	30.50%	2.738%
8	8.234	885	892	909	rBV	1044160	1679987	41.08%	3.688%
9	8.663	958	965	976	rBV	864834	1357088	33.19%	2.979%
10	9.110	1038	1041	1046	rVB6	5699	8639	0.21%	0.019%
11	9.375	1079	1086	1096	rBV	618198	1024009	25.04%	2.248%
12	9.910	1170	1177	1188	rBV	976868	1624635	39.73%	3.566%
13	10.022	1195	1196	1204	rVB6	5411	9022	0.22%	0.020%
14	10.281	1232	1240	1249	rBV	1030849	1616256	39.52%	3.548%
15	10.428	1256	1265	1288	rBV	809075	1554842	38.02%	3.413%
16	11.892	1509	1514	1521	rBV5	10484	24025	0.59%	0.053%
17	13.580	1794	1801	1814	rBV	1764314	2360671	57.73%	5.182%
18	13.851	1839	1847	1859	rBV	2021161	2886582	70.59%	6.337%
19	14.157	1893	1899	1908	rBV	1399109	2026563	49.56%	4.449%
20	14.386	1931	1938	1957	rBV	325936	719612	17.60%	1.580%
21	15.163	2062	2070	2082	rBV	2523269	3576558	87.46%	7.851%
22	15.286	2085	2091	2105	rVV	629614	844944	20.66%	1.855%
23	15.404	2108	2111	2116	rVB3	9773	14488	0.35%	0.032%
24	15.721	2161	2165	2170	rBV6	4177	7502	0.18%	0.016%
25	15.957	2201	2205	2210	rVB5	5399	9074	0.22%	0.020%
26	16.604	2309	2315	2320	rVB6	3043	5673	0.14%	0.012%
27	16.698	2327	2331	2335	rBV4	5994	7795	0.19%	0.017%
28	16.909	2359	2367	2376	rBV2	1662517	2193773	53.64%	4.816%
29	17.009	2378	2384	2398	rVV	2783925	3685064	90.11%	8.089%
30	18.880	2697	2702	2707	rVB4	23032	32016	0.78%	0.070%
31	18.951	2710	2714	2720	rVV	19768	28283	0.69%	0.062%
32	19.139	2743	2746	2747	rBV3	5335	4399	0.11%	0.010%
33	19.156	2747	2749	2754	rVV5	3138	4997	0.12%	0.011%
34	19.315	2770	2776	2790	rBV	3328022	4089432	100.00%	8.977%
35	21.139	3081	3086	3101	rBV	1371371	1966818	48.10%	4.318%
36	23.733	3519	3527	3547	rVB2	1567259	3362486	82.22%	7.381%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049368.D
Acq On : 21 Jan 2025 17:05
Operator : RC/JU
Sample : PB166157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK157

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Title : SVOA CALIBRATION

37	23.921	3551	3559	3577	rVB	852563	2004420	49.01%	4.400%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 45553968

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049368.D
Acq On : 21 Jan 2025 17:05
Operator : RC/JU
Sample : PB166157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

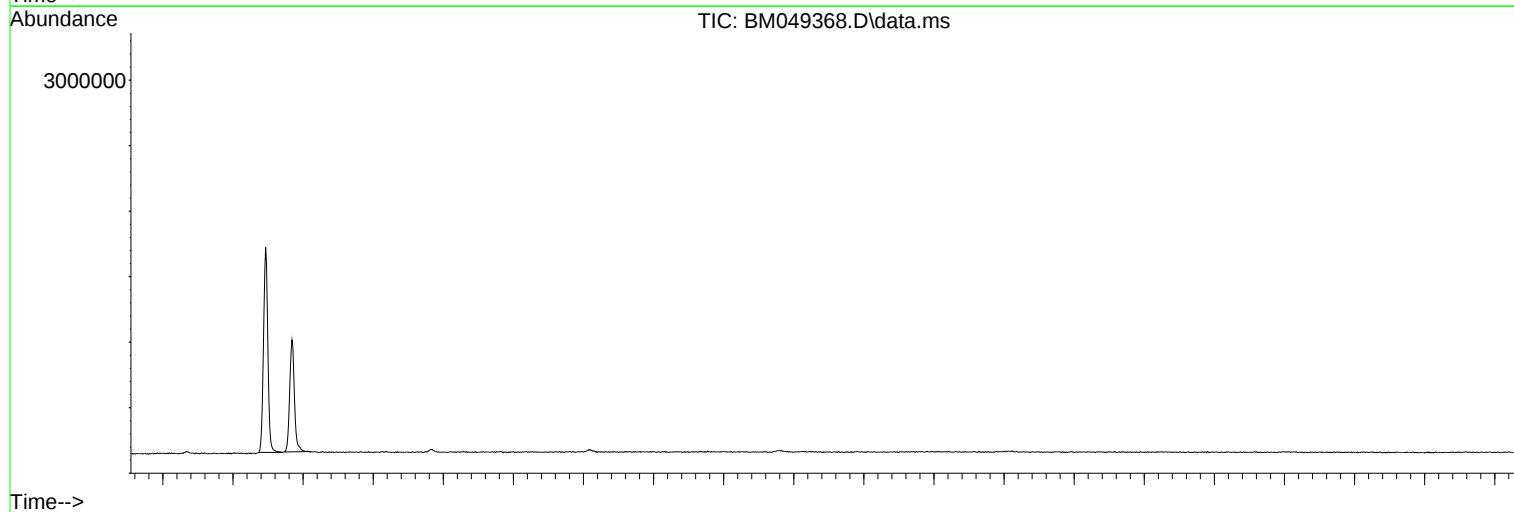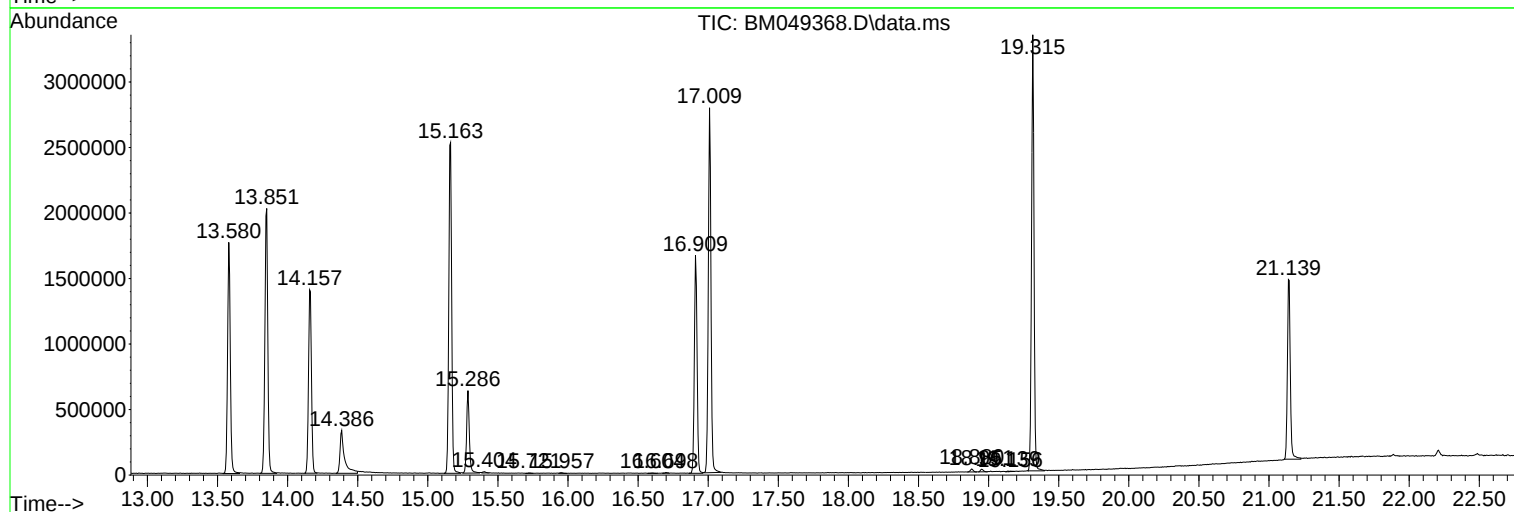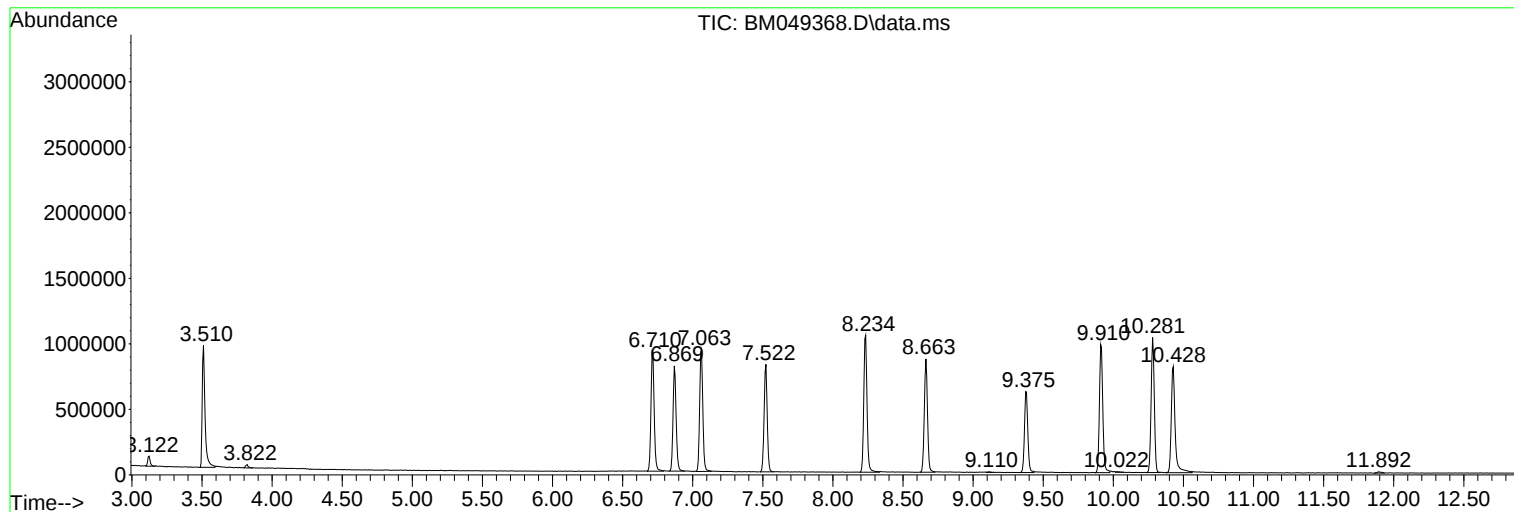

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049368.D
Acq On : 21 Jan 2025 17:05
Operator : RC/JU
Sample : PB166157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049368.D
Acq On : 21 Jan 2025 17:05
Operator : RC/JU
Sample : PB166157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc