

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049369.D
 Acq On : 21 Jan 2025 17:44
 Operator : RC/JU
 Sample : PB166156BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK156

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	31	rVB	66925	82813	2.72%	0.237%
2	3.510	85	89	111	rBV	871268	1201416	39.45%	3.431%
3	3.822	139	142	150	rVB6	12442	21069	0.69%	0.060%
4	5.022	344	346	349	rBV4	3639	3427	0.11%	0.010%
5	5.622	446	448	451	rVB3	3548	3353	0.11%	0.010%
6	6.716	627	634	646	rBV	793444	1217007	39.96%	3.476%
7	6.869	654	660	673	rVB	648695	985508	32.36%	2.815%
8	7.063	685	693	705	rBV	805926	1233640	40.50%	3.523%
9	7.522	764	771	781	rBV	636792	994662	32.66%	2.841%
10	8.234	884	892	904	rBV	860313	1346918	44.22%	3.847%
11	8.592	951	953	956	rVB4	2966	3447	0.11%	0.010%
12	8.663	956	965	977	rBV	651407	1074450	35.28%	3.069%
13	9.375	1079	1086	1096	rBV	468143	785076	25.78%	2.242%
14	9.751	1146	1150	1154	rVB5	2034	3134	0.10%	0.009%
15	9.916	1169	1178	1199	rBV	731971	1311485	43.06%	3.746%
16	10.281	1233	1240	1249	rVB	752819	1217583	39.98%	3.477%
17	10.428	1257	1265	1286	rBV	605289	1181780	38.80%	3.375%
18	11.892	1508	1514	1523	rVB8	8634	22231	0.73%	0.063%
19	12.816	1668	1671	1673	rBV3	3069	3101	0.10%	0.009%
20	13.580	1795	1801	1815	rBV	1173005	1618772	53.15%	4.623%
21	13.674	1815	1817	1820	rVB3	3803	3752	0.12%	0.011%
22	13.845	1838	1846	1860	rBV	1472895	2128897	69.90%	6.080%
23	13.939	1860	1862	1866	rVB3	2478	3162	0.10%	0.009%
24	14.163	1892	1900	1910	rVV	996545	1468755	48.22%	4.195%
25	14.386	1932	1938	1958	rBV	162456	472593	15.52%	1.350%
26	15.004	2041	2043	2047	rVB4	2557	3146	0.10%	0.009%
27	15.163	2063	2070	2085	rBV	1832590	2597484	85.28%	7.418%
28	15.286	2085	2091	2104	rVV	385741	535411	17.58%	1.529%
29	15.404	2108	2111	2115	rVB5	7184	10027	0.33%	0.029%
30	15.580	2137	2141	2142	rBV3	2211	3115	0.10%	0.009%
31	16.333	2267	2269	2274	rBV5	2365	3831	0.13%	0.011%
32	16.398	2277	2280	2283	rVB5	2188	3219	0.11%	0.009%
33	16.704	2326	2332	2337	rBV3	3873	6510	0.21%	0.019%
34	16.910	2361	2367	2378	rBV2	1132968	1579254	51.85%	4.510%
35	17.010	2378	2384	2404	rVV	1944130	2684837	88.15%	7.668%
36	17.151	2405	2408	2411	rVB5	2841	3304	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049369.D
Acq On : 21 Jan 2025 17:44
Operator : RC/JU
Sample : PB166156BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Title : SVOA CALIBRATION

37	17.257	2423	2426	2429	rBV5	2253	3713	0.12%	0.011%
38	17.374	2442	2446	2448	rBV4	2962	3149	0.10%	0.009%
39	17.798	2515	2518	2521	rBV4	2660	3226	0.11%	0.009%
40	18.315	2603	2606	2608	rBV3	3758	3904	0.13%	0.011%
41	18.833	2690	2694	2695	rBV4	3097	3103	0.10%	0.009%
42	18.880	2699	2702	2707	rVV5	17352	24826	0.82%	0.071%
43	18.951	2710	2714	2720	rVV3	15476	24623	0.81%	0.070%
44	19.004	2720	2723	2727	rVV4	3693	4913	0.16%	0.014%
45	19.315	2770	2776	2788	rBV	2389563	3045713	100.00%	8.698%
46	21.139	3081	3086	3096	rBV	1174696	1574988	51.71%	4.498%
47	23.733	3518	3527	3542	rBV	1253851	2796341	91.81%	7.986%
48	23.921	3551	3559	3578	rVB	711904	1708257	56.09%	4.879%




Sum of corrected areas: 35014925

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049369.D
Acq On : 21 Jan 2025 17:44
Operator : RC/JU
Sample : PB166156BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

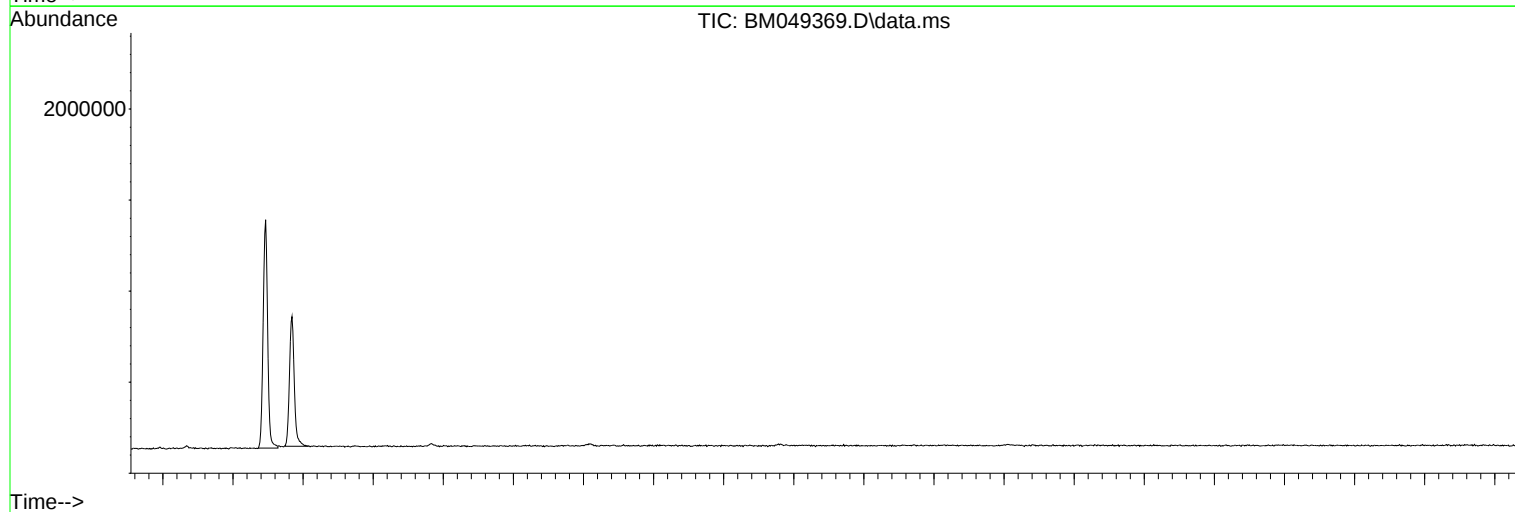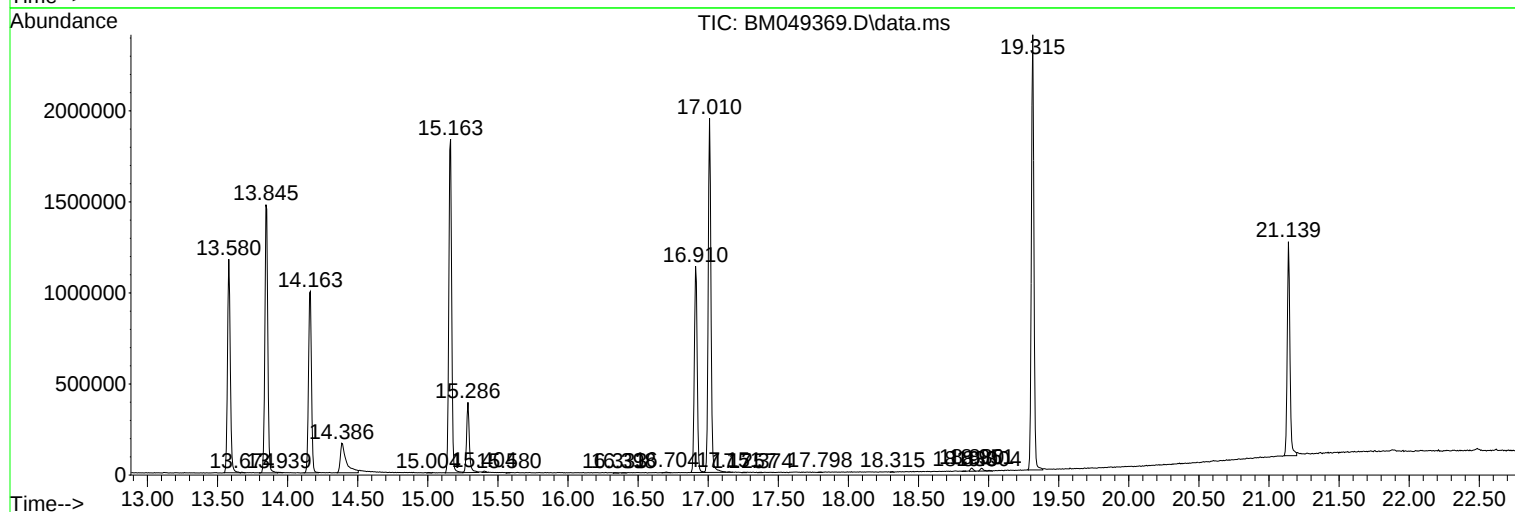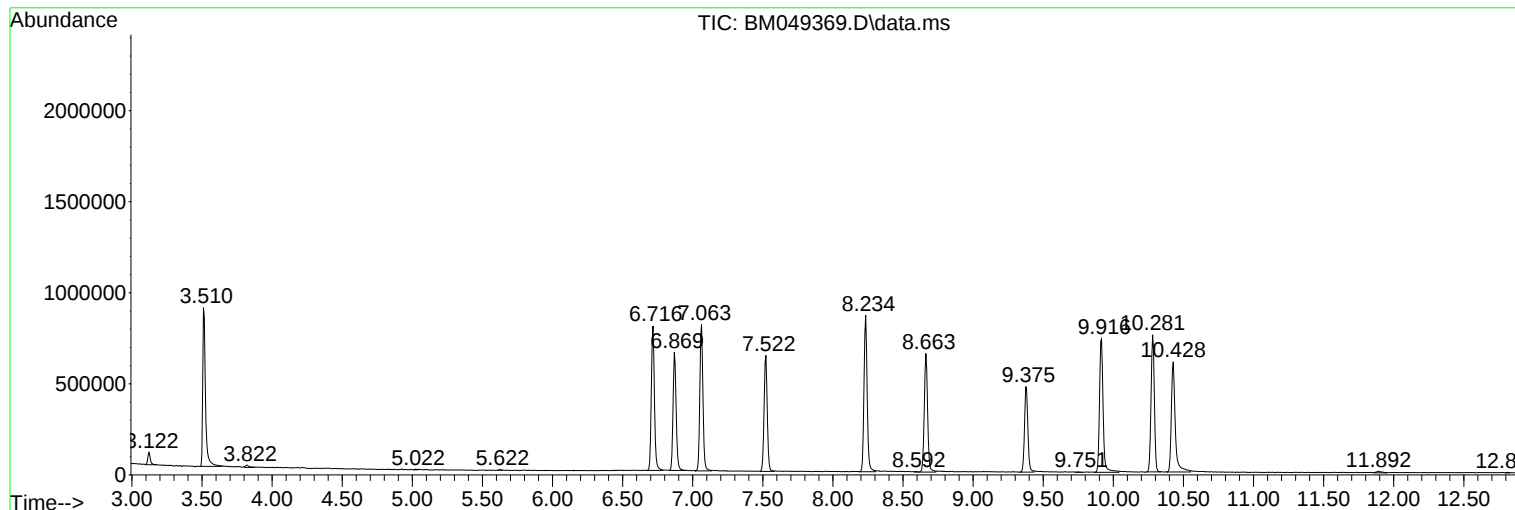

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049369.D
Acq On : 21 Jan 2025 17:44
Operator : RC/JU
Sample : PB166156BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049369.D
Acq On : 21 Jan 2025 17:44
Operator : RC/JU
Sample : PB166156BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
