

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049377.D
 Acq On : 21 Jan 2025 22:55
 Operator : RC/JU
 Sample : PB166133TB 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB133

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	28	rBV	87614	102635	2.65%	0.220%
2	3.510	85	89	105	rBV	1249419	1591373	41.02%	3.406%
3	3.822	138	142	145	rBV2	13752	20864	0.54%	0.045%
4	6.534	600	603	606	rBV5	3709	5538	0.14%	0.012%
5	6.716	627	634	654	rVB	1105351	1709325	44.07%	3.659%
6	6.869	654	660	674	rVB	877160	1339445	34.53%	2.867%
7	7.063	686	693	707	rBV	1130423	1728091	44.55%	3.699%
8	7.522	764	771	778	rBV	856539	1349437	34.79%	2.889%
9	8.234	885	892	903	rBV	1211914	1907420	49.17%	4.083%
10	8.516	937	940	942	rBV4	3284	4424	0.11%	0.009%
11	8.663	958	965	977	rBV	918198	1459198	37.62%	3.123%
12	9.222	1059	1060	1069	rBV8	3336	7670	0.20%	0.016%
13	9.375	1079	1086	1102	rBV	680325	1129877	29.13%	2.419%
14	9.786	1152	1156	1160	rVB6	4032	4530	0.12%	0.010%
15	9.910	1168	1177	1187	rBV	1086039	1842312	47.49%	3.944%
16	10.281	1233	1240	1251	rVB	1062859	1706295	43.99%	3.652%
17	10.428	1256	1265	1277	rBV	844376	1588561	40.95%	3.400%
18	11.128	1380	1384	1387	rBV5	2812	3914	0.10%	0.008%
19	11.310	1410	1415	1419	rBV7	3008	5208	0.13%	0.011%
20	11.580	1458	1461	1463	rBV4	4335	5630	0.15%	0.012%
21	11.886	1509	1513	1521	rBV6	9779	24181	0.62%	0.052%
22	12.228	1568	1571	1574	rVB4	3057	4382	0.11%	0.009%
23	12.651	1640	1643	1646	rBV4	2713	4168	0.11%	0.009%
24	13.439	1771	1777	1780	rBV8	2273	4520	0.12%	0.010%
25	13.580	1794	1801	1812	rVV	1714096	2354841	60.71%	5.041%
26	13.845	1839	1846	1856	rBV	2054006	2954032	76.15%	6.323%
27	14.157	1892	1899	1907	rBV	1454265	2056036	53.00%	4.401%
28	14.386	1931	1938	1959	rBV	254588	647854	16.70%	1.387%
29	14.839	2013	2015	2019	rVB5	4666	4426	0.11%	0.009%
30	15.074	2053	2055	2058	rBV4	3731	4308	0.11%	0.009%
31	15.157	2063	2069	2083	rBV	2542414	3577027	92.21%	7.657%
32	15.286	2085	2091	2101	rVV	498938	682045	17.58%	1.460%
33	15.404	2107	2111	2120	rVB6	11582	21326	0.55%	0.046%
34	15.945	2201	2203	2207	rBV5	4624	5260	0.14%	0.011%
35	16.439	2283	2287	2290	rBV4	4343	6883	0.18%	0.015%
36	16.698	2325	2331	2335	rBV5	6547	11821	0.30%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049377.D
 Acq On : 21 Jan 2025 22:55
 Operator : RC/JU
 Sample : PB166133TB 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB133

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

37	16.910	2361	2367	2377	rBV2	1591049	2148882	55.40%	4.600%
38	17.010	2377	2384	2398	rVV	2715214	3573420	92.12%	7.649%
39	17.133	2401	2405	2408	rVB6	3705	6505	0.17%	0.014%
40	17.374	2442	2446	2449	rVB5	3714	4973	0.13%	0.011%
41	17.604	2481	2485	2488	rBV5	5843	9896	0.26%	0.021%
42	17.739	2503	2508	2511	rVB6	3325	4464	0.12%	0.010%
43	18.468	2630	2632	2638	rVB6	4058	5431	0.14%	0.012%
44	18.527	2638	2642	2644	rBV5	3508	4531	0.12%	0.010%
45	18.609	2652	2656	2658	rBV5	2675	4454	0.11%	0.010%
46	18.839	2692	2695	2698	rVB3	4027	5113	0.13%	0.011%
47	18.880	2698	2702	2706	rBV2	23526	36687	0.95%	0.079%
48	18.951	2710	2714	2719	rVV	20726	28248	0.73%	0.060%
49	19.180	2751	2753	2755	rBV3	4475	4338	0.11%	0.009%
50	19.268	2766	2768	2769	rBV2	4974	4601	0.12%	0.010%
51	19.315	2770	2776	2791	rVV	3095009	3879048	100.00%	8.303%
52	21.139	3081	3086	3097	rBV	1362663	1904172	49.09%	4.076%
53	23.727	3519	3526	3541	rVB	1476502	3233846	83.37%	6.922%
54	23.915	3551	3558	3574	rVB	848515	1983784	51.14%	4.246%

Sum of corrected areas: 46717250




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049377.D
Acq On : 21 Jan 2025 22:55
Operator : RC/JU
Sample : PB166133TB 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB133

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

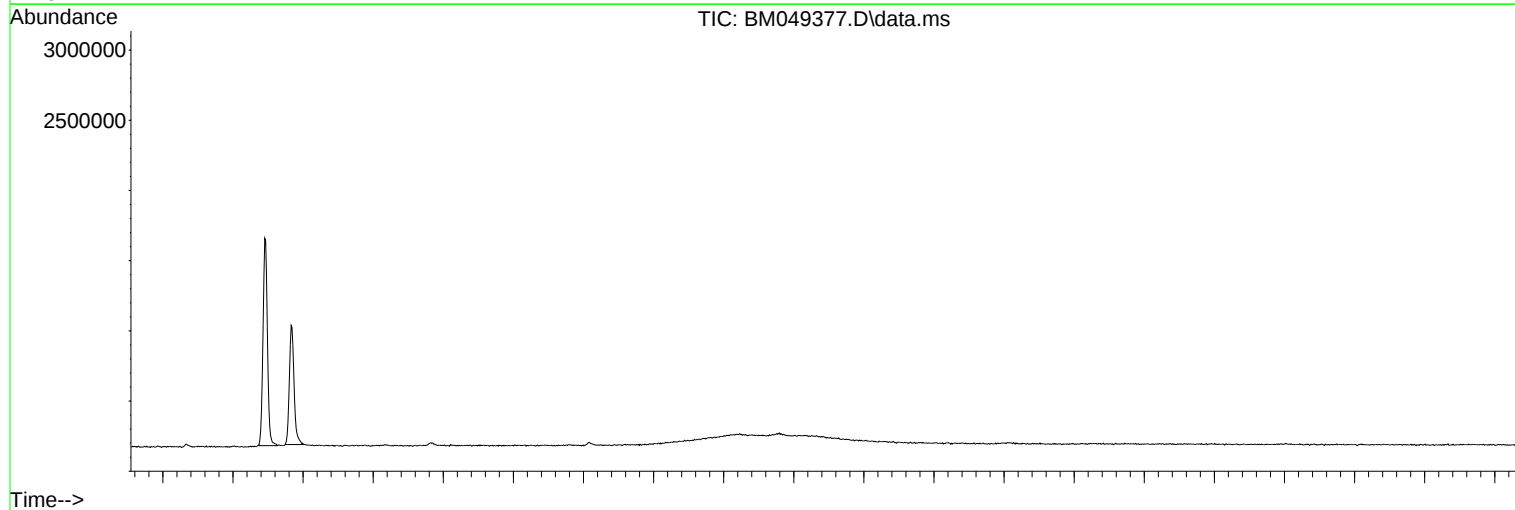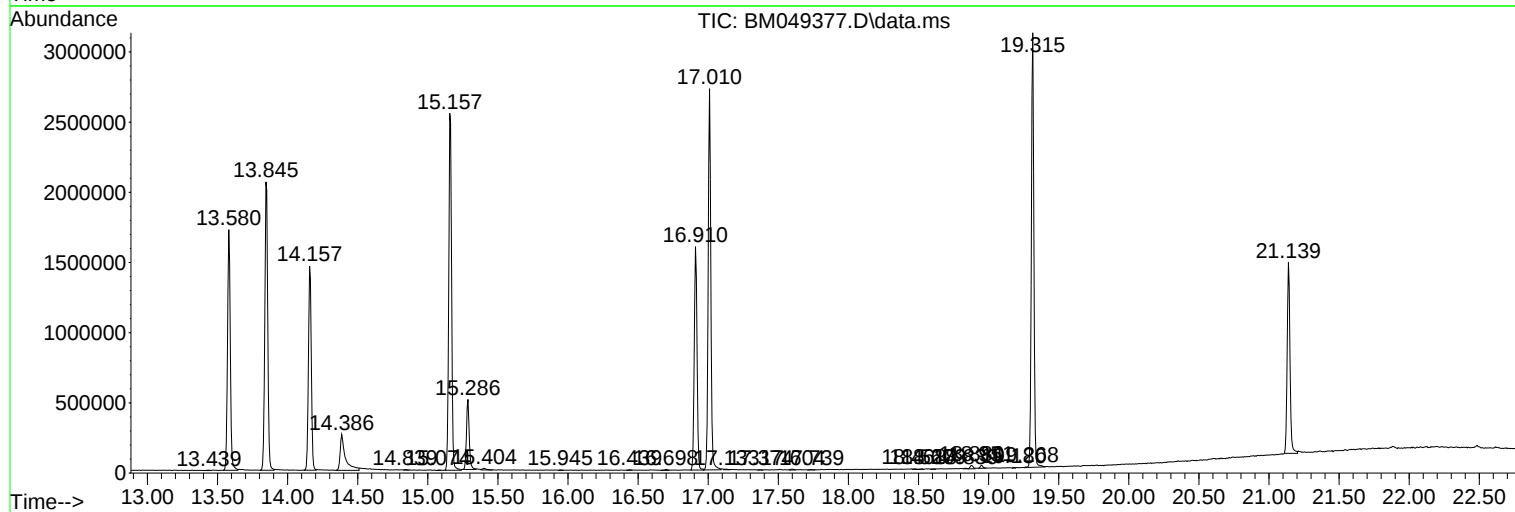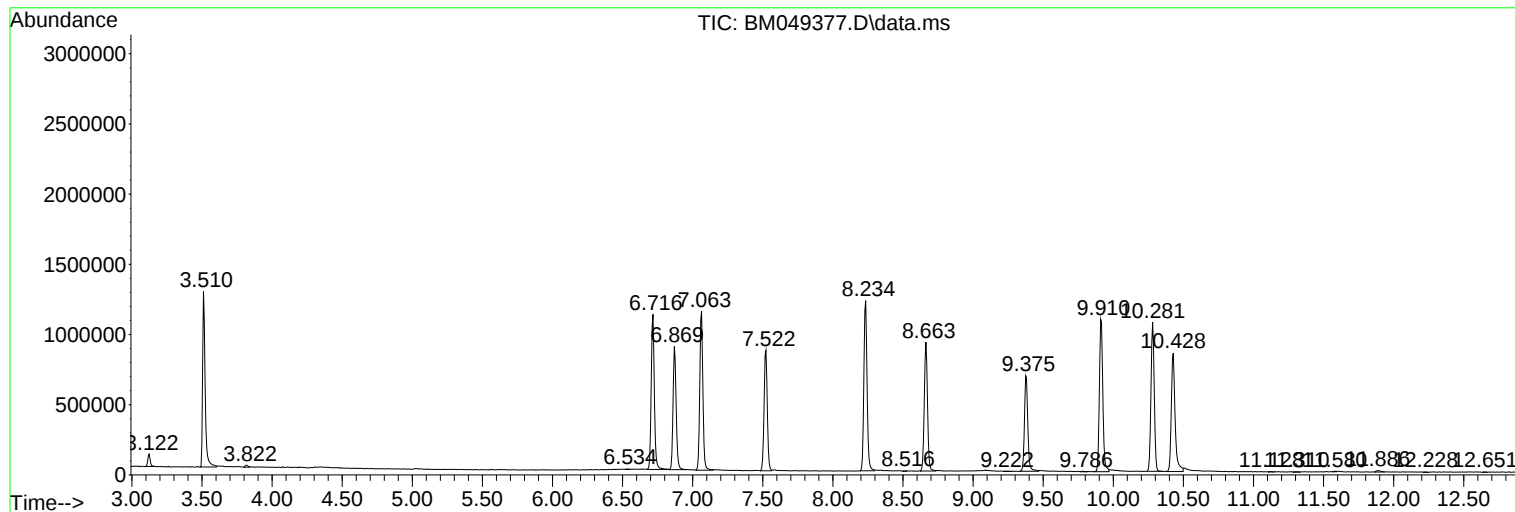

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049377.D
Acq On : 21 Jan 2025 22:55
Operator : RC/JU
Sample : PB166133TB 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB133

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049377.D
Acq On : 21 Jan 2025 22:55
Operator : RC/JU
Sample : PB166133TB 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB133

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
