

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049382.D
 Acq On : 22 Jan 2025 14:15
 Operator : RC/JU
 Sample : PB166160BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	19	22	29	rVB	61471	71680	2.45%	0.192%
2	3.510	85	89	103	rBV	779059	1085137	37.07%	2.912%
3	3.816	137	141	149	rVB	33724	47015	1.61%	0.126%
4	5.369	403	405	408	rVB4	3955	3141	0.11%	0.008%
5	5.616	445	447	452	rVB6	4091	5146	0.18%	0.014%
6	6.710	627	633	645	rVB	707153	1129549	38.58%	3.031%
7	6.869	654	660	671	rVB	599696	919210	31.40%	2.467%
8	7.057	686	692	708	rVB	740379	1172633	40.05%	3.147%
9	7.522	764	771	780	rBV	818206	1325939	45.29%	3.558%
10	7.857	826	828	831	rBV3	2889	3861	0.13%	0.010%
11	7.910	834	837	839	rBV4	3131	3338	0.11%	0.009%
12	8.228	885	891	905	rBV	778360	1287364	43.97%	3.454%
13	8.663	958	965	976	rBV	617239	998109	34.09%	2.678%
14	9.028	1026	1027	1030	rBV3	3324	3975	0.14%	0.011%
15	9.375	1080	1086	1096	rBV	440480	749251	25.59%	2.011%
16	9.910	1169	1177	1191	rBV	716291	1251027	42.73%	3.357%
17	10.157	1217	1219	1224	rVB6	2712	3062	0.10%	0.008%
18	10.192	1224	1225	1230	rVB5	2353	2971	0.10%	0.008%
19	10.280	1232	1240	1250	rBV	1053348	1697137	57.97%	4.554%
20	10.428	1257	1265	1278	rBV	570832	1097243	37.48%	2.944%
21	10.663	1303	1305	1310	rVB6	3291	3729	0.13%	0.010%
22	10.875	1338	1341	1343	rBV4	3283	3395	0.12%	0.009%
23	11.322	1413	1417	1419	rBV5	2492	2960	0.10%	0.008%
24	11.586	1458	1462	1464	rBV4	3757	4123	0.14%	0.011%
25	11.822	1499	1502	1504	rVB4	3179	3041	0.10%	0.008%
26	11.857	1504	1508	1511	rBV6	2409	4601	0.16%	0.012%
27	11.892	1511	1514	1517	rBV5	5848	9397	0.32%	0.025%
28	12.145	1553	1557	1558	rBV4	3096	2958	0.10%	0.008%
29	12.857	1674	1678	1683	rVB7	2113	3564	0.12%	0.010%
30	13.163	1727	1730	1732	rVB3	3140	3123	0.11%	0.008%
31	13.286	1747	1751	1752	rVB4	2681	2934	0.10%	0.008%
32	13.451	1776	1779	1781	rBV4	2374	2998	0.10%	0.008%
33	13.580	1793	1801	1812	rBV	1170837	1668948	57.01%	4.478%
34	13.845	1840	1846	1862	rBV	1421284	2089969	71.39%	5.608%
35	14.157	1893	1899	1912	rBV	1462933	2147746	73.36%	5.763%
36	14.386	1932	1938	1963	rBV	132757	433393	14.80%	1.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049382.D
 Acq On : 22 Jan 2025 14:15
 Operator : RC/JU
 Sample : PB166160BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK160

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

37	14.580	1969	1971	1977	rVV6	3853	5848	0.20%	0.016%
38	15.010	2040	2044	2049	rVB6	3722	6628	0.23%	0.018%
39	15.157	2063	2069	2080	rBV	1767877	2567432	87.70%	6.889%
40	15.286	2085	2091	2101	rVV	347383	505949	17.28%	1.358%
41	15.351	2101	2102	2105	rVV3	6730	5253	0.18%	0.014%
42	15.398	2105	2110	2115	rVB6	6505	12338	0.42%	0.033%
43	15.510	2126	2129	2132	rVB4	2459	2952	0.10%	0.008%
44	15.568	2136	2139	2141	rVB3	2974	3335	0.11%	0.009%
45	16.662	2321	2325	2327	rVB5	2419	3330	0.11%	0.009%
46	16.704	2327	2332	2335	rBV4	6551	11649	0.40%	0.031%
47	16.909	2359	2367	2378	rBV	1750881	2367714	80.87%	6.353%
48	17.009	2378	2384	2399	rVB	1885875	2617764	89.42%	7.024%
49	17.315	2432	2436	2437	rBV4	2856	2999	0.10%	0.008%
50	17.504	2466	2468	2471	rBV3	4224	4618	0.16%	0.012%
51	17.539	2471	2474	2477	rVV4	3335	4542	0.16%	0.012%
52	17.568	2477	2479	2481	rVV3	3701	3164	0.11%	0.008%
53	17.598	2481	2484	2487	rVV4	3247	4627	0.16%	0.012%
54	17.651	2490	2493	2498	rVV6	3278	6171	0.21%	0.017%
55	18.462	2628	2631	2634	rVB4	3316	4386	0.15%	0.012%
56	18.880	2698	2702	2708	rVB4	20339	26473	0.90%	0.071%
57	18.951	2708	2714	2719	rBV3	18514	31373	1.07%	0.084%
58	19.315	2770	2776	2789	rBV	2251156	2927641	100.00%	7.856%
59	21.139	3080	3086	3095	rBV	1657543	2214965	75.66%	5.944%
60	23.727	3518	3526	3541	rBV	1135318	2424433	82.81%	6.506%
61	23.915	3550	3558	3574	rBV	933839	2257250	77.10%	6.057%




Sum of corrected areas: 37266501

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049382.D
Acq On : 22 Jan 2025 14:15
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

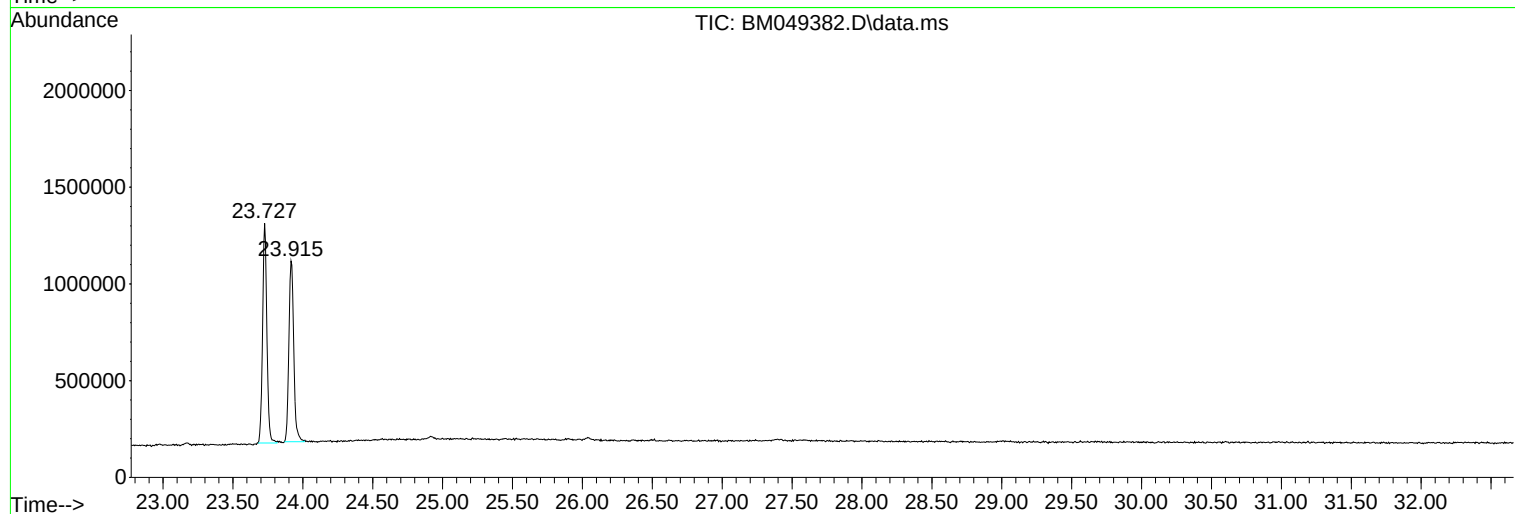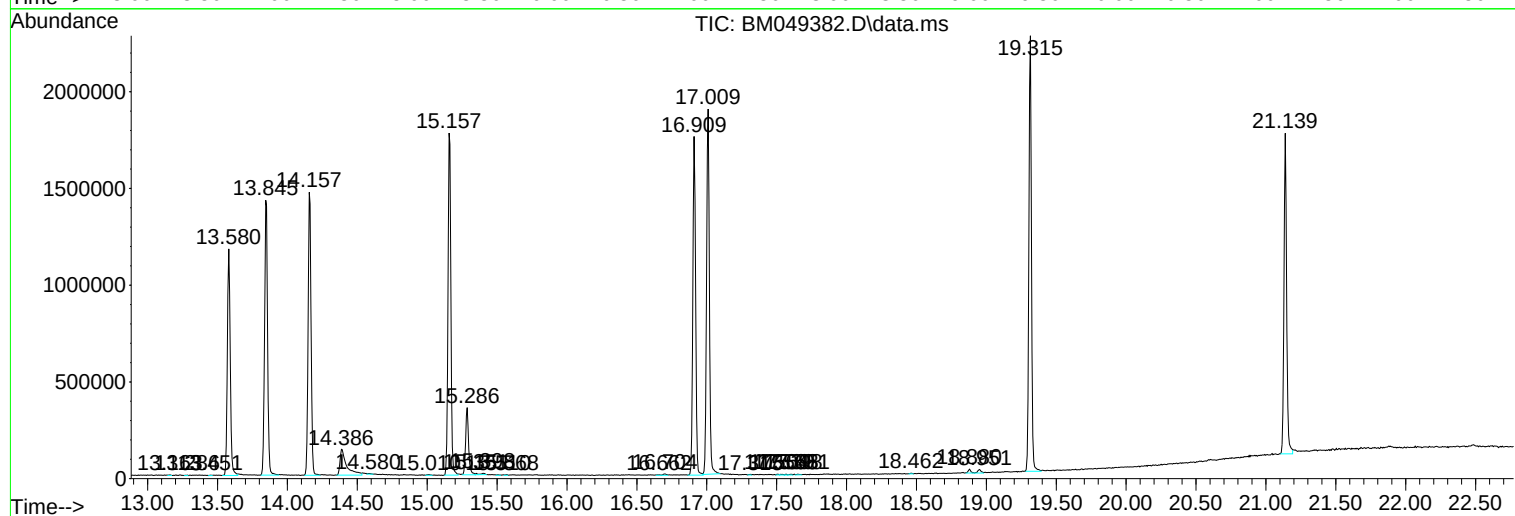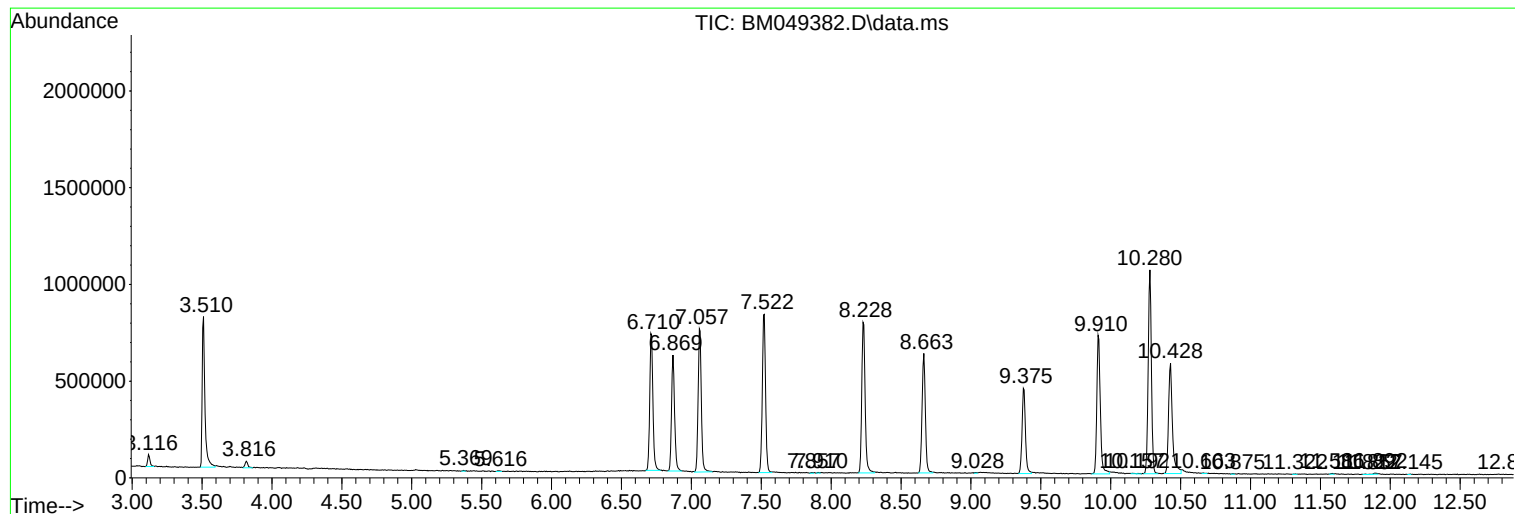

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049382.D
Acq On : 22 Jan 2025 14:15
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049382.D
Acq On : 22 Jan 2025 14:15
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------