

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
 Data File : BM049396.D
 Acq On : 22 Jan 2025 23:59
 Operator : RC/JU
 Sample : PB166160BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	31	rBV	87544	108010	2.57%	0.204%
2	3.505	84	88	104	rBV	1128530	1530710	36.38%	2.884%
3	3.816	137	141	145	rVB	40152	53468	1.27%	0.101%
4	4.675	285	287	292	rBV5	4884	4509	0.11%	0.008%
5	6.410	579	582	583	rBV3	4361	4571	0.11%	0.009%
6	6.710	627	633	645	rBV	1074745	1652476	39.28%	3.114%
7	6.869	654	660	675	rVB	847678	1299255	30.88%	2.448%
8	7.057	686	692	705	rBV	1099171	1656158	39.37%	3.121%
9	7.516	764	770	779	rBV	1206483	1849851	43.97%	3.486%
10	7.675	796	797	802	rBV5	3191	5203	0.12%	0.010%
11	8.004	852	853	858	rBV5	3510	4748	0.11%	0.009%
12	8.228	884	891	905	rBV	1211893	1889772	44.92%	3.561%
13	8.663	957	965	980	rVV	890460	1447899	34.42%	2.728%
14	9.169	1049	1051	1055	rBV4	3575	5198	0.12%	0.010%
15	9.375	1079	1086	1102	rBV	684171	1122163	26.67%	2.114%
16	9.910	1170	1177	1190	rBV	1100600	1834907	43.61%	3.457%
17	10.151	1215	1218	1223	rBV6	3190	6388	0.15%	0.012%
18	10.281	1232	1240	1250	rBV	1481219	2399734	57.04%	4.522%
19	10.422	1257	1264	1289	rBV	856771	1654774	39.33%	3.118%
20	11.886	1507	1513	1521	rBV4	11680	29350	0.70%	0.055%
21	13.580	1795	1801	1815	rBV	1701650	2381427	56.60%	4.487%
22	13.845	1837	1846	1860	rBV	2128753	3016810	71.71%	5.685%
23	14.157	1892	1899	1908	rBV	2212446	3043298	72.34%	5.734%
24	14.380	1931	1937	1960	rBV	293782	731109	17.38%	1.378%
25	14.580	1969	1971	1976	rVB6	4127	5300	0.13%	0.010%
26	14.833	2012	2014	2019	rVB6	3612	4787	0.11%	0.009%
27	15.010	2039	2044	2047	rVB6	4021	5213	0.12%	0.010%
28	15.157	2063	2069	2080	rBV	2631011	3656886	86.92%	6.891%
29	15.286	2084	2091	2101	rBV	497504	715761	17.01%	1.349%
30	15.404	2106	2111	2116	rVB5	13552	20203	0.48%	0.038%
31	15.727	2165	2166	2171	rVB4	4227	4386	0.10%	0.008%
32	15.892	2193	2194	2200	rVB5	2907	4818	0.11%	0.009%
33	15.951	2200	2204	2207	rBV5	4700	8594	0.20%	0.016%
34	16.433	2283	2286	2294	rVB7	3662	7376	0.18%	0.014%
35	16.698	2326	2331	2336	rVB4	6769	12783	0.30%	0.024%
36	16.910	2360	2367	2377	rBV	2446330	3334844	79.27%	6.284%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049396.D
Acq On : 22 Jan 2025 23:59
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Title : SVOA CALIBRATION

37	17.010	2377	2384	2398	rVB	2682651	3726673	88.58%	7.022%
38	17.598	2481	2484	2486	rBV4	2909	4280	0.10%	0.008%
39	18.880	2697	2702	2709	rBV4	22704	35185	0.84%	0.066%
40	18.951	2709	2714	2718	rBV	22378	29957	0.71%	0.056%
41	19.309	2765	2775	2790	rBV	3229160	4207154	100.00%	7.927%
42	21.139	3080	3086	3098	rBV	2292920	3090132	73.45%	5.823%
43	23.727	3518	3526	3541	rVB	1564857	3336853	79.31%	6.288%
44	23.915	3550	3558	3575	rVB	1362821	3127496	74.34%	5.893%




Sum of corrected areas: 53070469

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049396.D
Acq On : 22 Jan 2025 23:59
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

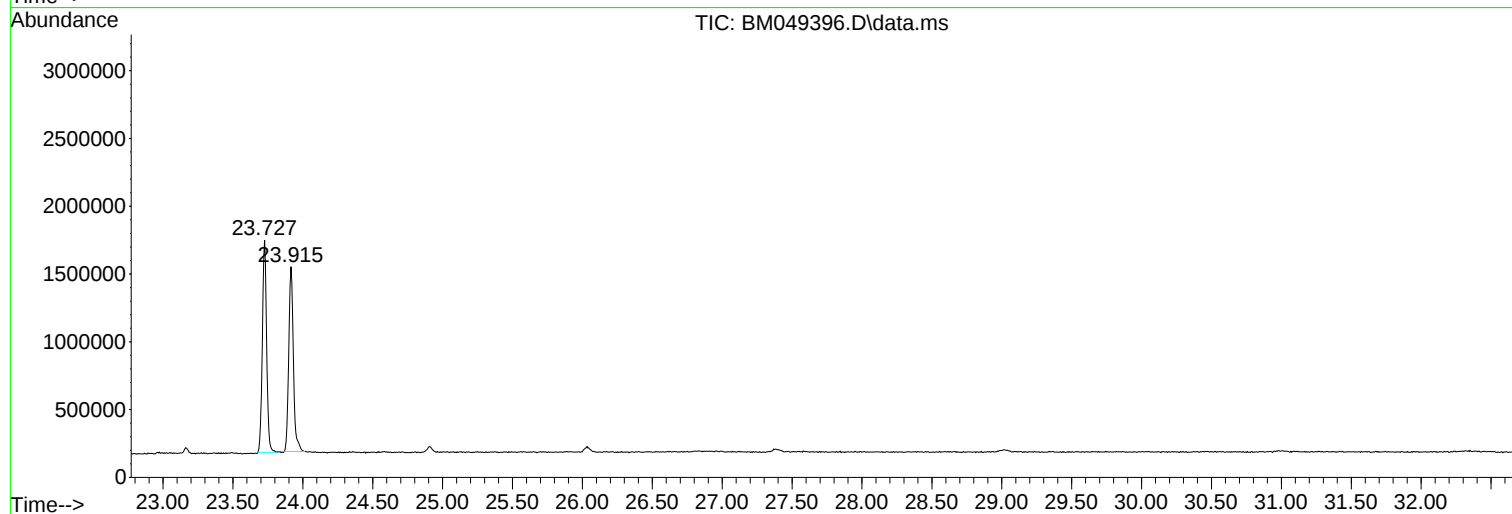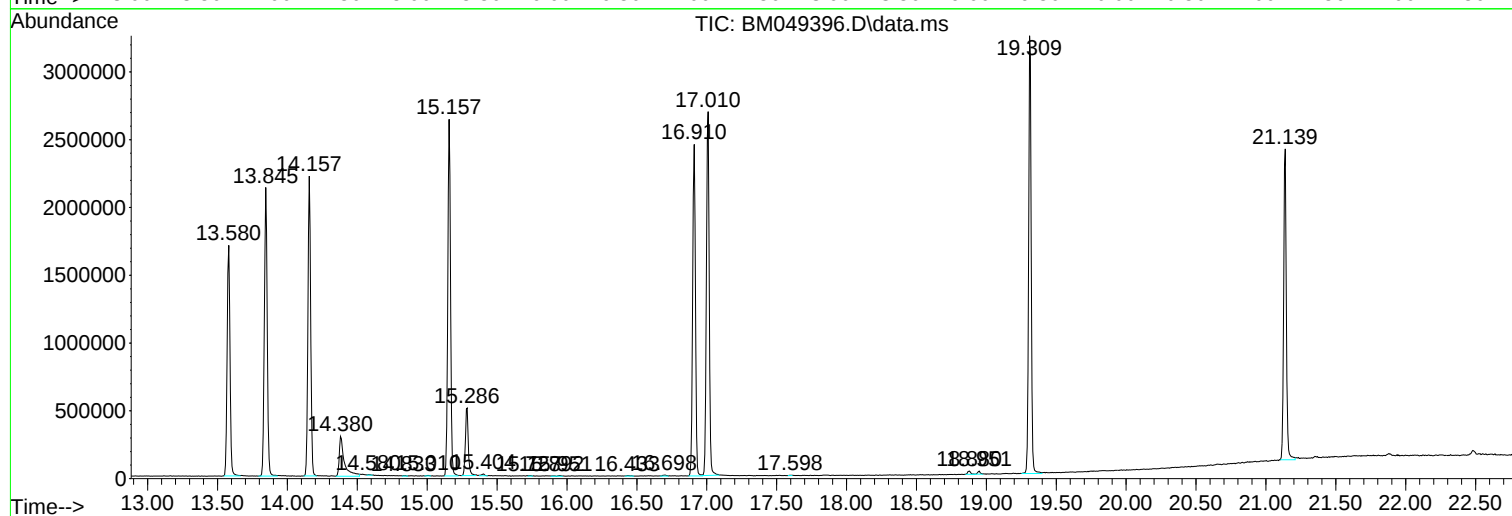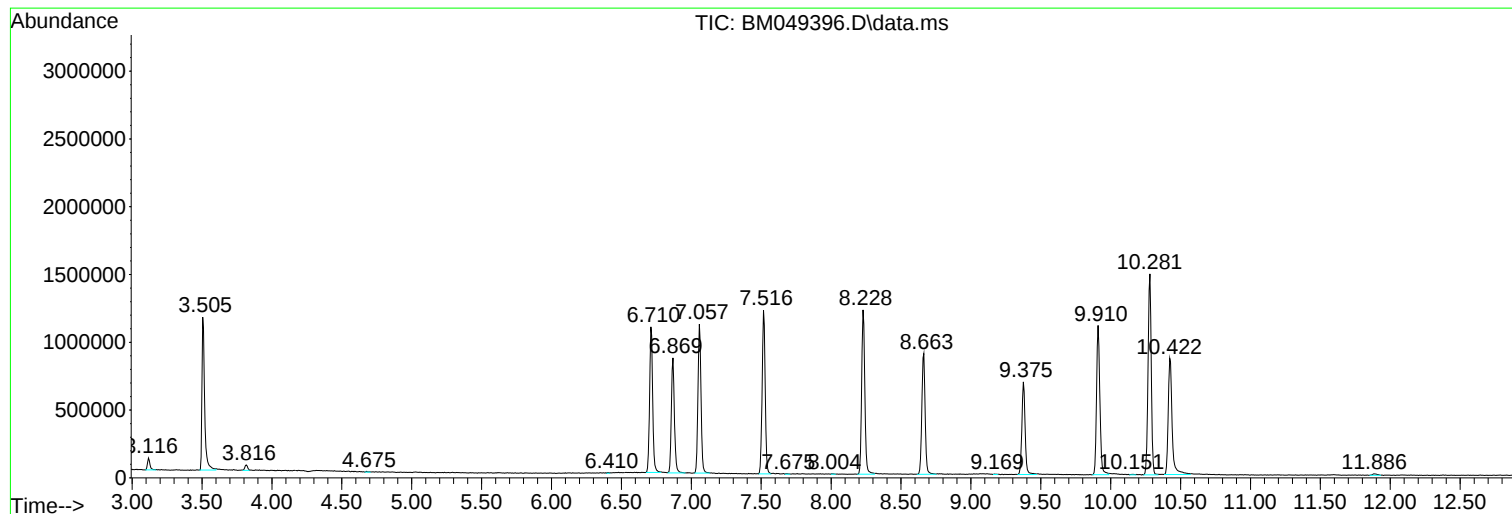

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049396.D
Acq On : 22 Jan 2025 23:59
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012225\
Data File : BM049396.D
Acq On : 22 Jan 2025 23:59
Operator : RC/JU
Sample : PB166160BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK160

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------