

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000323.D
 Acq On : 24 Jan 2015 08:33
 Operator : TP/IZ
 Sample : PB81490BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 26 11:48:34 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	103747	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	445365	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	197111	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	794046	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1066571	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	593035	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	18926	8.00	ng/uL	0.00
5) Phenol-d5	6.97	99	267688	30.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	207701	34.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	203647	32.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	198528	29.31	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	115705	34.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	109200	35.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	209152	30.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	39349	4.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	903859	63.86	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	158834	9.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	115204	49.19	ng/ul	0.00
57) Fluorene-d10	15.45	176	773451	60.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	115458	27.57	ng/ul	0.00
70) Anthracene-d10	17.29	188	699918	18.56	ng/ul	0.00
76) Pyrene-d10	19.59	212	1195235	25.25	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	613532	22.75	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.51	70	7371	1.07	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
Data File : BM000323.D
Acq On : 24 Jan 2015 08:33
Operator : TP/IZ
Sample : PB81490BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 26 11:48:34 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 24 04:15:00 2015
Response via : Initial Calibration

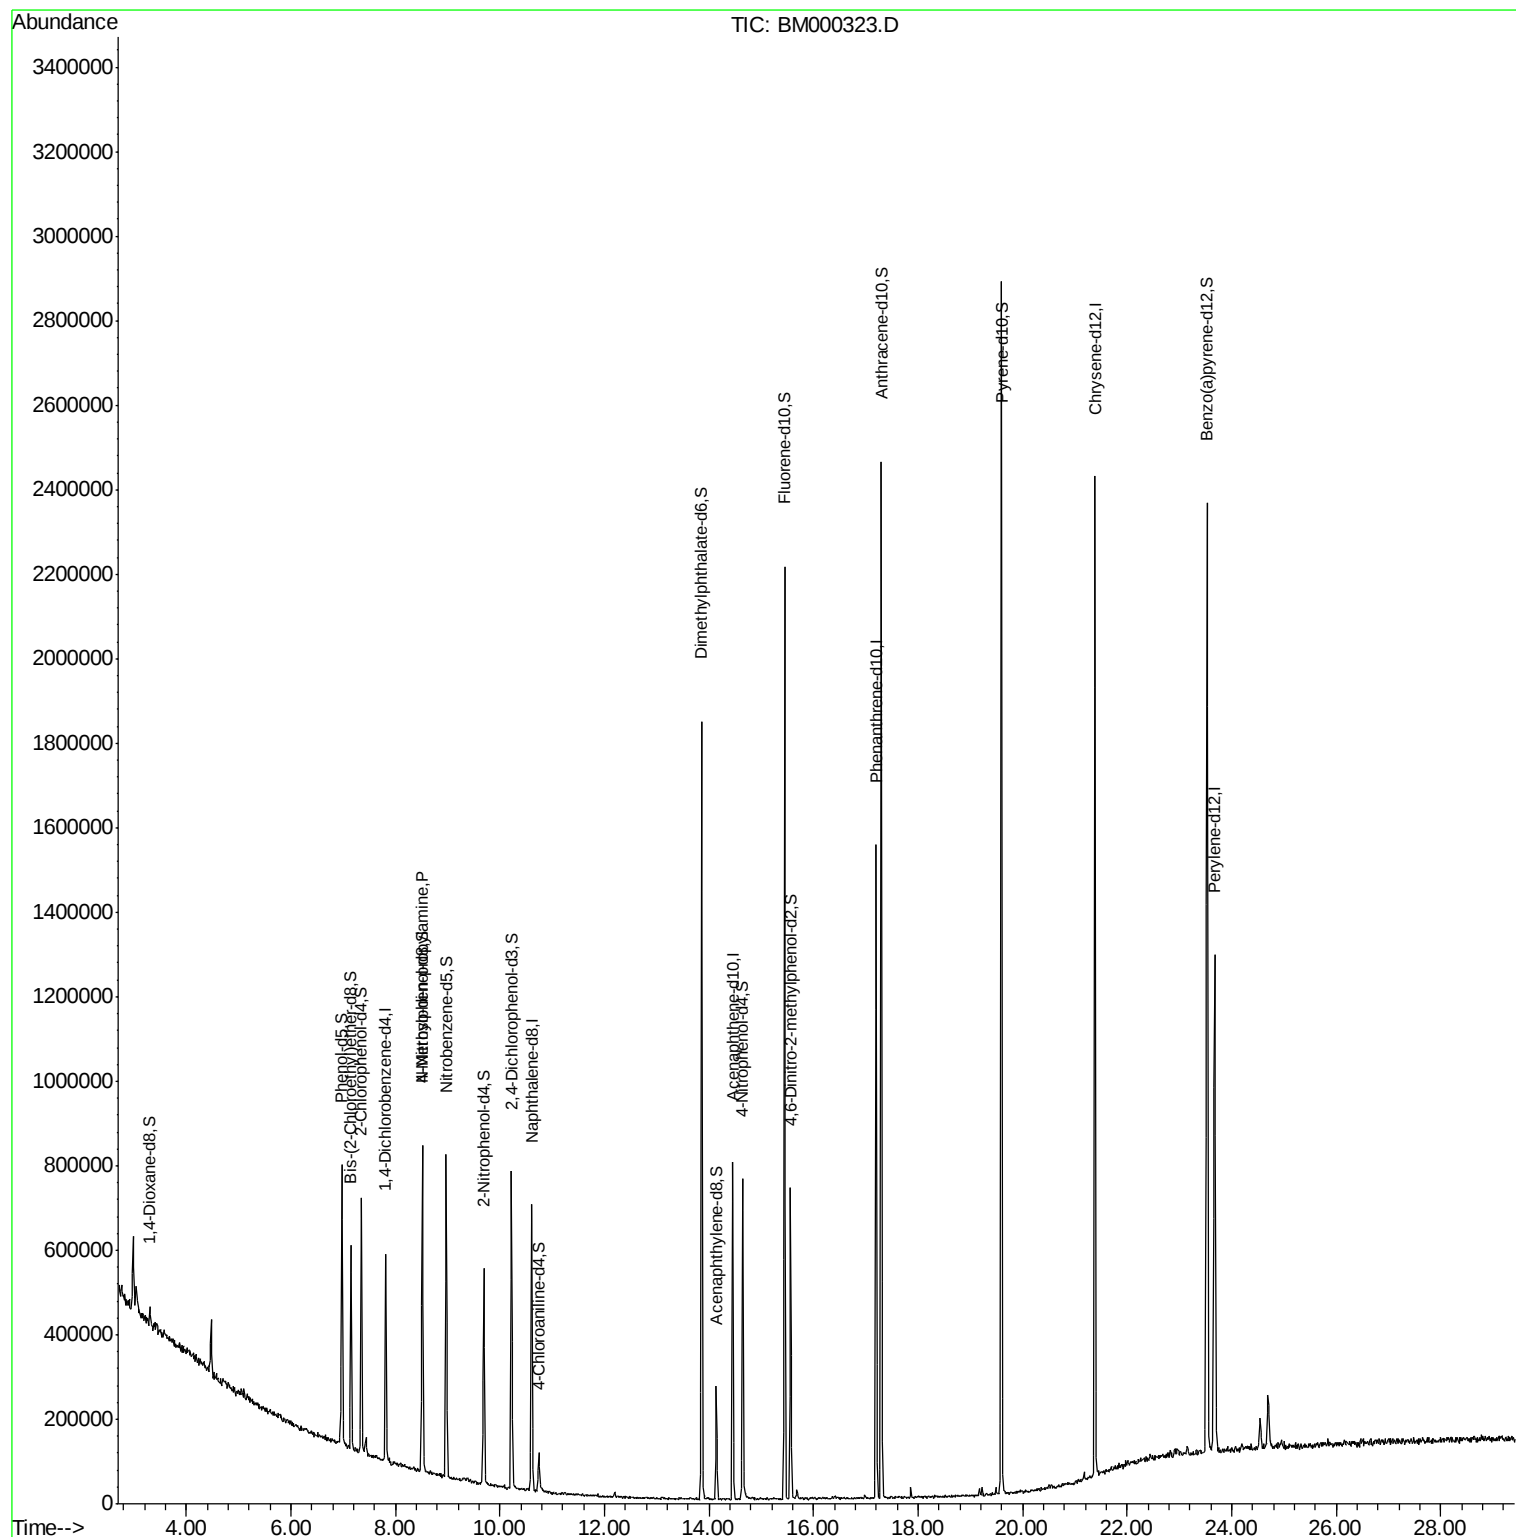

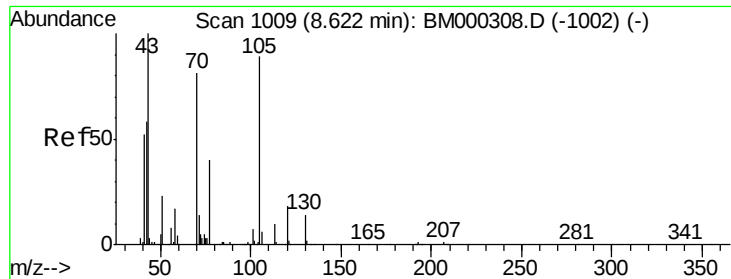

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.07 ng/ul
 RT: 8.51 min Scan# 990
 Delta R.T. -0.11 min
 Lab File: BM000323.D
 Acq: 24 Jan 2015 08:33

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 7371
 Ion Ratio Lower Upper
 70 100
 42 398.5 58.9 88.3#
 101 0.0 7.0 10.6#
 130 0.0 13.4 20.2#

