

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000334.D
 Acq On : 24 Jan 2015 15:39
 Operator : TP/IZ
 Sample : G1134-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 26 12:54:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 26 12:45:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	103305	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	423372	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	321107	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	758266	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1059181	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1112905	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	2328	0.99	ng/uL	0.00
5) Phenol-d5	6.97	99	40347	4.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	138593	22.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	112904	18.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	74572	11.06	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	80964	25.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	74982	25.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	141120	21.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	4107	0.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	744790	32.30	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	860781	30.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	17233	4.52	ng/ul	0.00
57) Fluorene-d10	15.44	176	687142	33.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	91080	22.77	ng/ul	0.00
70) Anthracene-d10	17.29	188	1192392	33.12	ng/ul	0.00
76) Pyrene-d10	19.59	212	1476849	31.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1468053	29.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.86	165	6546	1.51	ng/ul#	26




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
Data File : BM000334.D
Acq On : 24 Jan 2015 15:39
Operator : TP/IZ
Sample : G1134-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 26 12:54:28 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 26 12:45:18 2015
Response via : Initial Calibration

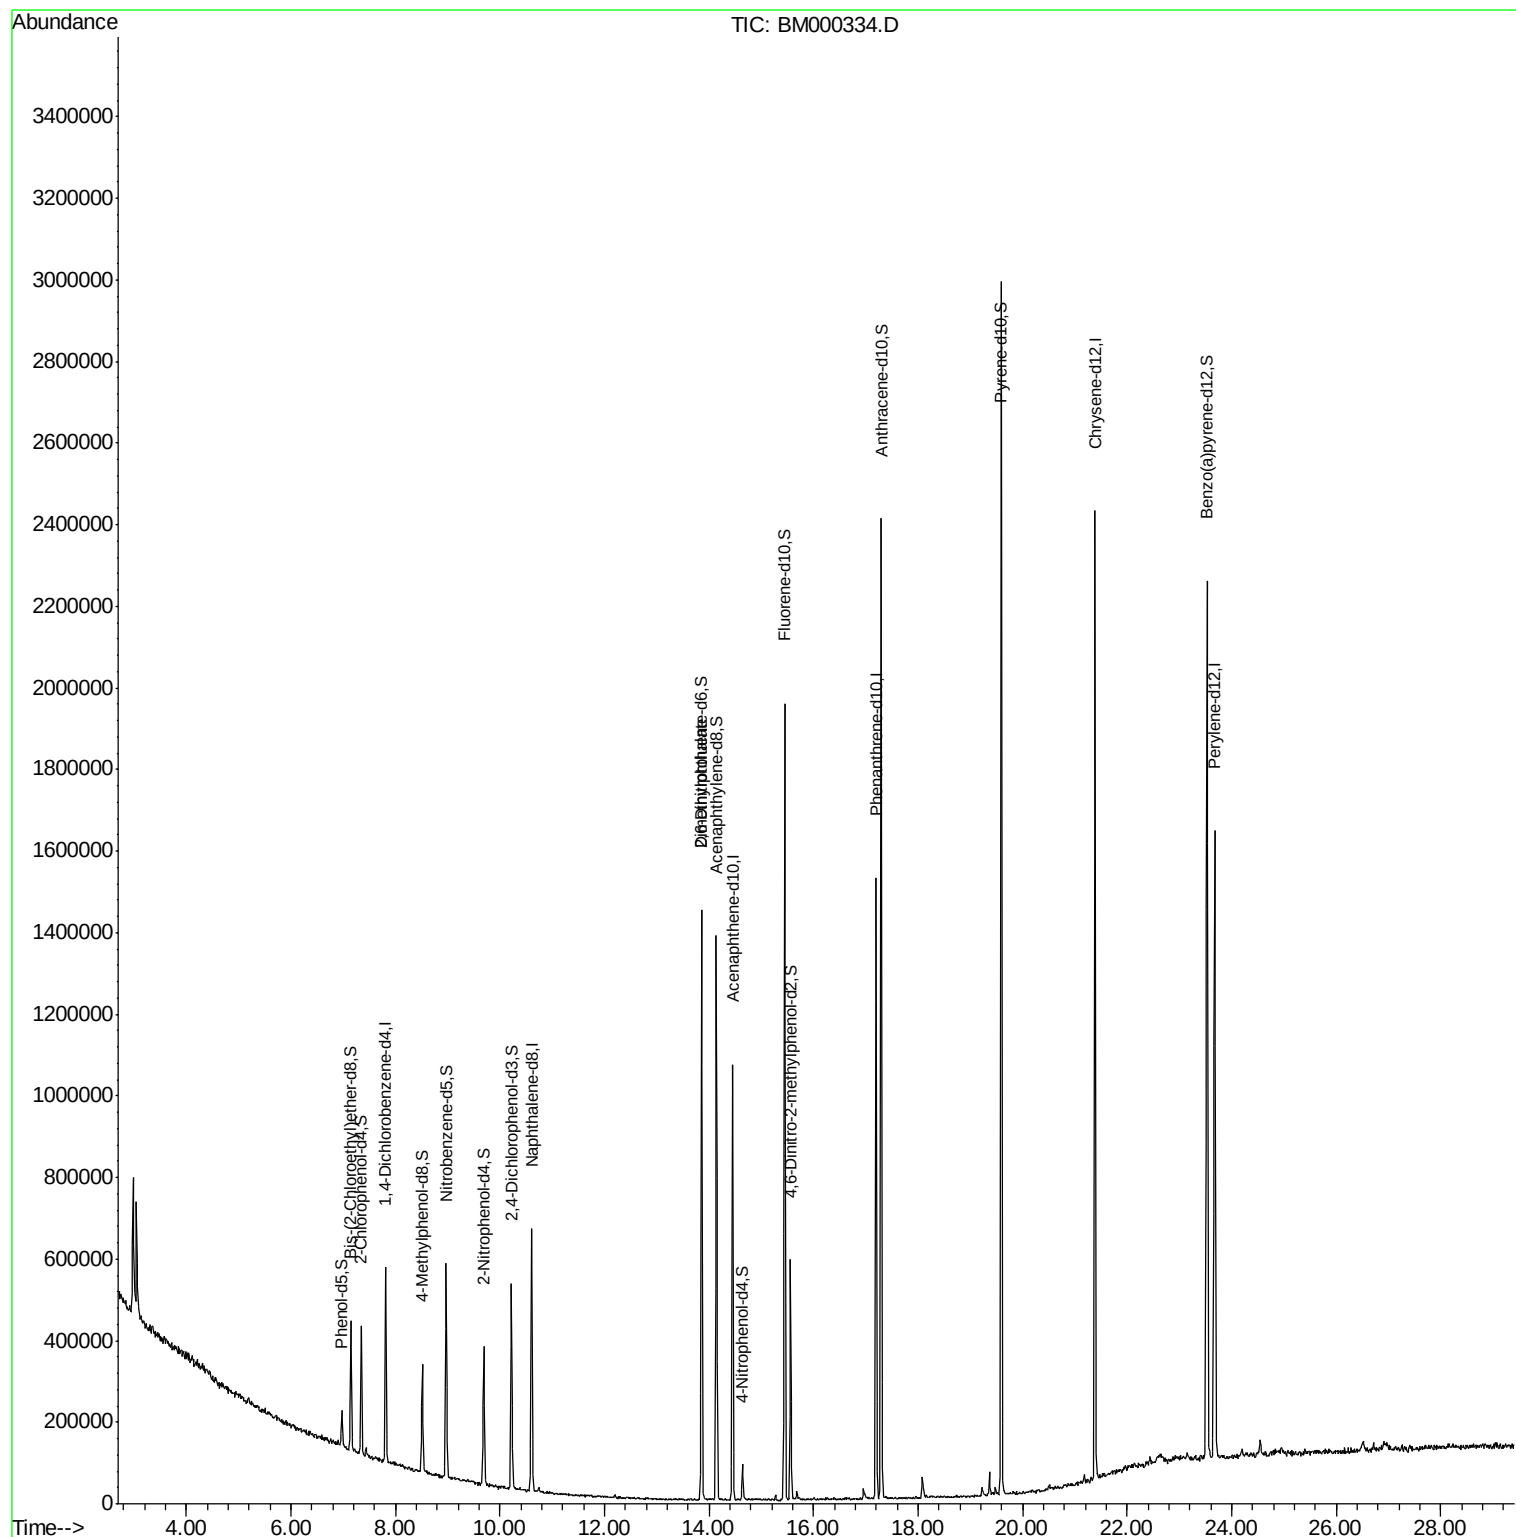

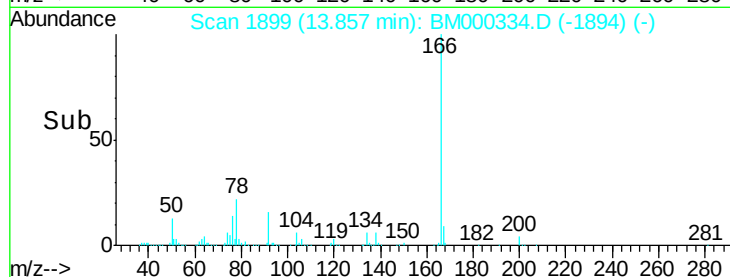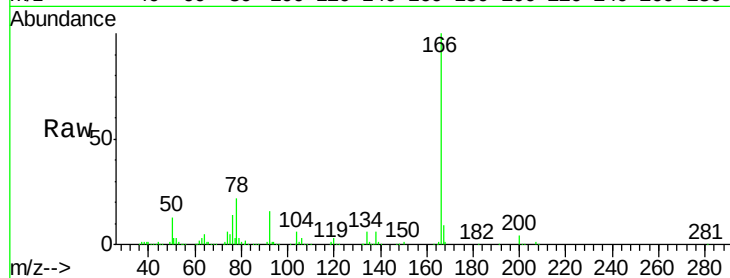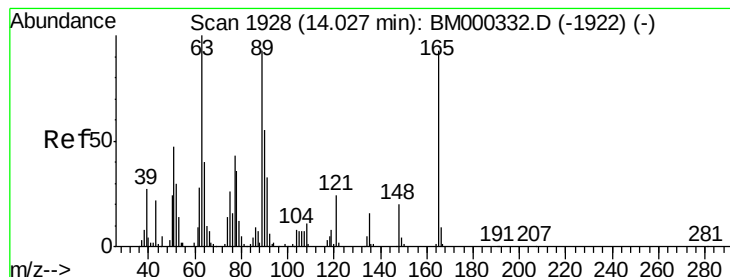

#45

2,6-Dinitrotoluene

Concen: 1.51 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. -0.17 min

Lab File: BM000334.D

Acq: 24 Jan 2015 15:39

Instrument :

BNA_M

ClientSampleId :

Tot Ion:165 Resp: 6546

Ion Ratio Lower Upper

165 100

89 0.0 69.5 104.3#

121 34.6 22.3 33.5#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

