

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000349.D
 Acq On : 25 Jan 2015 01:06
 Operator : TP/IZ
 Sample : PB81493BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 26 13:42:50 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 26 13:29:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	92913	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	383677	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	270356	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	698417	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	980782	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	895041	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	15378	7.26	ng/uL	0.00
5) Phenol-d5	6.97	99	198067	25.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	158072	29.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	155654	27.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	142908	23.56	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	86007	29.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	80671	30.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	154540	26.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	21638	3.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	643193	33.13	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	479337	20.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	83580	26.02	ng/ul	0.00
57) Fluorene-d10	15.44	176	612799	35.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	87625	23.79	ng/ul	0.00
70) Anthracene-d10	17.29	188	945879	28.52	ng/ul	0.00
76) Pyrene-d10	19.59	212	1205627	27.70	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	1074868	26.40	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.86	165	5535	1.52	ng/ul#	19




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
Data File : BM000349.D
Acq On : 25 Jan 2015 01:06
Operator : TP/IZ
Sample : PB81493BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 26 13:42:50 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 26 13:29:32 2015
Response via : Initial Calibration

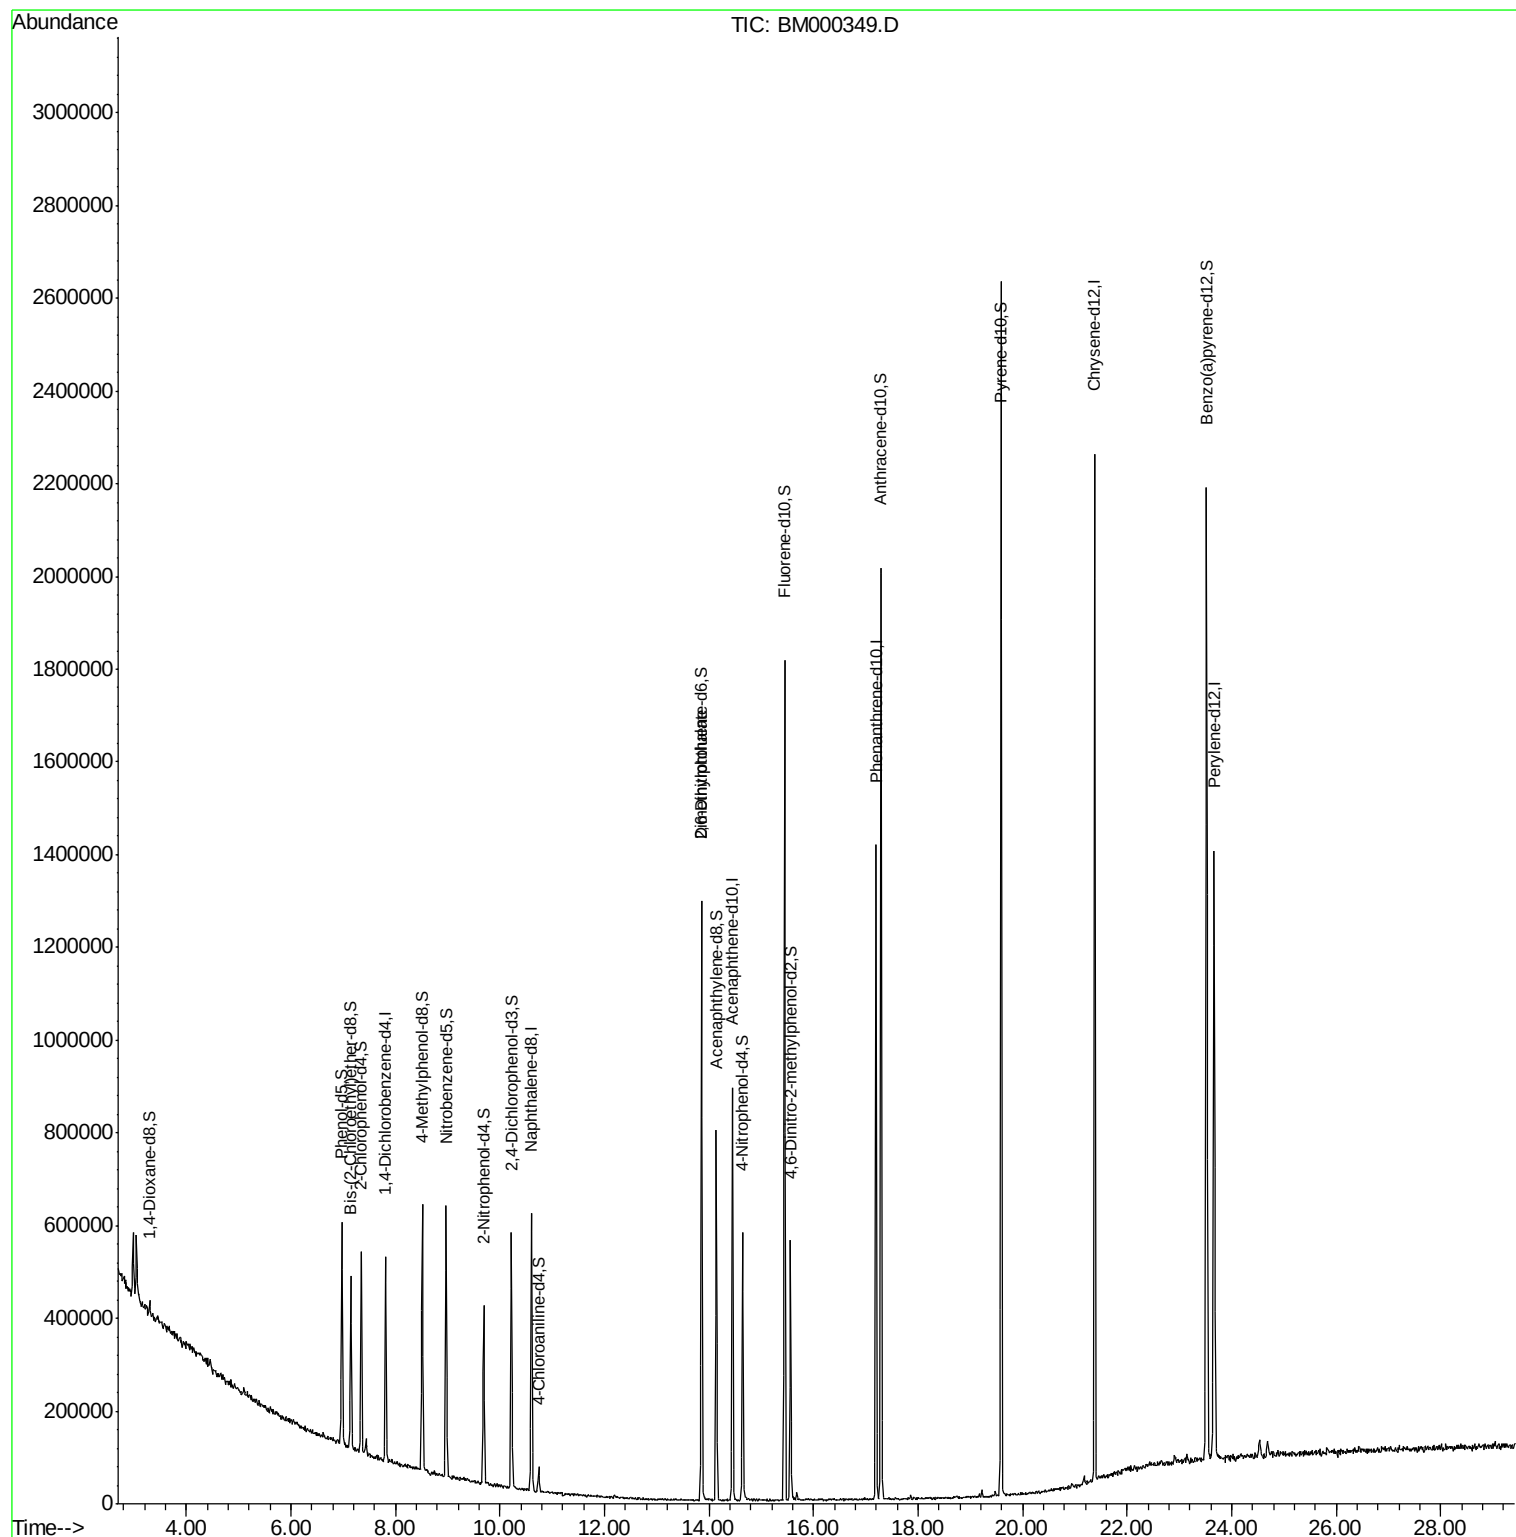

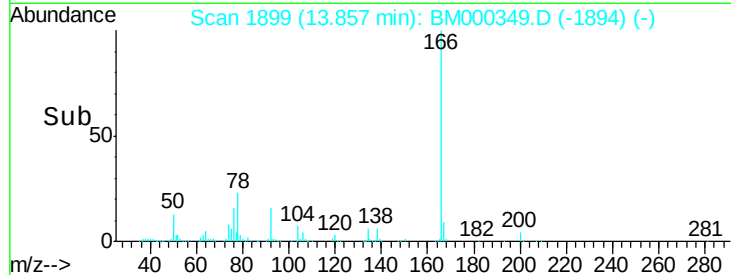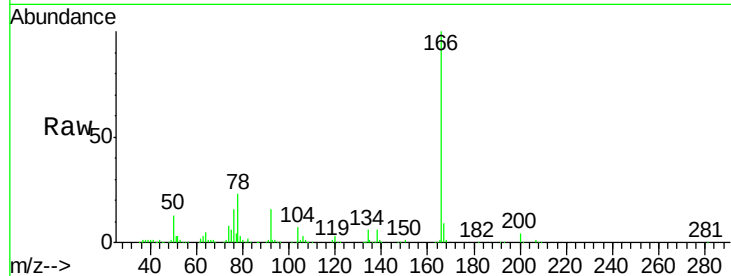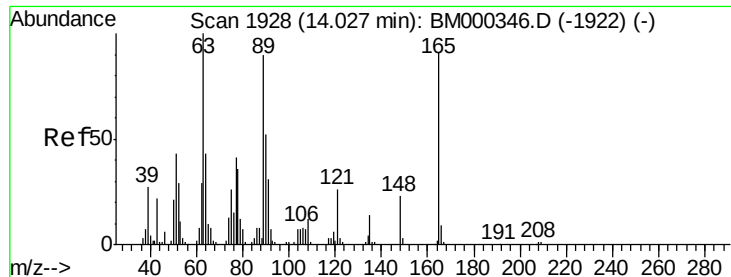

#45
 2,6-Dinitrotoluene
 Concen: 1.52 ng/ul
 RT: 13.86 min Scan# 1899
 Delta R.T. -0.17 min
 Lab File: BM000349.D
 Acq: 25 Jan 2015 01:06

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	69.5	104.3
121	48.6	22.3	33.5

