

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000351.D
 Acq On : 25 Jan 2015 02:17
 Operator : TP/IZ
 Sample : G1115-06DL 2X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 26 13:43:02 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 26 13:29:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	87220	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	350604	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	270871	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	646427	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	895700	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	944044	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	741112	372.66	ng/uL	-0.03
5) Phenol-d5	6.97	99	13087	1.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	45126	8.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	35809	6.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	23575	4.14	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	26764	10.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	23197	9.46	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.22	165	41754	7.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	1672	0.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	235442	12.11	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	284509	11.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	6510	2.02	ng/ul	-0.01
57) Fluorene-d10	15.44	176	243637	13.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	31405	9.21	ng/ul	-0.01
70) Anthracene-d10	17.29	188	445027	14.50	ng/ul	0.00
76) Pyrene-d10	19.59	212	546143	13.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	571221	13.30	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) 1,4-Dioxane	3.33	88	59677	22.16	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
Data File : BM000351.D
Acq On : 25 Jan 2015 02:17
Operator : TP/IZ
Sample : G1115-06DL 2X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 26 13:43:02 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 26 13:29:32 2015
Response via : Initial Calibration

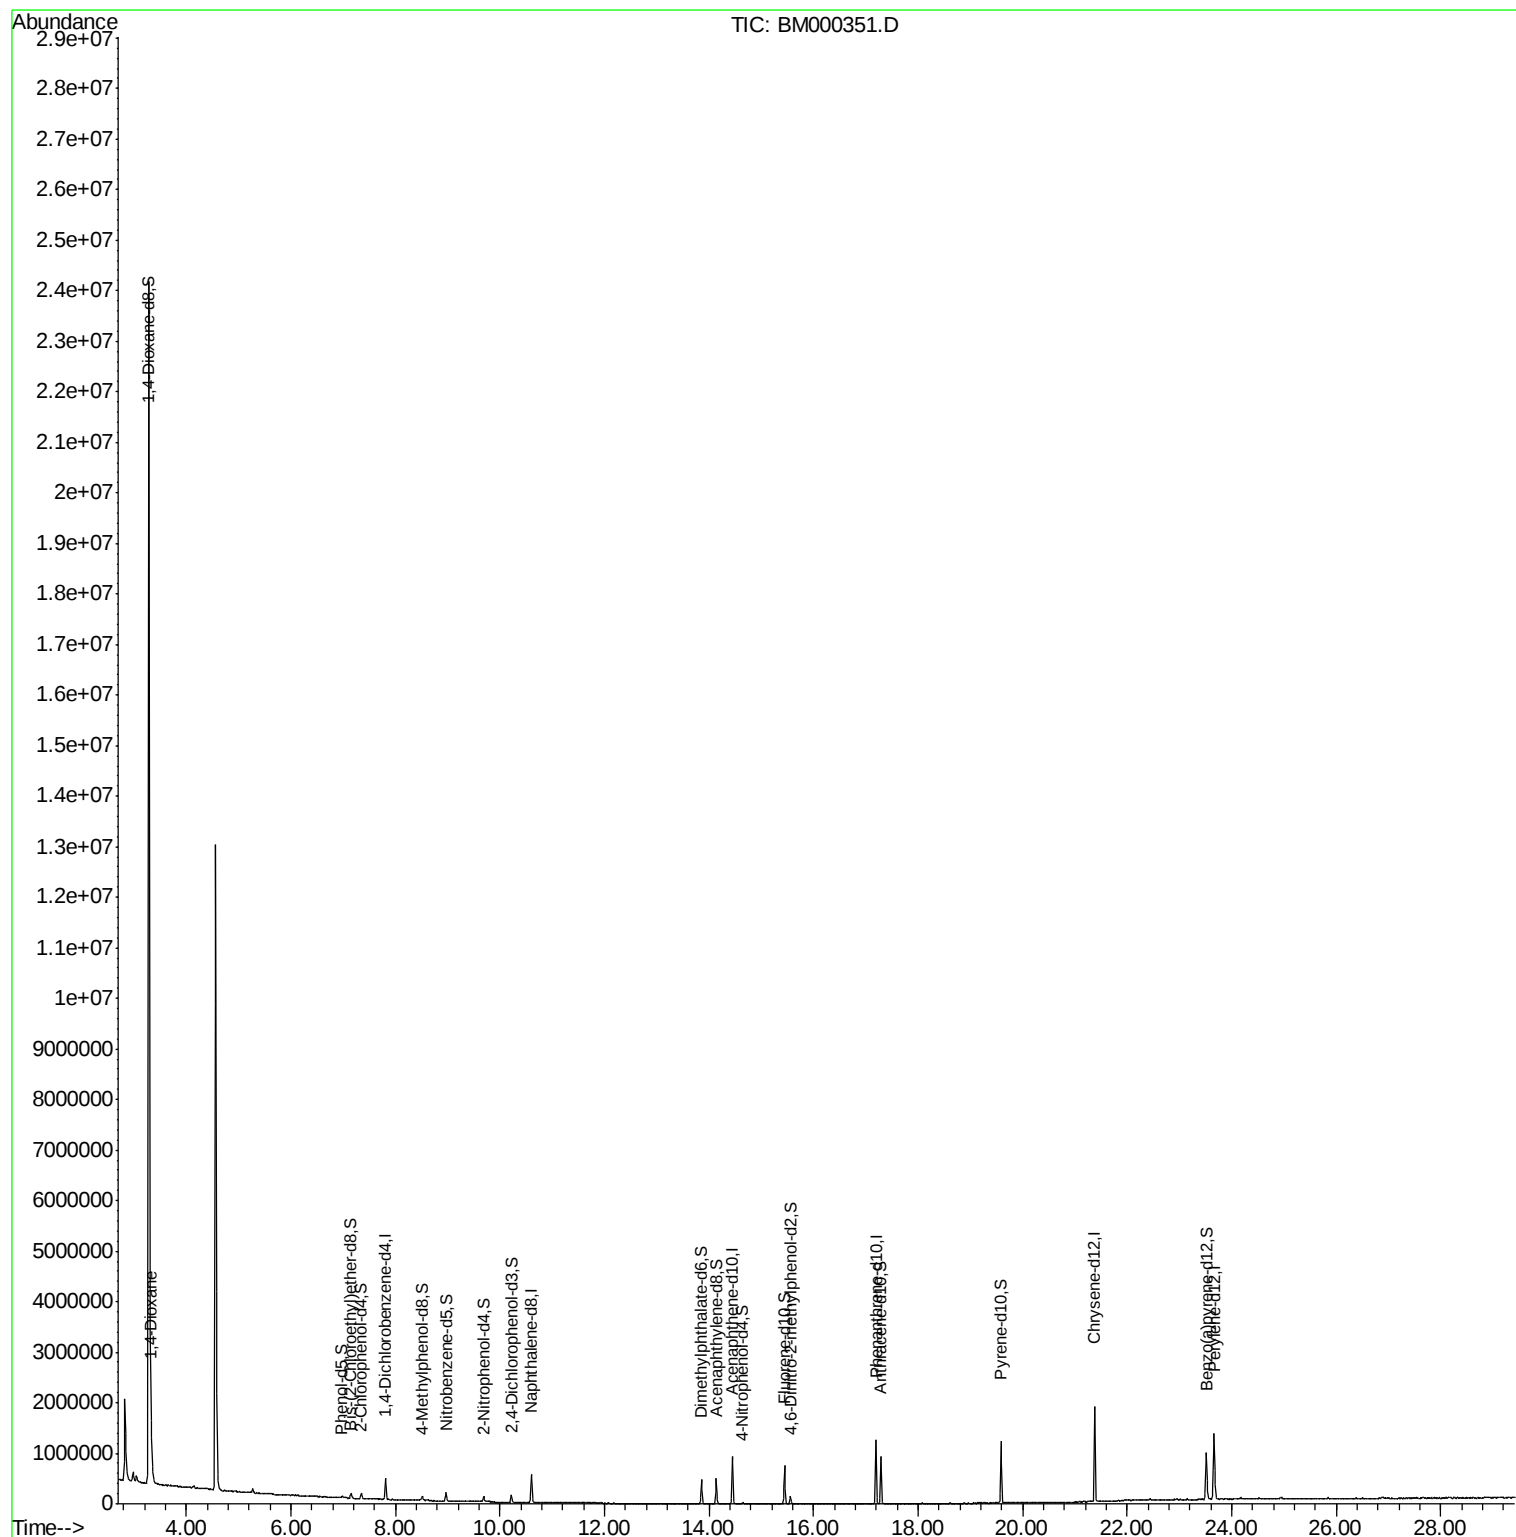

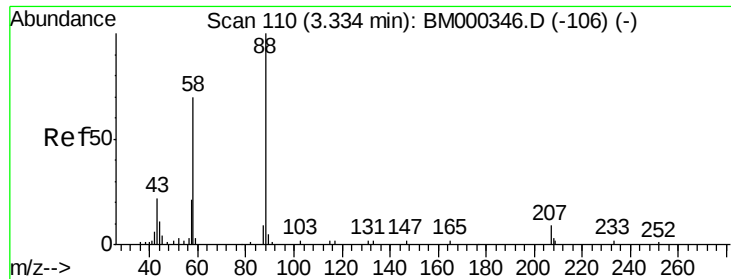

#2

1,4-Dioxane

Concen: 22.16 ng/uL

RT: 3.33 min Scan# 110

Delta R.T. -0.01 min

Lab File: BM000351.D

Acq: 25 Jan 2015 02:17

Instrument :

BNA_M

ClientSampleId :

Tot Ion: 88 Resp: 59677

Ion	Ratio	Lower	Upper
88	100		
43	26.4	22.4	33.6
58	66.8	57.4	86.2

