

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000320.D
 Acq On : 24 Jan 2015 06:47
 Operator : TP/IZ
 Sample : G1115-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COANO

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:17 PM

Quant Time: Jan 26 11:58:27 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

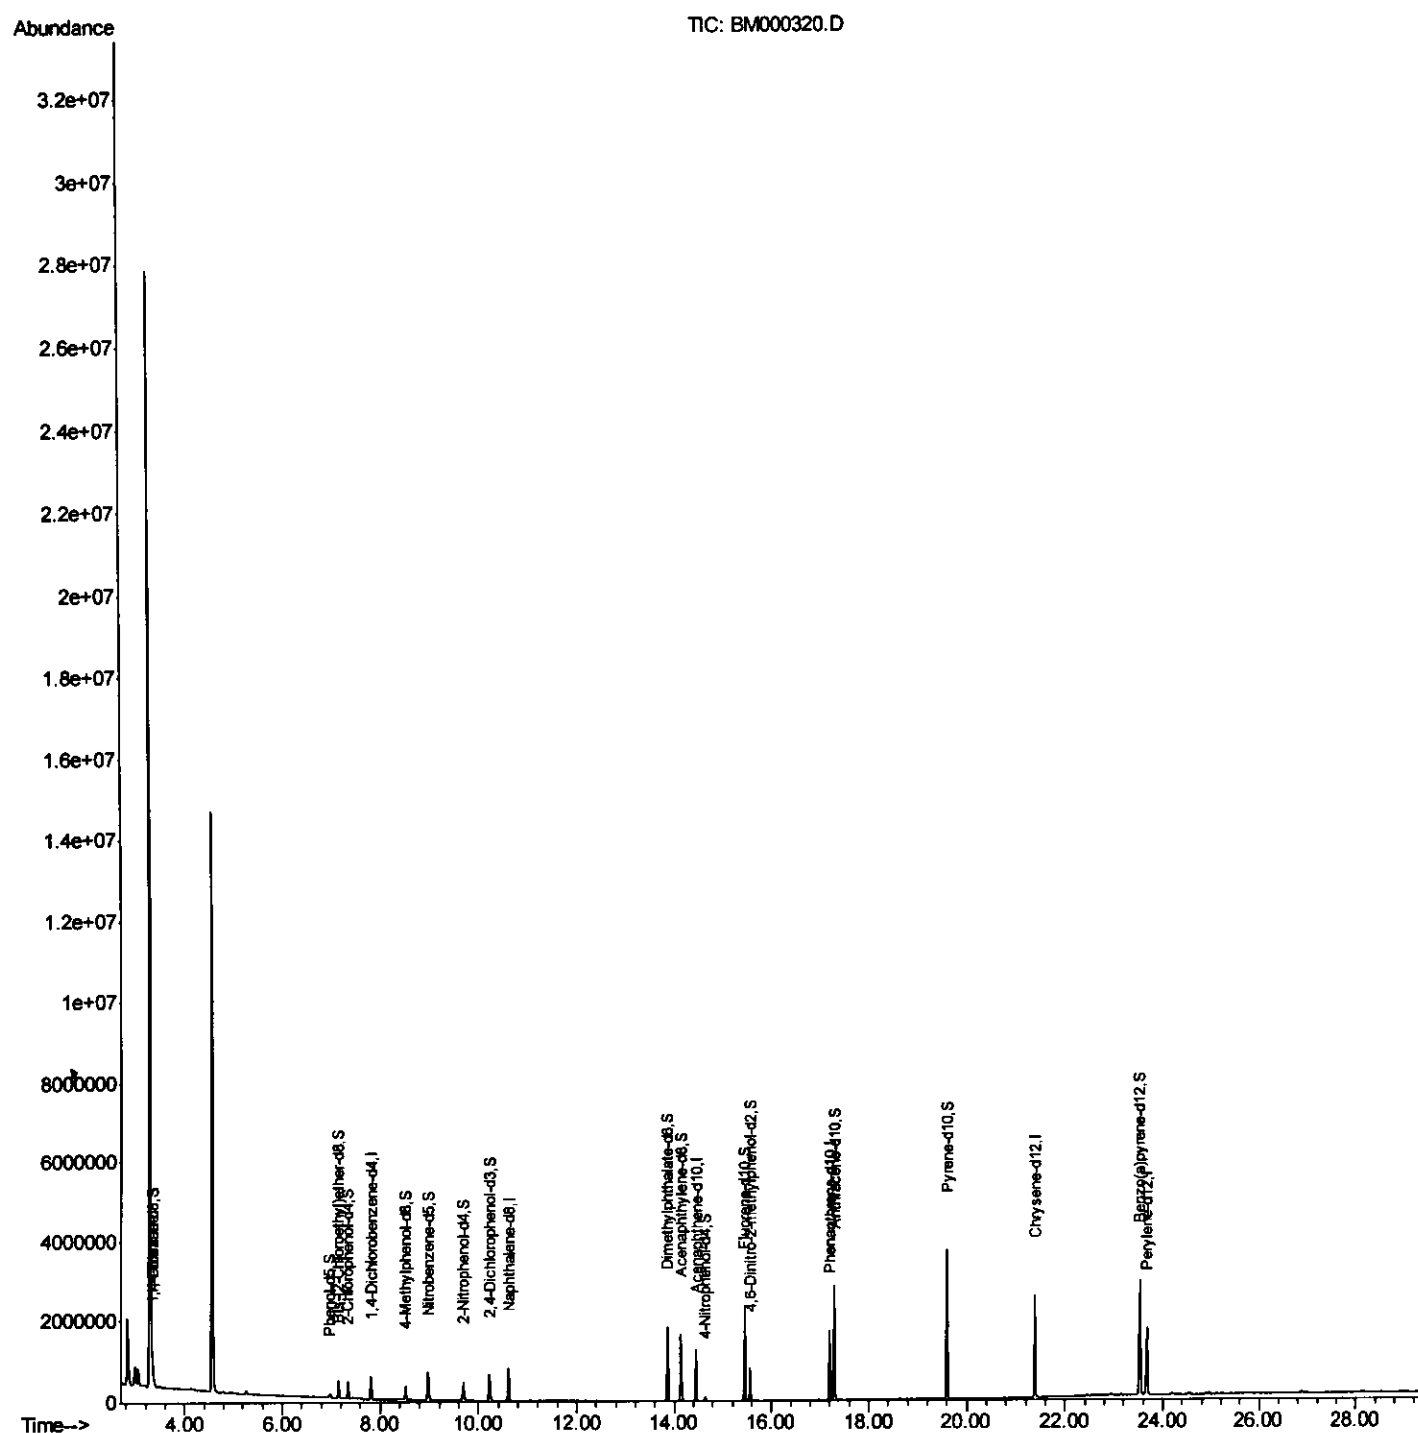

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000320.D
 Acq On : 24 Jan 2015 06:47
 Operator : TP/IZ
 Sample : G1115-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAN0

Quant Time: Jan 26 11:48:15 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:17 PM

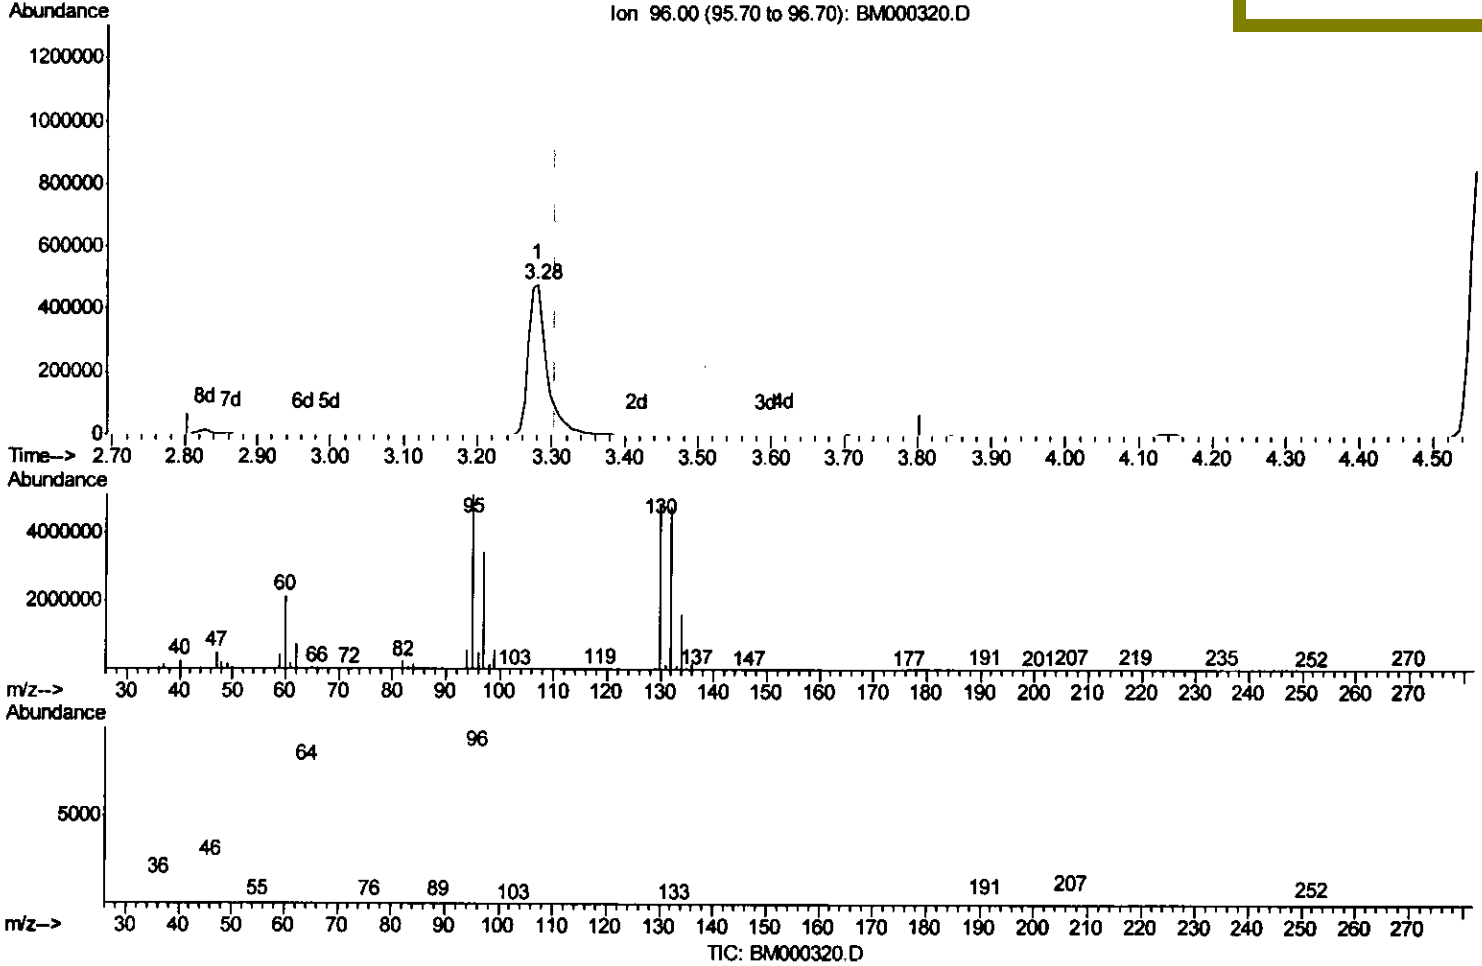

(3) 1,4-Dioxane-d8 (S)

3.281min (-0.024) 305.93ng/uL

response 830364

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	0.06#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000320.D
 Acq On : 24 Jan 2015 06:47
 Operator : TP/IZ
 Sample : G1115-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COANO

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:17 PM

Quant Time: Jan 26 11:48:15 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

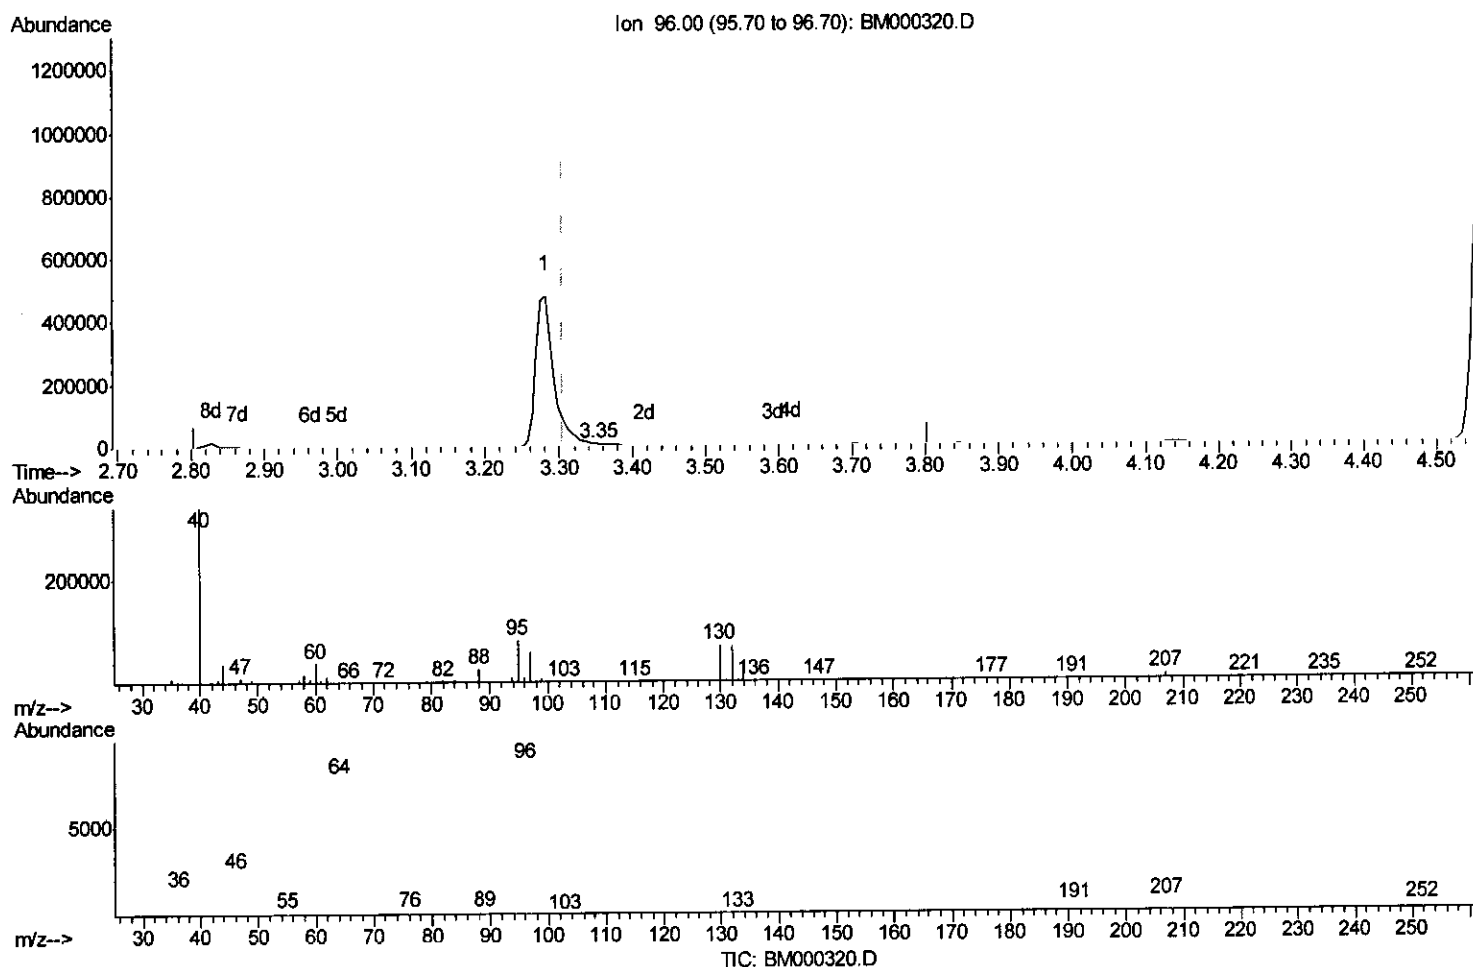

(3) 1,4-Dioxane-d8 (S)

3.346min (+0.041) 3.54ng/uL m

response 9618

Ion Exp% Act%

96.00	100	100
64.00	74.90	5.42#
34.00	0.00	0.00
0.00	0.00	0.00

T.P
 1/30/15

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000320.D
 Acq On : 24 Jan 2015 06:47
 Operator : TP/IZ
 Sample : G1115-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 COANO

Quant Time: Jan 26 11:58:27 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:17 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	119040	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	502840	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	379092	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	875238	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1154261	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1194867	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.35	96	9618m	3.54	ng/uL	0.04
5) Phenol-d5	6.97	99	48403	4.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	172281	24.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	135302	18.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	90886	11.69	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	101583	26.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	91650	26.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	173541	22.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	3700	0.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	908174	33.36	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	1027149	30.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	19584	4.35	ng/ul	0.00
57) Fluorene-d10	15.44	176	813668	33.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	119956	25.98	ng/ul	0.00
70) Anthracene-d10	17.29	188	1401243	33.72	ng/ul	0.00
76) Pyrene-d10	19.59	212	1731669	33.80	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1841687	33.89	ng/ul	0.00

Target Compounds					Ovalue
2) 1,4-Dioxane	3.34	88	54496	14.83	ng/uL 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

T.P.
 1/30/15