

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000322.D
 Acq On : 24 Jan 2015 07:58
 Operator : TP/IZ
 Sample : G1115-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW1

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:25 PM

Quant Time: Jan 26 12:06:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

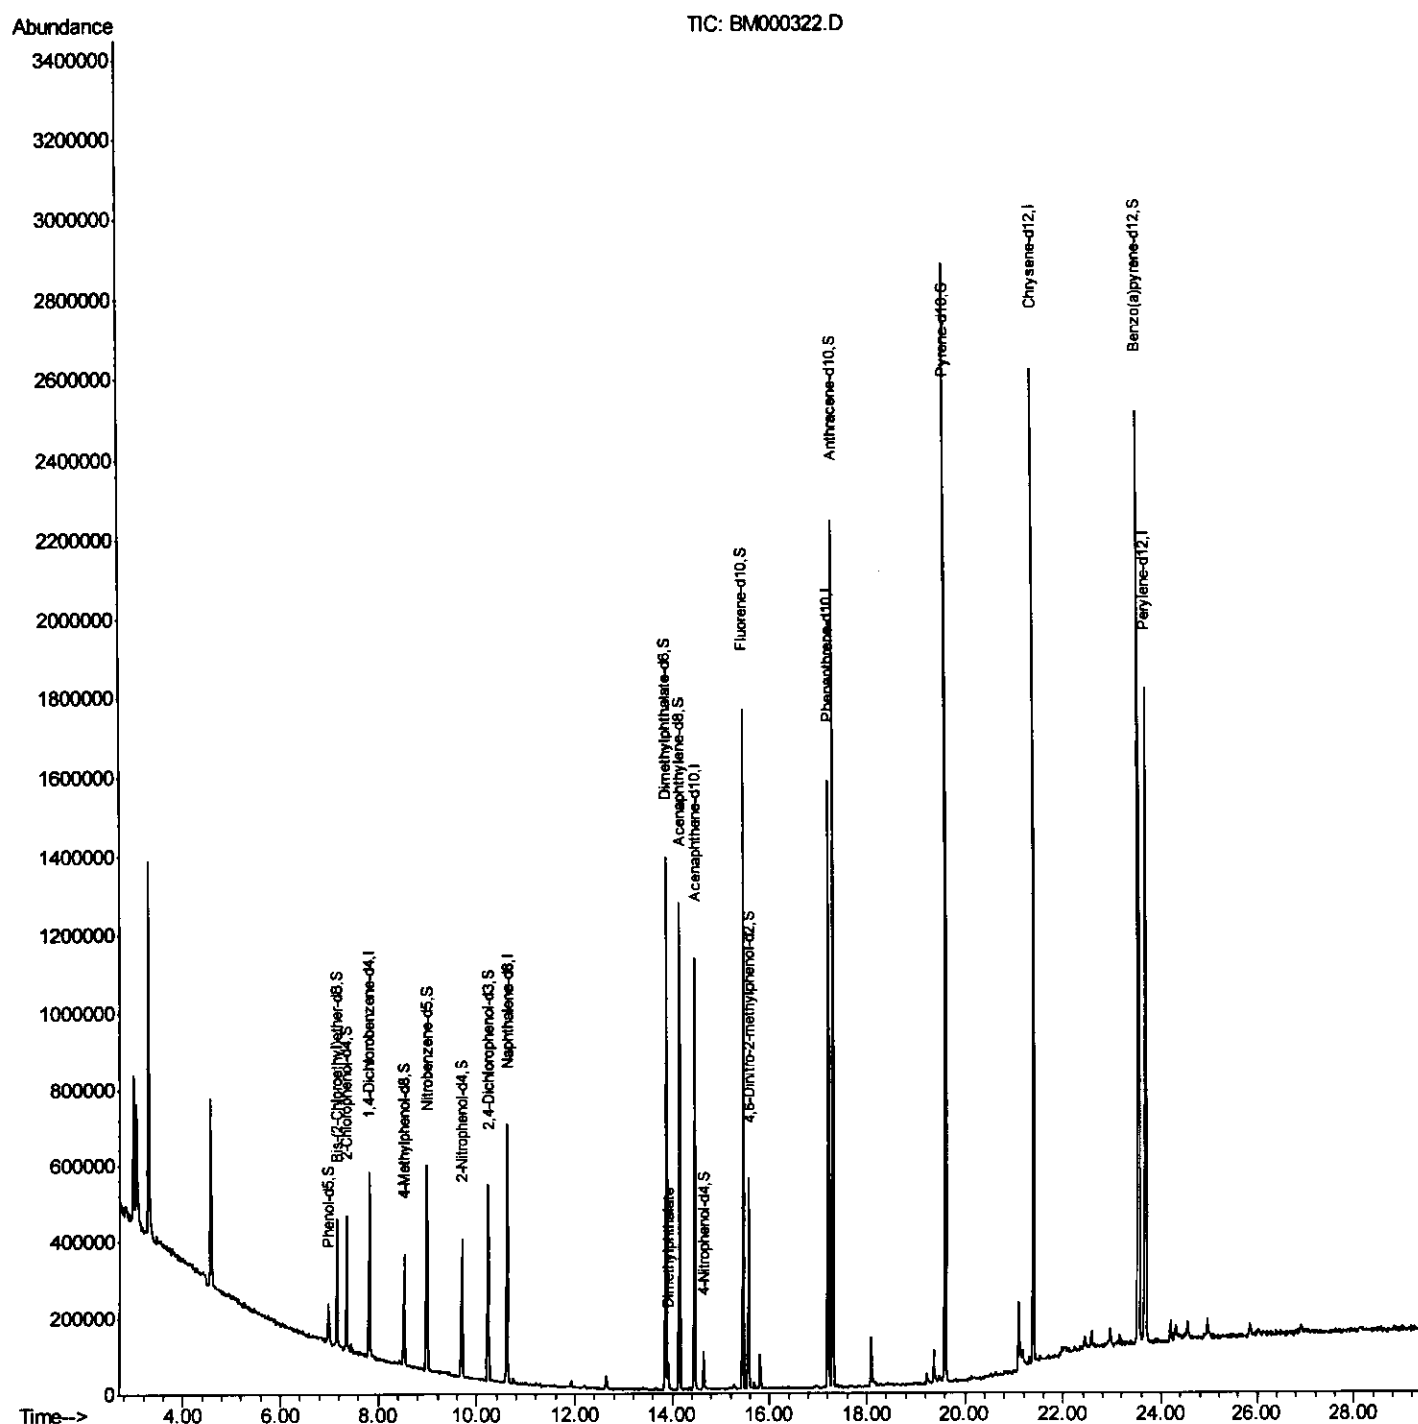

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000322.D
 Acq On : 24 Jan 2015 07:58
 Operator : TP/IZ
 Sample : G1115-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW1

Quant Time: Jan 26 11:48:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:25 PM

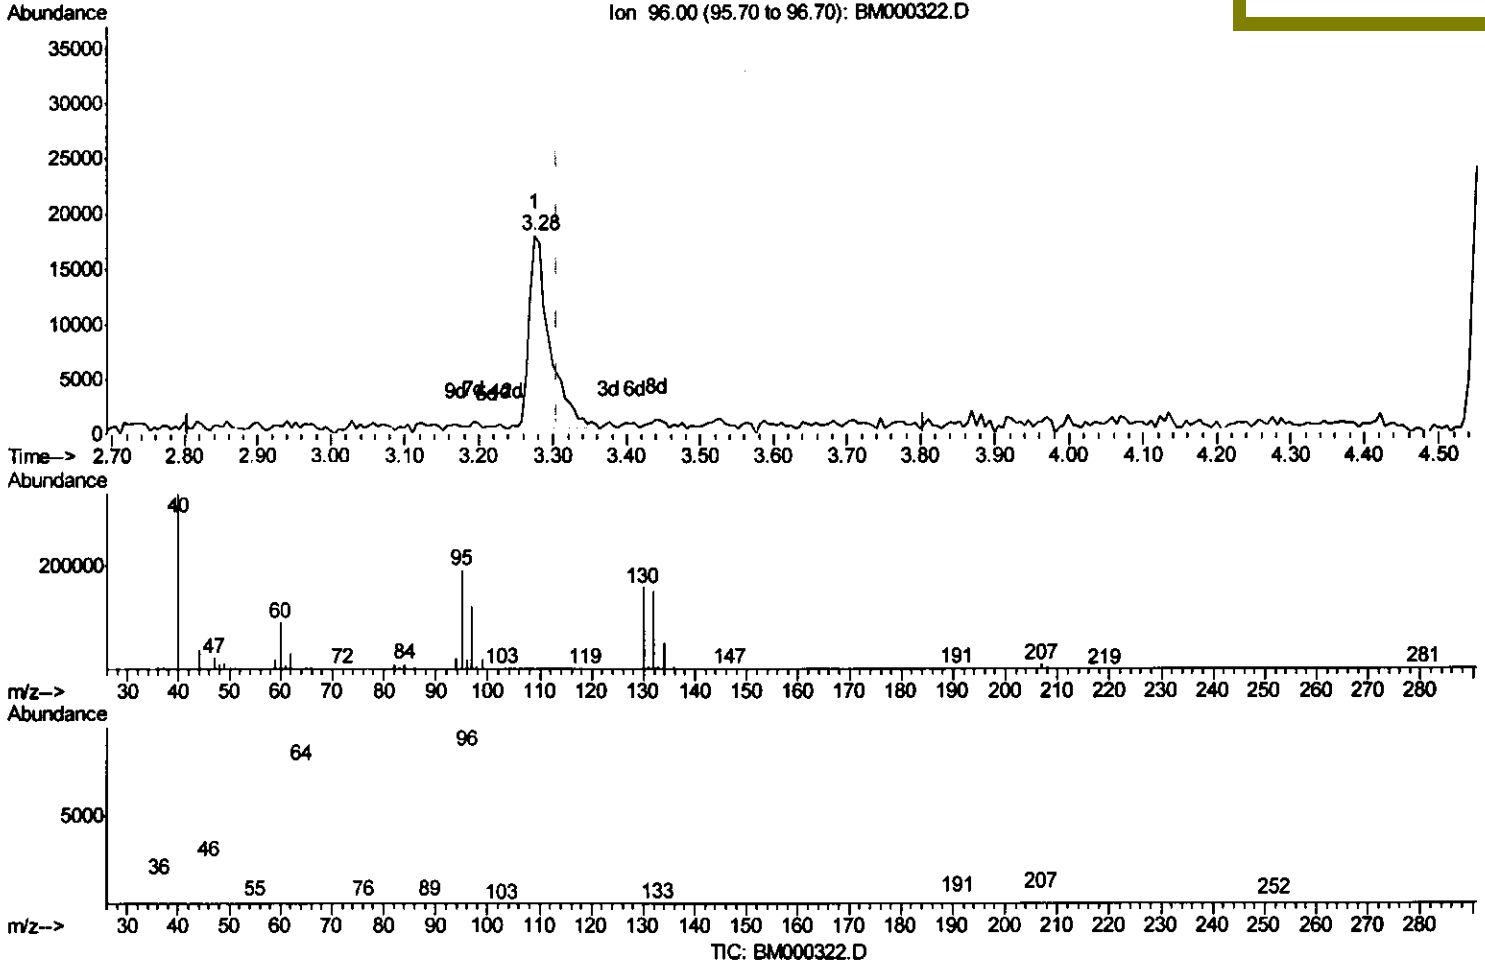

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.029) 13.77ng/uL

response 33386

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000322.D
 Acq On : 24 Jan 2015 07:58
 Operator : TP/IZ
 Sample : G1115-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW1

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:25 PM

Quant Time: Jan 26 11:48:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

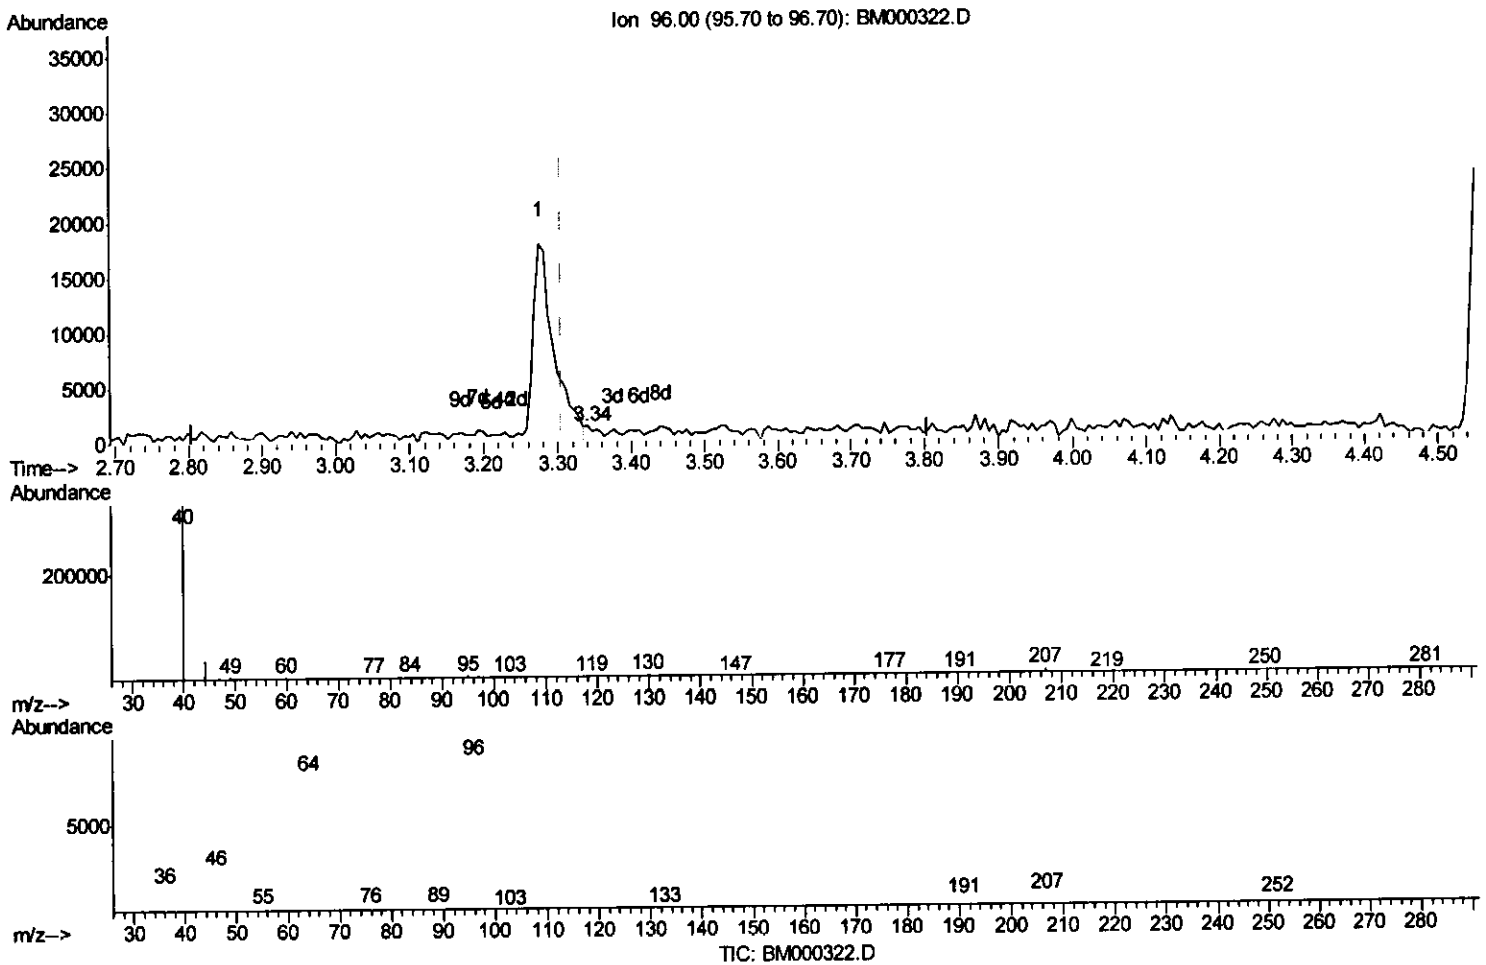

(3) 1,4-Dioxane-d8 (S)

3.340min (+0.035) 0.68ng/uL m

response 1638

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

T.P
 1/30/15

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000322.D
 Acq On : 24 Jan 2015 07:58
 Operator : TP/IZ
 Sample : G1115-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW1

Quant Time: Jan 26 12:06:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:52:25 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	106358	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	444672	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	337417	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	799060	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1130481	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1197534	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.34	96	1638m	0.68	ng/uL	0.04
5) Phenol-d5	6.97	99	44924	4.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	140959	22.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	117562	18.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	81944	11.80	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	81805	24.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	74575	23.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	144474	21.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	5136	0.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	671704	27.72	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	774360	26.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	18159	4.53	ng/ul	0.00
57) Fluorene-d10	15.44	176	627812	28.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	83678	19.85	ng/ul	0.00
70) Anthracene-d10	17.29	188	1095352	28.87	ng/ul	0.00
76) Pyrene-d10	19.59	212	1392077	27.75	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1578853	28.99	ng/ul	0.00

T.P.
 1/30/15

Target Compounds					Ovalue
44) Dimethylphthalate	13.90	163	29856	1.20	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed