

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000315.D
 Acq On : 24 Jan 2015 03:15
 Operator : TP/IZ
 Sample : G1115-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:51:45 PM

Quant Time: Jan 26 11:34:11 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 24 04:15:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	127175	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	550738	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	423465	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	958875	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1302707	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	1347895	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	2905m	1.00	ng/uL	0.02
5) Phenol-d5	6.97	99	72561	6.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	220525	29.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	182519	23.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	130984	15.77	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	126087	30.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	121129	31.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	220277	26.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	10589	1.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	1002030	32.96	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	1184548	31.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	26066	5.18	ng/ul	0.00
57) Fluorene-d10	15.44	176	897144	32.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	118235	23.38	ng/ul	0.00
70) Anthracene-d10	17.29	188	1486341	32.64	ng/ul	0.00
76) Pyrene-d10	19.59	212	1813559	31.37	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1973991	32.20	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	90214	2.89	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
Data File : BM000315.D
Acq On : 24 Jan 2015 03:15
Operator : TP/IZ
Sample : G1115-03
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

apatel
1/26/2015 4:51:45 PM

Quant Time: Jan 26 11:34:11 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 24 04:15:00 2015
Response via : Initial Calibration

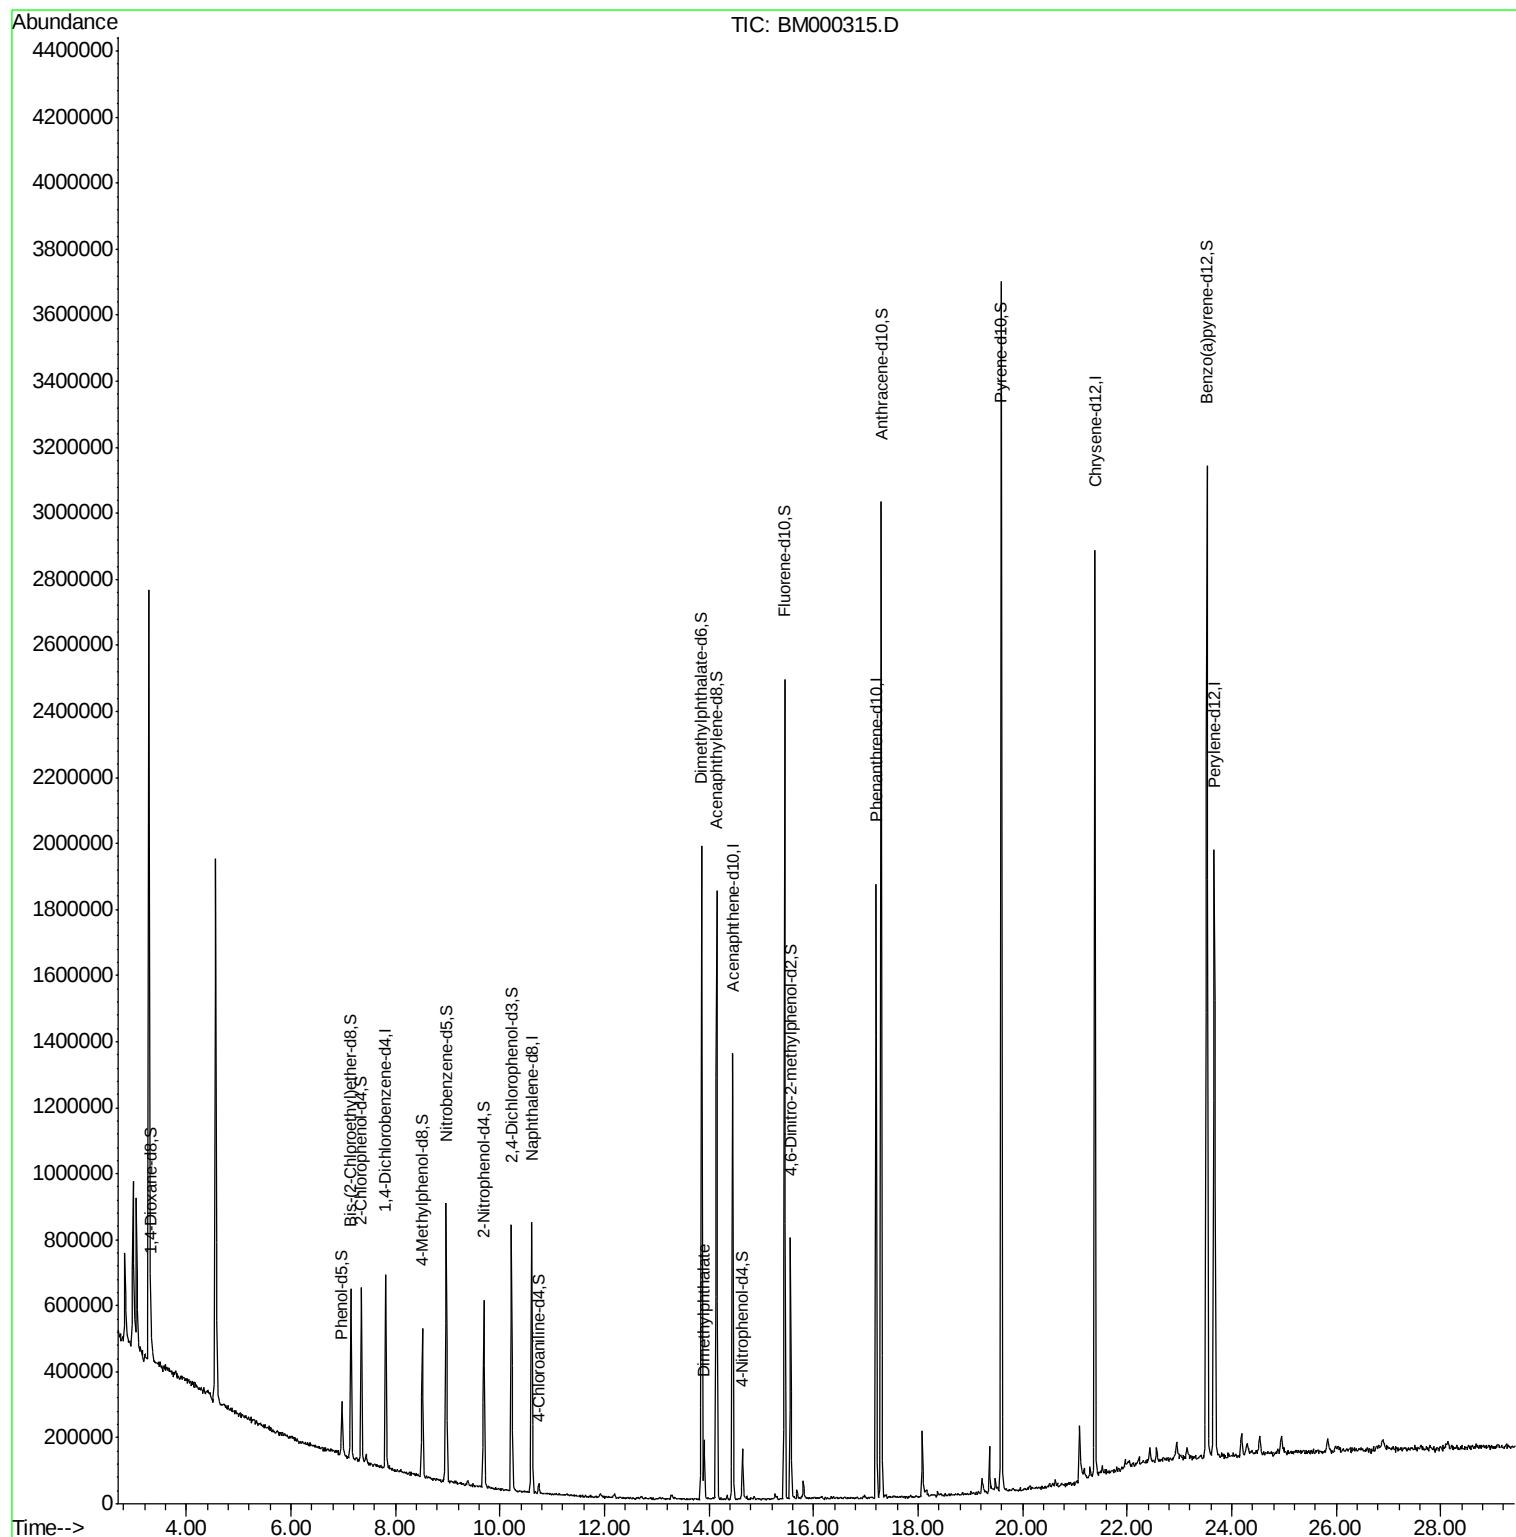

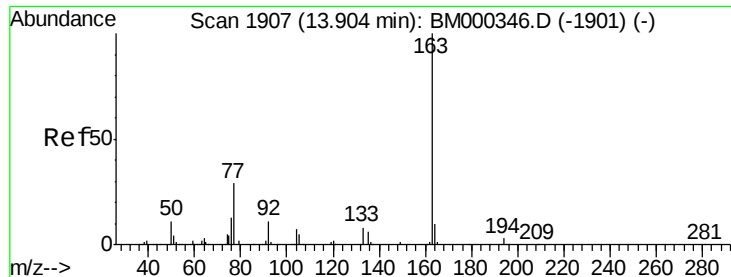

#44
 Dimethylphthalate
 Concen: 2.89 ng/ul
 RT: 13.90 min Scan# 1907
 Delta R.T. 0.00 min
 Lab File: BM000315.D
 Acq: 24 Jan 2015 03:15

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.4	3.1	4.7
164	9.2	8.1	12.1

Manual Integrations
 APPROVED

apatel
 1/26/2015 4:51:45 PM

