

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
 Data File : BM000337.D
 Acq On : 24 Jan 2015 17:25
 Operator : TP/IZ
 Sample : G1134-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW8

Quant Time: Jan 26 12:54:48 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 26 12:45:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	105634	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	477403	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	364983	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	876572	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	1226681	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	1278590	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	4362	1.81	ng/uL	0.00
5) Phenol-d5	6.97	99	49638	5.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	156301	25.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	131443	20.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	96373	13.97	ng/ul	-0.01
19) Nitrobenzene-d5	8.97	128	95557	26.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	88069	26.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	173558	23.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	10409	1.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	812734	31.01	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	957985	29.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	21264	4.90	ng/ul	0.00
57) Fluorene-d10	15.44	176	743757	31.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	102884	22.25	ng/ul	0.00
70) Anthracene-d10	17.29	188	1281630	30.79	ng/ul	0.00
76) Pyrene-d10	19.59	212	1616613	29.69	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1585332	27.26	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	37023	1.38	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012315\
Data File : BM000337.D
Acq On : 24 Jan 2015 17:25
Operator : TP/IZ
Sample : G1134-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AW8

Quant Time: Jan 26 12:54:48 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 26 12:45:18 2015
Response via : Initial Calibration

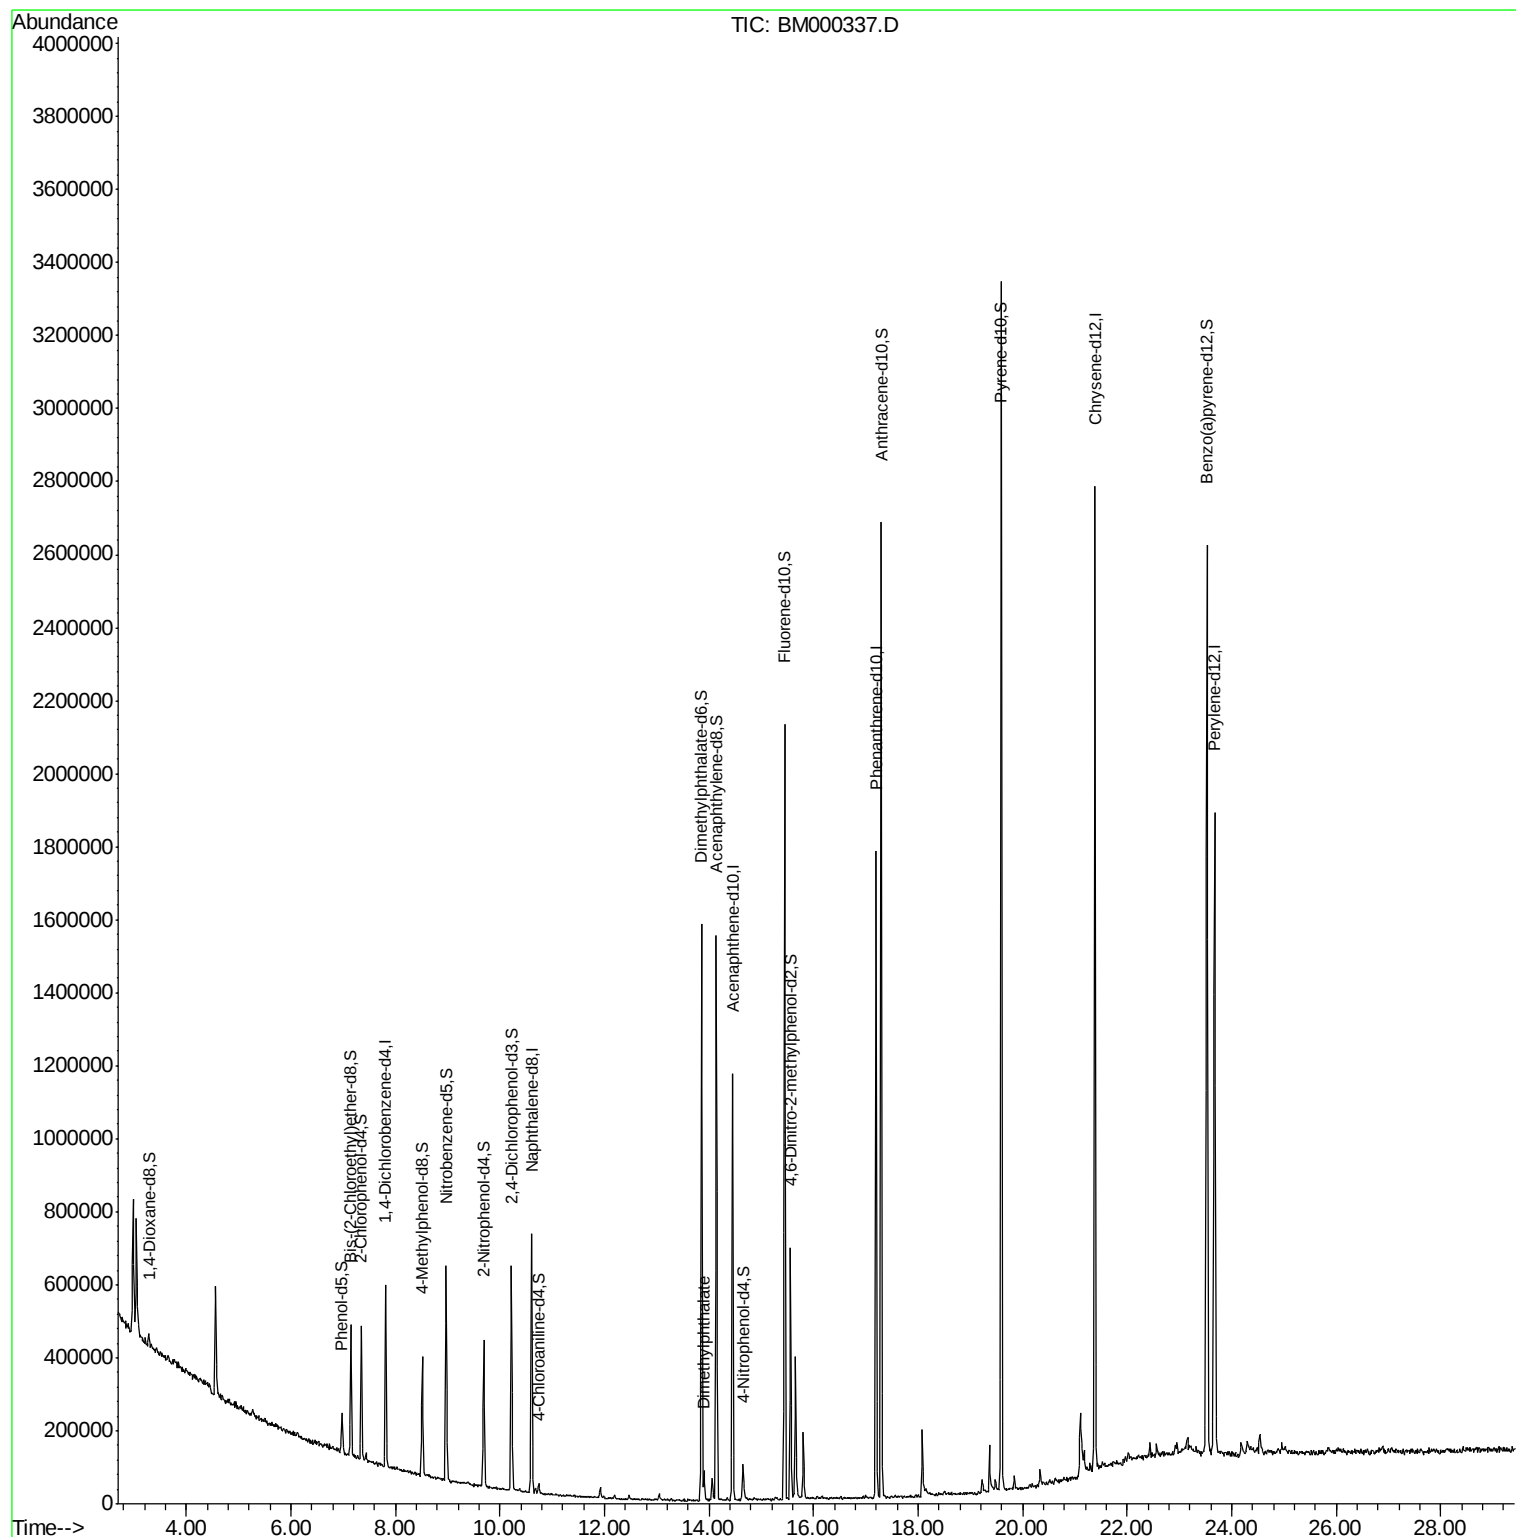

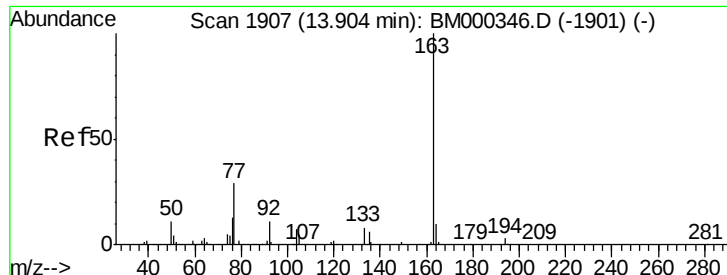

#44

Dimethylphthalate

Concen: 1.38 ng/ul

RT: 13.90 min Scan# 1907

Delta R.T. 0.00 min

Lab File: BM000337.D

Acq: 24 Jan 2015 17:25

Instrument :

BNA_M

ClientSampleId :

C0AW8


Tot Ion:163 Resp: 37023

Ion Ratio Lower Upper

163 100

194 2.4 3.1 4.7#

164 11.5 8.1 12.1

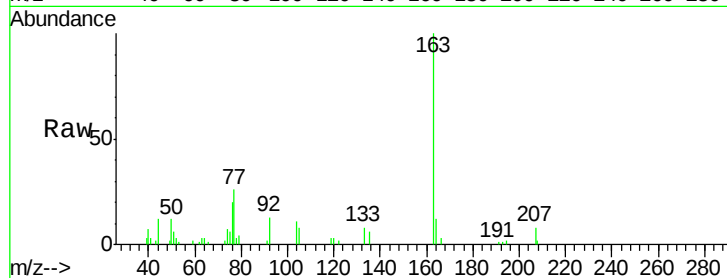

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

