

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
 Data File : BM000352.D
 Acq On : 25 Jan 2015 02:52
 Operator : TP/IZ
 Sample : G1115-12DL 2X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AS2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.822	19	23	38	rVB	805415	1355112	5.05%	2.459%
2	2.975	46	49	57	rVV	179137	274007	1.02%	0.497%
3	3.046	59	61	72	rVB2	164322	264288	0.98%	0.480%
4	3.275	95	100	125	rVB	16026656	26856313	100.00%	48.736%
5	4.557	312	318	332	rVB	5410173	8580407	31.95%	15.571%
6	5.263	436	438	446	rVB2	63559	97115	0.36%	0.176%
7	7.146	753	758	764	rVB	121818	198853	0.74%	0.361%
8	7.340	787	791	799	rVB2	111771	191601	0.71%	0.348%
9	7.810	865	871	879	rVB	378821	600514	2.24%	1.090%
10	8.504	985	989	994	rVB2	90338	136659	0.51%	0.248%
11	8.963	1062	1067	1075	rVB	195208	317207	1.18%	0.576%
12	9.681	1184	1189	1197	rVB2	114599	190154	0.71%	0.345%
13	10.216	1275	1280	1288	rVB2	157550	253995	0.95%	0.461%
14	10.598	1339	1345	1351	rVB	482232	799062	2.98%	1.450%
15	13.851	1893	1898	1903	rBV	501394	656235	2.44%	1.191%
16	13.898	1903	1906	1912	rVB3	19033	27052	0.10%	0.049%
17	14.139	1938	1947	1954	rVB	514427	714696	2.66%	1.297%
18	14.445	1993	1999	2007	rVB	831998	1184855	4.41%	2.150%
19	14.633	2025	2031	2038	rBV5	28456	48179	0.18%	0.087%
20	15.439	2161	2168	2175	rVB	741955	1014321	3.78%	1.841%
21	15.551	2181	2187	2194	rBV2	148335	210696	0.78%	0.382%
22	15.804	2225	2230	2236	rBV3	33451	48118	0.18%	0.087%
23	17.192	2459	2466	2472	rBV	1140138	1629788	6.07%	2.958%
24	17.286	2476	2482	2491	rBV	947908	1284522	4.78%	2.331%
25	18.074	2611	2616	2623	rBV7	22337	34436	0.13%	0.062%
26	19.586	2867	2873	2881	rBV	1196295	1568908	5.84%	2.847%
27	21.286	3159	3162	3167	rBV6	23937	30357	0.11%	0.055%
28	21.374	3172	3177	3183	rBV	1879566	2357041	8.78%	4.277%
29	23.515	3533	3541	3548	rBV2	955190	1775859	6.61%	3.223%
30	23.662	3558	3566	3576	rVB	1272115	2405238	8.96%	4.365%


Sum of corrected areas: 55105588

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
Data File : BM000352.D
Acq On : 25 Jan 2015 02:52
Operator : TP/IZ
Sample : G1115-12DL 2X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AS2DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

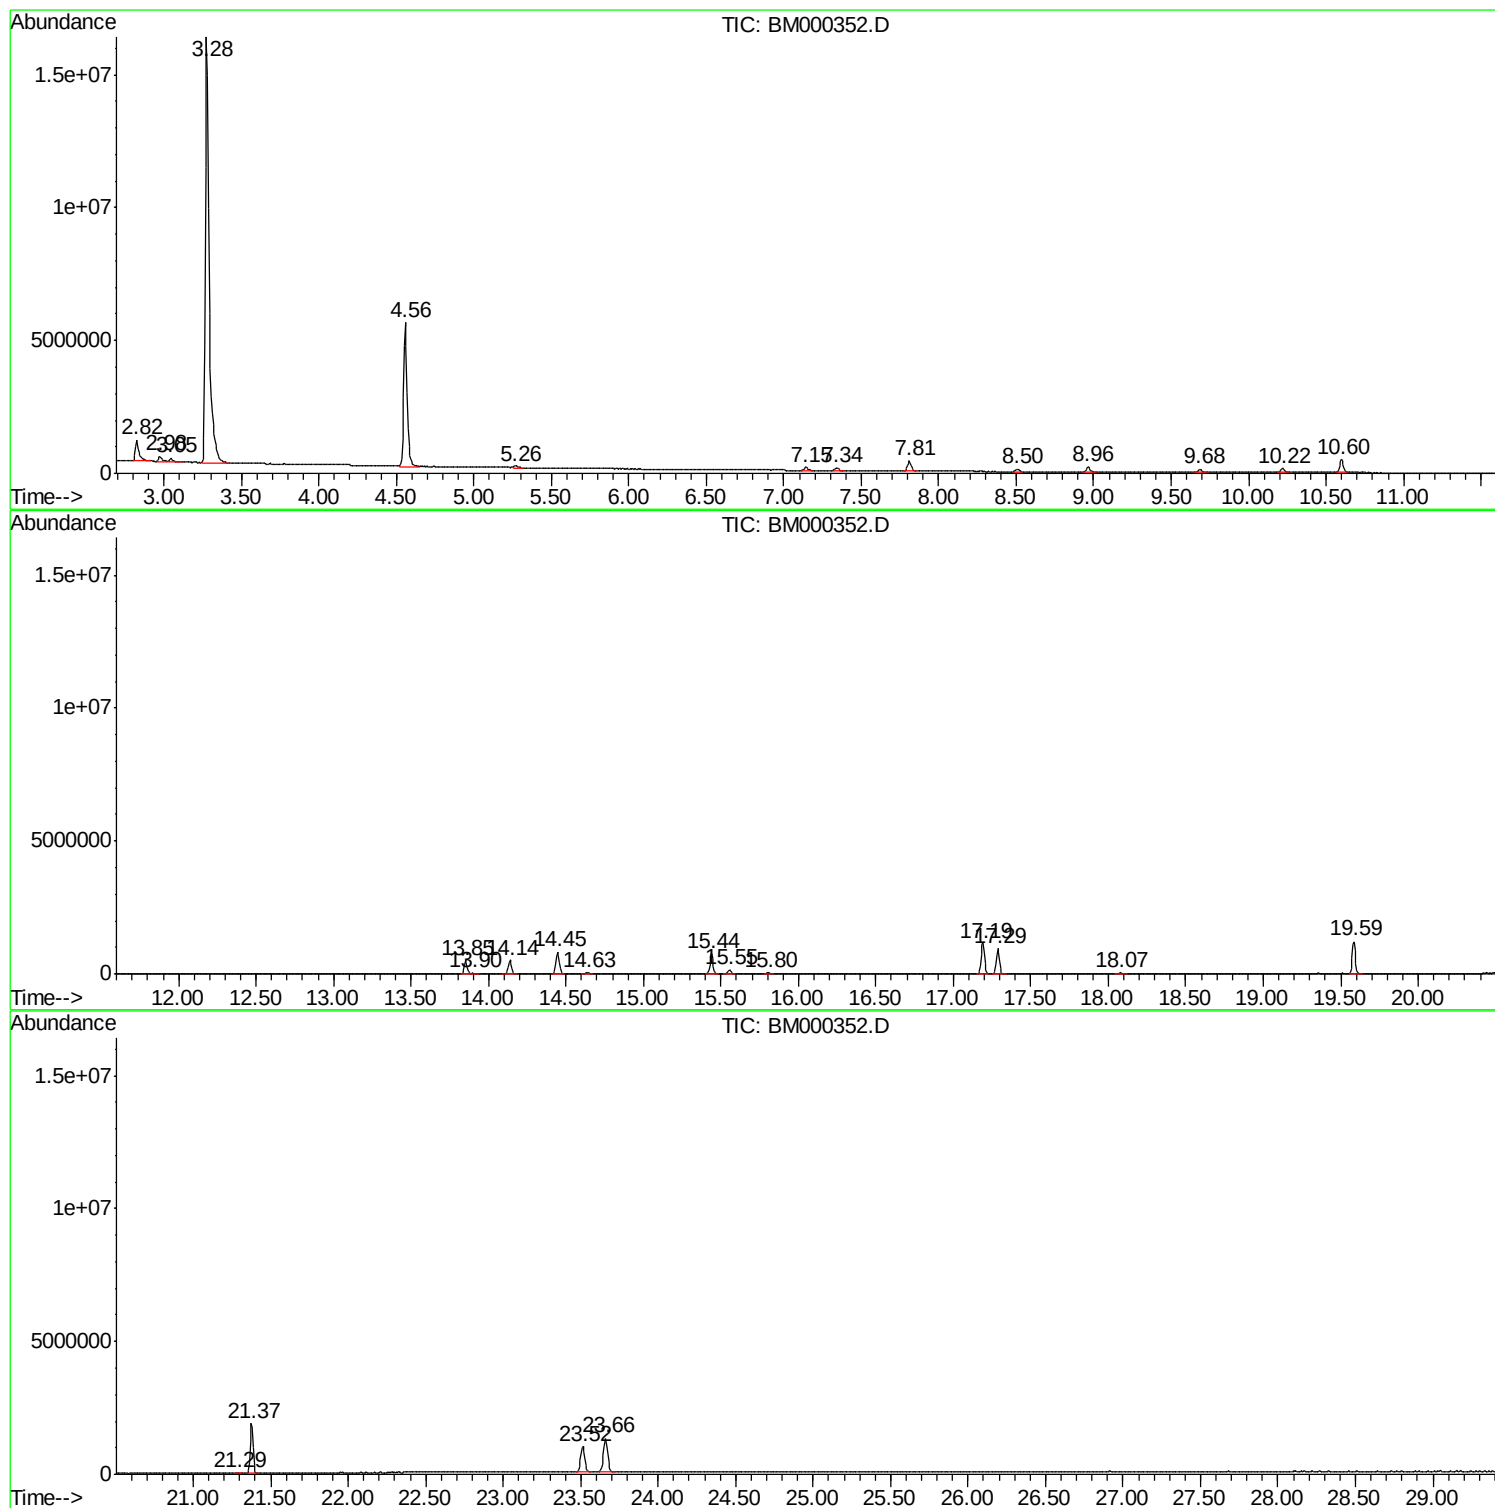

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
Data File : BM000352.D
Acq On : 25 Jan 2015 02:52
Operator : TP/IZ
Sample : G1115-12DL 2X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AS2DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
Data File : BM000352.D
Acq On : 25 Jan 2015 02:52
Operator : TP/IZ
Sample : G1115-12DL 2X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AS2DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc