

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
 Data File : BM000354.D
 Acq On : 25 Jan 2015 04:03
 Operator : TP/IZ
 Sample : G1115-02DL 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	98	100	107	rVB3	107570	140172	7.58%	1.843%
2	4.558	315	318	324	rVB2	105398	158008	8.55%	2.077%
3	7.810	865	871	880	rVB	292294	475211	25.71%	6.247%
4	9.216	1109	1110	1113	rBV	9030	7796	0.42%	0.102%
5	9.681	1187	1189	1191	rBV	5736	4669	0.25%	0.061%
6	10.334	1298	1300	1303	rVB2	6218	4594	0.25%	0.060%
7	10.598	1339	1345	1351	rBV	374626	609967	33.00%	8.018%
8	10.669	1355	1357	1358	rBV2	3475	2898	0.16%	0.038%
9	10.828	1383	1384	1387	rVB2	4435	2969	0.16%	0.039%
10	11.098	1428	1430	1434	rBV3	4399	5088	0.28%	0.067%
11	11.375	1475	1477	1480	rBV2	2669	3044	0.16%	0.040%
12	11.504	1497	1499	1503	rBV2	2008	2460	0.13%	0.032%
13	11.663	1524	1526	1528	rVV2	2954	3043	0.16%	0.040%
14	11.698	1530	1532	1534	rVV	3414	3287	0.18%	0.043%
15	11.739	1538	1539	1543	rVB2	3301	3251	0.18%	0.043%
16	11.781	1543	1546	1547	rBV2	3539	2482	0.13%	0.033%
17	12.016	1583	1586	1591	rBV3	2088	2765	0.15%	0.036%
18	12.157	1608	1610	1614	rBV2	4054	4190	0.23%	0.055%
19	12.381	1646	1648	1651	rVV2	2864	2985	0.16%	0.039%
20	12.757	1711	1712	1716	rVB2	3137	3356	0.18%	0.044%
21	12.992	1748	1752	1753	rVB2	3776	4060	0.22%	0.053%
22	13.010	1753	1755	1757	rBV	3310	3167	0.17%	0.042%
23	13.286	1800	1802	1804	rBV2	3074	2607	0.14%	0.034%
24	13.304	1804	1805	1809	rVV2	2738	2670	0.14%	0.035%
25	13.357	1811	1814	1817	rVB3	2473	3209	0.17%	0.042%
26	13.380	1817	1818	1821	rBV2	3619	2777	0.15%	0.037%
27	13.680	1866	1869	1873	rBV2	2244	2822	0.15%	0.037%
28	13.851	1894	1898	1902	rBV3	4123	5711	0.31%	0.075%
29	13.904	1905	1907	1909	rBV2	3047	2497	0.14%	0.033%
30	14.051	1926	1932	1938	rVB4	4007	8404	0.45%	0.110%
31	14.127	1944	1945	1946	rBV	3550	2432	0.13%	0.032%
32	14.145	1946	1948	1950	rVB2	3587	2586	0.14%	0.034%
33	14.245	1960	1965	1968	rBV4	2849	5180	0.28%	0.068%
34	14.445	1992	1999	2005	rBV	645799	884882	47.87%	11.632%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
 Data File : BM000354.D
 Acq On : 25 Jan 2015 04:03
 Operator : TP/IZ
 Sample : G1115-02DL 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
 Title : SVOA CALIBRATION

35	14.486	2005	2006	2011	rVB3	3316	4477	0.24%	0.059%
36	14.533	2011	2014	2015	rBV3	2875	2724	0.15%	0.036%
37	15.139	2114	2117	2121	rBV	3630	2530	0.14%	0.033%
38	15.439	2163	2168	2171	rVB5	10475	12113	0.66%	0.159%
39	15.574	2188	2191	2194	rVB2	2603	2670	0.14%	0.035%
40	15.663	2203	2206	2210	rVV2	2026	3018	0.16%	0.040%
41	15.827	2231	2234	2237	rBV2	2560	3147	0.17%	0.041%
42	15.910	2245	2248	2255	rBV3	2520	4990	0.27%	0.066%
43	16.133	2283	2286	2288	rVB3	2815	2958	0.16%	0.039%
44	16.392	2326	2330	2333	rVB2	1889	2971	0.16%	0.039%
45	16.574	2358	2361	2364	rBV3	2665	3817	0.21%	0.050%
46	16.886	2412	2414	2416	rBV2	3609	2465	0.13%	0.032%
47	16.927	2418	2421	2423	rVB2	2755	3252	0.18%	0.043%
48	17.039	2437	2440	2443	rBV3	2979	3782	0.20%	0.050%
49	17.086	2446	2448	2454	rVB3	2862	3548	0.19%	0.047%
50	17.186	2459	2465	2472	rBV	907163	1257005	68.00%	16.524%
51	17.286	2478	2482	2486	rVV3	7603	11674	0.63%	0.153%
52	17.445	2507	2509	2513	rBV4	1749	2471	0.13%	0.032%
53	17.657	2542	2545	2547	rVB3	2787	2703	0.15%	0.036%
54	17.704	2550	2553	2556	rVB4	3409	4652	0.25%	0.061%
55	17.727	2556	2557	2560	rBV3	2658	3267	0.18%	0.043%
56	17.957	2593	2596	2601	rBV4	4219	5764	0.31%	0.076%
57	18.080	2615	2617	2620	rBV2	4426	3458	0.19%	0.045%
58	18.133	2624	2626	2628	rVB2	2684	2679	0.14%	0.035%
59	18.227	2640	2642	2644	rBV2	3182	3258	0.18%	0.043%
60	18.327	2658	2659	2662	rVB	4087	2474	0.13%	0.033%
61	18.357	2662	2664	2666	rBV3	3540	3673	0.20%	0.048%
62	18.510	2685	2690	2691	rBV3	3511	3925	0.21%	0.052%
63	18.610	2703	2707	2708	rVB3	2986	3361	0.18%	0.044%
64	18.639	2708	2712	2715	rBV2	4682	6503	0.35%	0.085%
65	18.786	2735	2737	2738	rBV	4663	2503	0.14%	0.033%
66	18.833	2743	2745	2748	rVB3	3749	3547	0.19%	0.047%
67	18.862	2748	2750	2752	rBV2	2921	2728	0.15%	0.036%
68	19.115	2791	2793	2796	rVV2	4381	3667	0.20%	0.048%
69	19.157	2798	2800	2805	rVV3	2230	4673	0.25%	0.061%
70	19.386	2836	2839	2842	rVV4	3718	3247	0.18%	0.043%
71	19.433	2846	2847	2849	rBV2	4366	3220	0.17%	0.042%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
 Data File : BM000354.D
 Acq On : 25 Jan 2015 04:03
 Operator : TP/IZ
 Sample : G1115-02DL 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
 Title : SVOA CALIBRATION

72	19.509	2857	2860	2862	rVB3	3304	3488	0.19%	0.046%
73	19.545	2862	2866	2867	rBV3	3940	4192	0.23%	0.055%
74	19.562	2867	2869	2870	rVV2	3268	2680	0.14%	0.035%
75	19.586	2870	2873	2877	rVB3	11561	14339	0.78%	0.188%
76	19.686	2889	2890	2893	rVB2	3242	2439	0.13%	0.032%
77	19.792	2906	2908	2910	rBV2	3020	4037	0.22%	0.053%
78	19.851	2916	2918	2921	rBV3	4209	3894	0.21%	0.051%
79	19.915	2926	2929	2932	rBV4	2435	3474	0.19%	0.046%
80	20.098	2956	2960	2961	rBV3	5831	5098	0.28%	0.067%
81	20.133	2964	2966	2968	rVB3	6348	6005	0.32%	0.079%
82	20.168	2968	2972	2974	rBV4	4967	5801	0.31%	0.076%
83	20.198	2976	2977	2979	rBV2	4557	2573	0.14%	0.034%
84	20.345	3001	3002	3005	rBV2	3775	4300	0.23%	0.057%
85	20.374	3005	3007	3008	rVB2	5993	3090	0.17%	0.041%
86	20.398	3008	3011	3013	rBV3	5370	6017	0.33%	0.079%
87	20.556	3033	3038	3040	rBV4	7337	11326	0.61%	0.149%
88	20.604	3044	3046	3049	rVV4	5667	6606	0.36%	0.087%
89	20.656	3053	3055	3058	rBV2	5331	4314	0.23%	0.057%
90	20.927	3099	3101	3103	rVB3	5107	3884	0.21%	0.051%
91	21.062	3123	3124	3130	rBV5	5358	7464	0.40%	0.098%
92	21.109	3130	3132	3135	rBV3	5188	5756	0.31%	0.076%
93	21.168	3138	3142	3146	rVB6	12391	17442	0.94%	0.229%
94	21.203	3146	3148	3149	rBV2	6198	5718	0.31%	0.075%
95	21.374	3172	3177	3183	rBV	1511970	1820021	98.46%	23.925%
96	21.574	3209	3211	3214	rBV3	10292	11113	0.60%	0.146%
97	22.015	3284	3286	3287	rBV2	9546	5929	0.32%	0.078%
98	22.086	3296	3298	3299	rBV2	10793	6126	0.33%	0.081%
99	22.380	3346	3348	3349	rBV2	10777	7400	0.40%	0.097%
100	23.656	3558	3565	3574	rBV	989940	1848491	100.00%	24.299%




Sum of corrected areas: 7607170

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
Data File : BM000354.D
Acq On : 25 Jan 2015 04:03
Operator : TP/IZ
Sample : G1115-02DL 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

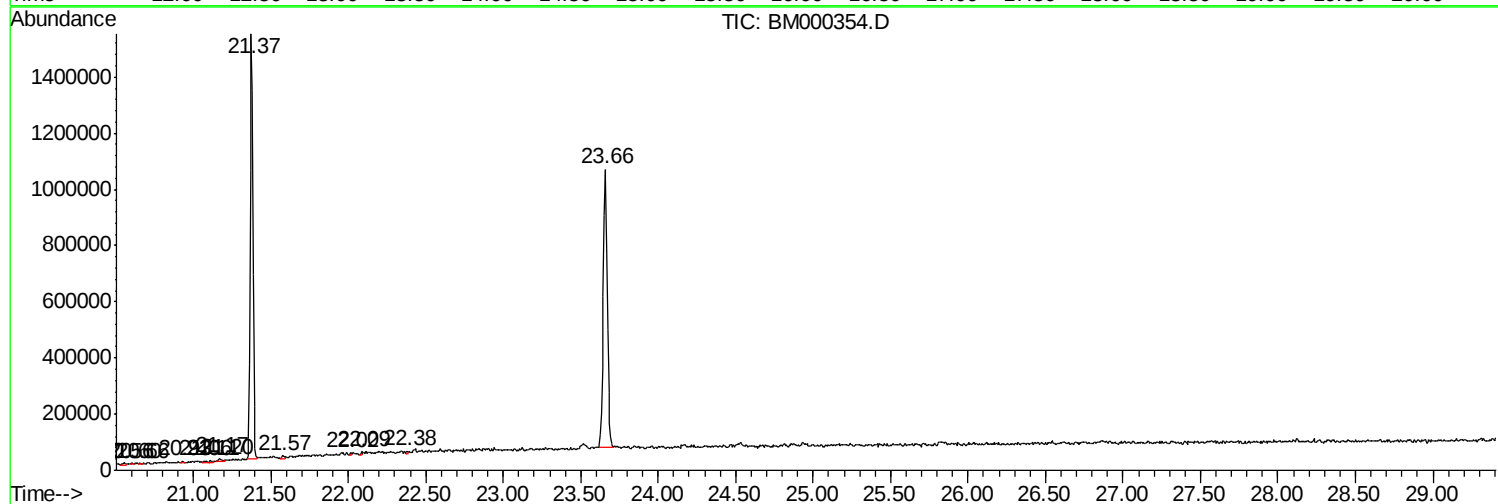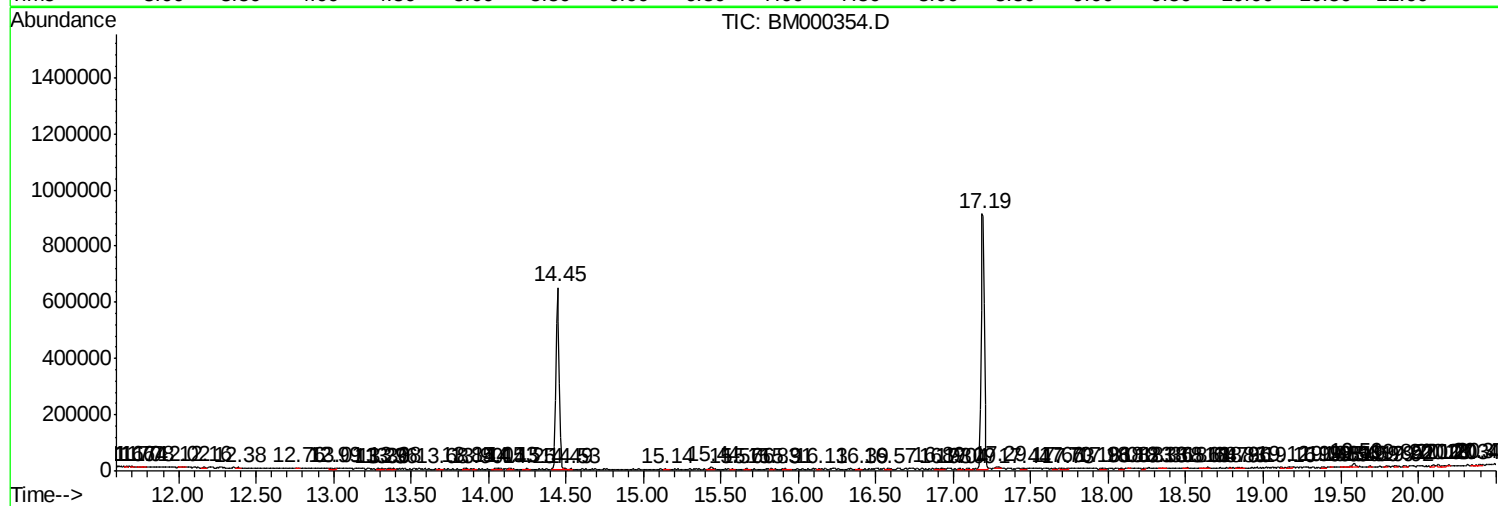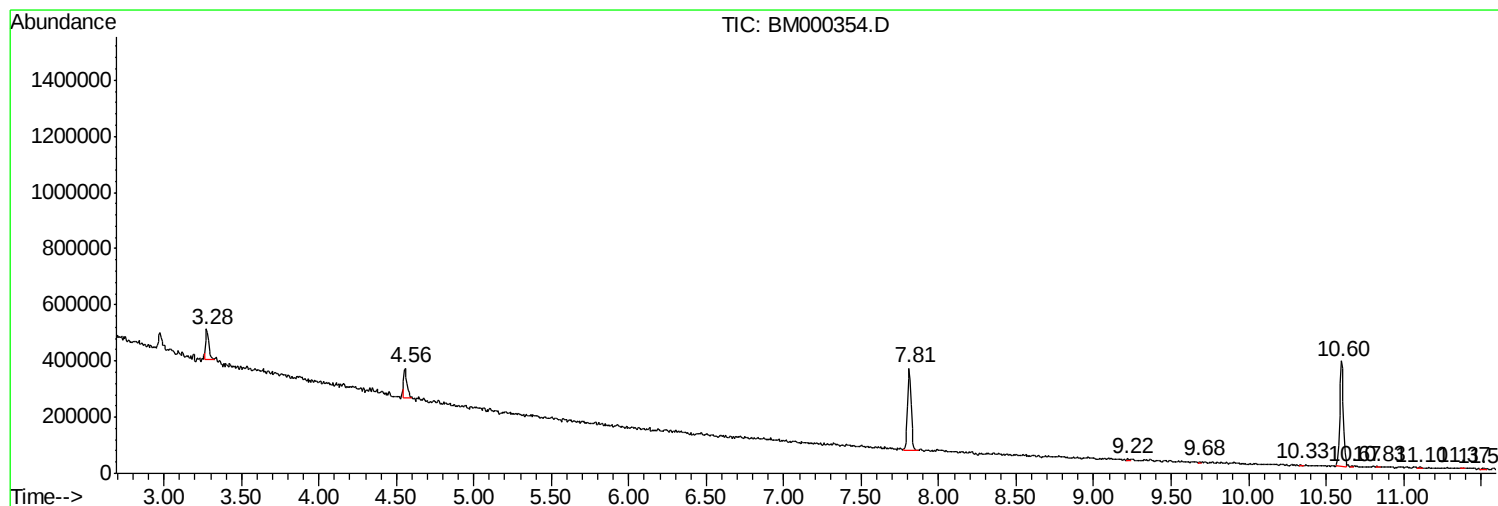

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
Data File : BM000354.D
Acq On : 25 Jan 2015 04:03
Operator : TP/IZ
Sample : G1115-02DL 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012315\
Data File : BM000354.D
Acq On : 25 Jan 2015 04:03
Operator : TP/IZ
Sample : G1115-02DL 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK4DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc