


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012316\
Data File : BM004116.D
Acq On : 22 Jan 2016 18:14
Operator : SJ/UM
Sample : DFTPP43
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP43

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Title : SVOA CALIBRATION
Last Update : Mon Jan 25 13:26:07 2016

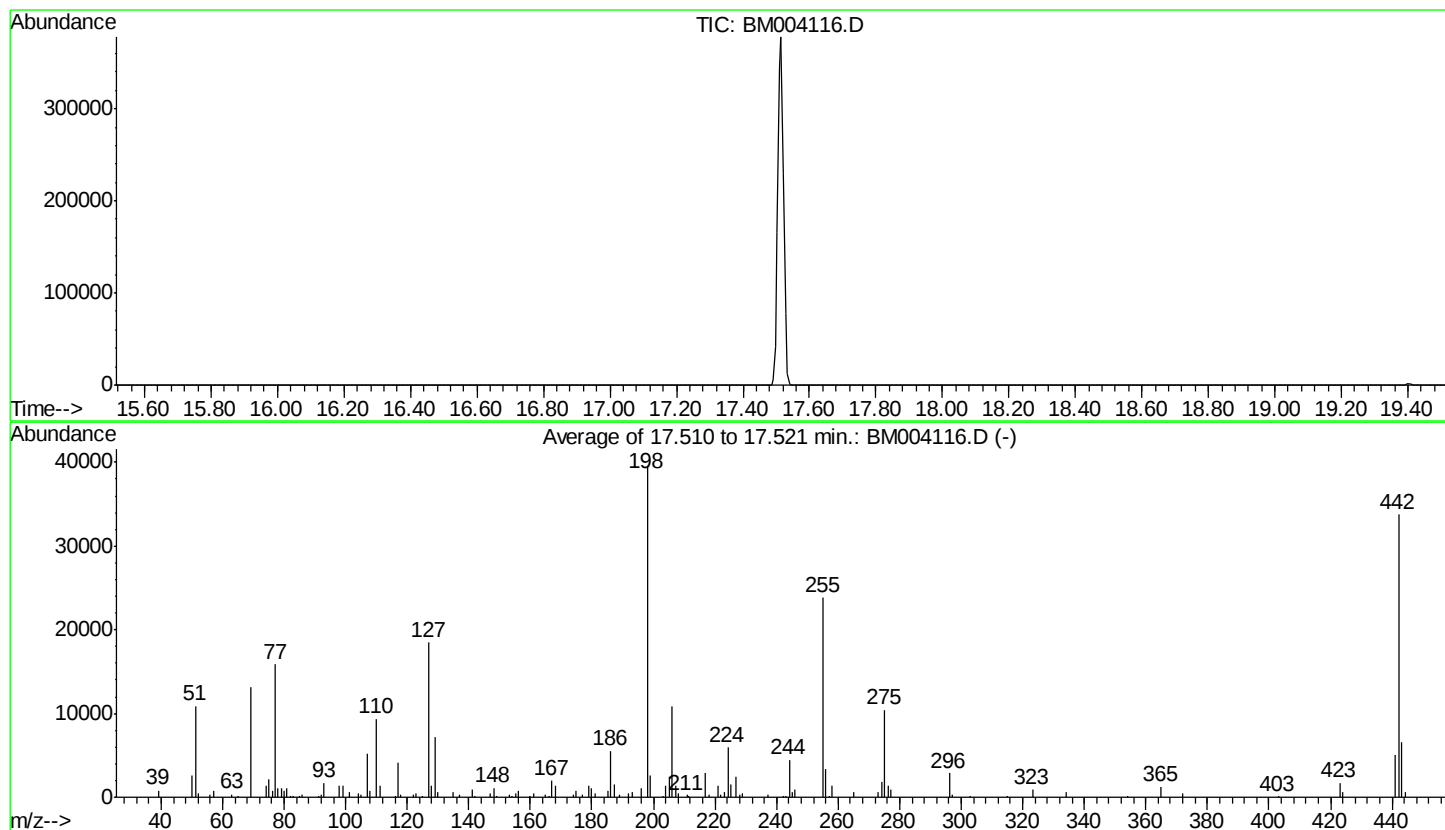

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	10881	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.2	13163	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	18487	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39597	PASS
199	198	5	9	6.4	2535	PASS
275	198	10	60	26.3	10430	PASS
365	198	1	100	3.3	1294	PASS
441	443	0.01	100	75.9	5036	PASS
442	198	50	100	85.3	33765	PASS
443	442	15	24	19.7	6637	PASS

m/z	Abundance
39.00	968.0
50.10	3195.0
51.10	13341.0
52.00	682.0
56.00	386.0
57.00	936.0
63.00	599.0
69.00	16078.0
74.00	1665.0
75.00	2779.0
76.10	890.0
77.10	19440.0
78.10	1311.0
79.00	1244.0
80.00	976.0
81.00	1404.0
82.00	319.0
83.00	306.0
85.00	312.0
86.00	383.0
92.00	370.0
93.00	2084.0
98.10	1609.0
99.00	1631.0
101.00	789.0
104.00	448.0
105.00	464.0
107.00	6081.0
108.00	910.0
110.00	10919.0
111.00	1690.0
116.00	300.0
117.00	4818.0
118.00	434.0
122.00	411.0
123.00	607.0
127.10	21120.0
128.00	1579.0
129.00	8066.0
130.00	734.0
135.00	674.0
137.00	426.0
141.00	1088.0
147.00	668.0
148.00	1181.0
149.00	320.0
153.00	344.0
155.00	558.0
156.10	903.0
160.00	339.0
161.00	472.0
165.00	404.0
165.90	305.0
167.00	2243.0
168.00	1682.0
174.00	456.0
175.00	905.0
177.00	395.0
179.00	1512.0
180.00	1281.0
181.00	535.0
185.00	778.0
186.10	6171.0
187.10	1844.0
189.00	398.0
192.00	566.0
193.00	584.0
196.00	1199.0
198.00	43312.0
199.00	2864.0
204.10	1586.0
205.10	2780.0
206.10	11658.0
207.10	1833.0
208.00	465.0
210.90	458.0
217.00	3021.0
218.00	387.0
221.00	1576.0
222.00	386.0
223.00	687.0
224.10	6393.0
225.10	1643.0
227.00	2728.0
228.00	369.0
229.00	596.0
237.00	405.0
242.00	327.0
244.10	4660.0
245.10	679.0
246.00	930.0

Instrument :
BNA_M
ClientSampleId :
DFTPP43

255.10	24584.0
256.10	3736.0
257.00	358.0
258.10	1418.0
265.00	569.0
273.00	714.0
274.10	1785.0
275.10	10446.0
276.10	1512.0
277.10	882.0
296.10	2662.0
297.00	466.0
303.00	339.0
323.10	886.0
334.10	541.0
365.00	1270.0
372.10	504.0
423.10	1471.0
424.20	618.0
441.10	4213.0
442.10	27864.0
443.10	5796.0
444.10	544.0

Instrument :
BNA_M
ClientSampleId :
DFTPP43

m/z	Abundance
39.10	881.0
50.10	2979.0
51.10	12674.0
52.00	529.0
56.00	414.0
57.00	956.0
63.00	534.0
65.00	301.0
69.00	15181.0
74.00	1498.0
75.00	2464.0
76.10	828.0
77.10	18600.0
78.10	1267.0
79.00	1178.0
80.00	864.0
81.00	1275.0
83.00	307.0
85.00	326.0
86.00	354.0
91.00	307.0
92.00	382.0
93.00	2034.0
98.00	1580.0
99.00	1555.0
101.00	758.0
103.90	466.0
105.00	403.0
107.00	6145.0
108.00	898.0
110.00	10800.0
111.00	1575.0
117.00	4727.0
118.00	305.0
122.00	350.0
123.00	618.0
125.00	307.0
127.00	21776.0
128.00	1718.0
129.00	8558.0
130.00	622.0
135.00	756.0
137.00	402.0
141.00	1070.0
142.00	373.0
147.00	578.0
148.00	1319.0
153.00	365.0
154.00	306.0
155.10	547.0
156.00	1019.0
160.00	318.0
161.10	571.0
165.00	443.0
167.00	2316.0
168.00	1475.0
174.00	541.0
175.00	918.0
177.00	447.0
179.00	1681.0
180.00	1298.0
181.00	590.0
185.10	888.0
186.10	6517.0
187.10	1858.0
189.00	410.0
192.00	560.0
193.00	664.0
196.00	1316.0
198.00	46616.0
199.00	3078.0
203.00	327.0
204.00	1710.0
205.10	2973.0
206.10	13039.0
207.00	1798.0
208.00	504.0
211.20	446.0
217.00	3314.0
218.00	424.0
221.10	1681.0
221.90	539.0
223.00	769.0
224.10	6991.0
225.10	1804.0
227.00	2981.0
228.00	393.0
229.00	608.0
237.10	321.0
242.00	344.0
243.00	393.0

Instrument :
BNA_M
ClientSampleId :
DFTPP43

244.10	5242.0
245.10	621.0
246.10	1013.0
255.10	28464.0
256.10	4058.0
257.00	326.0
258.00	1490.0
265.00	628.0
273.10	849.0
274.10	2328.0
275.10	12419.0
276.10	1637.0
277.10	1059.0
296.10	3626.0
297.00	458.0
303.00	337.0
315.00	365.0
323.10	1077.0
334.00	678.0
354.10	326.0
365.10	1483.0
372.10	549.0
403.10	391.0
423.10	2124.0
424.10	752.0
441.10	6098.0
442.10	40832.0
443.10	7991.0
444.20	773.0

Instrument :
BNA_M
ClientSampleId :
DFTPP43

m/z	Abundance
39.00	469.0
50.00	1544.0
51.10	6628.0
52.00	315.0
57.00	486.0
69.00	8232.0
74.00	783.0
75.00	1378.0
76.00	411.0
77.10	9561.0
78.10	672.0
79.00	606.0
80.00	465.0
81.00	685.0
93.00	1073.0
98.00	818.0
99.00	807.0
101.00	395.0
104.00	300.0
107.00	3416.0
108.00	530.0
110.00	6464.0
111.00	892.0
117.00	2725.0
127.00	12566.0
128.00	909.0
129.00	4750.0
130.00	391.0
135.00	416.0
141.00	604.0
147.00	344.0
148.00	723.0
155.00	419.0
156.00	558.0
161.00	336.0
167.00	1256.0
168.00	761.0
175.10	509.0
179.00	1001.0
180.00	717.0
181.00	325.0
185.00	489.0
186.10	3908.0
187.00	1121.0
192.00	341.0
193.00	442.0
196.00	814.0
198.00	28864.0
199.00	1663.0
204.00	1072.0
205.00	1712.0
206.10	7886.0
207.10	1276.0
208.00	350.0
211.00	337.0
217.00	2244.0
221.10	1070.0
223.00	469.0
224.10	4441.0
225.10	1167.0
227.00	1839.0
229.00	338.0
244.10	3410.0
245.10	428.0
246.00	630.0
255.10	18392.0
256.00	2497.0
258.00	1059.0
265.00	429.0
273.10	515.0
274.00	1539.0
275.10	8426.0
276.10	1173.0
277.00	765.0
296.10	2345.0
323.10	782.0
334.00	568.0
365.00	1129.0
372.10	416.0
423.10	1670.0
424.10	566.0
441.10	4797.0
442.10	32600.0
443.20	6124.0
444.10	515.0

Instrument :
BNA_M
ClientSampleId :
DFTPP43

m/z	Abundance
207.10	300.0

Instrument :
BNA_M
ClientSampleId :
DFTPP43