

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012317\
 Data File : BM008809.D
 Acq On : 23 Jan 2017 19:42
 Operator : UM/SJ
 Sample : PB96205BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Quant Time: Jan 24 02:51:59 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 24 02:47:47 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.94	152	95415	20.00	ng/ul	0.00
18) Naphthalene-d8	10.75	136	382844	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.57	164	301378	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.42	188	1330143	20.00	ng/ul	0.09
75) Chrysene-d12	21.49	240	671569	20.00	ng/ul	0.00
83) Perylene-d12	23.85	264	384081	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.39	96	18354	9.51	ng/uL	0.00
5) Phenol-d5	7.09	99	327491	40.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.27	67	269203	41.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.47	132	227754	43.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	257348	40.67	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	116220	47.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.83	143	132008	44.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	252113	40.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.88	131	184761	27.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.98	166	939139	47.56	ng/ul	0.00
46) Acenaphthylene-d8	14.27	160	1063339	45.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.76	143	133056	40.28	ng/ul	0.00
57) Fluorene-d10	15.57	176	802315	42.77	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	157845	19.93	ng/ul	0.00
70) Anthracene-d10	17.42	188	1330143	22.87	ng/ul	0.00
76) Pyrene-d10	19.70	212	1508718	51.22	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.70	264	778709	47.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.63	70	11843	1.57	ng/ul#	1
21) Isophorone	9.82	82	30237	1.74	ng/ul#	71
45) 2,6-Dinitrotoluene	13.98	165	7711	2.04	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012317\
Data File : BM008809.D
Acq On : 23 Jan 2017 19:42
Operator : UM/SJ
Sample : PB96205BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Time: Jan 24 02:51:59 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 24 02:47:47 2017
Response via : Initial Calibration




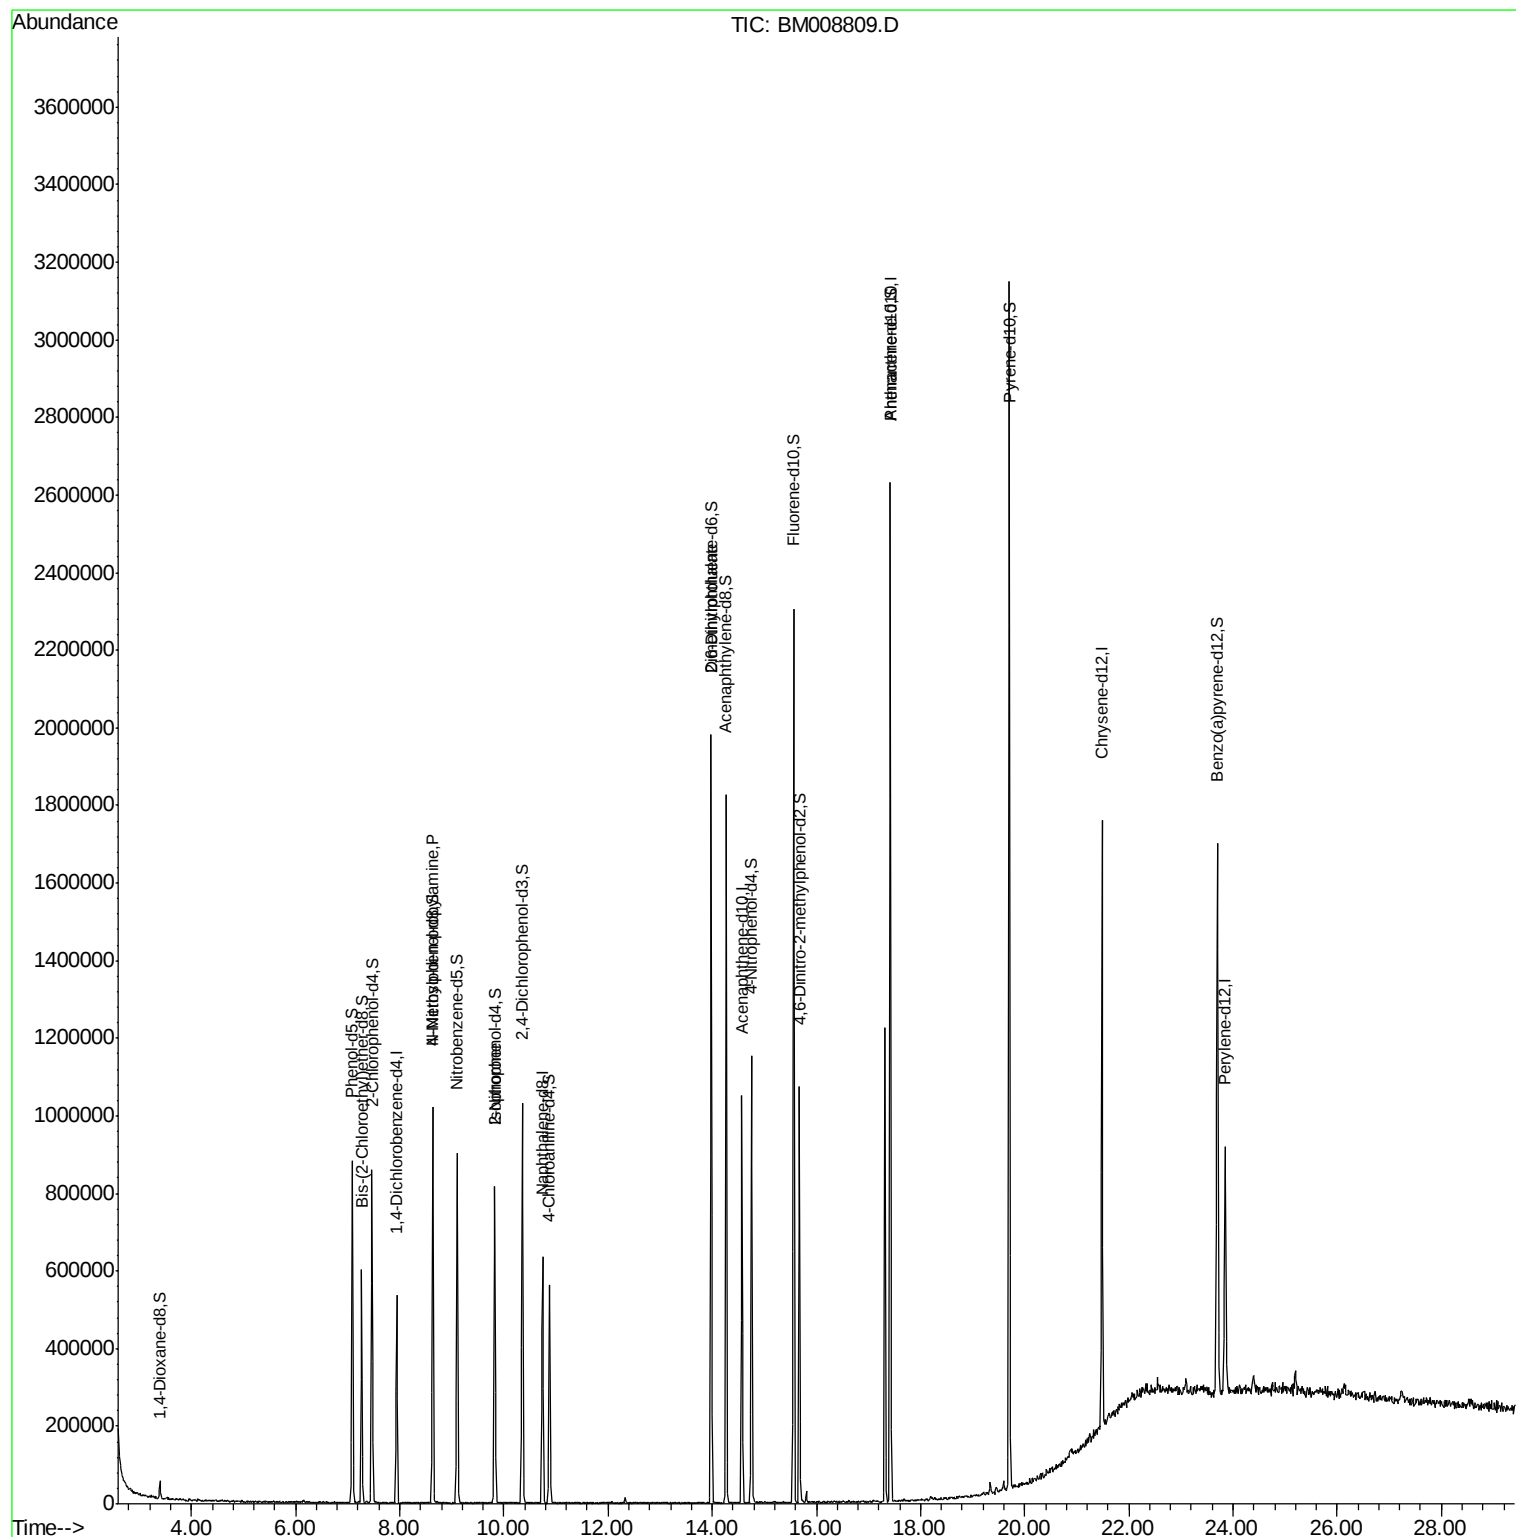


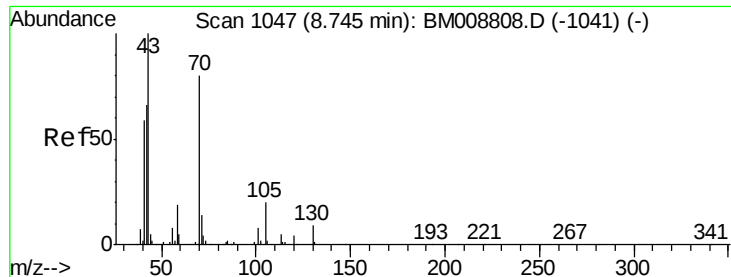

#15
N-Nitroso-di-n-propylamine
Concen: 1.57 ng/ul
RT: 8.63 min Scan# 1028
Delta R.T. -0.11 min
Lab File: BM008809.D
Acq: 23 Jan 2017 19:42




Instrument :
BNA_M
ClientSampleId :
SBLK05


Tgt Ion: 70 Resp: 11843
Ion Ratio Lower Upper
70 100
42 385.6 37.5 56.3#
101 0.0 7.8 11.8#
130 0.0 16.6 25.0#

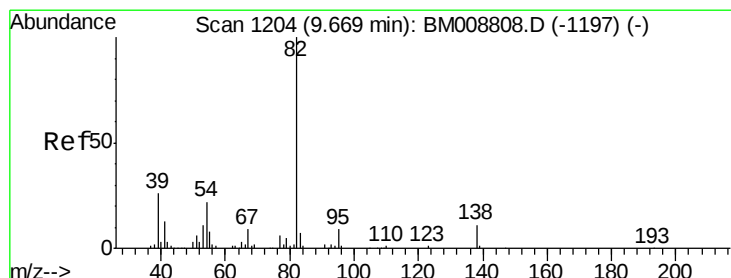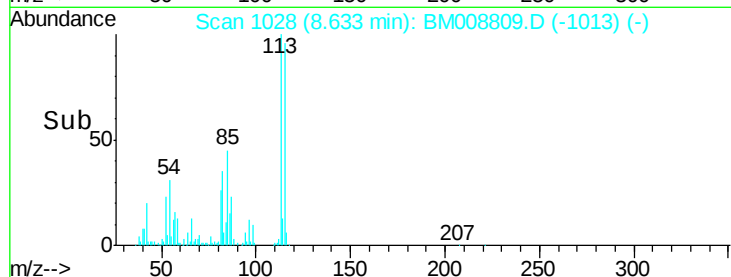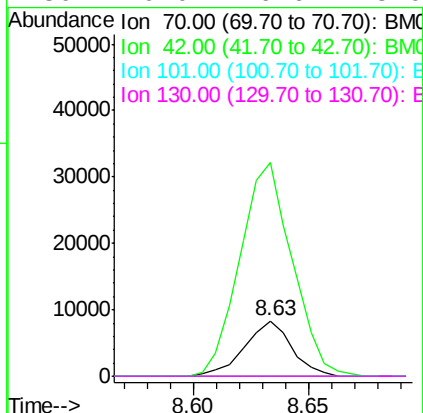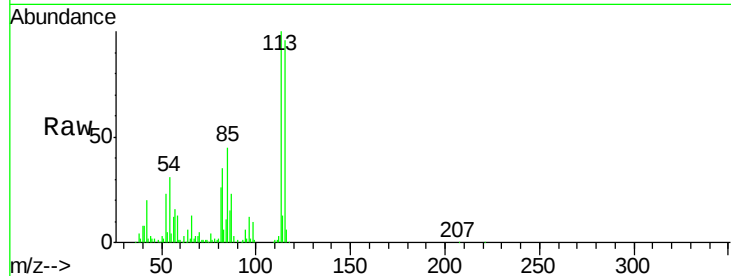

#21
Isophorone
Concen: 1.74 ng/ul
RT: 9.82 min Scan# 1230
Delta R.T. 0.15 min
Lab File: BM008809.D
Acq: 23 Jan 2017 19:42

Tgt Ion: 82 Resp: 30237
Ion Ratio Lower Upper
82 100
95 4.8 6.1 9.1#
138 0.0 13.4 20.2#

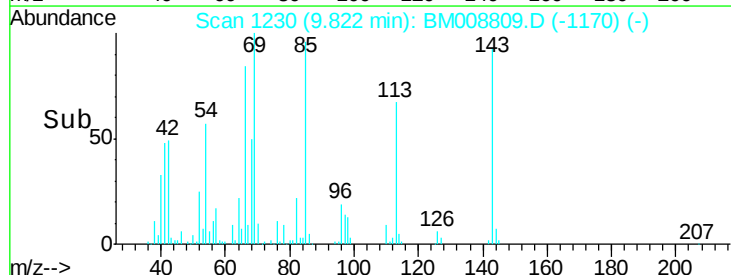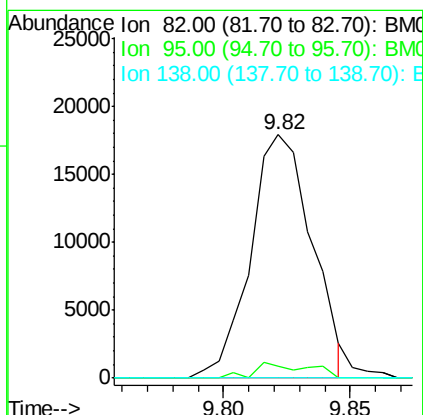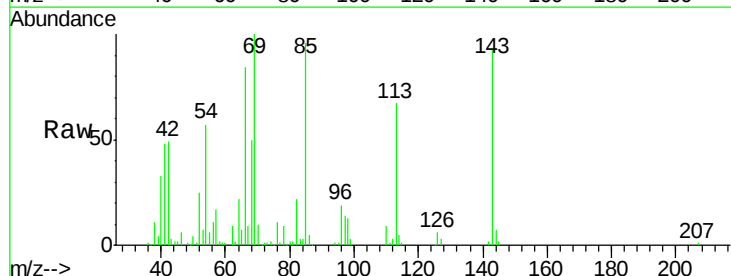

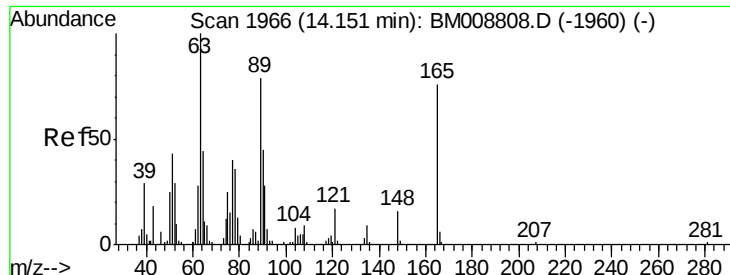

#45

2,6-Dinitrotoluene

Concen: 2.04 ng/ul

RT: 13.98 min Scan# 1937

Delta R.T. -0.17 min

Lab File: BM008809.D

Acq: 23 Jan 2017 19:42

Instrument :

BNA_M

ClientSampleId :

SBLK05



Tgt Ion:165 Resp: 7711

Ion Ratio Lower Upper

165 100

89 6.8 50.6 76.0#

121 33.2 18.2 27.2#

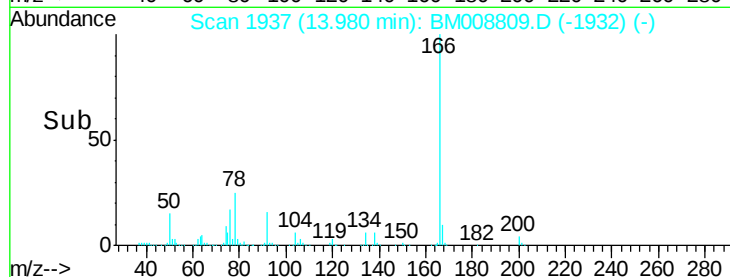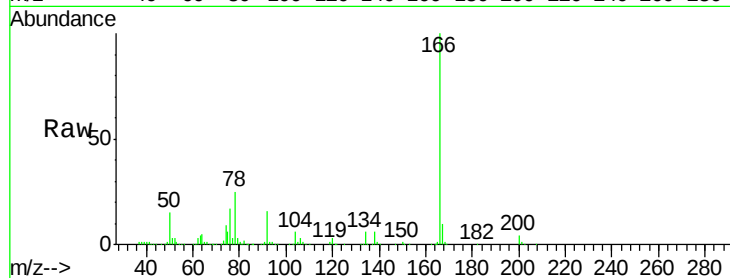

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

