

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_M\DATA\BM012318\
 Data File : BM013734.D
 Acq On : 23 Jan 2018 17:09
 Operator : SJ/JU
 Sample : J1220-08
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6A10

Quant Time: Jan 24 03:44:15 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 24 03:42:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	147902	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	581266	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	320515	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	693843	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	668203	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	663918	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	13781	3.68	ng/uL	0.00
5) Phenol-d5	6.79	99	303659	26.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	193461	28.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	276398	29.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	259186	29.69	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	136513	30.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	154560	32.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	265015	28.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	335138	41.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	785999	29.76	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1032633	30.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	95178	22.17	ng/ul	0.00
57) Fluorene-d10	15.26	176	674643	29.04	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	90984	21.79	ng/ul	0.00
70) Anthracene-d10	17.12	188	1009757	29.88	ng/ul	0.00
76) Pyrene-d10	19.42	212	1088040	34.97	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	976582	32.00	ng/ul	0.00


Target Compounds					Qvalue
6) Phenol	6.82	94	29576	2.597 ng/ul	94
44) Dimethylphthalate	13.73	163	239835	9.234 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_M\DATA\BM012318\
Data File : BM013734.D
Acq On : 23 Jan 2018 17:09
Operator : SJ/JU
Sample : J1220-08
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6A10

Quant Time: Jan 24 03:44:15 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 24 03:42:30 2018
Response via : Initial Calibration

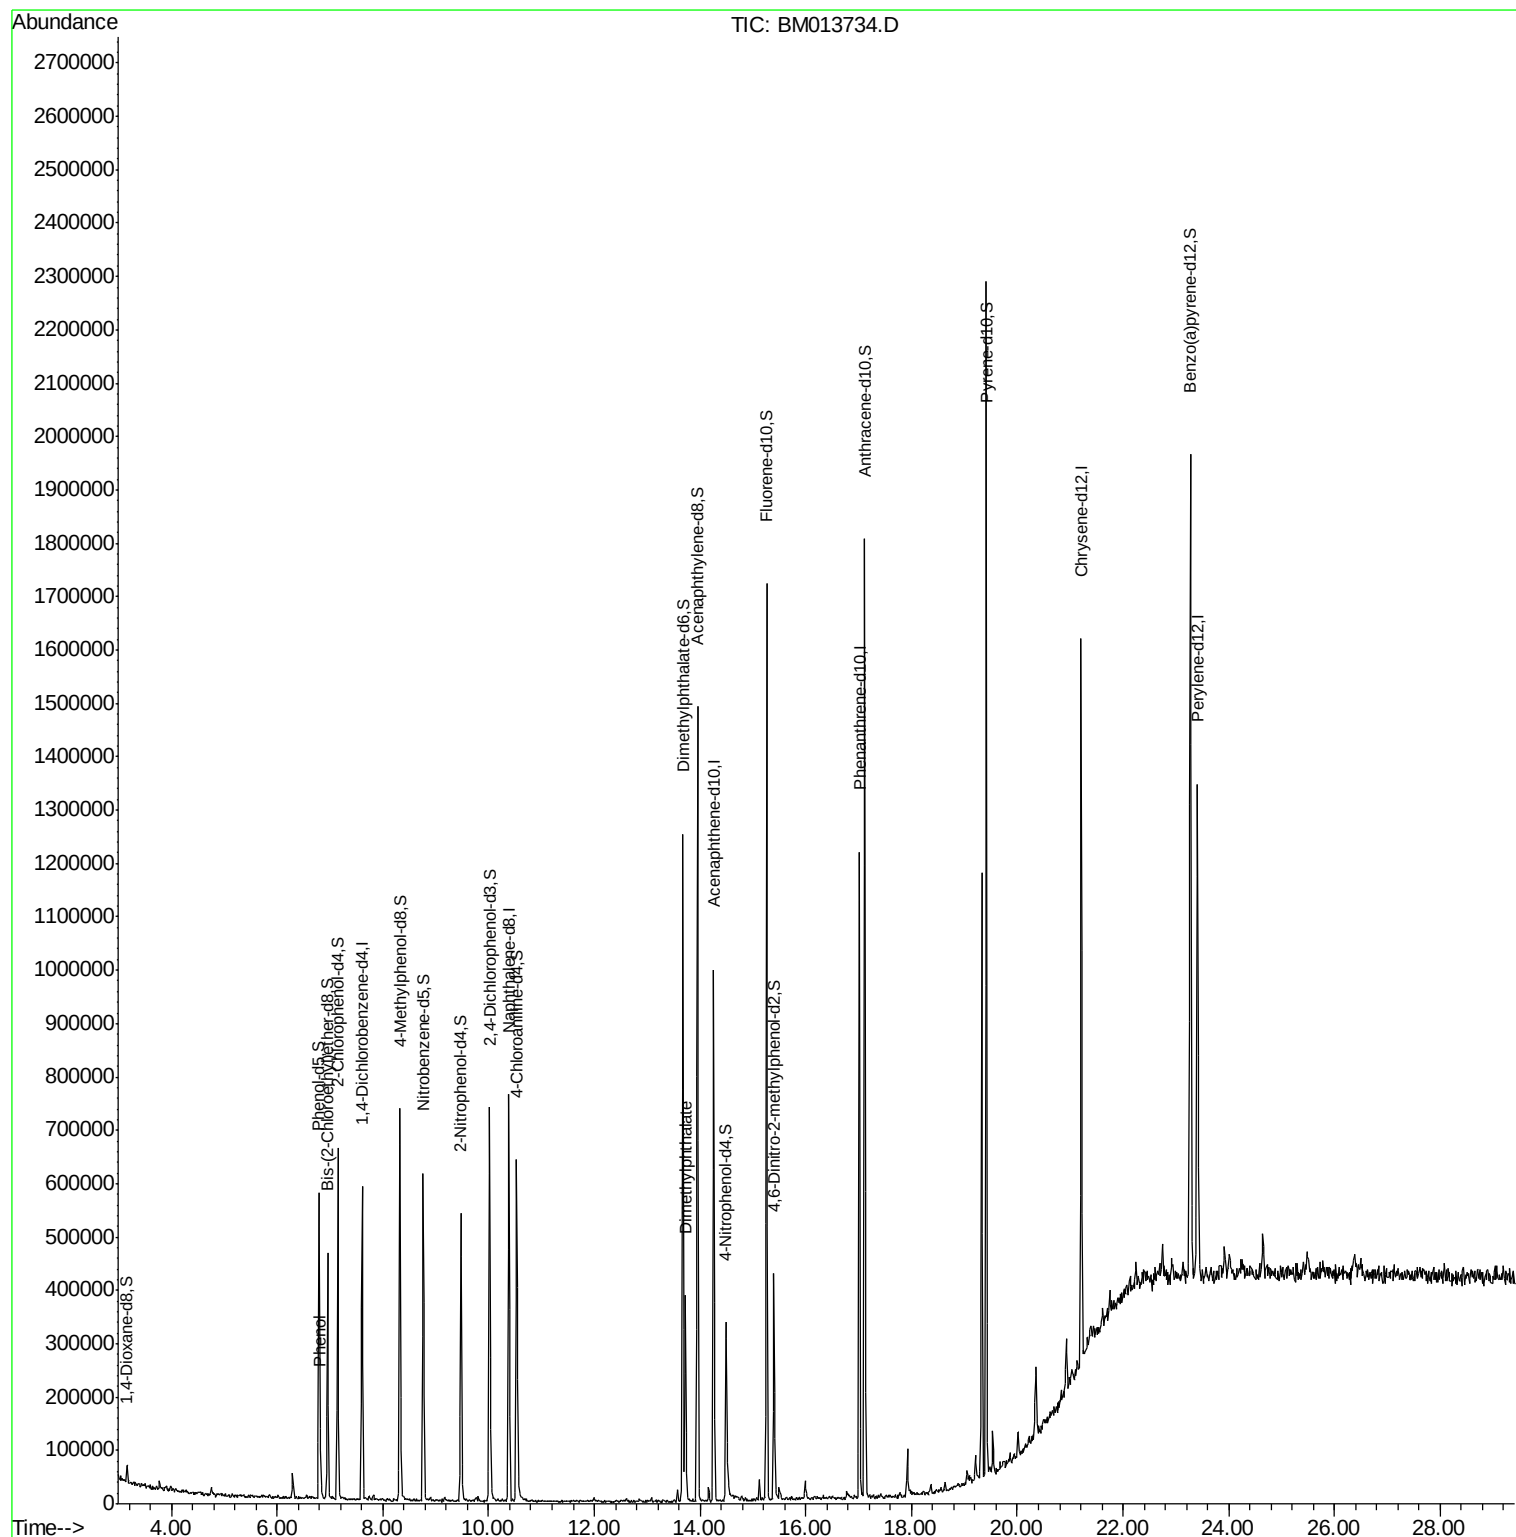

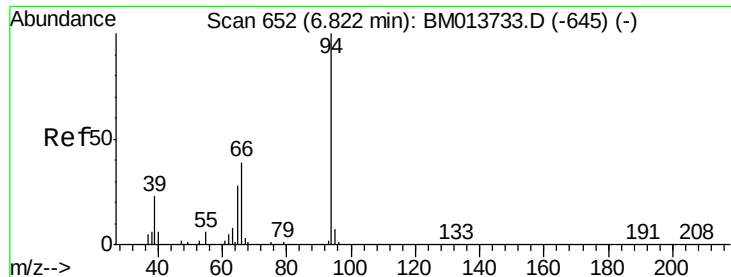

#6

Phenol

Concen: 2.597 ng/ul

RT: 6.82 min Scan# 652

Delta R.T. -0.00 min

Lab File: BM013734.D

Acq: 23 Jan 2018 17:09

Instrument :

BNA_M

ClientSampleId :

F6A10


Tgt Ion: 94 Resp: 29576

Ion Ratio Lower Upper




94 100

65 35.2 28.2 42.4

66 52.3 47.2 70.8

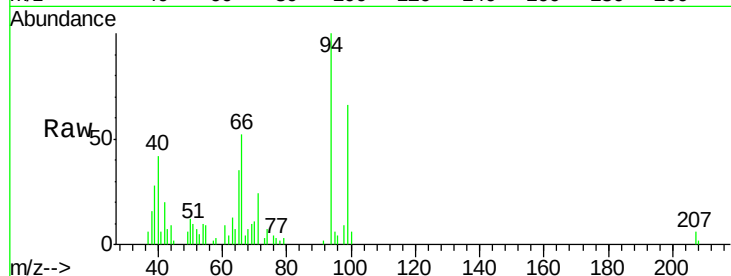

Abundance Ion 94.00 (93.70 to 94.70): BM013734.D (-618) (-)

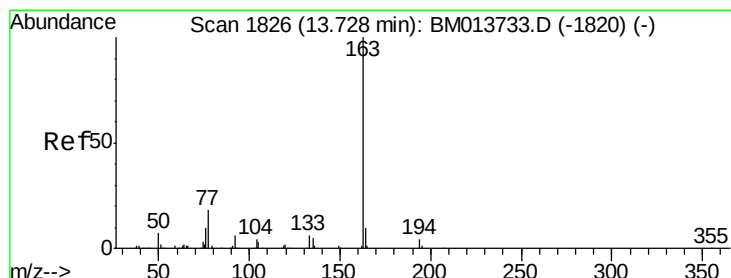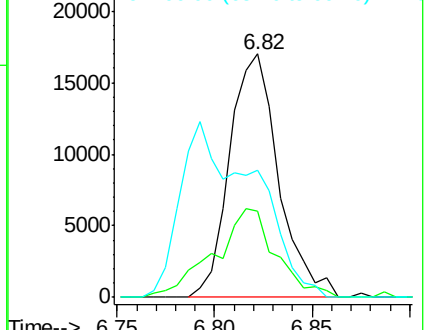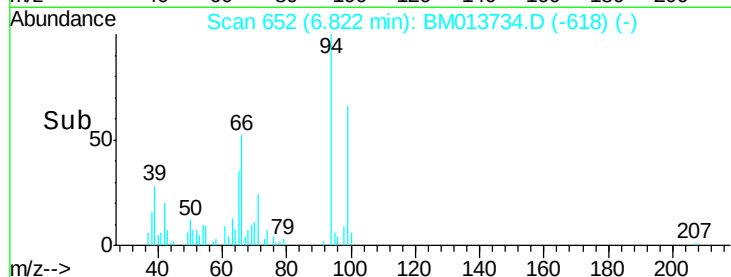

#44

Dimethylphthalate

Concen: 9.234 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.00 min

Lab File: BM013734.D

Acq: 23 Jan 2018 17:09


Tgt Ion: 163 Resp: 239835

Ion Ratio Lower Upper

163 100

194 5.2 3.5 5.3

164 10.5 8.2 12.4

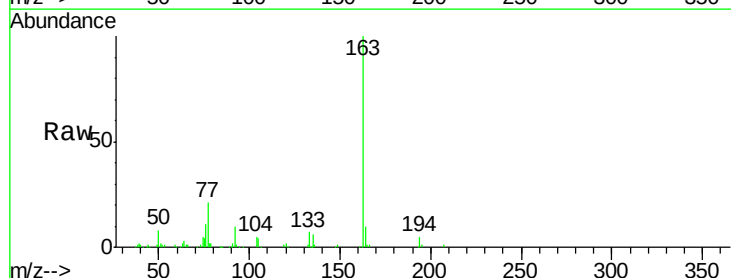

Abundance Ion 163.00 (162.70 to 163.70): BM013734.D (-1792) (-)

