

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_M\DATA\BM012318\
 Data File : BM013737.D
 Acq On : 23 Jan 2018 18:58
 Operator : SJ/JU
 Sample : J1221-19
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6A43

Quant Time: Jan 24 04:47:27 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 24 03:42:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	151116	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	595947	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	340973	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	730849	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	743223	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	729766	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	19098	5.00	ng/uL	0.00
5) Phenol-d5	6.79	99	465510	40.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	268141	38.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	387783	41.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	386532	43.34	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	197713	42.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	212219	43.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	388468	41.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	482857	58.96	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	1142605	40.66	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1486803	41.49	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	165317	36.20	ng/ul	0.00
57) Fluorene-d10	15.26	176	989506	40.04	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	149882	34.07	ng/ul	0.00
70) Anthracene-d10	17.12	188	1471973	41.35	ng/ul	0.00
76) Pyrene-d10	19.42	212	1628406	47.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1518916	45.28	ng/ul	0.00


Target Compounds					Qvalue
6) Phenol	6.82	94	82186	7.063 ng/ul	89
44) Dimethylphthalate	13.72	163	416271	15.066 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_M\DATA\BM012318\
Data File : BM013737.D
Acq On : 23 Jan 2018 18:58
Operator : SJ/JU
Sample : J1221-19
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6A43

Quant Time: Jan 24 04:47:27 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 24 03:42:30 2018
Response via : Initial Calibration

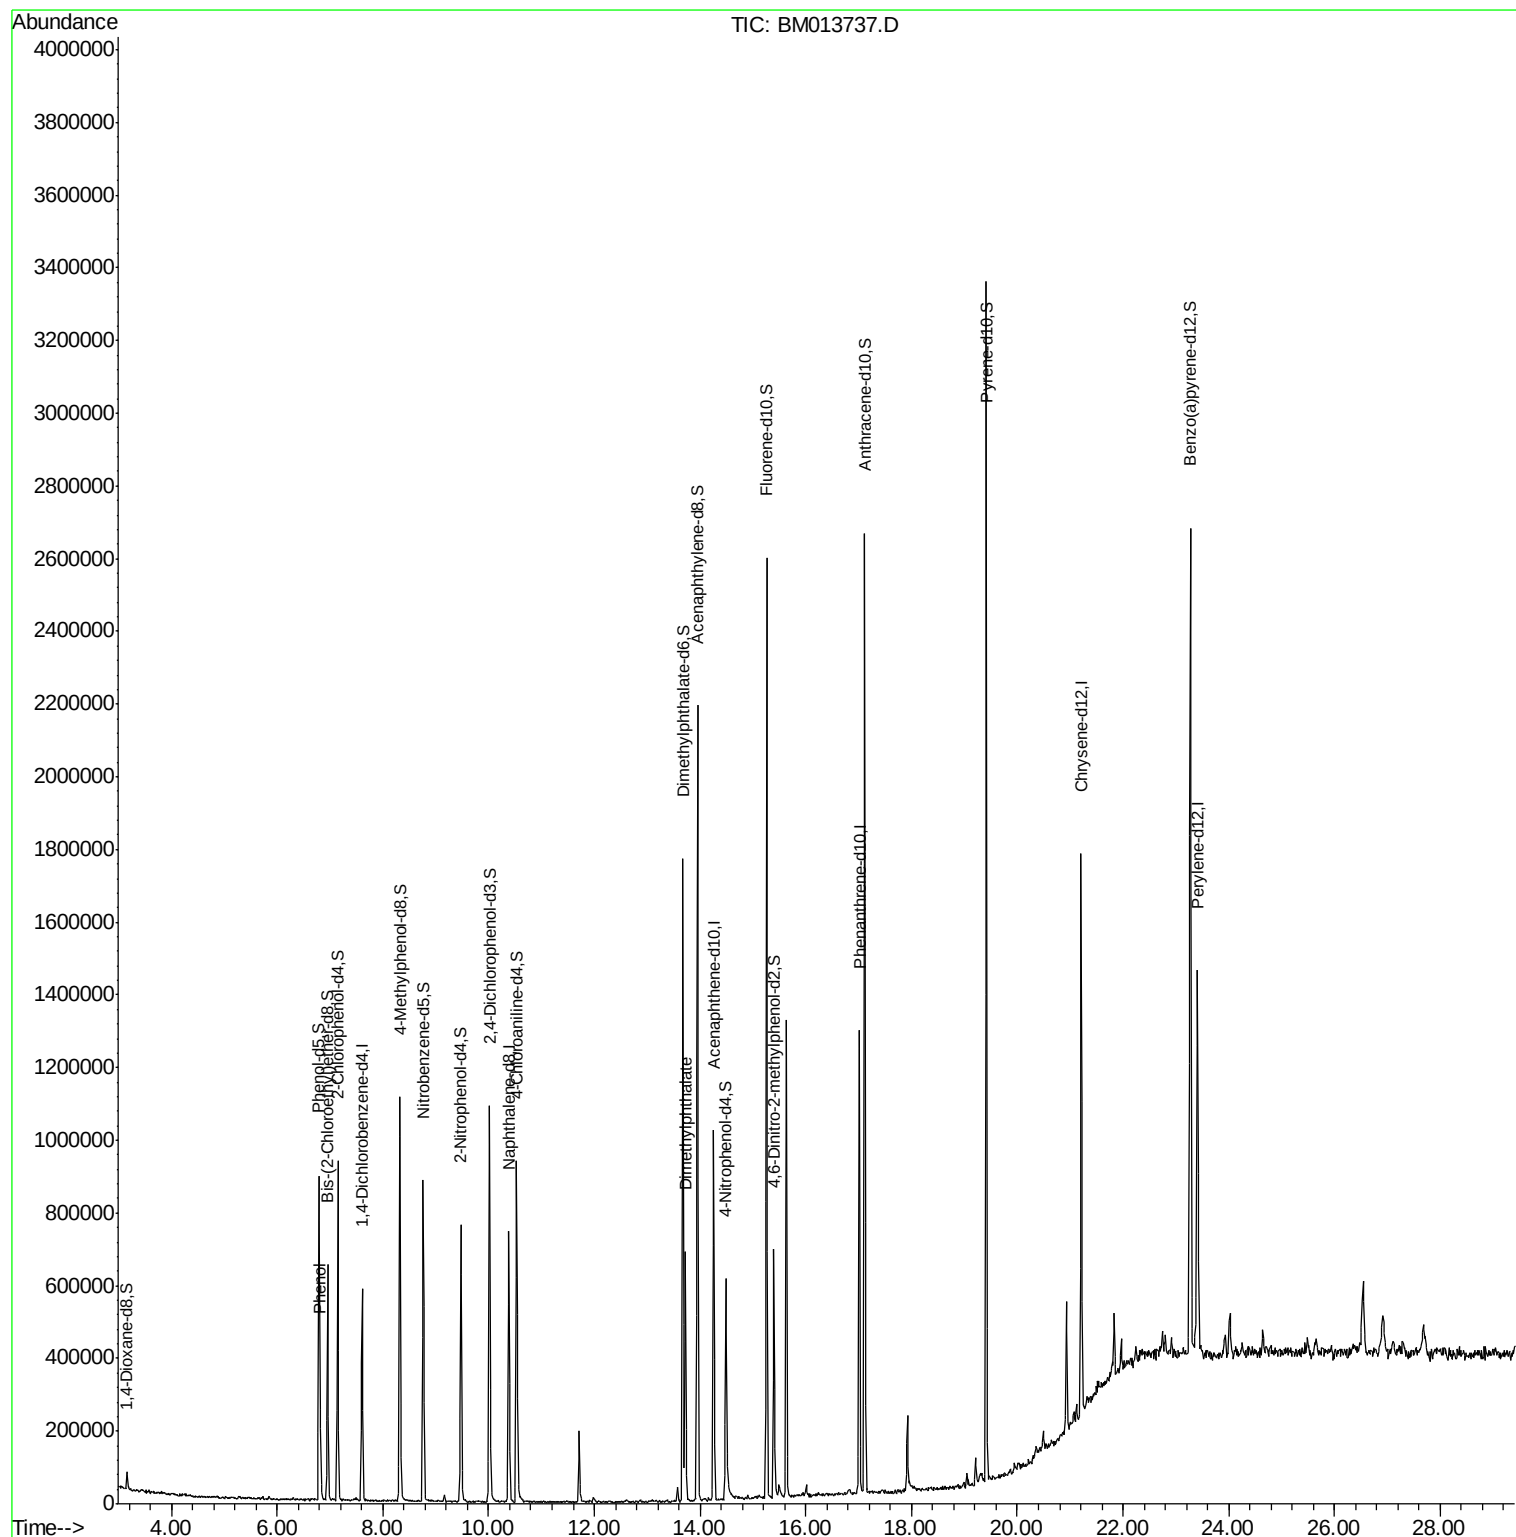

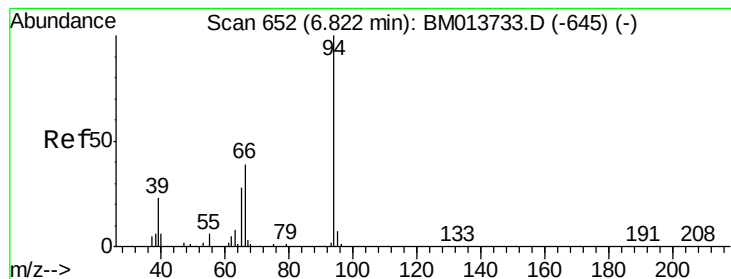





#6

Phenol

Concen: 7.063 ng/ul
 RT: 6.82 min Scan# 651
 Delta R.T. -0.01 min
 Lab File: BM013737.D
 Acq: 23 Jan 2018 18:58

Instrument :
 BNA_M
 ClientSampleId :
 F6A43

Tgt Ion: 94 Resp: 82186
 Ion Ratio Lower Upper
 94 100
 65 33.3 28.2 42.4
 66 47.6 47.2 70.8

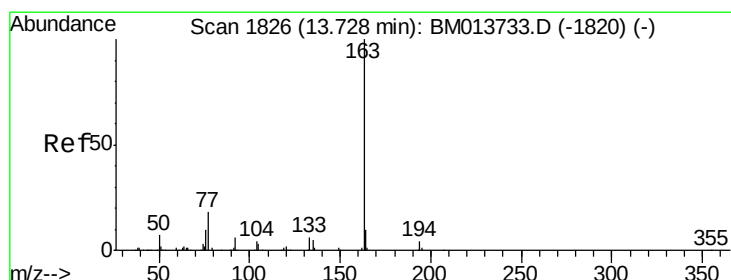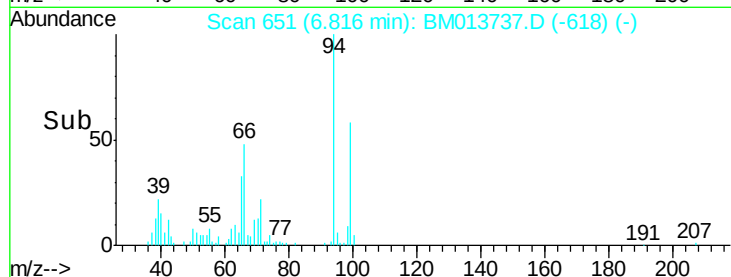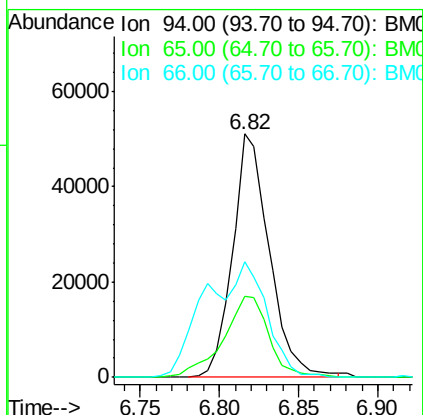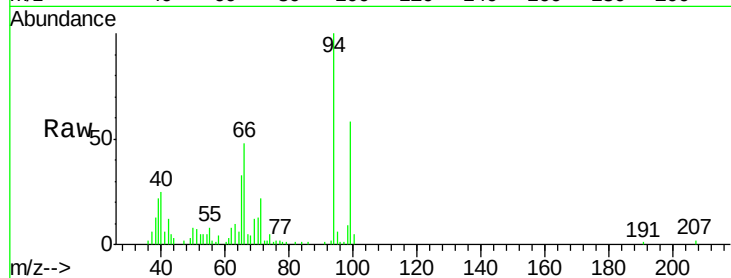

#44

Dimethylphthalate

Concen: 15.066 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BM013737.D
 Acq: 23 Jan 2018 18:58

Tgt Ion: 163 Resp: 416271
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.5 5.3
 164 9.4 8.2 12.4

