

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_M\DATA\BM012318\
 Data File : BM013745.D
 Acq On : 23 Jan 2018 23:46
 Operator : SJ/JU
 Sample : J1221-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6A23

Quant Time: Jan 24 05:47:44 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 24 03:42:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	160326	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	654590	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	378074	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	873534	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	973426	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	961568	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	19862	4.90	ng/uL	0.00
5) Phenol-d5	6.79	99	467377	37.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	269594	36.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	387918	38.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	390412	41.26	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	197145	38.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	226032	42.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	399495	38.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	345153	38.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	1180431	37.88	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1563175	39.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	157138	31.03	ng/ul	0.00
57) Fluorene-d10	15.26	176	1047657	38.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	161720	30.76	ng/ul	0.00
70) Anthracene-d10	17.11	188	1618837	38.05	ng/ul	0.00
76) Pyrene-d10	19.42	212	1827361	40.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1817472	41.12	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	6.82	94	80606	6.529 ng/ul#	85
44) Dimethylphthalate	13.72	163	408978	13.349 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_M\DATA\BM012318\
Data File : BM013745.D
Acq On : 23 Jan 2018 23:46
Operator : SJ/JU
Sample : J1221-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6A23

Quant Time: Jan 24 05:47:44 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 24 03:42:30 2018
Response via : Initial Calibration

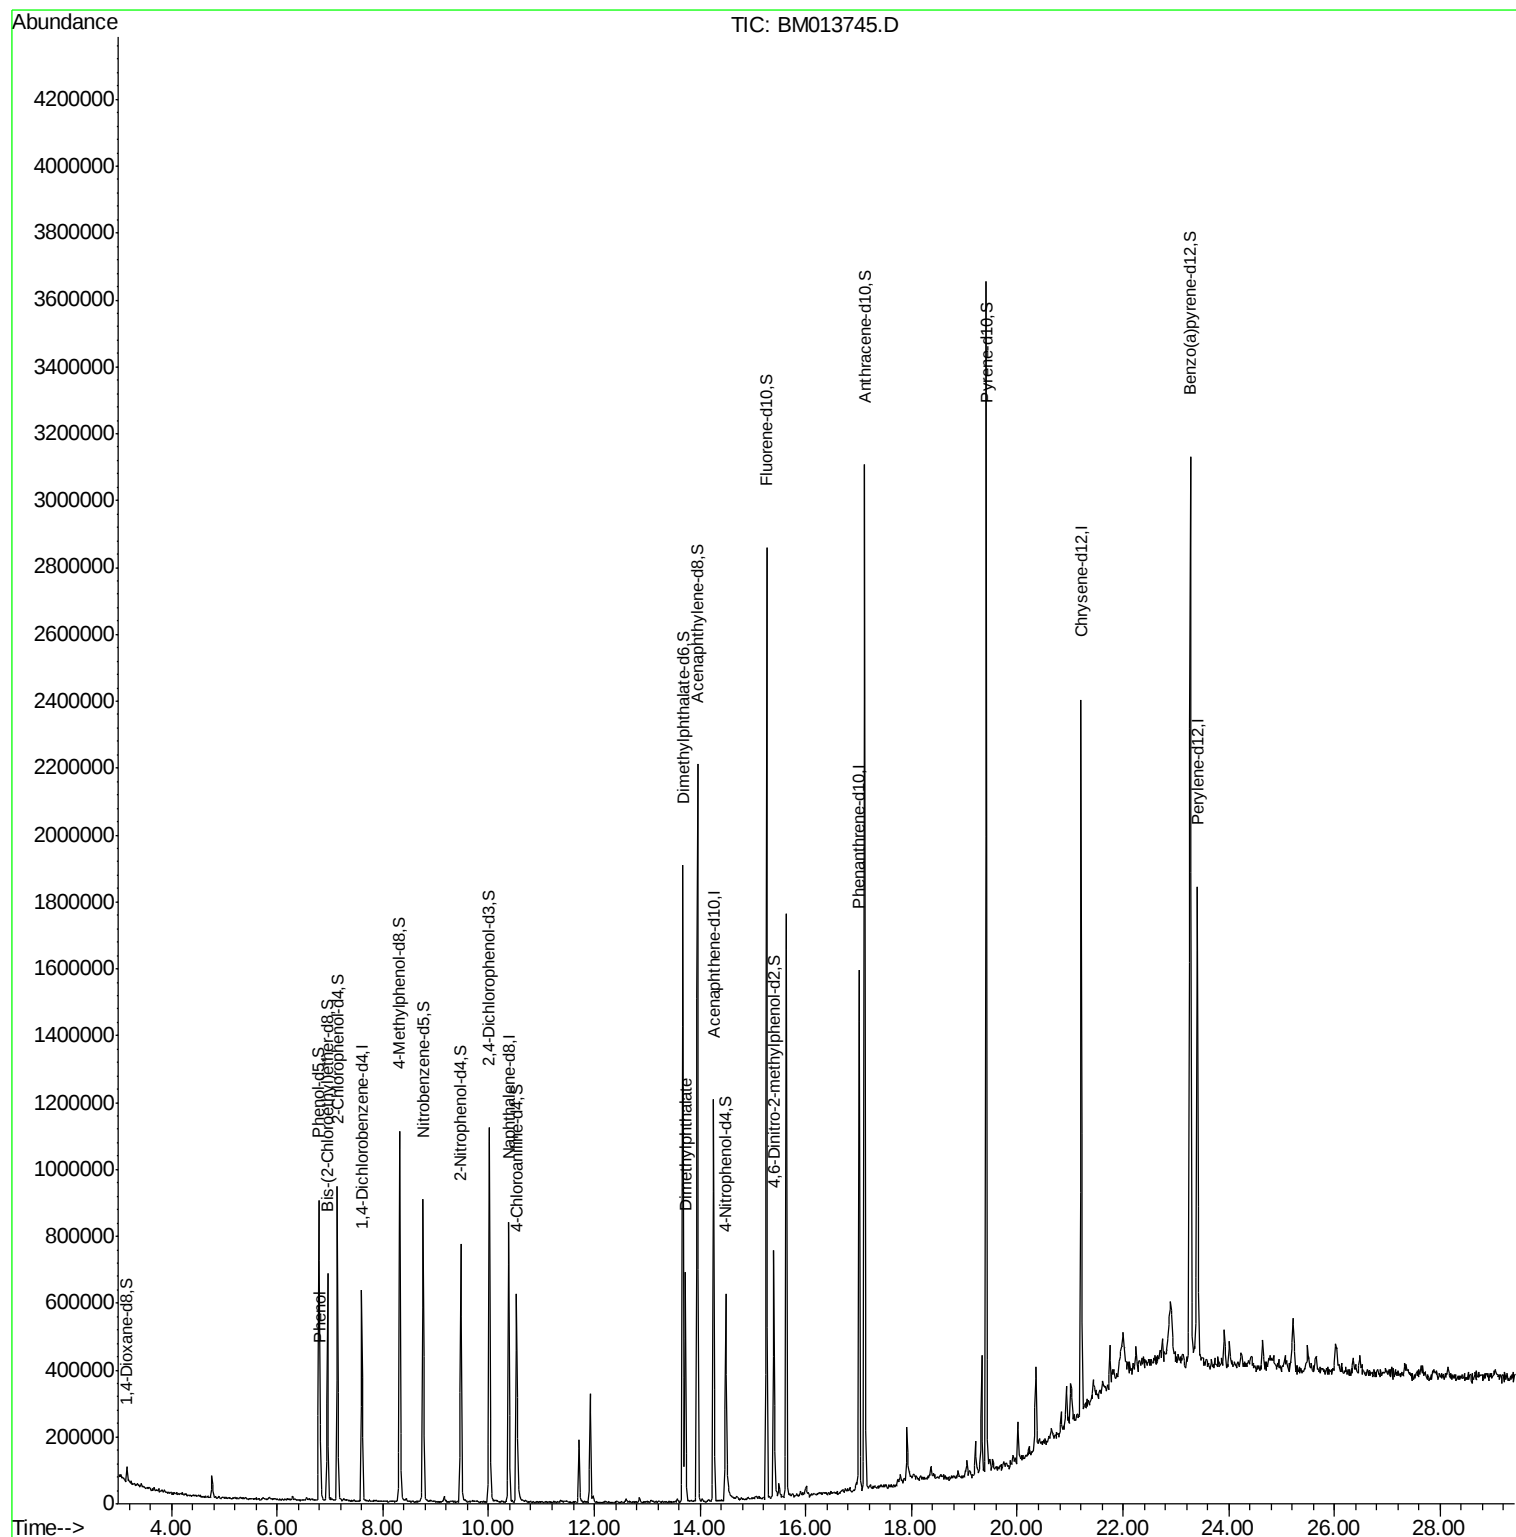

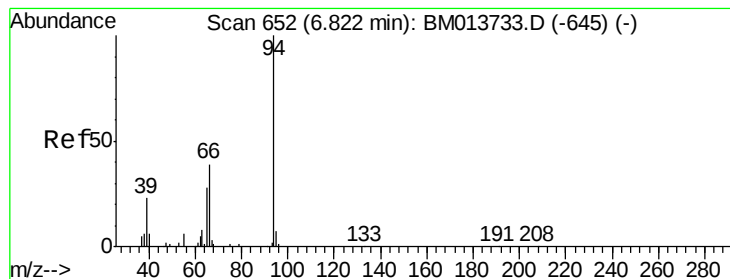





#6

Phenol

Concen: 6.529 ng/ul
 RT: 6.82 min Scan# 651
 Delta R.T. -0.01 min
 Lab File: BM013745.D
 Acq: 23 Jan 2018 23:46

Instrument :
 BNA_M
 ClientSampleId :
 F6A23

Tgt Ion: 94 Resp: 80606
 Ion Ratio Lower Upper
 94 100
 65 35.2 28.2 42.4
 66 41.3 47.2 70.8#

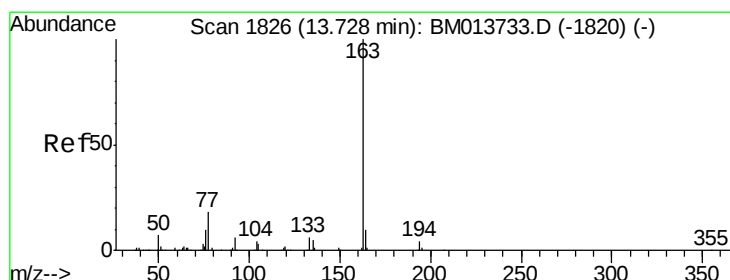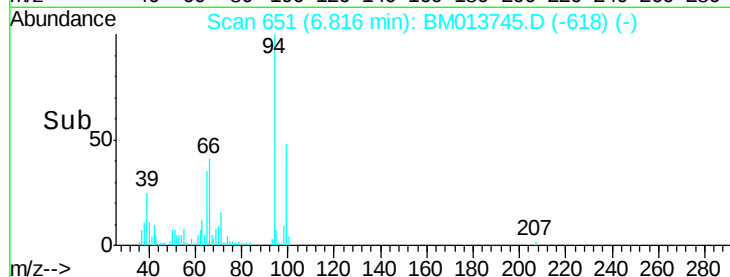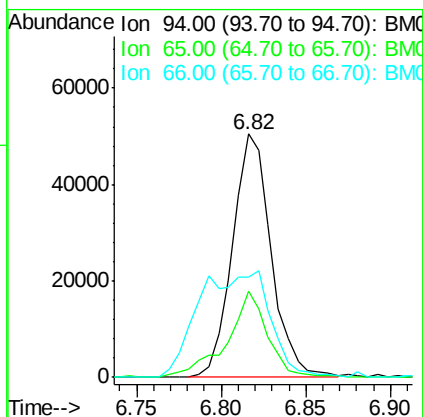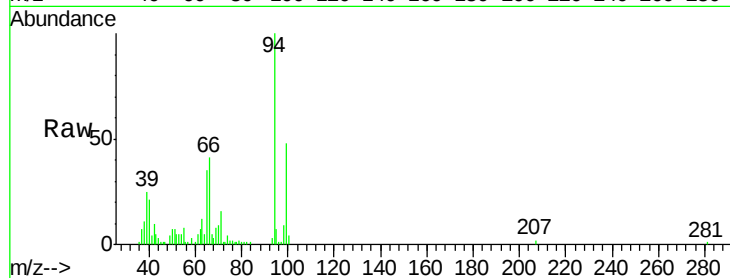

#44

Dimethylphthalate

Concen: 13.349 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BM013745.D
 Acq: 23 Jan 2018 23:46

Tgt Ion: 163 Resp: 408978
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.5 5.3
 164 10.3 8.2 12.4

