


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012320\
 Data File : BM024599.D
 Acq On : 23 Jan 2020 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 23 14:57:07 2020

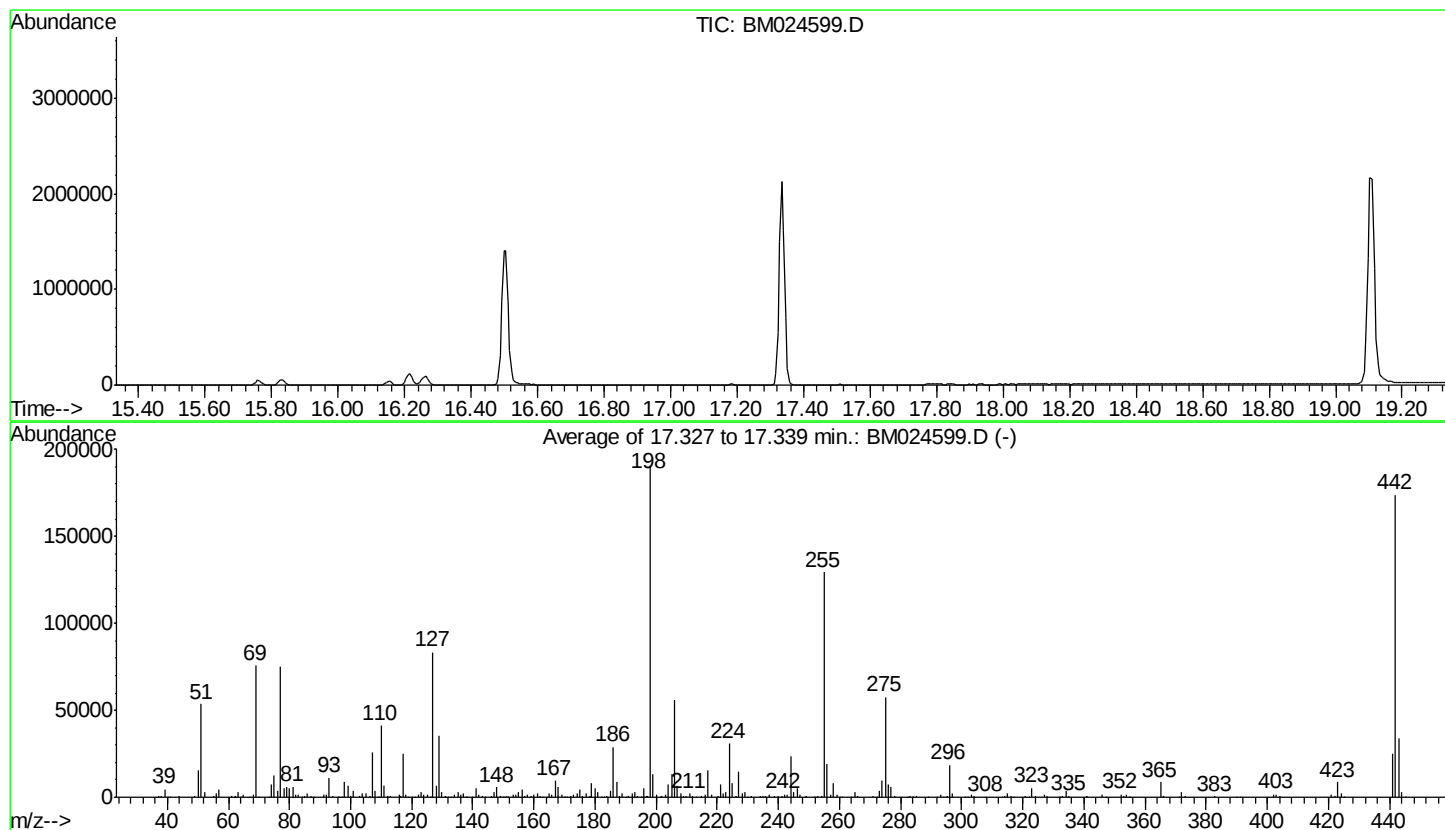

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	53661	PASS
68	69	0.00	2	1.8	1351	PASS
69	198	0.00	100	39.6	75520	PASS
70	69	0.00	2	0.4	328	PASS
127	198	10	80	43.7	83344	PASS
197	198	0.00	2	0.5	943	PASS
198	198	100	100	100.0	190677	PASS
199	198	5	9	7.0	13308	PASS
275	198	10	60	30.3	57722	PASS
365	198	1	100	4.6	8745	PASS
441	198	0.01	100	13.1	25026	PASS
442	198	50	100	91.3	174101	PASS
443	442	15	24	19.5	33944	PASS