

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012417\
 Data File : BM008849.D
 Acq On : 24 Jan 2017 21:40
 Operator : UM/SJ
 Sample : I1315-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDN11

Quant Time: Jan 25 03:39:46 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 25 03:34:06 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	56188	20.00	ng/ul	0.00
18) Naphthalene-d8	10.74	136	215047	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.57	164	156491	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.32	188	356755	20.00	ng/ul	0.00
75) Chrysene-d12	21.48	240	464836	20.00	ng/ul	0.00
83) Perylene-d12	23.84	264	449571	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.39	96	4206	3.70	ng/uL	0.00
5) Phenol-d5	7.08	99	114002	23.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	97065	25.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	74857	24.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	81308	21.82	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	37873	27.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	38201	22.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	84131	24.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	54944	14.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	231736	22.60	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	334218	27.55	ng/ul	0.00
51) 4-Nitrophenol-d4	14.75	143	37582	21.91	ng/ul	0.00
57) Fluorene-d10	15.56	176	258797	26.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	35760	16.83	ng/ul	0.00
70) Anthracene-d10	17.42	188	454187	29.11	ng/ul	0.00
76) Pyrene-d10	19.70	212	572207	28.07	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.69	264	563022	29.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	7.11	94	21208	4.09	ng/ul#	33
15) N-Nitroso-di-n-propylamine	8.62	70	5053	1.14	ng/ul#	1
44) Dimethylphthalate	14.02	163	43659	4.26	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012417\
Data File : BM008849.D
Acq On : 24 Jan 2017 21:40
Operator : UM/SJ
Sample : I1315-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDN11

Quant Time: Jan 25 03:39:46 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 25 03:34:06 2017
Response via : Initial Calibration

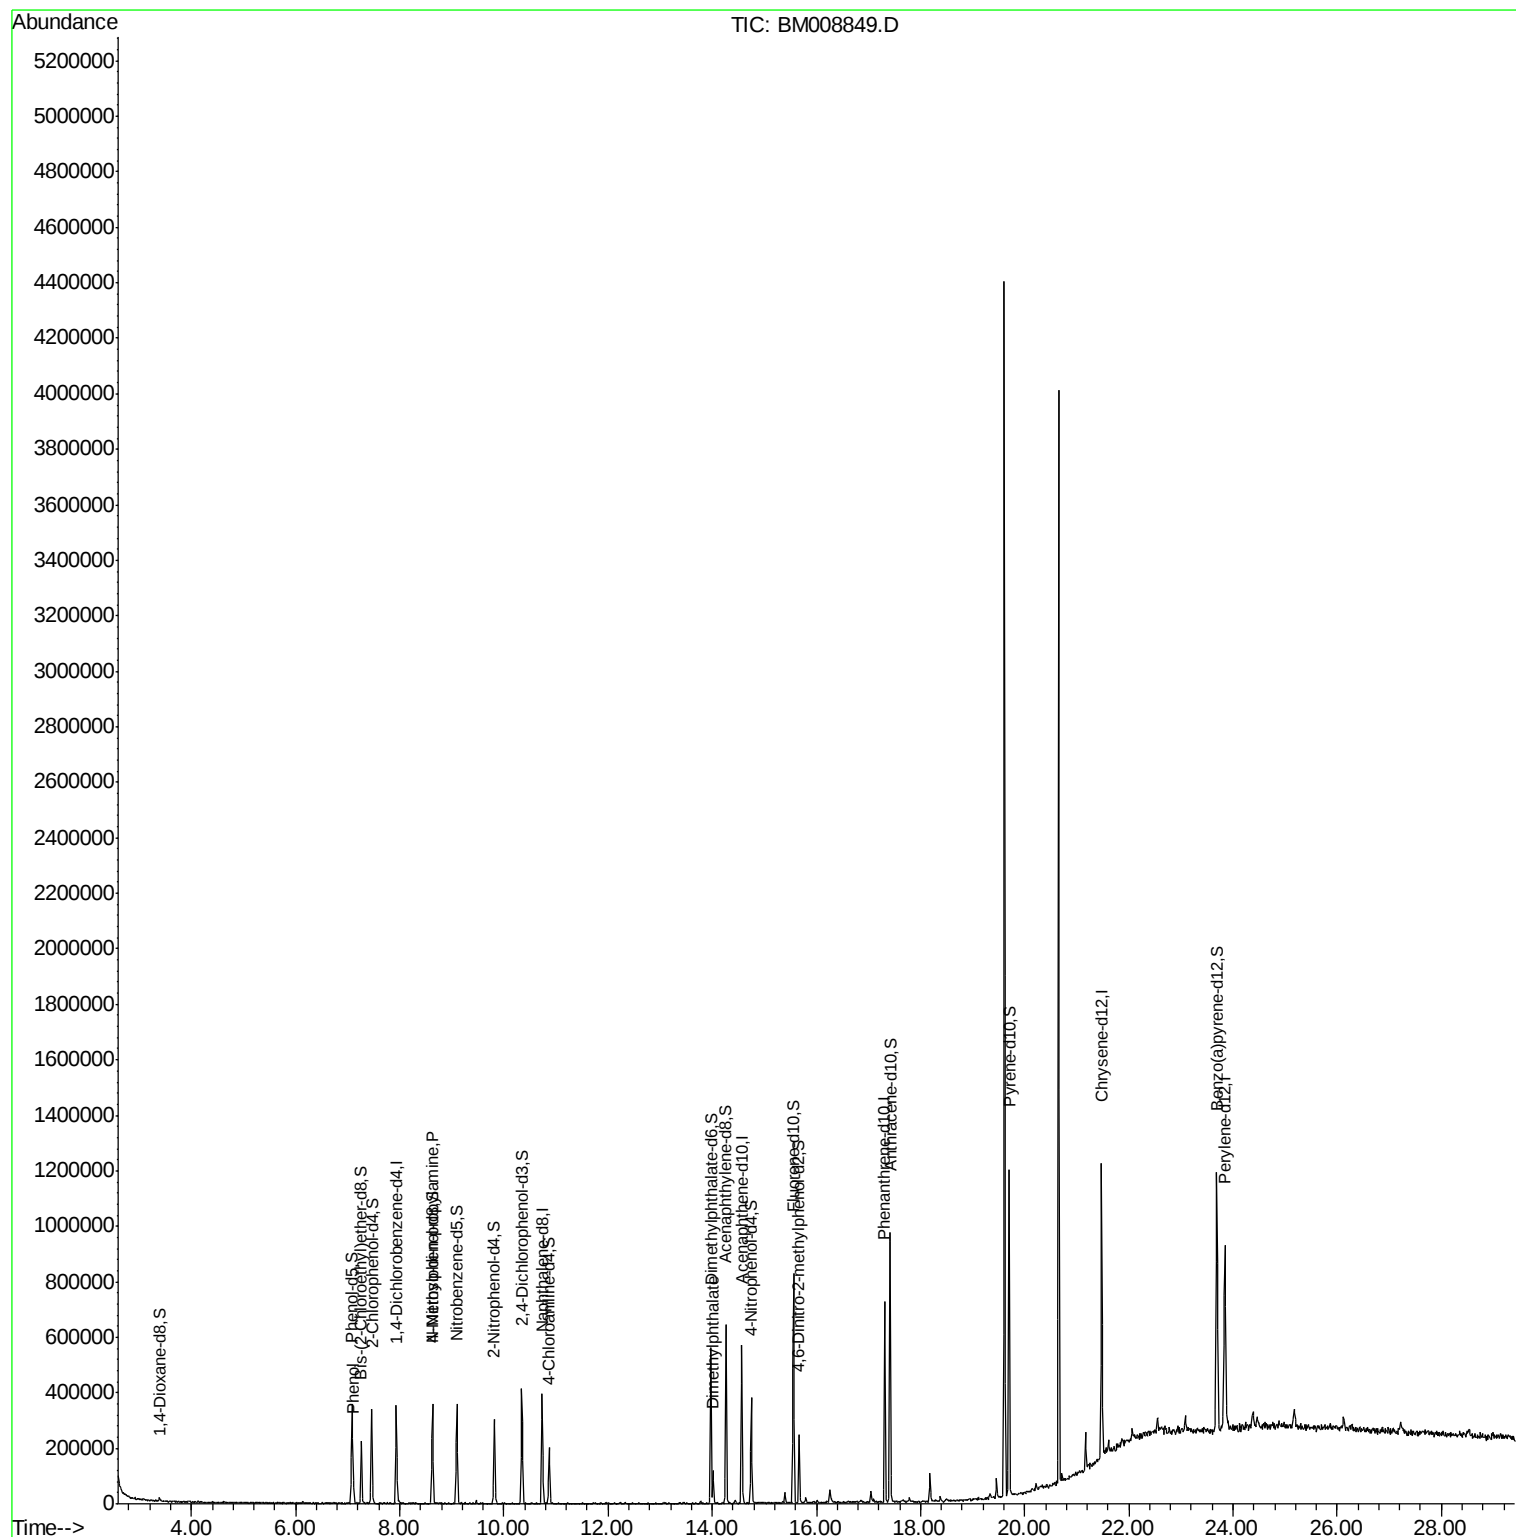

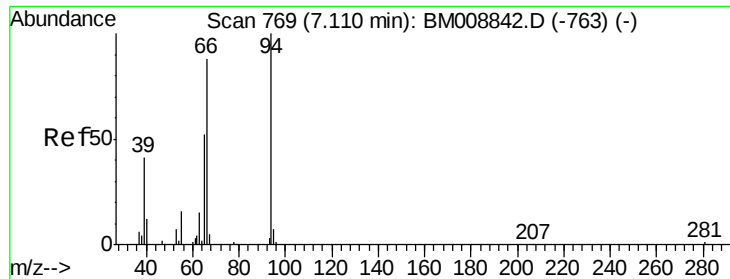

#6

Phenol

Concen: 4.09 ng/ul

RT: 7.11 min Scan# 769

Delta R.T. -0.00 min

Lab File: BM008849.D

Acq: 24 Jan 2017 21:40

Instrument :

BNA_M

ClientSampleId :

BDN11





Tgt Ion: 94 Resp: 21208

Ion Ratio Lower Upper

94 100

65 60.7 23.1 34.7#

66 88.1 33.7 50.5#

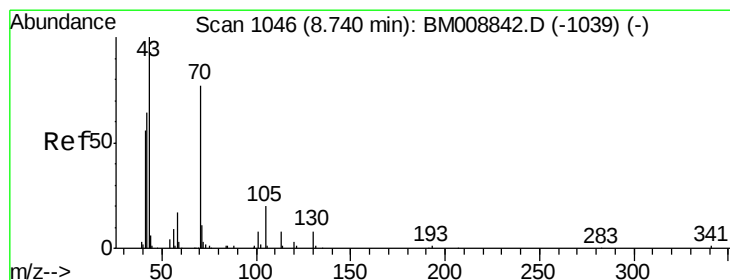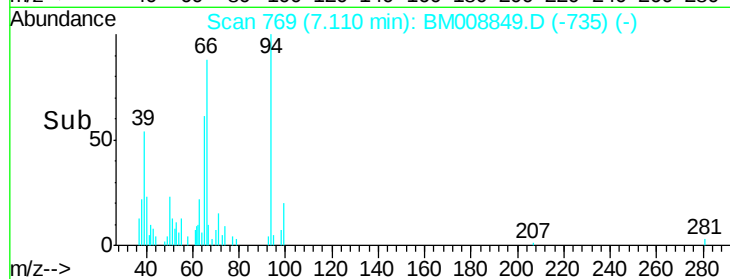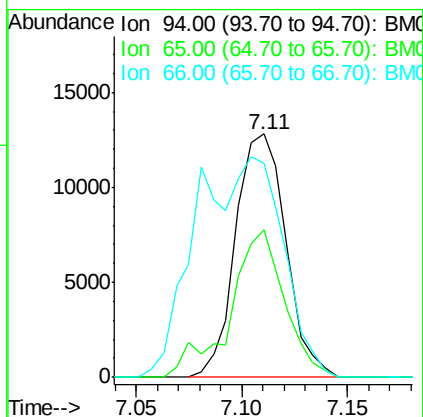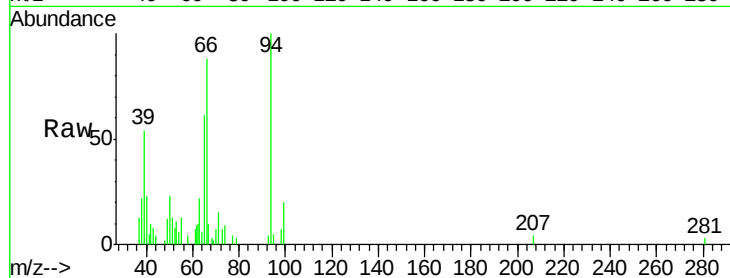

#15

N-Nitroso-di-n-propylamine

Concen: 1.14 ng/ul

RT: 8.62 min Scan# 1026

Delta R.T. -0.12 min

Lab File: BM008849.D

Acq: 24 Jan 2017 21:40

Tgt Ion: 70 Resp: 5053




Ion Ratio Lower Upper


70 100

42 423.6 37.5 56.3#

101 0.0 7.8 11.8#

130 0.0 16.6 25.0#

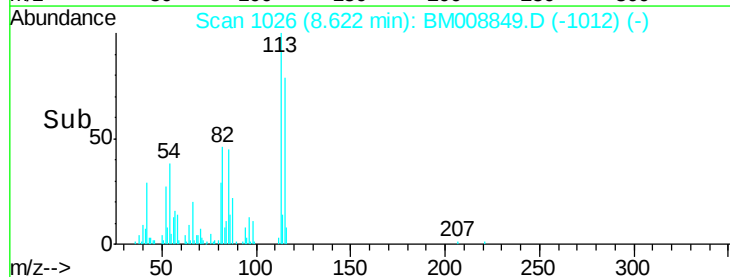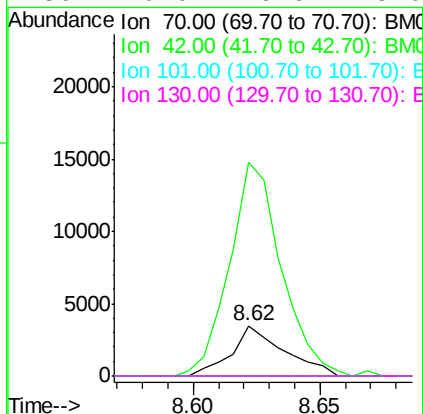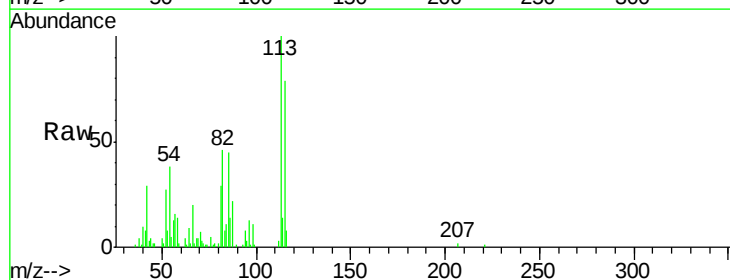

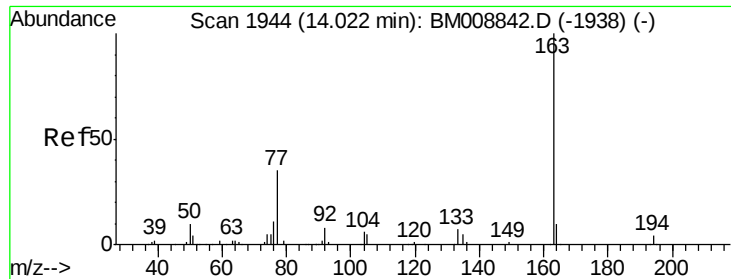

#44
 Dimethylphthalate
 Concen: 4.26 ng/ul
 RT: 14.02 min Scan# 1944
 Delta R.T. -0.00 min
 Lab File: BM008849.D
 Acq: 24 Jan 2017 21:40

Instrument :
 BNA_M
 ClientSampleId :
 BDN11

Tgt Ion:163 Resp: 43659
 Ion Ratio Lower Upper
 163 100
 194 5.7 3.4 5.0#
 164 9.9 8.2 12.4

