

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012418\
 Data File : BM013774.D
 Acq On : 24 Jan 2018 18:50
 Operator : SJ/JU
 Sample : J1223-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 25 00:33:06 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 25 00:32:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	148587	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	602002	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	349114	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	721354	20.00	ng/ul	0.00
75) Chrysene-d12	21.20	240	744599	20.00	ng/ul	0.00
83) Perylene-d12	23.40	264	781982	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	12518	3.33	ng/uL	0.00
5) Phenol-d5	6.78	99	268010	23.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	168278	24.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	231903	24.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	195243	22.27	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	121485	26.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	128691	26.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	233402	24.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	282114	34.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	740224	25.73	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	942345	25.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	98581	21.08	ng/ul	0.00
57) Fluorene-d10	15.25	176	651816	25.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	98942	22.79	ng/ul	0.00
70) Anthracene-d10	17.10	188	976448	27.79	ng/ul	0.00
76) Pyrene-d10	19.40	212	1092921	31.53	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.26	264	1053383	29.31	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	6.81	94	28575	2.498	ng/ul#	83
28) Naphthalene	10.42	128	99777	3.332	ng/ul	97
34) 2-Methylnaphthalene	12.04	142	494079	22.127	ng/ul	95
40) 1,1'-Biphenyl	13.07	154	37583	1.293	ng/ul	96
44) Dimethylphthalate	13.72	163	162143	5.731	ng/ul#	94
49) Acenaphthene	14.32	153	610570	26.260	ng/ul	98
53) Dibenzofuran	14.65	168	712724	20.376	ng/ul	97
58) Fluorene	15.30	166	700998	24.466	ng/ul	98
64) N-Nitrosodiphenylamine	15.52	169	21546	1.016	ng/ul#	81
68) Pentachlorophenol	16.66	266	8901	1.826	ng/ul#	79
69) Phenanthrene	17.05	178	3592784	89.602	ng/ul	99
71) Anthracene	17.14	178	596680	14.427	ng/ul	99
74) Fluoranthene	19.07	202	2468375	51.571	ng/ul#	93
77) Pyrene	19.43	202	1638583	36.199	ng/ul#	94
80) Benzo(a)anthracene	21.19	228	354311	7.875	ng/ul	98
82) Chrysene	21.24	228	300633	7.284	ng/ul	98
85) Benzo(b)fluoranthene	22.74	252	191417	3.986	ng/ul#	89
86) Benzo(k)fluoranthene	22.79	252	63954	1.378	ng/ul#	87
88) Benzo(a)pyrene	23.30	252	94559	2.084	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012418\
Data File : BM013774.D
Acq On : 24 Jan 2018 18:50
Operator : SJ/JU
Sample : J1223-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 25 00:33:06 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 25 00:32:09 2018
Response via : Initial Calibration

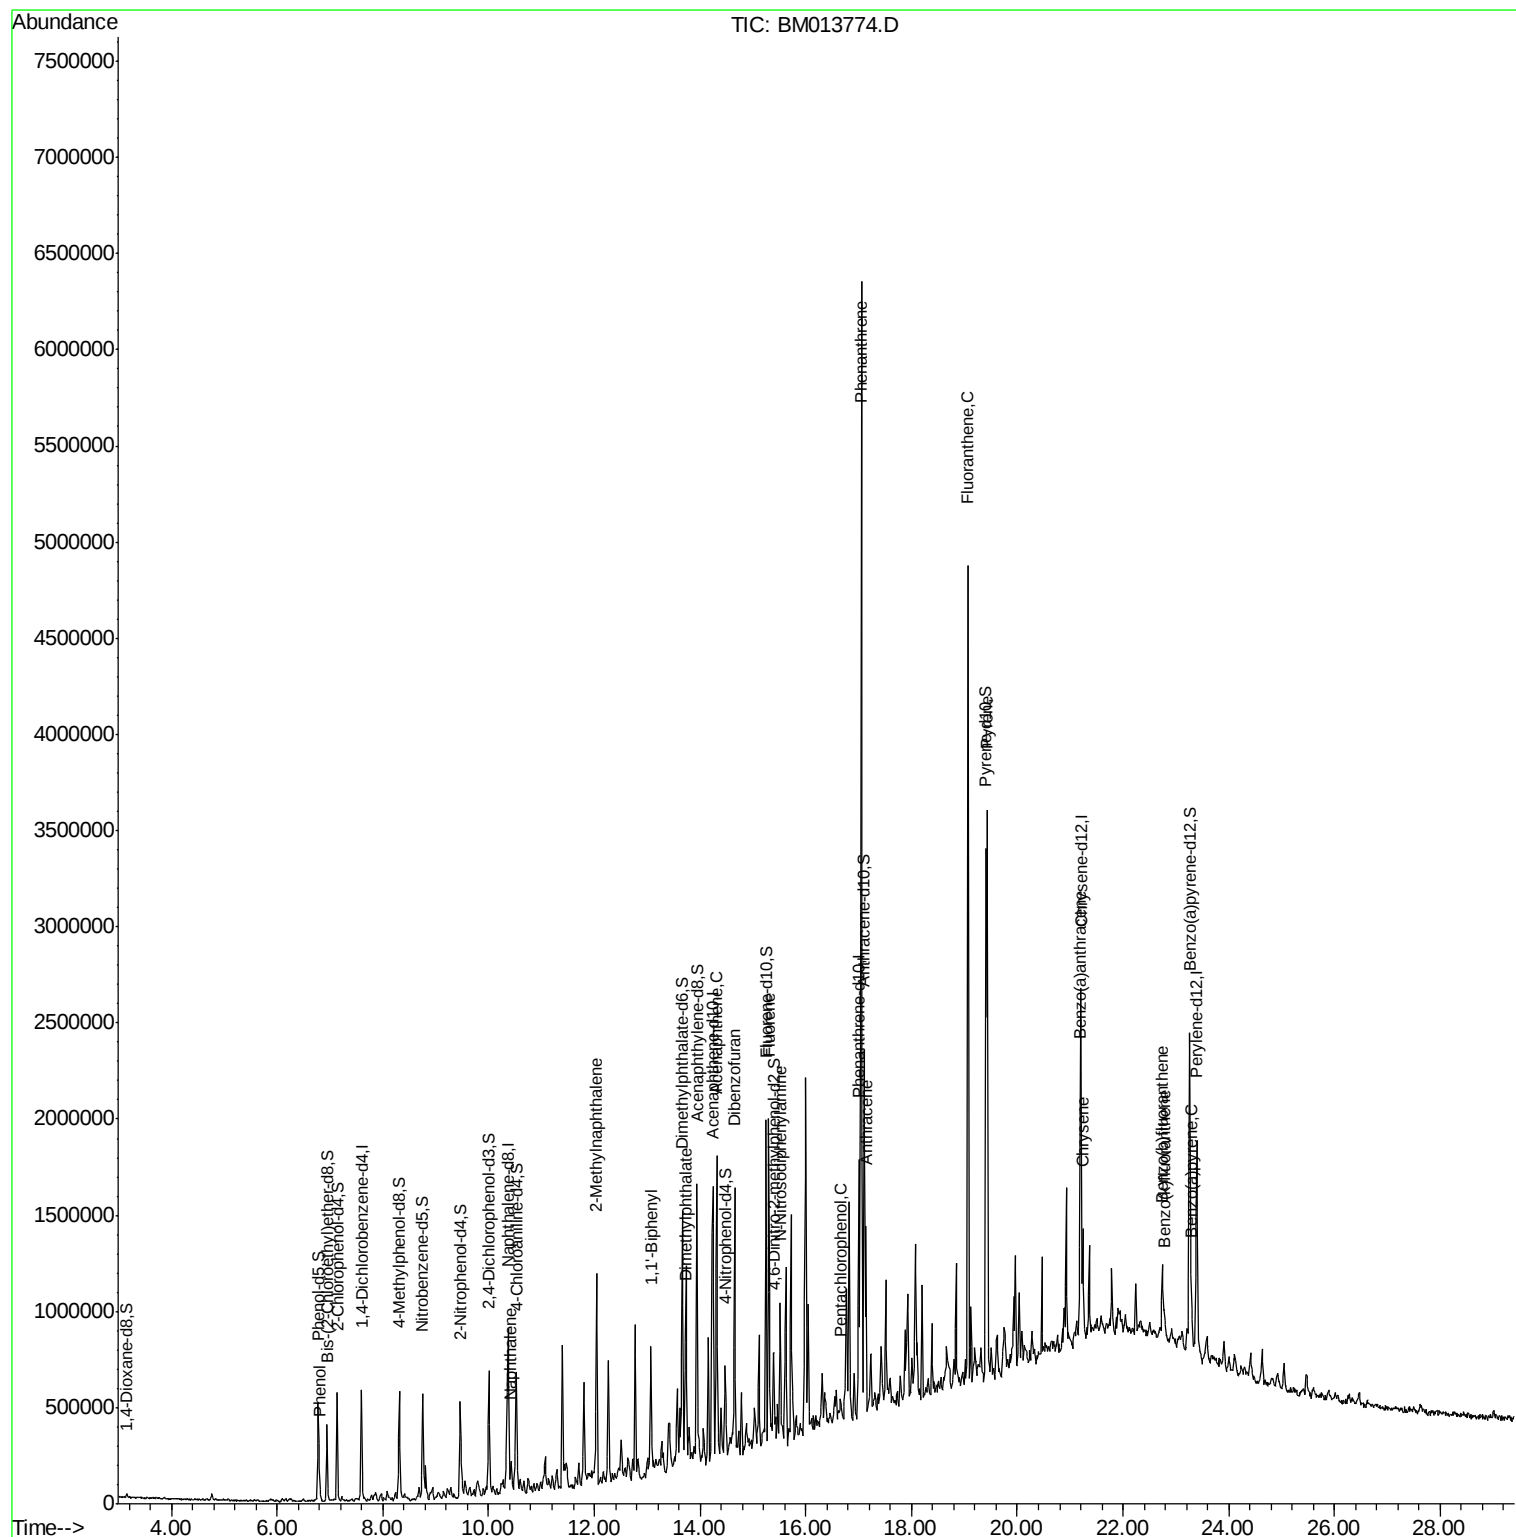

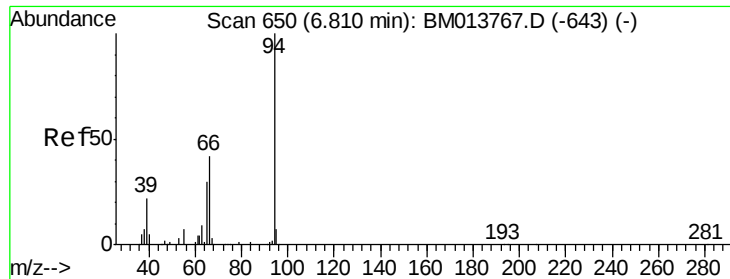

#6

Phenol

Concen: 2.498 ng/ul

RT: 6.81 min Scan# 650

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampled :


Tot Ion: 94 Resp: 28575

Ion Ratio Lower Upper

94 100

65 28.9 28.2 42.4




66 43.2 47.2 70.8#

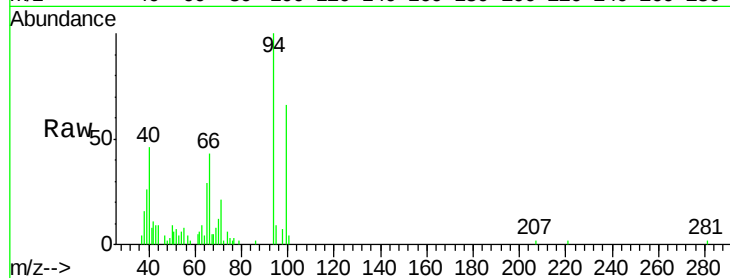

Abundance Ion 94.00 (93.70 to 94.70): BM013767.D (-643) (-)

Ion 65.00 (64.70 to 65.70): BM013767.D (-643) (-)

Ion 66.00 (65.70 to 66.70): BM013767.D (-643) (-)

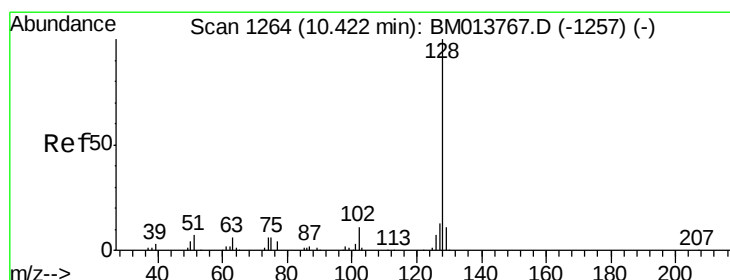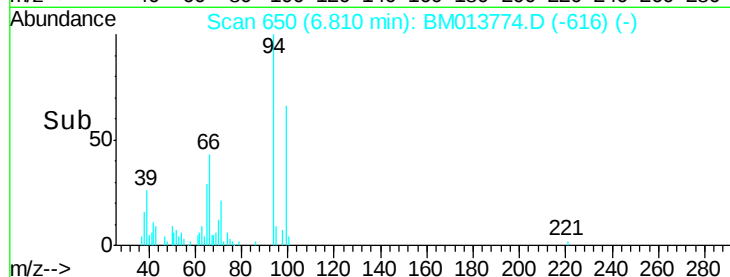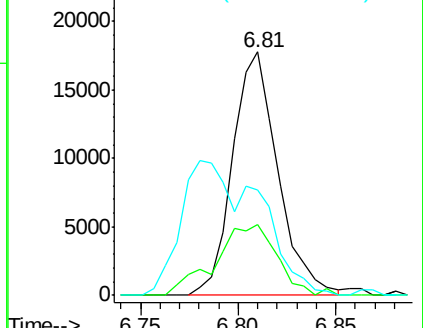

#28

Naphthalene

Concen: 3.332 ng/ul

RT: 10.42 min Scan# 1264

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50


Tgt Ion: 128 Resp: 99777

Ion Ratio Lower Upper

128 100

129 12.7 8.8 13.2



127 12.9 10.6 16.0

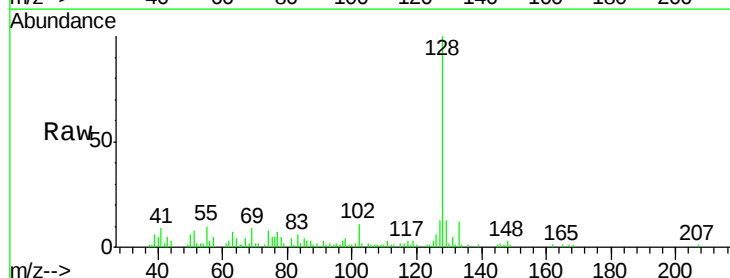


Abundance Ion 128.00 (127.70 to 128.70): BM013767.D (-1257) (-)

Ion 129.00 (128.70 to 129.70): BM013767.D (-1257) (-)

Ion 127.00 (126.70 to 127.70): BM013767.D (-1257) (-)

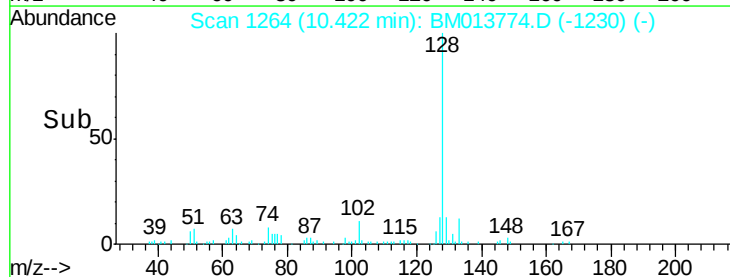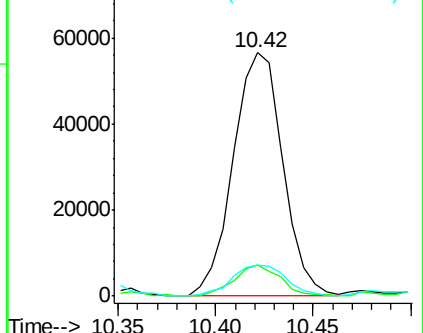

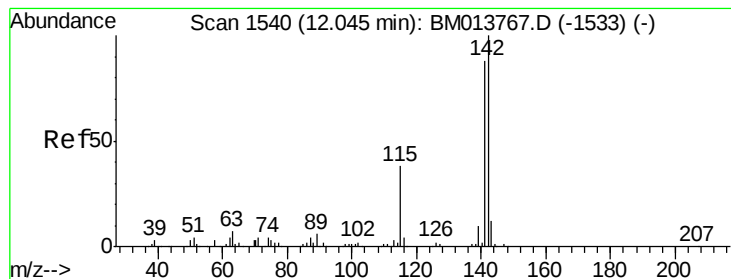

#34

2-Methylnaphthalene

Concen: 22.127 ng/ul

RT: 12.04 min Scan# 1540

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M


ClientSampleId :

Tot Ion:142 Resp: 494079

Ion Ratio Lower Upper

142 100

141 87.4 74.1 111.1



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

12.04

300000



200000

100000

0

Time-->

12.00 12.05 12.10

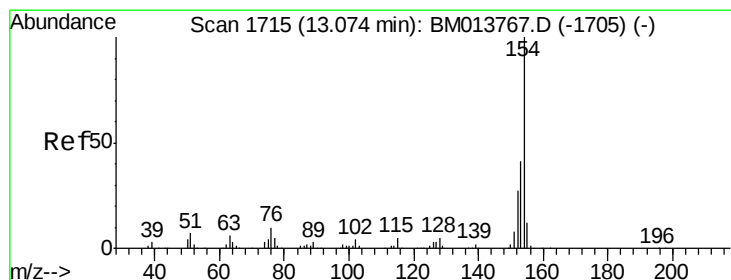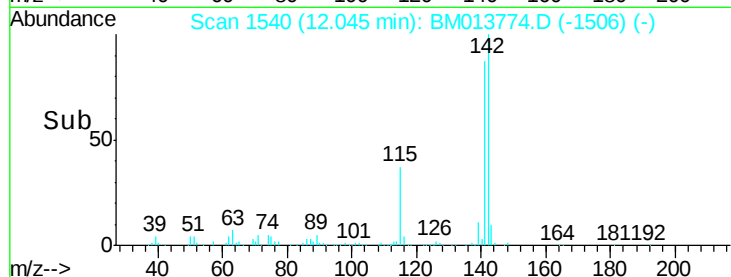

#40

1,1'-Biphenyl

Concen: 1.293 ng/ul

RT: 13.07 min Scan# 1715

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50


Tgt Ion:154 Resp: 37583

Ion Ratio Lower Upper

154 100

153 38.2 32.6 48.8

76 12.4 8.5 12.7



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

13.07

30000


20000


10000

0

Time-->

13.05 13.10

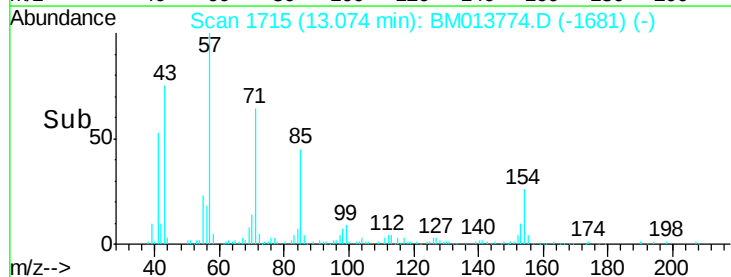

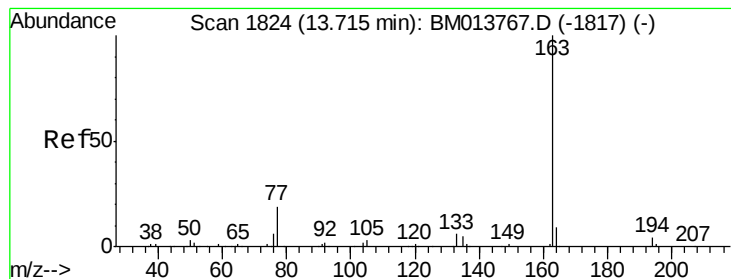

#44

Dimethylphthalate

Concen: 5.731 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 162143

Ion Ratio Lower Upper

163 100

194 5.5 3.5 5.3#




164 13.2 8.2 12.4#



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

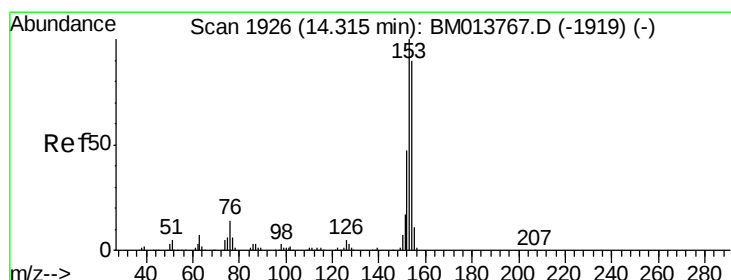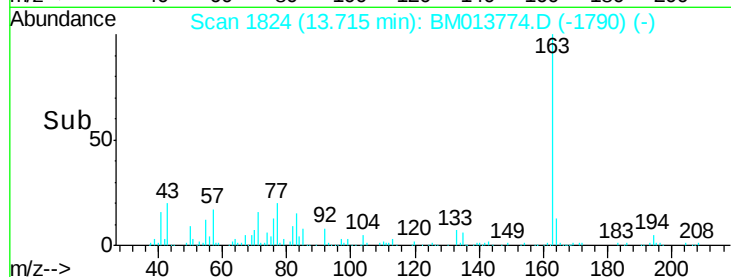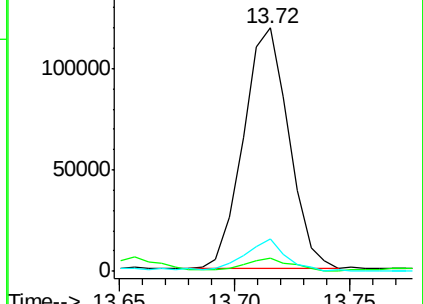

#49

Acenaphthene

Concen: 26.260 ng/ul

RT: 14.32 min Scan# 1926

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50


Tgt Ion:153 Resp: 610570

Ion Ratio Lower Upper

153 100

152 43.7 37.6 56.4



154 87.6 70.4 105.6




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

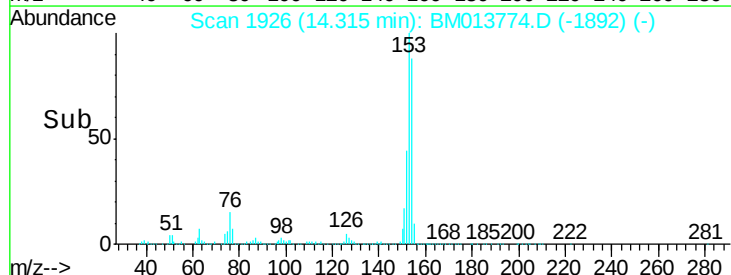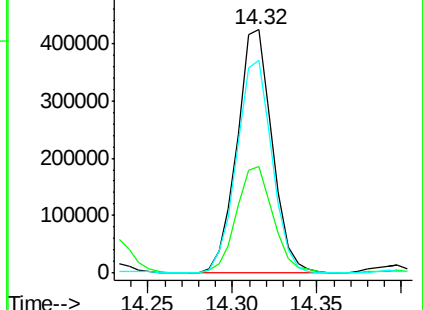

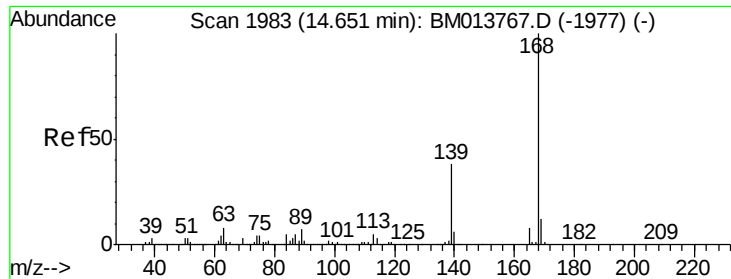

#53

Dibenzenofuran

Concen: 20.376 ng/ul

RT: 14.65 min Scan# 1983

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M


ClientSampleId :

Tot Ion:168 Resp: 712724

Ion Ratio Lower Upper




168 100

139 40.2 30.8 46.2

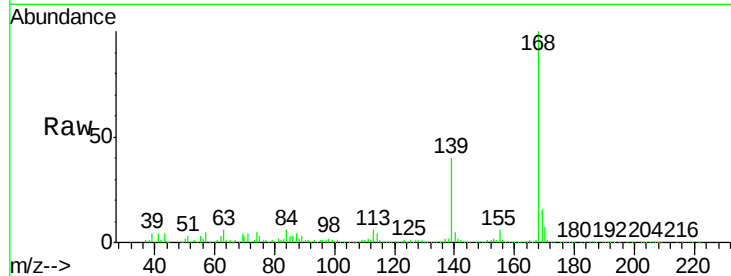

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

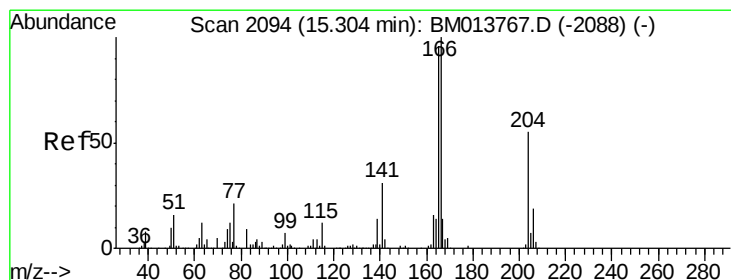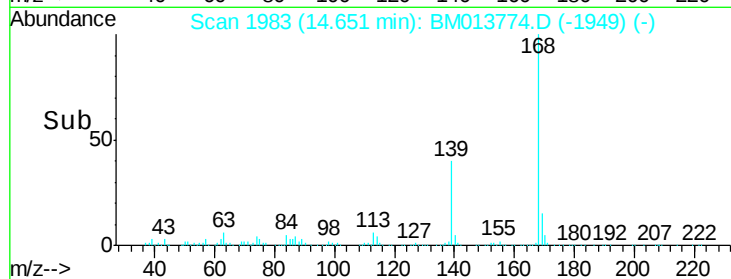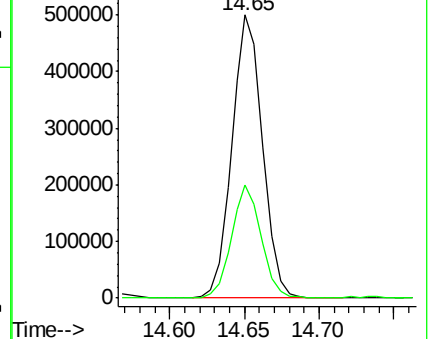

#58

Fluorene

Concen: 24.466 ng/ul

RT: 15.30 min Scan# 2094

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50


Tgt Ion:166 Resp: 700998

Ion Ratio Lower Upper

166 100

165 99.1 77.9 116.9



167 14.9 10.6 16.0




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

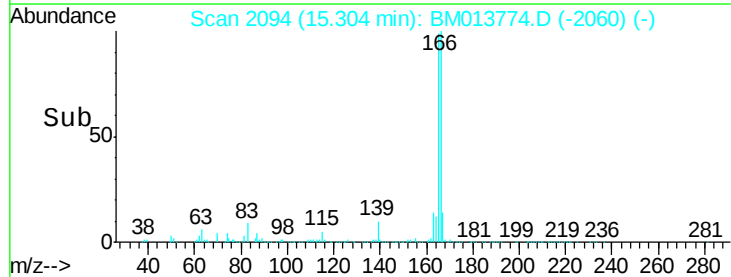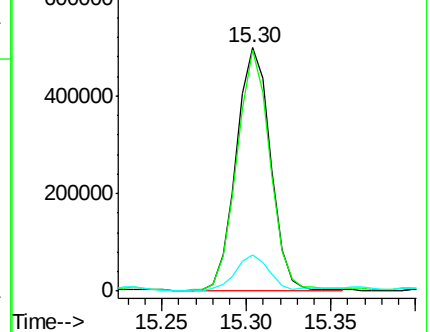

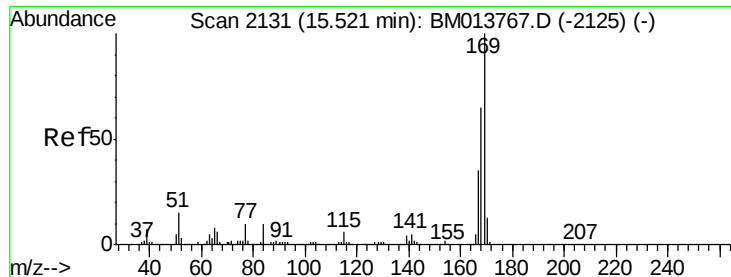

#64

N-Nitrosodiphenylamine

Concen: 1.016 ng/ul

RT: 15.52 min Scan# 2131

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampled :


Tot Ion:169 Resp: 21546

Ion Ratio Lower Upper

169 100

168 52.4 54.0 81.0#




167 24.6 29.1 43.7#

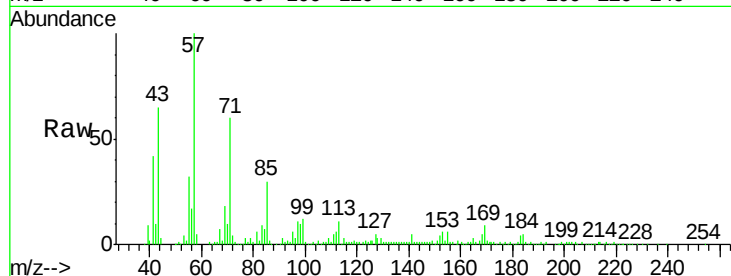

Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

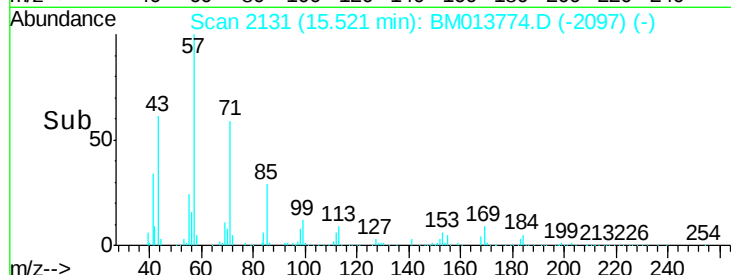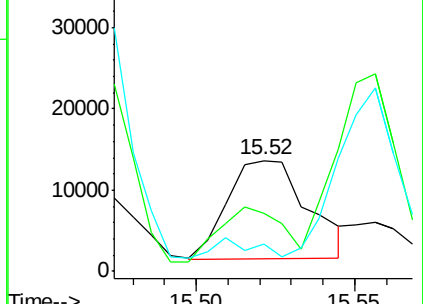

#68

Pentachlorophenol

Concen: 1.826 ng/ul

RT: 16.66 min Scan# 2325

Delta R.T. 0.01 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50


Tgt Ion:266 Resp: 8901

Ion Ratio Lower Upper

266 100

264 83.3 49.3 73.9#



268 54.9 52.6 78.8




Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

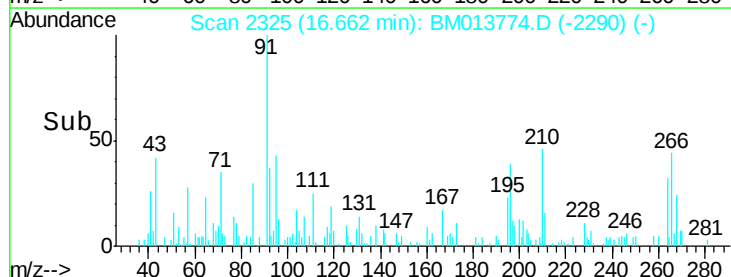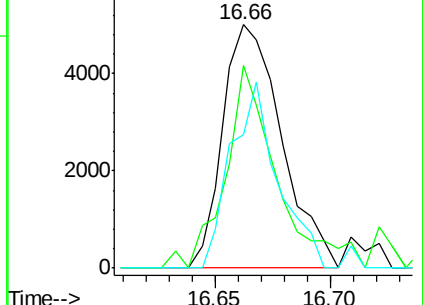

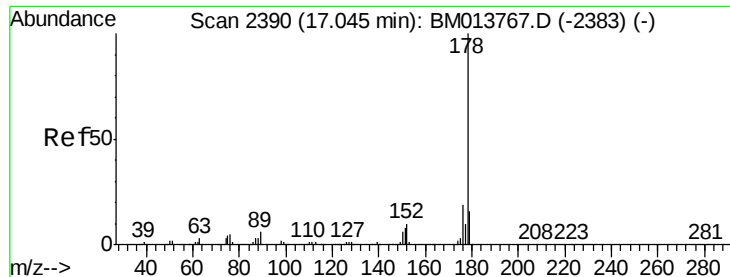

#69

Phenanthrene

Concen: 89.602 ng/ul

RT: 17.05 min Scan# 2391

Delta R.T. 0.01 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 3592784

Ion Ratio Lower Upper

178 100

179 15.4 12.6 19.0




176 18.4 14.9 22.3

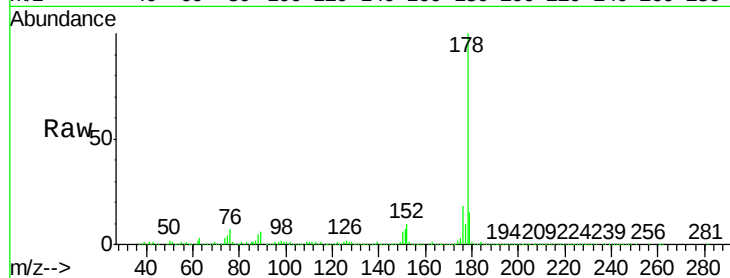

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

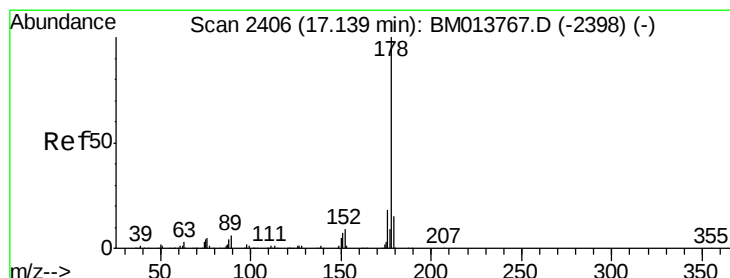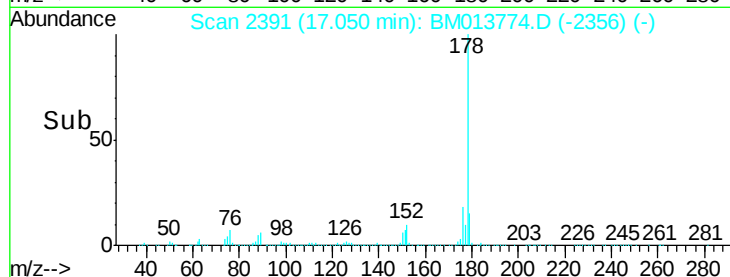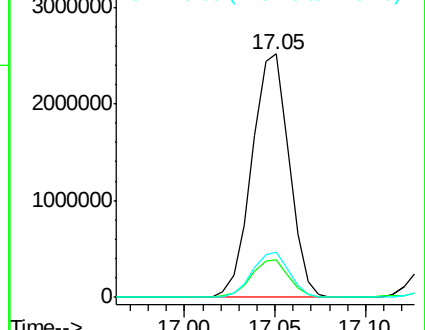

#71

Anthracene

Concen: 14.427 ng/ul

RT: 17.14 min Scan# 2406

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50


Tgt Ion:178 Resp: 596680

Ion Ratio Lower Upper

178 100

179 14.6 11.7 17.5



176 17.4 14.6 21.8

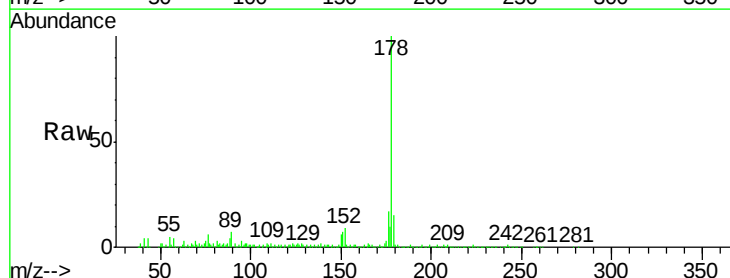


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



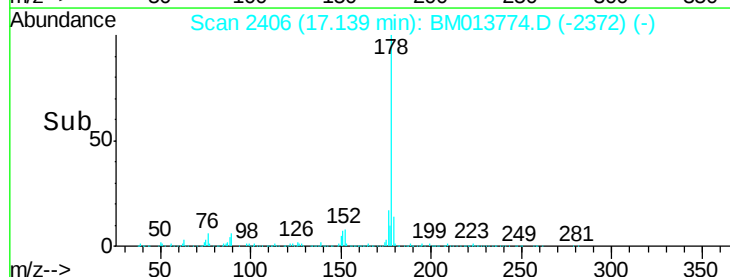
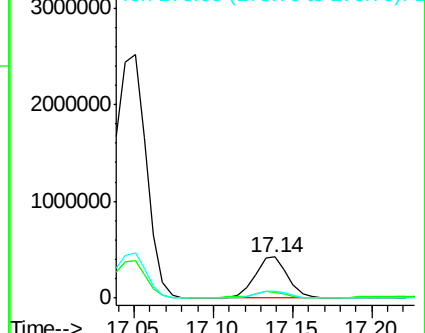


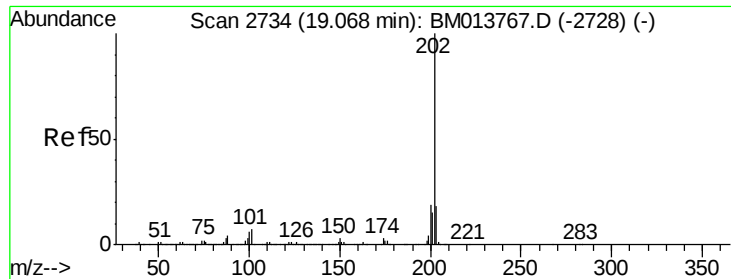

#74
 Fluoranthene
 Concen: 51.571 ng/ul
 RT: 19.07 min Scan# 2734
 Delta R.T. -0.00 min
 Lab File: BM013774.D
 Acq: 24 Jan 2018 18:50




Instrument :
 BNA_M
 ClientSampled :


Tot Ion:202 Resp: 2468375
 Ion Ratio Lower Upper
 202 100
 101 8.3 4.6 7.0#
 100 6.1 3.4 5.2#

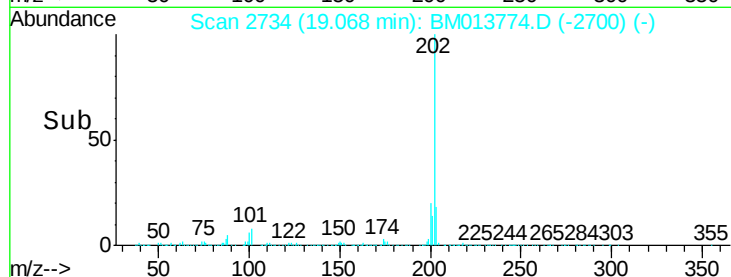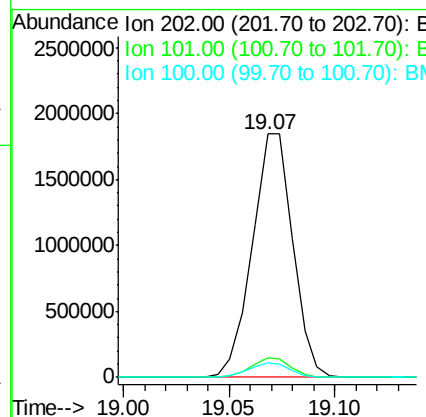

#77
 Pyrene
 Concen: 36.199 ng/ul
 RT: 19.43 min Scan# 2796
 Delta R.T. -0.00 min
 Lab File: BM013774.D
 Acq: 24 Jan 2018 18:50

Tgt Ion:202 Resp: 1638583
 Ion Ratio Lower Upper
 202 100
 101 9.4 5.1 7.7#
 100 7.2 4.9 7.3

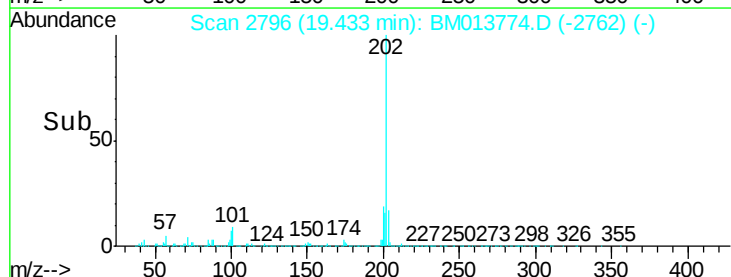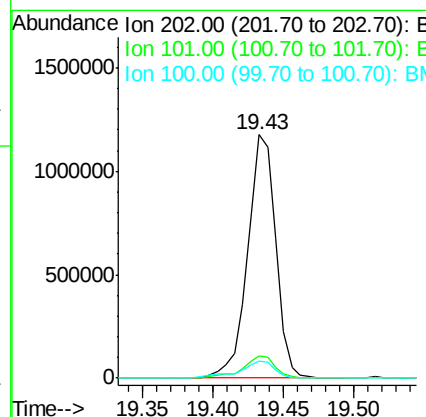

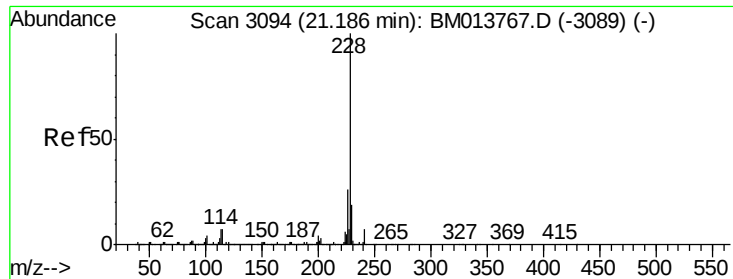

#80

Benzo(a)anthracene

Concen: 7.875 ng/ul

RT: 21.19 min Scan# 3094

Delta R.T. -0.00 min

Lab File: BM013774.D





Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampleId :

Tot	Ion:228	Resp:	354311
Ion	Ratio	Lower	Upper
228	100		
229	21.0	15.4	23.0
226	26.5	21.4	32.0

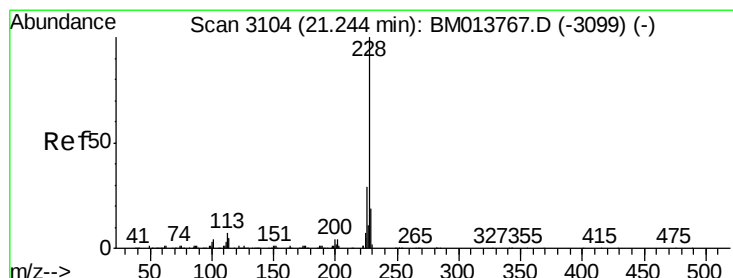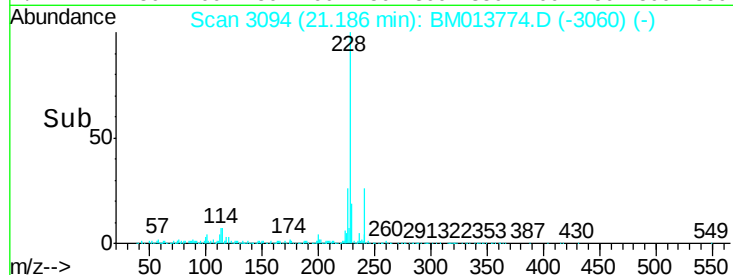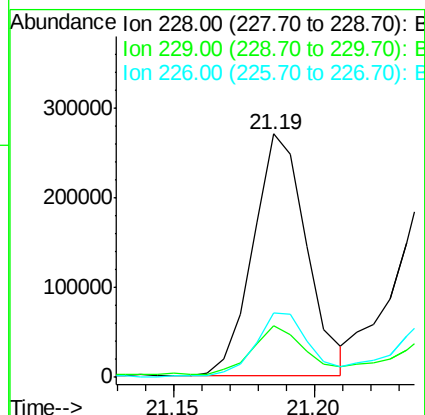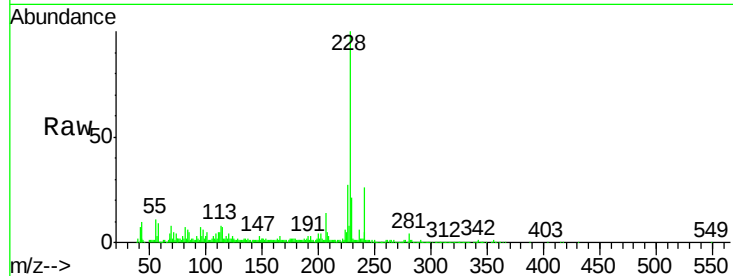

#82

Chrysene

Concen: 7.284 ng/ul




RT: 21.24 min Scan# 3103


Delta R.T. -0.01 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Tgt	Ion:228	Resp:	300633
Ion	Ratio	Lower	Upper
228	100		
226	28.2	23.4	35.2
229	20.5	15.5	23.3

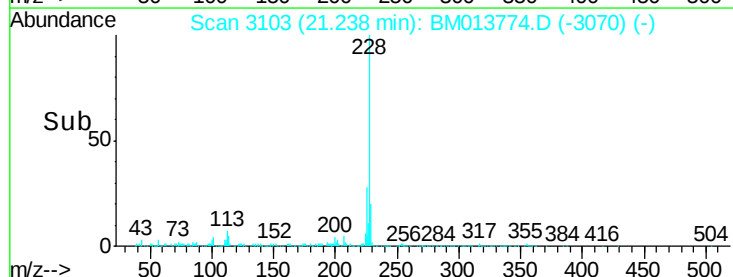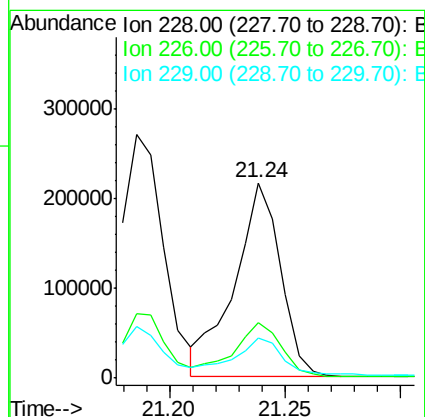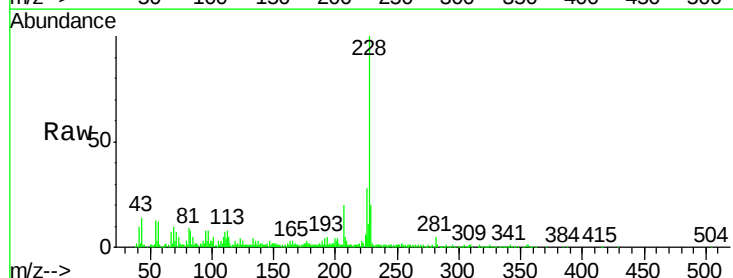

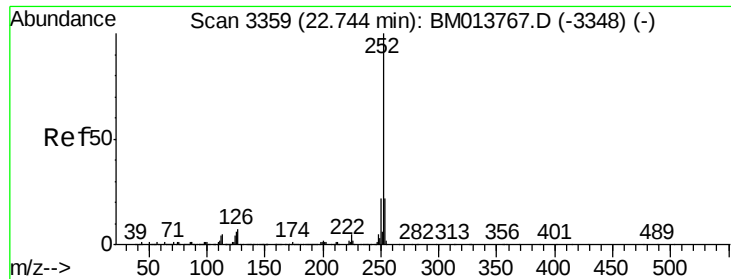

#85

Benzo(b)fluoranthene

Concen: 3.986 ng/ul

RT: 22.74 min Scan# 3359

Delta R.T. -0.00 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampled :





Tot Ion:252 Resp: 191417

Ion Ratio Lower Upper

252 100

253 26.7 17.9 26.9

125 11.9 3.6 5.4#

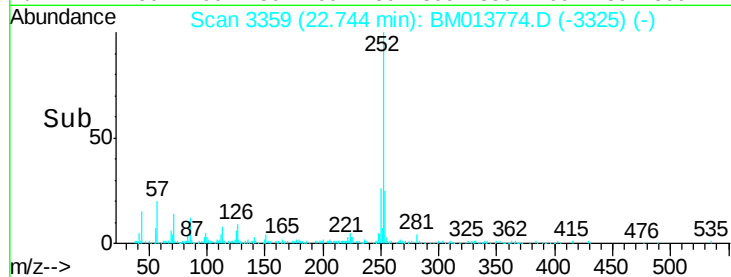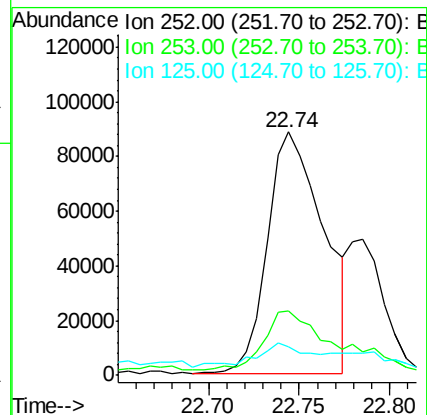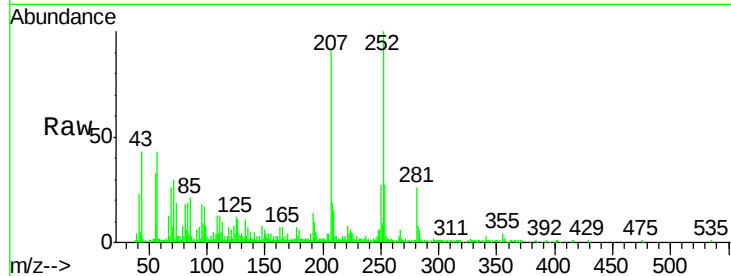

#86

Benzo(k)fluoranthene

Concen: 1.378 ng/ul

RT: 22.79 min Scan# 3366

Delta R.T. -0.01 min

Lab File: BM013774.D

Acq: 24 Jan 2018 18:50




Tgt Ion:252 Resp: 63954


Ion Ratio Lower Upper

252 100

253 17.4 17.1 25.7

125 16.2 3.4 5.2#

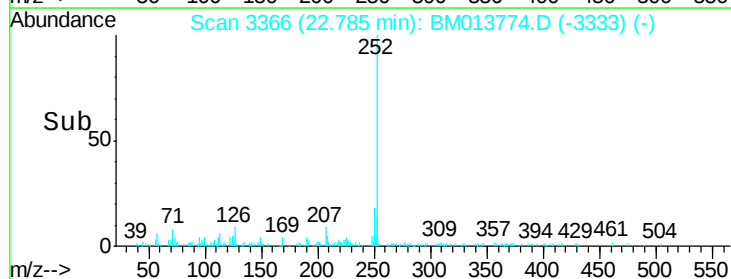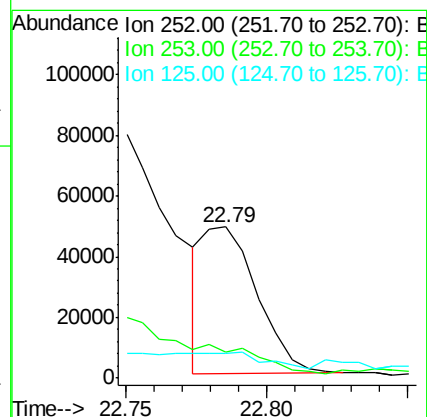

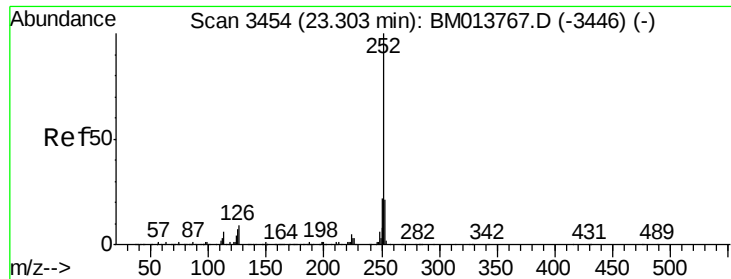

#88

Benzo(a)pyrene

Concen: 2.084 ng/ul

RT: 23.30 min Scan# 3454

Delta R.T. -0.00 min

Lab File: BM013774.D


Acq: 24 Jan 2018 18:50

Instrument :

BNA_M

ClientSampleId :

Tot Ion:	252	Resp:	94559
Ion	Ratio	Lower	Upper
252	100		
253	22.9	18.2	27.2
125	14.6	4.0	6.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

