

Data Path : U:\HPCHEM1\BNA M\DATA\BM012418\
 Data File : BM013785.D
 Acq On : 25 Jan 2018 01:25
 Operator : SJ/JU
 Sample : J1222-09DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6A82DL

Manual Integrations
 APPROVED

Sohil
 1/25/2018 5:35:40 PM

Quant Time: Jan 25 04:14:31 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 25 03:36:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	133071	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	513212	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	297186	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	689773	20.00	ng/ul	0.00
75) Chrysene-d12	21.20	240	762078	20.00	ng/ul	0.00
83) Perylene-d12	23.39	264	774232	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	1500m	0.45	ng/uL	0.00
5) Phenol-d5	6.79	99	26257	2.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	17219	2.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	25353	3.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	20562	2.62	ng/ul	0.01
19) Nitrobenzene-d5	8.75	128	12470	3.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	12171	2.89	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.02	165	21883	2.69	ng/ul	0.01
29) 4-Chloroaniline-d4	10.54	131	12662	1.80	ng/ul	0.02
43) Dimethylphthalate-d6	13.66	166	82535	3.37	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	99550	3.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	5225m	1.31	ng/ul	0.02
57) Fluorene-d10	15.24	176	74366	3.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	7937	1.91	ng/ul	0.00
70) Anthracene-d10	17.10	188	114387	3.40	ng/ul	0.00
76) Pyrene-d10	19.40	212	133657	3.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.26	264	128339	3.61	ng/ul	0.00

Target Compounds

					Ovalue
28) Naphthalene	10.42	128	48597	1.903 ng/ul	97
34) 2-Methylnaphthalene	12.04	142	148568	7.805 ng/ul	94
55) 2,3,4,6-Tetrachlorophenol	14.89	232	16810	2.695 ng/ul#	96
68) Pentachlorophenol	16.66	266	233492	50.105 ng/ul	98
69) Phenanthrene	17.04	178	88536	2.309 ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : U:\HPCHEM1\BNA M\DATA\BM012418\
Data File : BM013785.D
Acq On : 25 Jan 2018 01:25
Operator : SJ/JU
Sample : J1222-09DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6A82DL

Manual Integrations
APPROVED

Sohil
1/25/2018 5:35:40 PM

Quant Time: Jan 25 04:14:31 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 25 03:36:03 2018
Response via : Initial Calibration

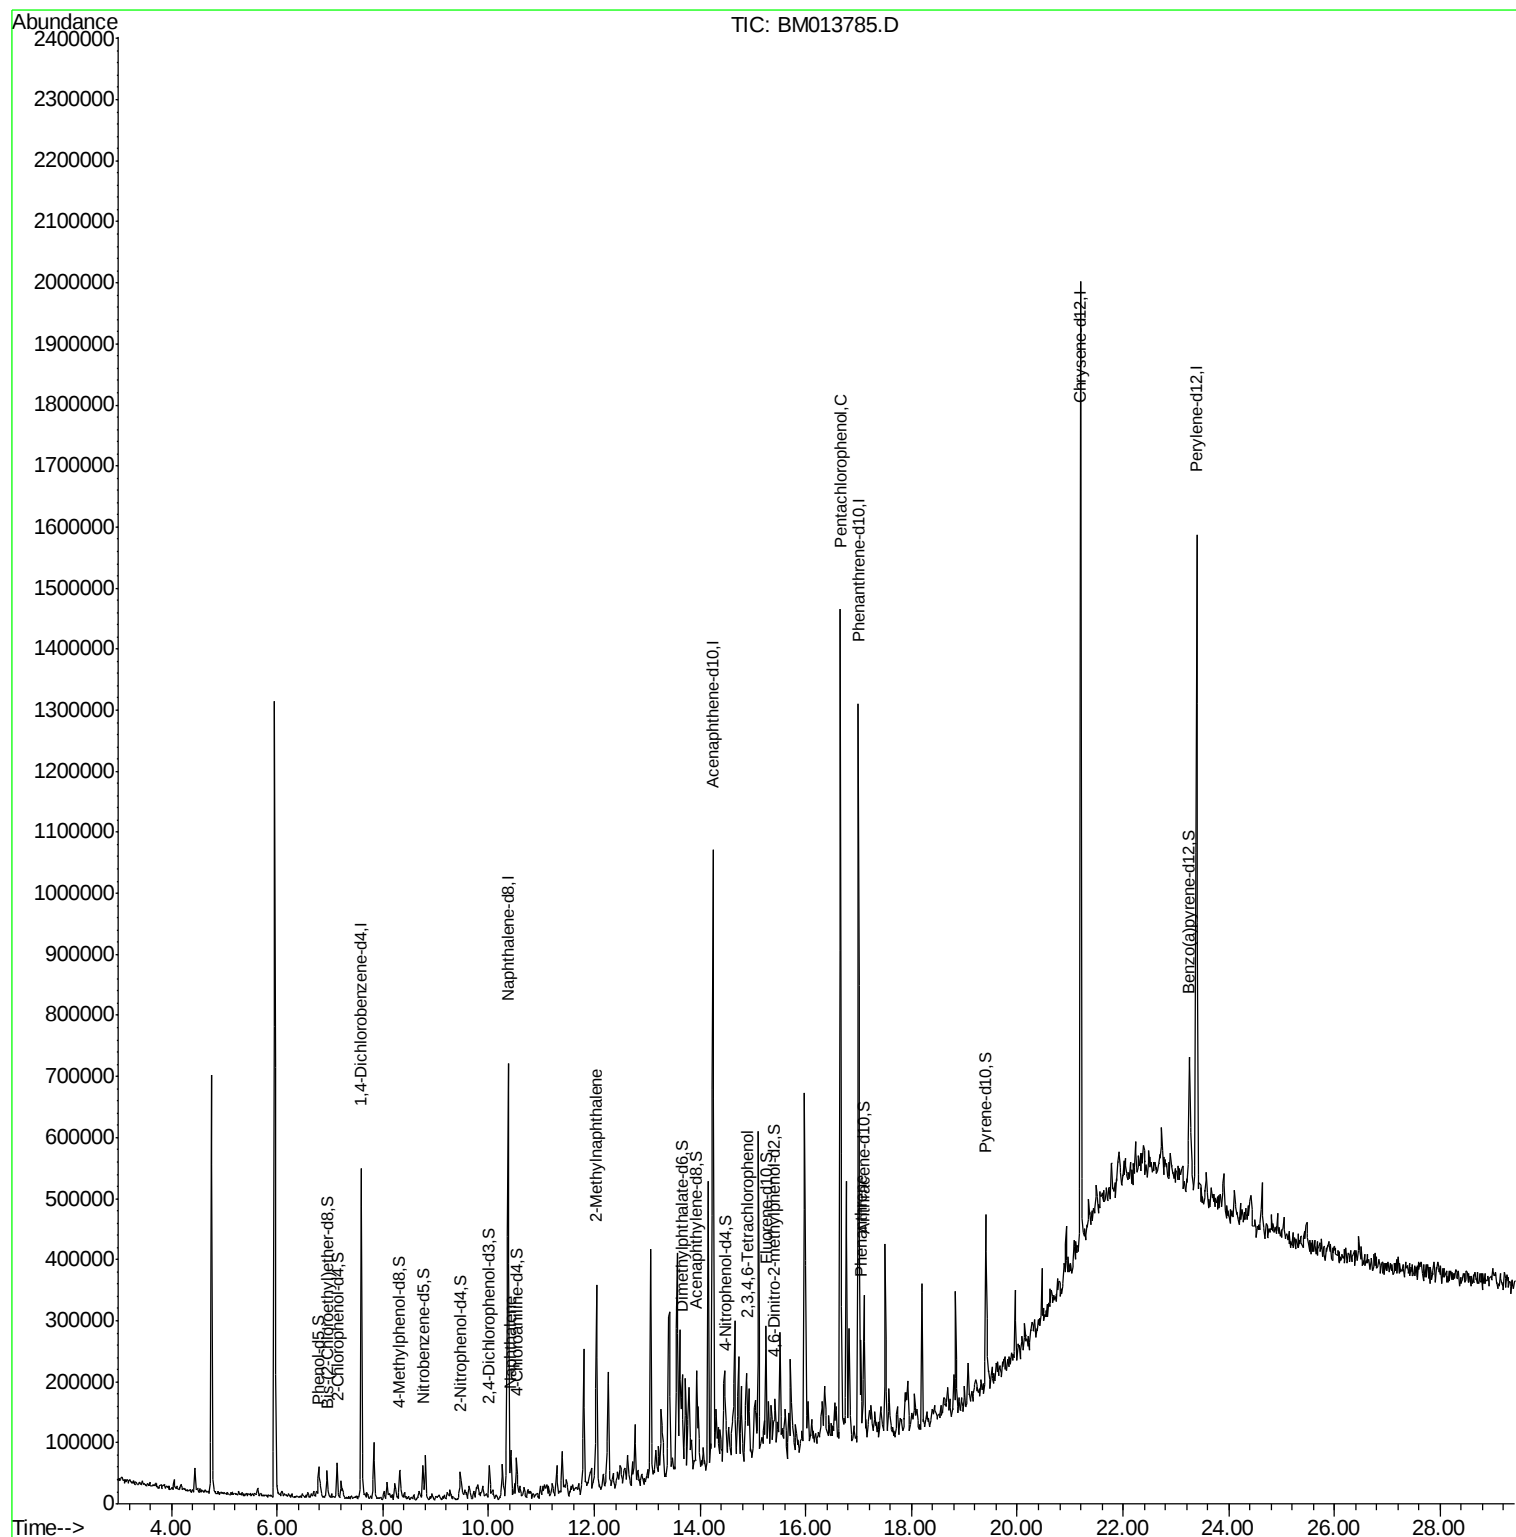

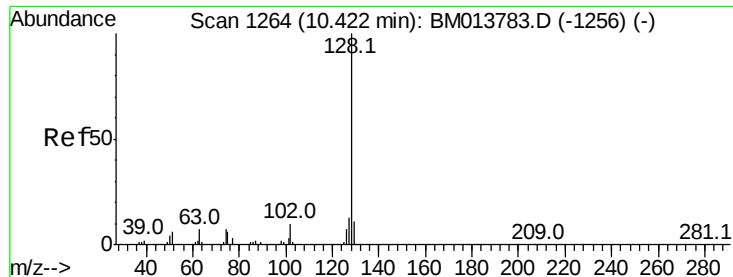





#28
Naphthalene
Concen: 1.903 ng/ul
RT: 10.42 min Scan# 1264
Delta R.T. 0.00 min
Lab File: BM013785.D
Acq: 25 Jan 2018 01:25

Instrument :
BNA_M
ClientSampleId :
F6A82DL

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.5	8.8	13.2
127	14.8	10.6	16.0




Manual Integrations
APPROVED


Sohil
1/25/2018 5:35:40 PM

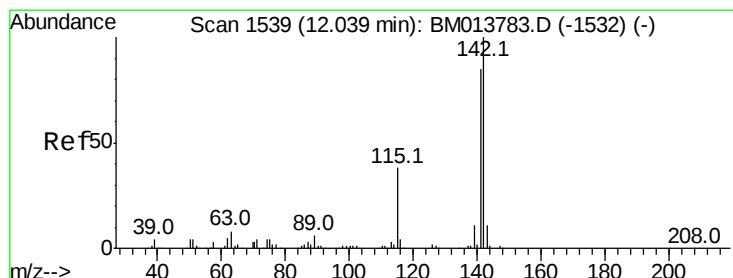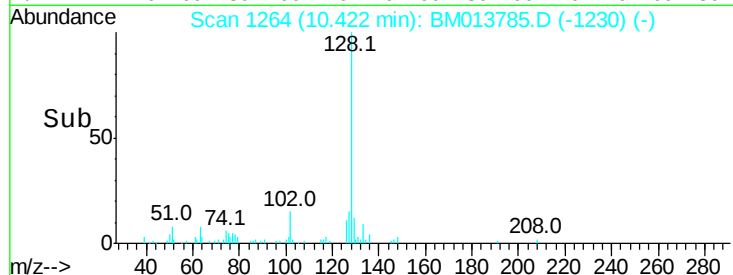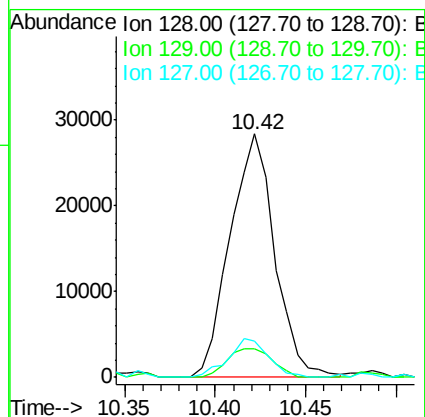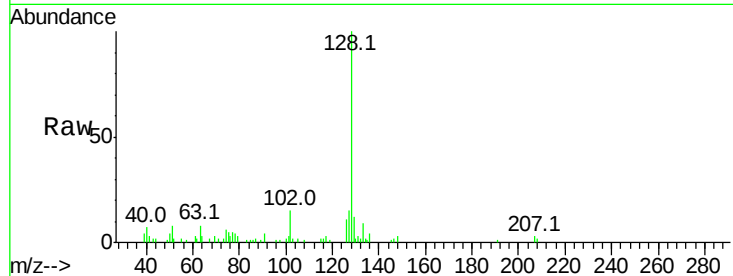

#34
2-Methylnaphthalene
Concen: 7.805 ng/ul
RT: 12.04 min Scan# 1539
Delta R.T. 0.00 min
Lab File: BM013785.D
Acq: 25 Jan 2018 01:25

Tgt Ion	Ratio	Lower	Upper
142	100		
141	87.1	74.1	111.1

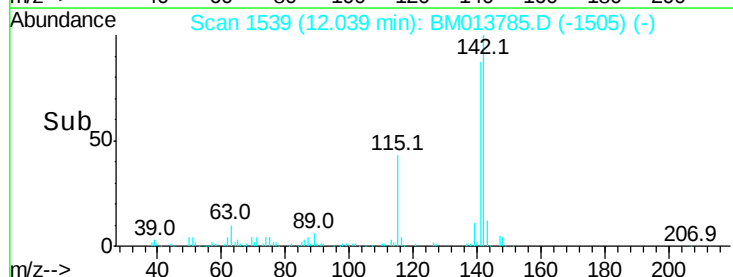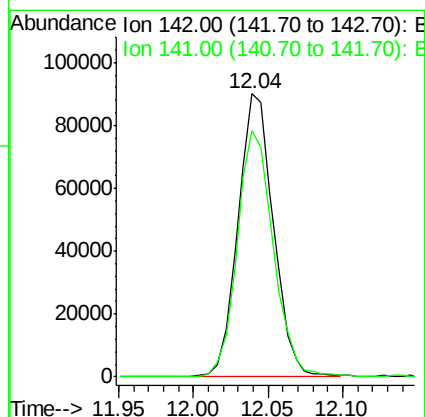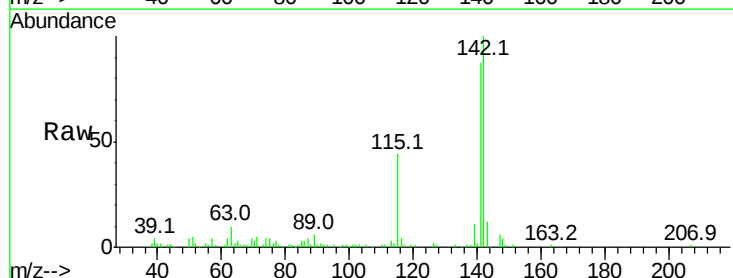

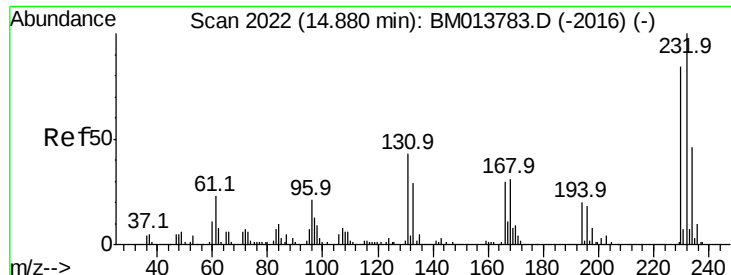

#55

2,3,4,6-Tetrachlorophenol

Concen: 2.695 ng/ul

RT: 14.89 min Scan# 2024

Delta R.T. 0.01 min

Lab File: BM013785.D

Acq: 25 Jan 2018 01:25

Instrument :

BNA_M

ClientSampleId :

F6A82DL

Tot Ion:232 Resp: 16810

Ion Ratio Lower Upper

232 100

131 33.7 29.0 43.4


130 0.0 2.0 3.0#

166 28.5 21.4 32.2

Manual Integrations
APPROVED

Sohil

1/25/2018 5:35:40 PM



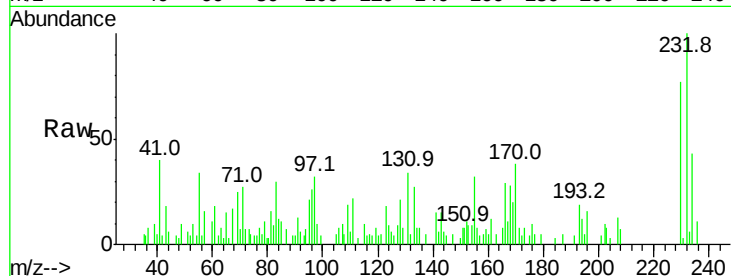


Abundance Ion 232.00 (231.70 to 232.70): E

Ion 131.00 (130.70 to 131.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 166.00 (165.70 to 166.70): E

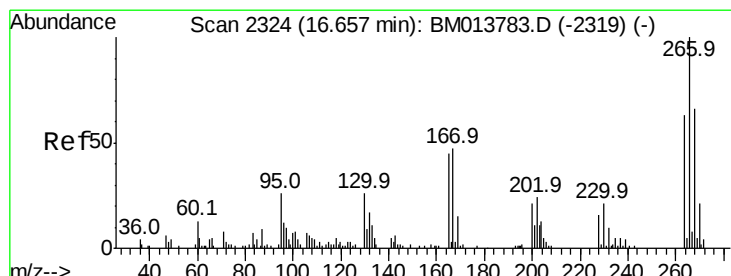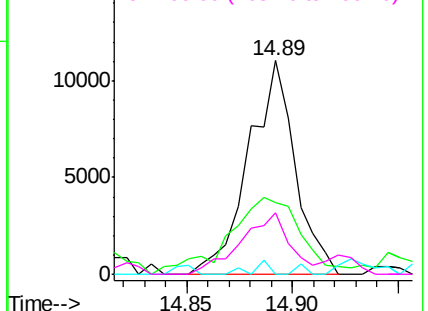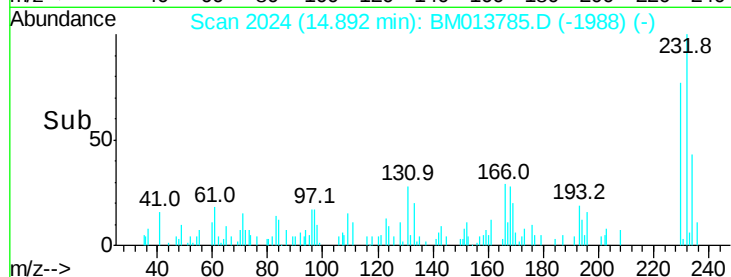

#68

Pentachlorophenol

Concen: 50.105 ng/ul

RT: 16.66 min Scan# 2324

Delta R.T. 0.00 min

Lab File: BM013785.D

Acq: 25 Jan 2018 01:25


Tgt Ion:266 Resp: 233492

Ion Ratio Lower Upper

266 100

264 61.8 49.3 73.9



268 62.8 52.6 78.8

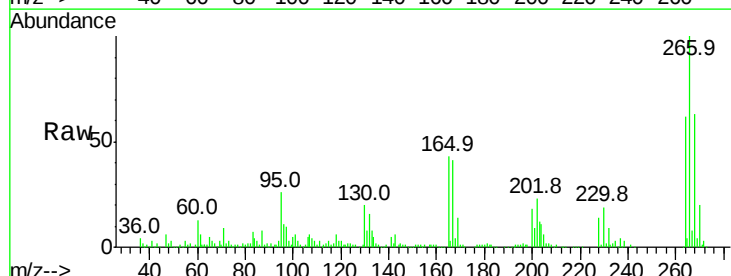


Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

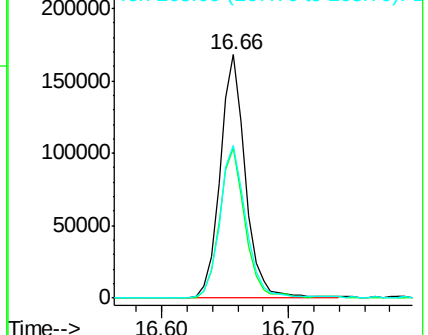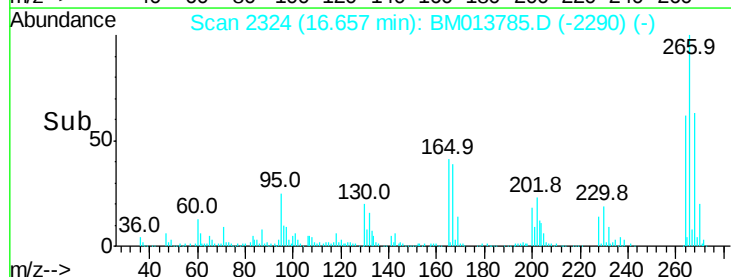

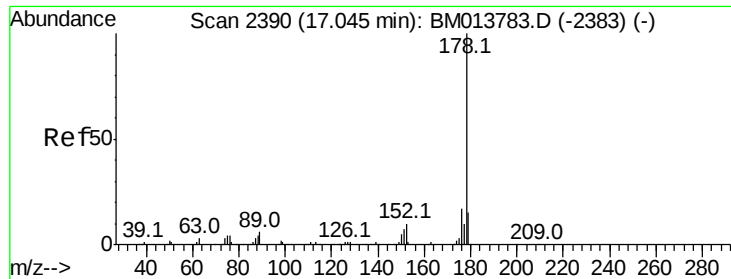

#69

Phenanthrene

Concen: 2.309 ng/ul

RT: 17.04 min Scan# 2390

Delta R.T. 0.00 min

Lab File: BM013785.D

Acq: 25 Jan 2018 01:25

Instrument :

BNA_M

ClientSampleId :

F6A82DL

Tot Ion:178 Resp: 88536

Ion Ratio Lower Upper

178 100

179 16.7 12.6 19.0

176 20.7 14.9 22.3

Manual Integrations

APPROVED

Sohil

1/25/2018 5:35:40 PM

