
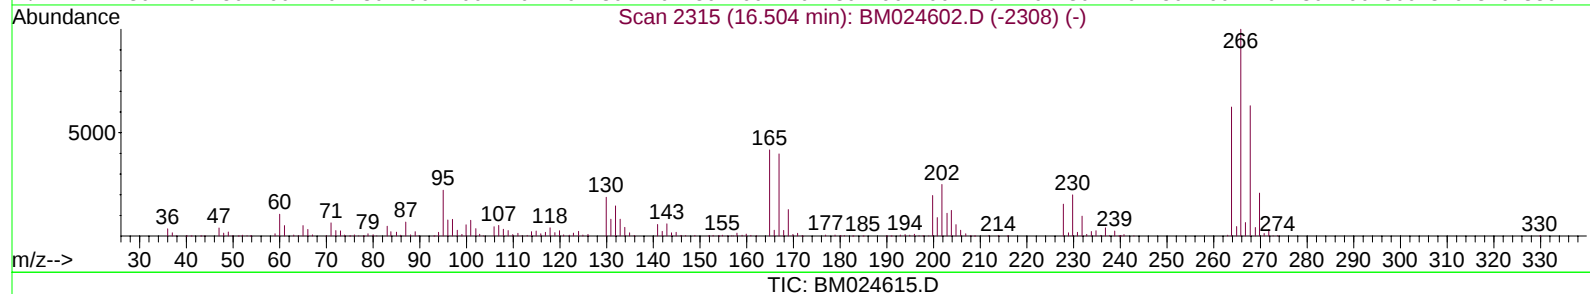
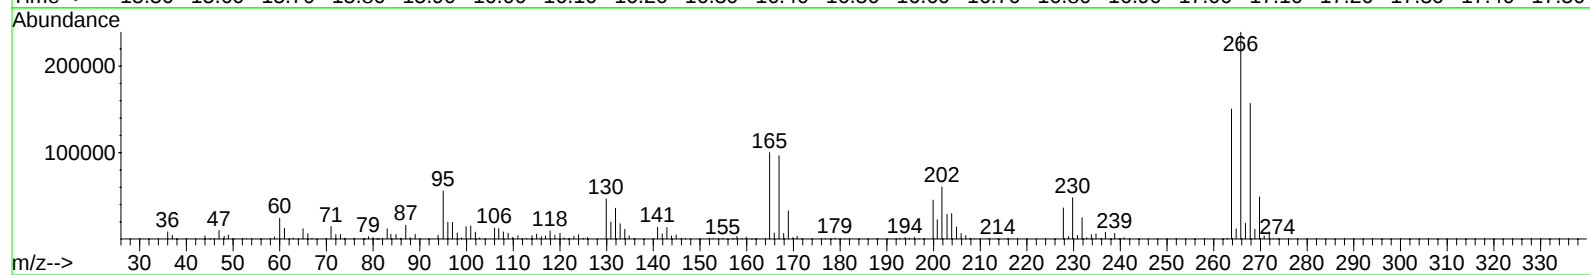


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012420\
Data File : BM024615.D
Acq On : 24 Jan 2020 10:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 17:41:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 23 14:57:07 2020
Response via : Initial Calibration

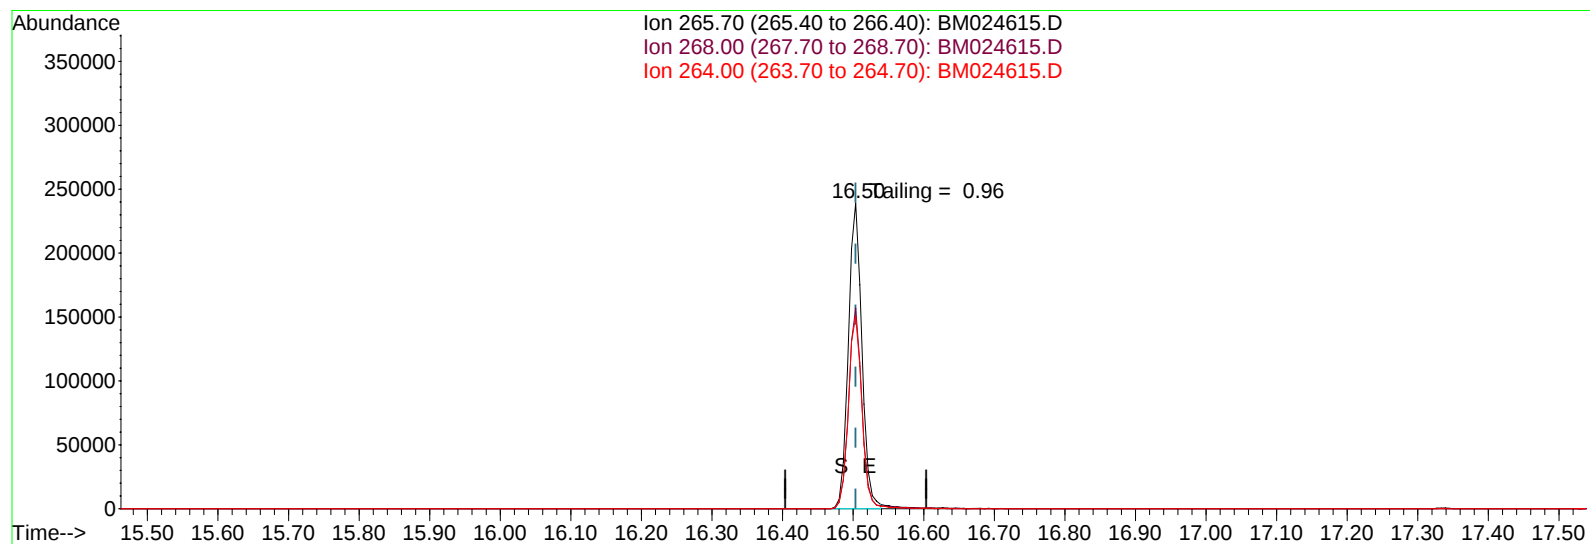

(70) Pentachlorophenol (C)




16.504min (-0.000) 321828.62ng

response 318916

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	65.60
264.00	62.40	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012420\
Data File : BM024615.D
Acq On : 24 Jan 2020 10:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 17:41:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 23 14:57:07 2020
Response via : Initial Calibration

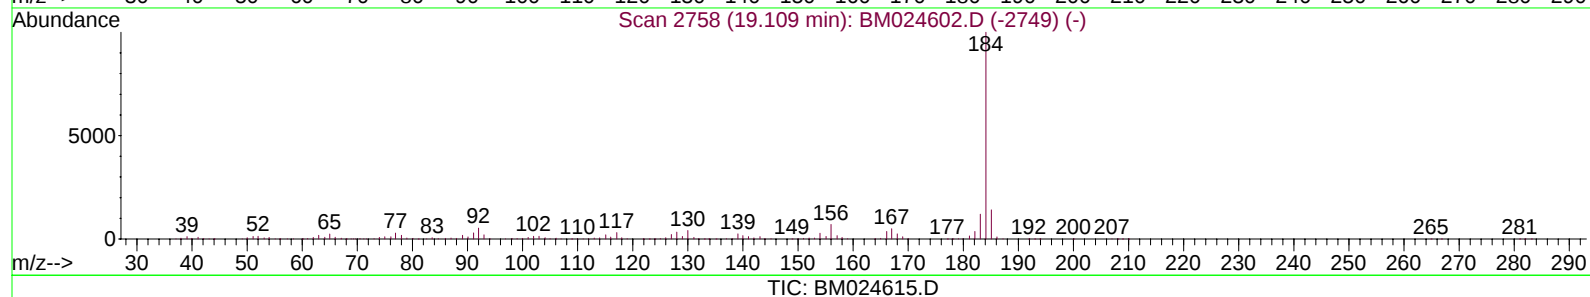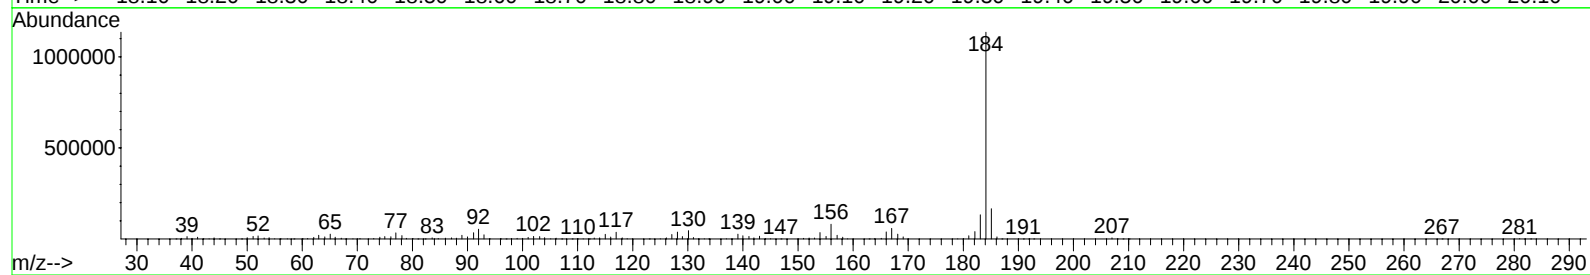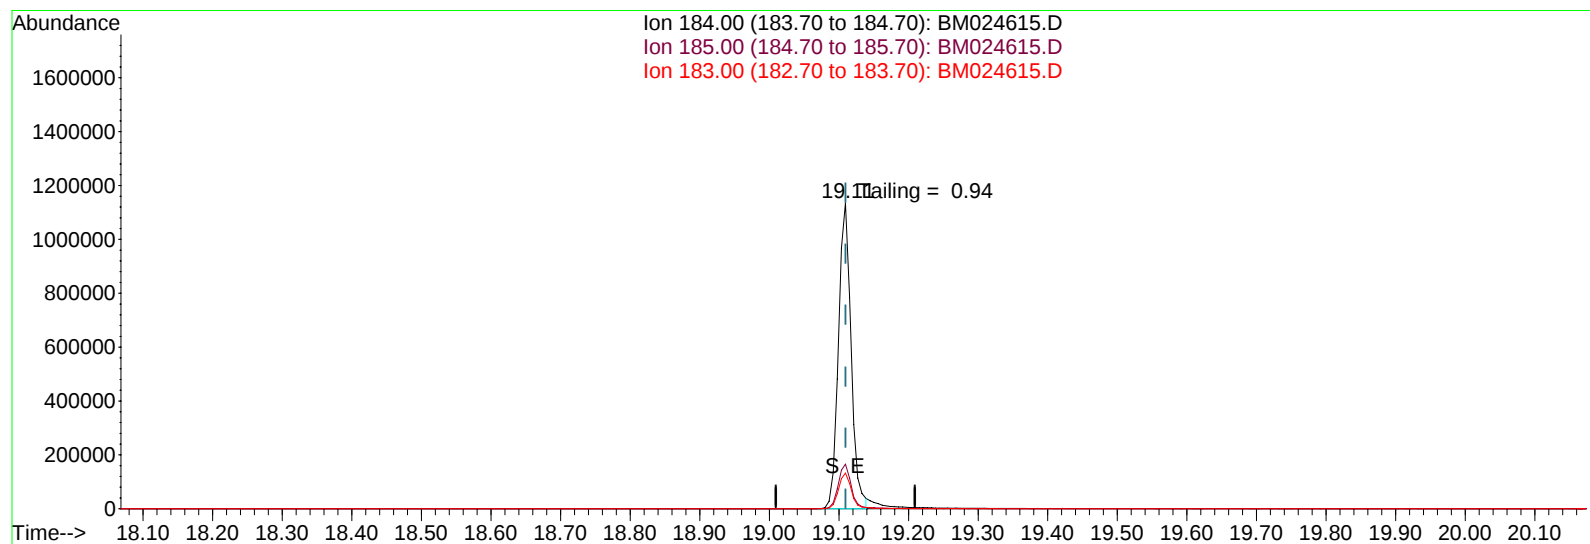

(77) Benzidine

19.109min (-0.000) 97240.86ng

response 1469732

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.62
183.00	12.00	11.69
0.00	0.00	0.00