


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012420\
 Data File : BM024615.D
 Acq On : 24 Jan 2020 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 23 14:57:07 2020

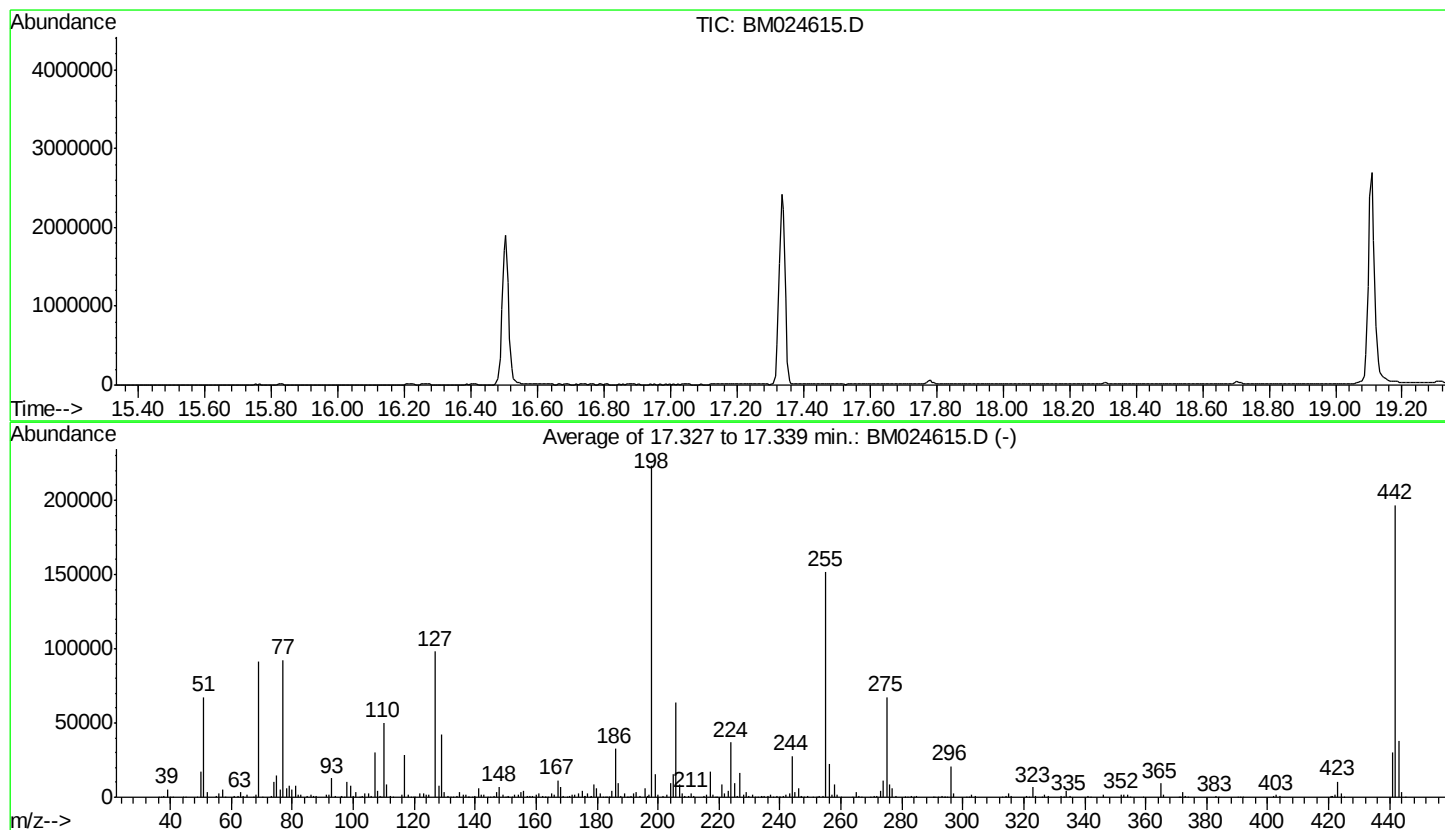

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	67229	PASS
68	69	0.00	2	2.0	1809	PASS
69	198	0.00	100	40.9	91392	PASS
70	69	0.00	2	0.4	404	PASS
127	198	10	80	44.0	98200	PASS
197	198	0.00	2	0.7	1616	PASS
198	198	100	100	100.0	223210	PASS
199	198	5	9	6.8	15196	PASS
275	198	10	60	30.2	67352	PASS
365	198	1	100	4.1	9263	PASS
441	198	0.01	100	13.5	30180	PASS
442	198	50	100	88.0	196488	PASS
443	442	15	24	19.4	38061	PASS