

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
 Data File : BM038521.D
 Acq On : 24 Jan 2023 11:08
 Operator : CG/JU
 Sample : PB150200BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150200BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	311	317	324	rBV	512785	705693	25.58%	4.283%
2	5.516	389	396	409	rBV	1501230	2036691	73.83%	12.362%
3	7.128	663	670	686	rBV	1310515	1989651	72.12%	12.077%
4	7.963	806	812	823	rVB	295589	457312	16.58%	2.776%
5	9.139	1005	1012	1025	rBV	740750	1166155	42.27%	7.078%
6	10.775	1282	1290	1298	rBV	322012	529376	19.19%	3.213%
7	13.227	1700	1707	1717	rBV	1809913	2480976	89.93%	15.059%
8	14.598	1932	1940	1950	rBV	433018	621907	22.54%	3.775%
9	16.086	2187	2193	2203	rBV	1248494	1692986	61.37%	10.276%
10	17.339	2400	2406	2415	rBV	464058	642852	23.30%	3.902%
11	19.950	2845	2850	2861	rBV	2277530	2758747	100.00%	16.745%
12	21.515	3111	3116	3123	rBV	512240	651898	23.63%	3.957%
13	23.927	3520	3526	3537	rVB2	373814	740513	26.84%	4.495%




Sum of corrected areas: 16474757

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
Data File : BM038521.D
Acq On : 24 Jan 2023 11:08
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150200BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

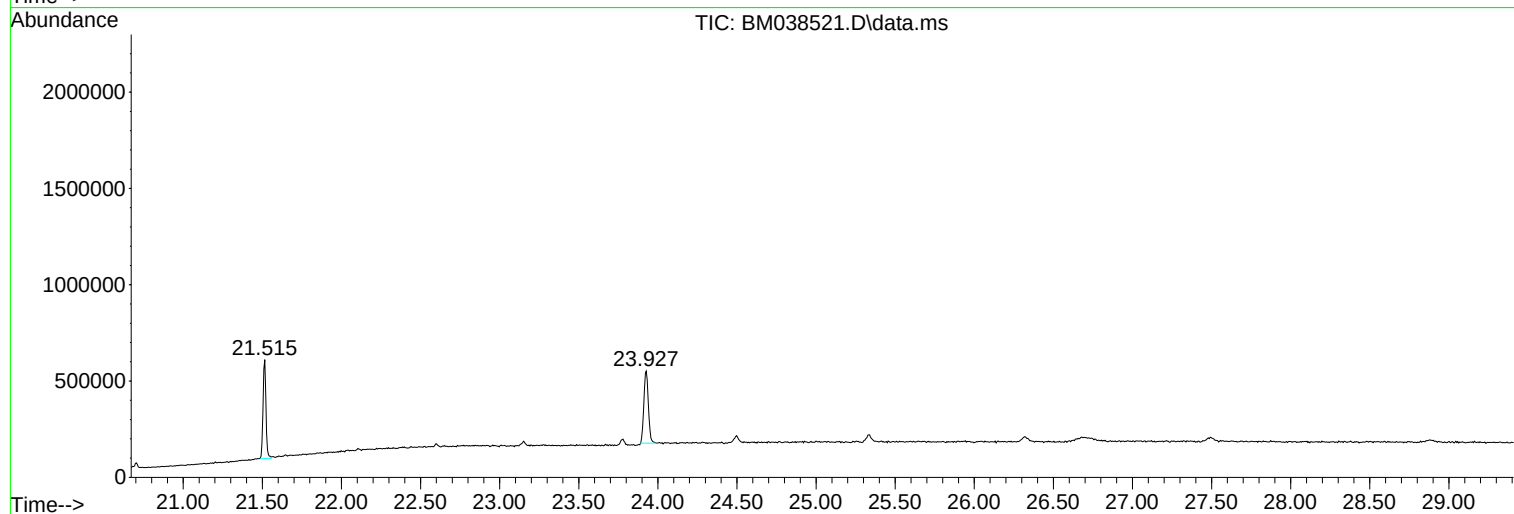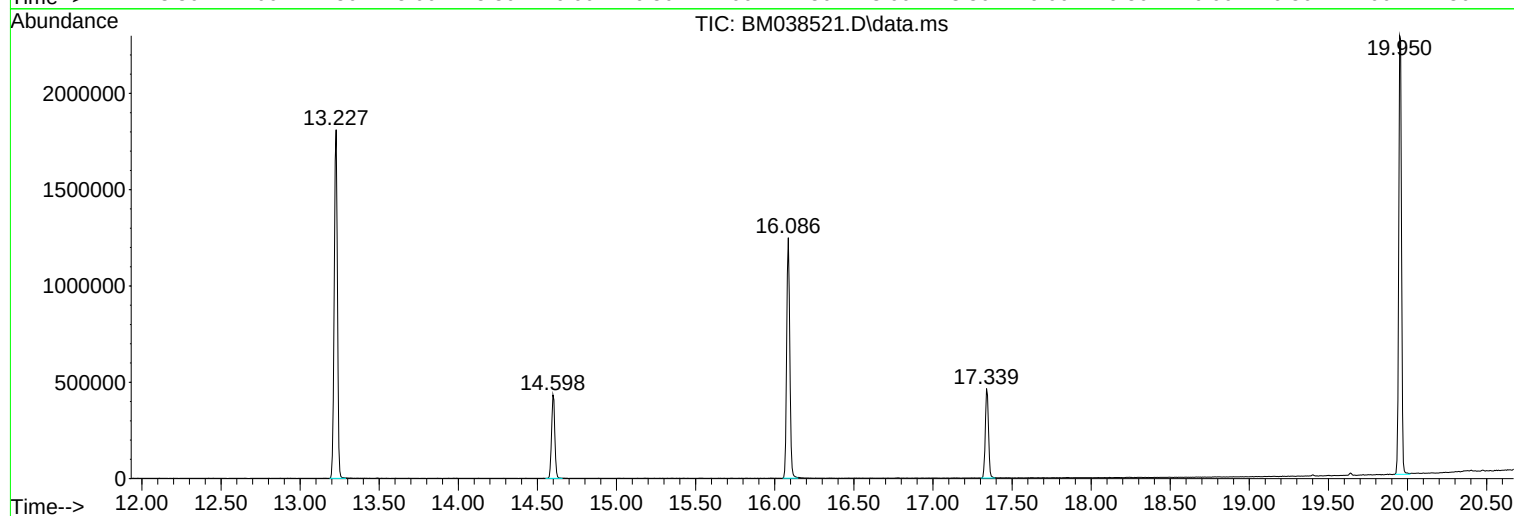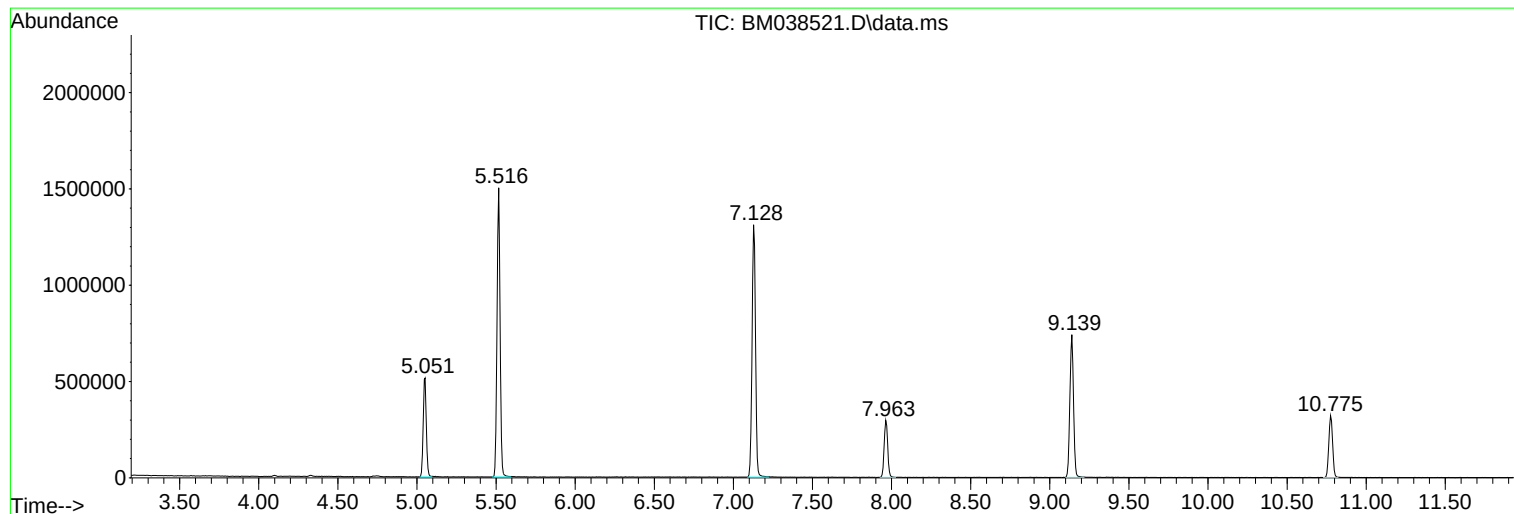

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
Data File : BM038521.D
Acq On : 24 Jan 2023 11:08
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150200BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.051	30.86 ng	705693	1,4-Dichlorobenzene-d4	7.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

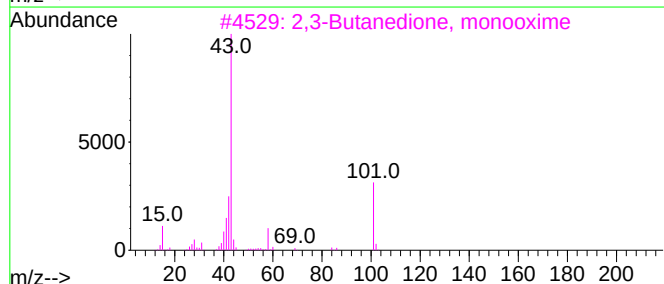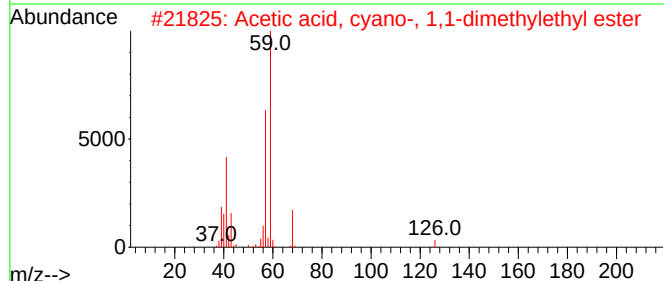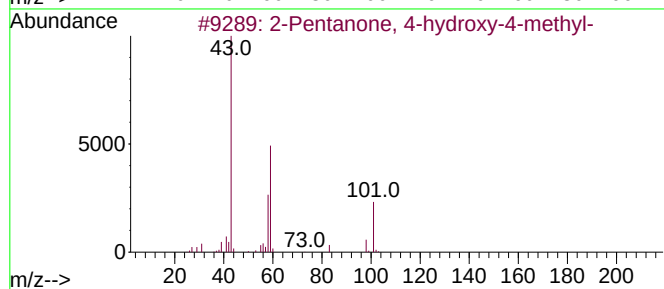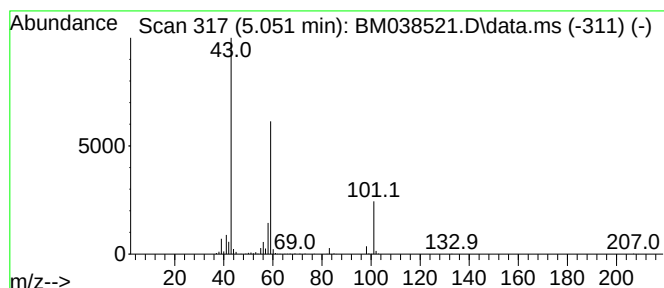

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
Data File : BM038521.D
Acq On : 24 Jan 2023 11:08
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150200BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.051	30.9	ng	705693	1	7.963	457312	20.0