


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
Data File : BM038519.D
Acq On : 24 Jan 2023 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 21 01:21:49 2023

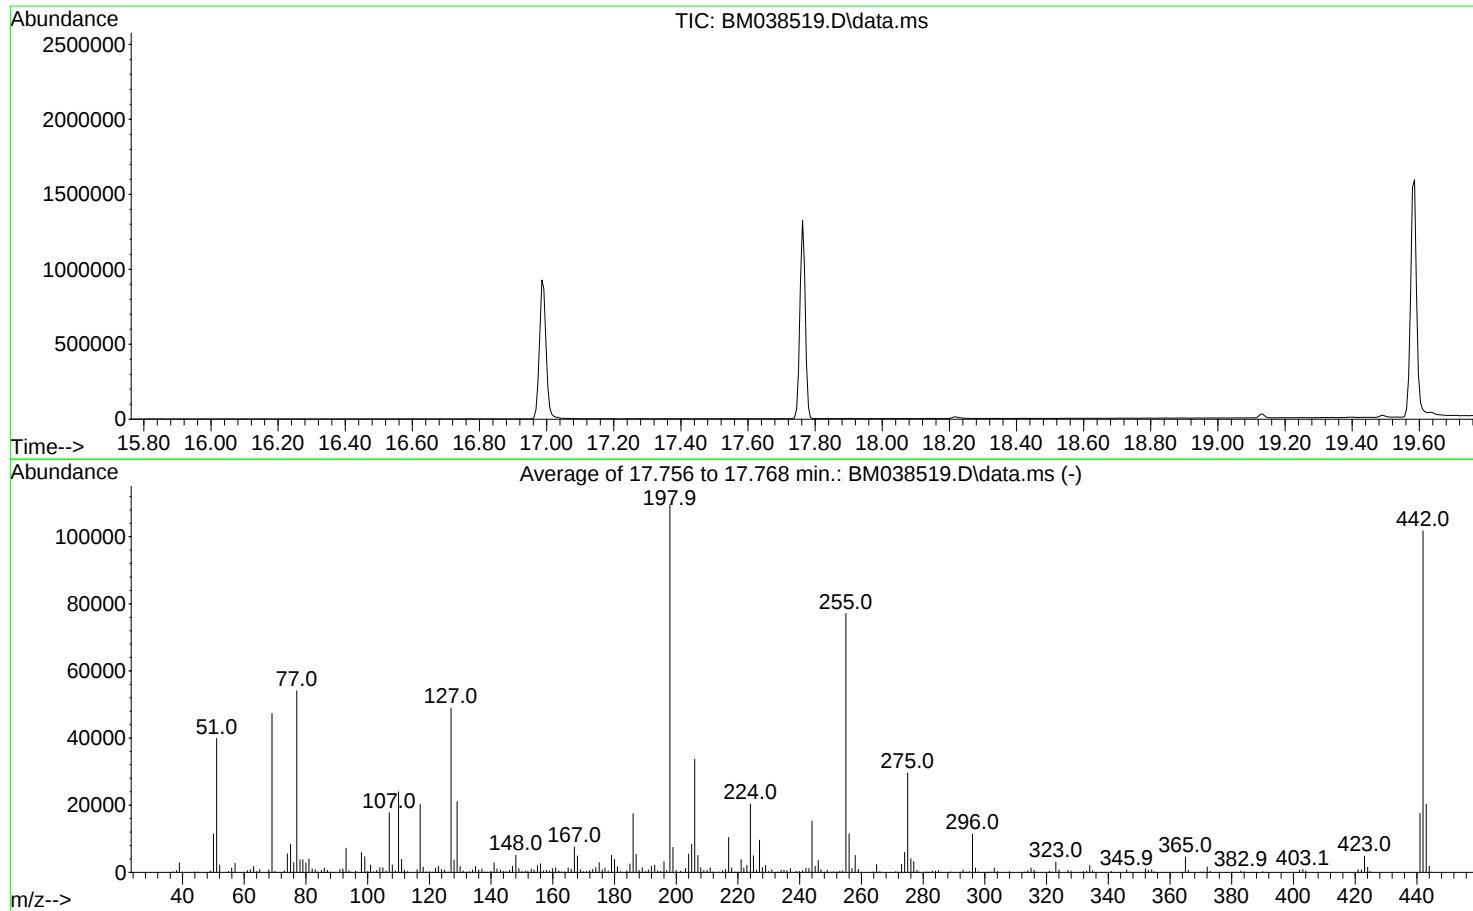




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	39904	PASS
68	69	0.00	2	1.5	715	PASS
69	198	0.00	100	43.2	47315	PASS
70	69	0.00	2	0.5	243	PASS
127	198	10	80	44.6	48944	PASS
197	198	0.00	2	0.4	484	PASS
198	198	100	100	100.0	109627	PASS
199	198	5	9	6.8	7403	PASS
275	198	10	60	27.0	29600	PASS
365	198	1	100	4.2	4579	PASS
441	198	0.01	100	16.0	17512	PASS
442	442	50	100	100.0	101736	PASS
443	442	15	24	20.0	20302	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
Data File : BM038519.D
Acq On : 24 Jan 2023 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 25 06:11:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 21 01:21:49 2023
Response via : Initial Calibration

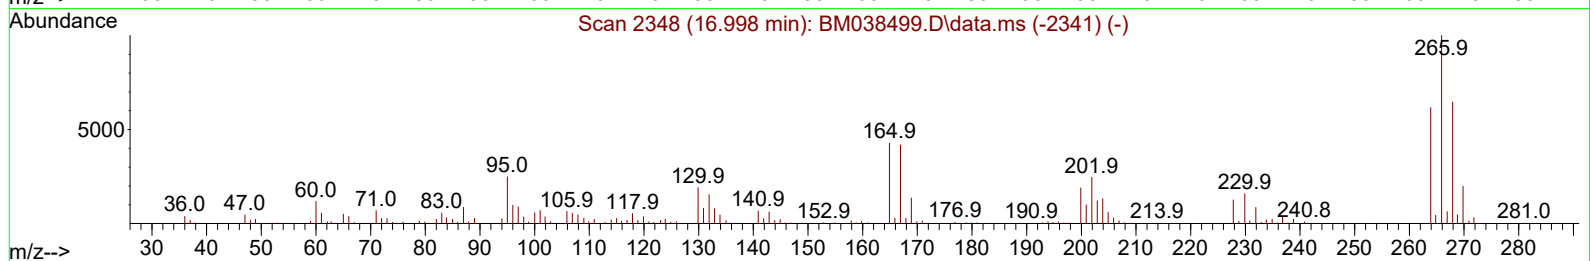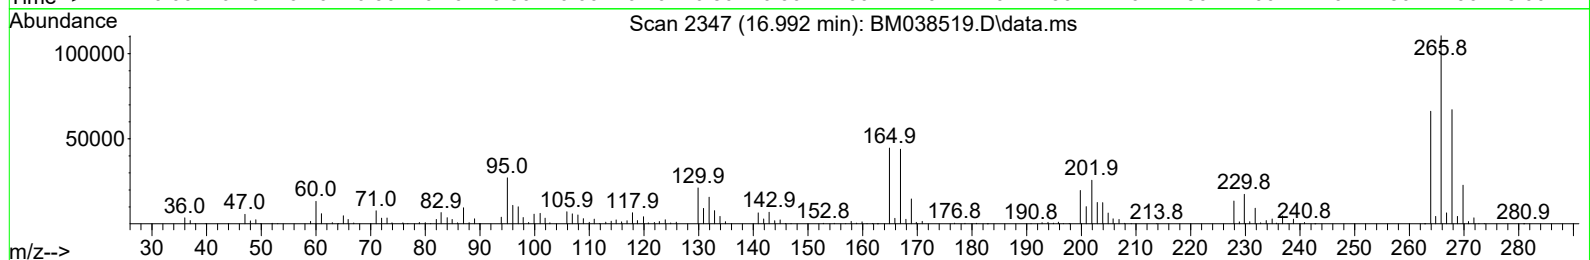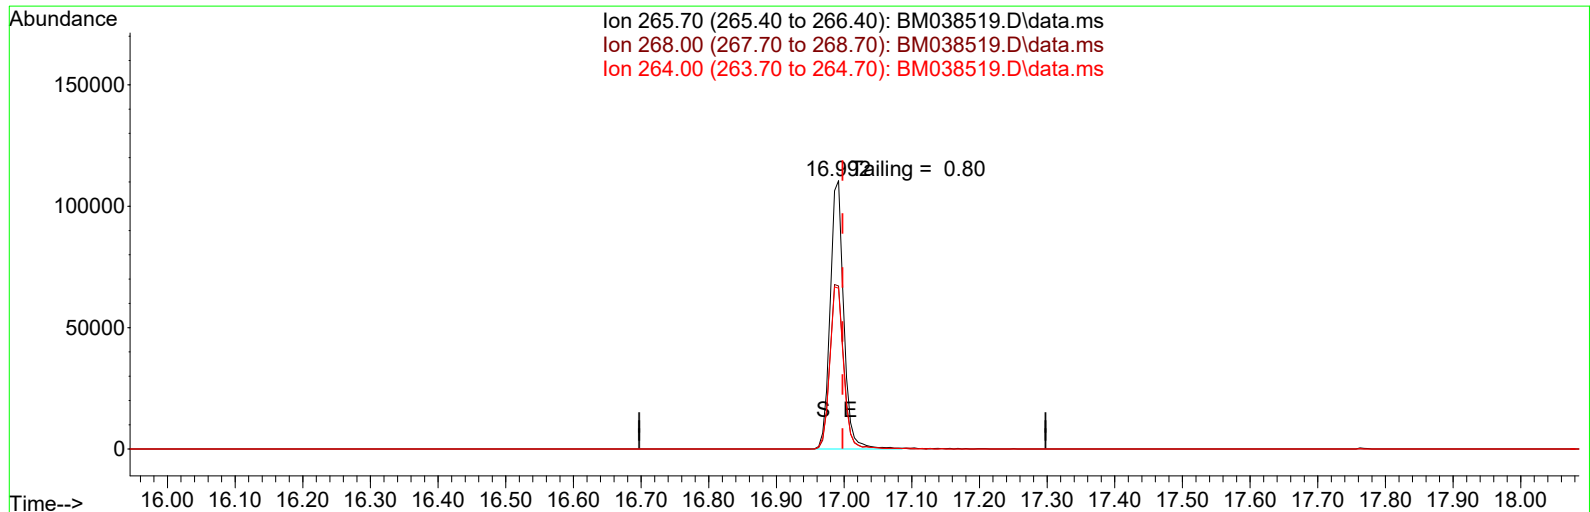

TIC: BM038519.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.006) 0.00 ng




response 154061

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	60.77
264.00	61.70	59.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012423\
Data File : BM038519.D
Acq On : 24 Jan 2023 09:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 25 06:11:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 21 01:21:49 2023
Response via : Initial Calibration

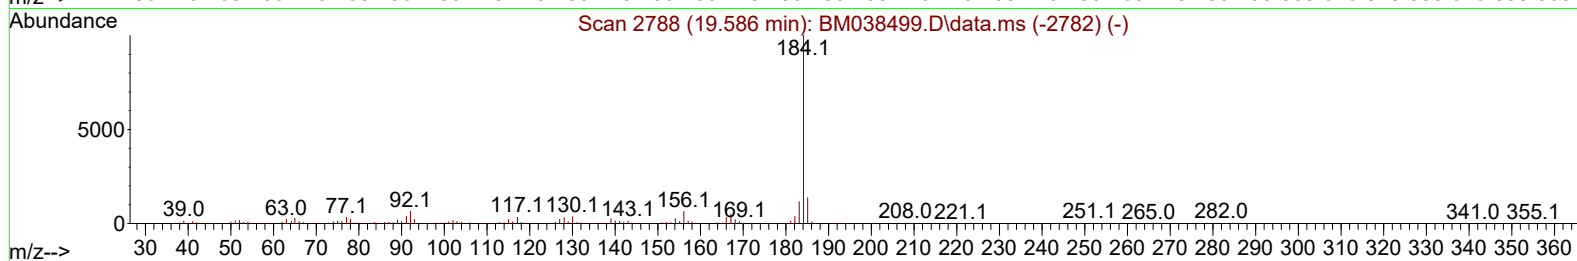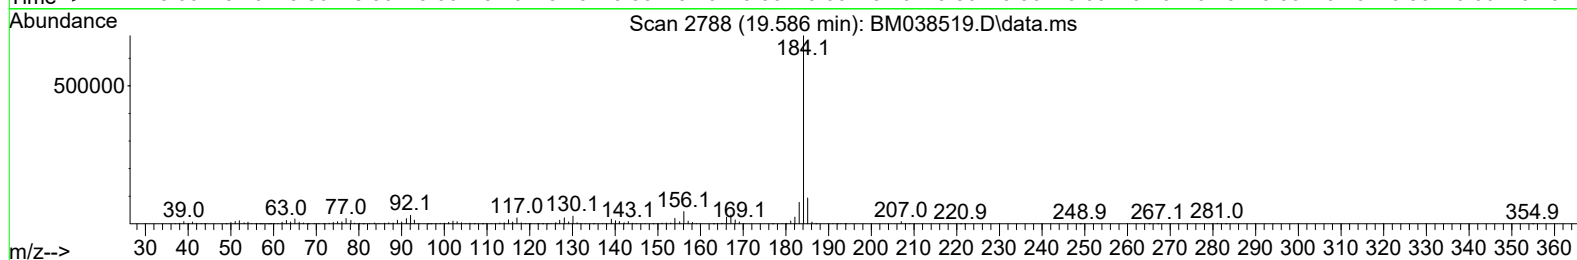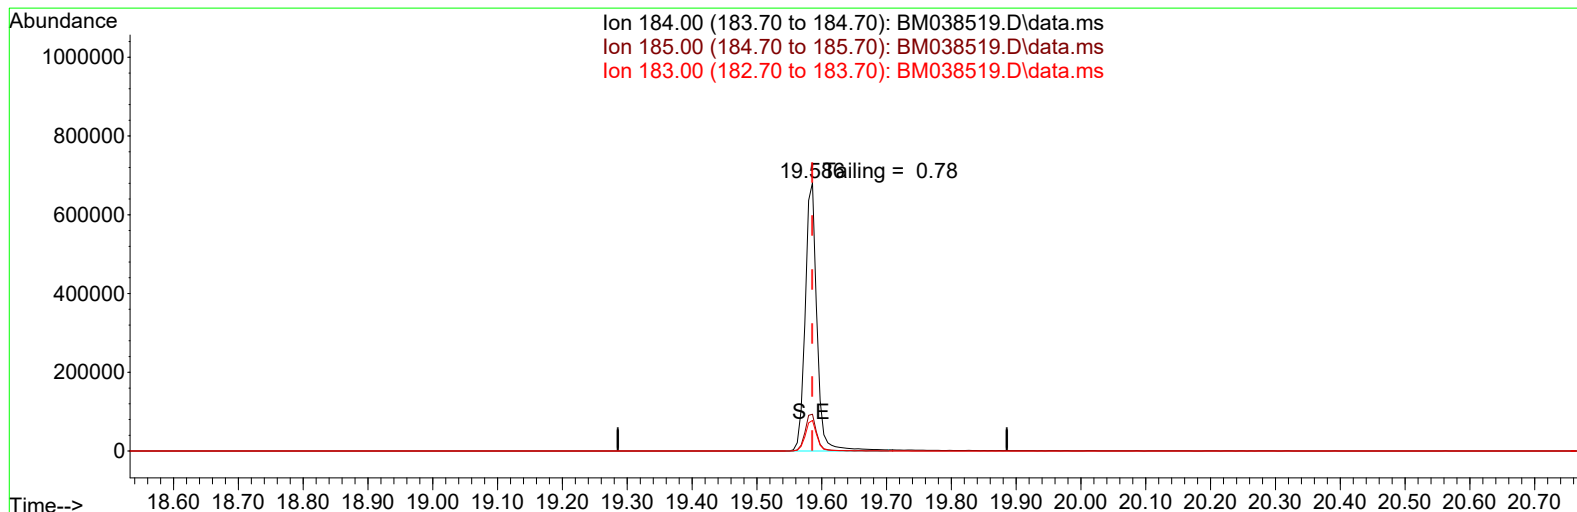

TIC: BM038519.D\data.ms

(77) Benzidine

19.586min (+ 0.000) 0.00 ng

response 865302

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.72
183.00	11.60	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2023	BNA_M	<u>BM038519.D</u>
Compound Name	Response	Retention Time
DDT	496879	20.803
DDD	4548	20.415
DDE	56	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4604	501483	0.92

Instrument :
BNA_M
ClientSampleId :
DFTPP