

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012425\
 Data File : BM049436.D
 Acq On : 24 Jan 2025 15:05
 Operator : RC/JU
 Sample : PB166197BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK197

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	28	rVB	66797	88774	2.08%	0.184%
2	3.505	84	88	104	rBV	923429	1302247	30.49%	2.701%
3	3.810	136	140	147	rVB	33340	46860	1.10%	0.097%
4	6.710	626	633	648	rBV	910706	1417345	33.18%	2.940%
5	6.863	652	659	678	rVB	710902	1109844	25.98%	2.302%
6	7.057	685	692	703	rBV	908493	1395734	32.68%	2.895%
7	7.516	763	770	777	rBV	874618	1376347	32.22%	2.854%
8	8.228	882	891	904	rBV	1030758	1630883	38.18%	3.382%
9	8.657	957	964	979	rBV	762339	1209662	28.32%	2.509%
10	9.369	1079	1085	1098	rBV	578749	959095	22.45%	1.989%
11	9.910	1169	1177	1190	rBV	939242	1600596	37.47%	3.320%
12	10.275	1231	1239	1249	rVB	1096924	1771632	41.48%	3.674%
13	10.422	1256	1264	1284	rBV	787360	1464408	34.28%	3.037%
14	11.886	1506	1513	1520	rBV3	9624	19660	0.46%	0.041%
15	13.580	1794	1801	1813	rBV	1562725	2219479	51.96%	4.603%
16	13.845	1838	1846	1857	rBV	1921493	2673429	62.59%	5.545%
17	14.010	1871	1874	1879	rBV6	4610	8832	0.21%	0.018%
18	14.157	1892	1899	1911	rBV	1699088	2411572	56.46%	5.001%
19	14.380	1928	1937	1960	rBV	383252	854256	20.00%	1.772%
20	15.157	2061	2069	2083	rBV	2405573	3345063	78.31%	6.938%
21	15.280	2084	2090	2104	rVV	608672	867399	20.31%	1.799%
22	15.398	2106	2110	2114	rVV5	11671	18255	0.43%	0.038%
23	16.698	2327	2331	2340	rVB4	7076	12620	0.30%	0.026%
24	16.910	2360	2367	2376	rBV	2155777	2892888	67.73%	6.000%
25	17.004	2377	2383	2396	rVV	2552746	3592791	84.11%	7.451%
26	17.298	2425	2433	2436	rBV8	2073	5186	0.12%	0.011%
27	17.833	2519	2524	2533	rBV	107144	184876	4.33%	0.383%
28	18.874	2697	2701	2707	rBV	28952	39983	0.94%	0.083%
29	18.951	2709	2714	2718	rVV	23433	37662	0.88%	0.078%
30	19.004	2721	2723	2726	rVV4	4788	4570	0.11%	0.009%
31	19.127	2739	2744	2751	rBV2	64367	107969	2.53%	0.224%
32	19.309	2767	2775	2785	rBV	3263767	4271362	100.00%	8.859%
33	21.139	3081	3086	3095	rBV	2099771	2917609	68.31%	6.051%
34	23.733	3519	3527	3542	rVB	1563508	3419077	80.05%	7.091%
35	23.921	3551	3559	3576	rVB	1211005	2939146	68.81%	6.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012425\
Data File : BM049436.D
Acq On : 24 Jan 2025 15:05
Operator : RC/JU
Sample : PB166197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 48217111

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012425\
Data File : BM049436.D
Acq On : 24 Jan 2025 15:05
Operator : RC/JU
Sample : PB166197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

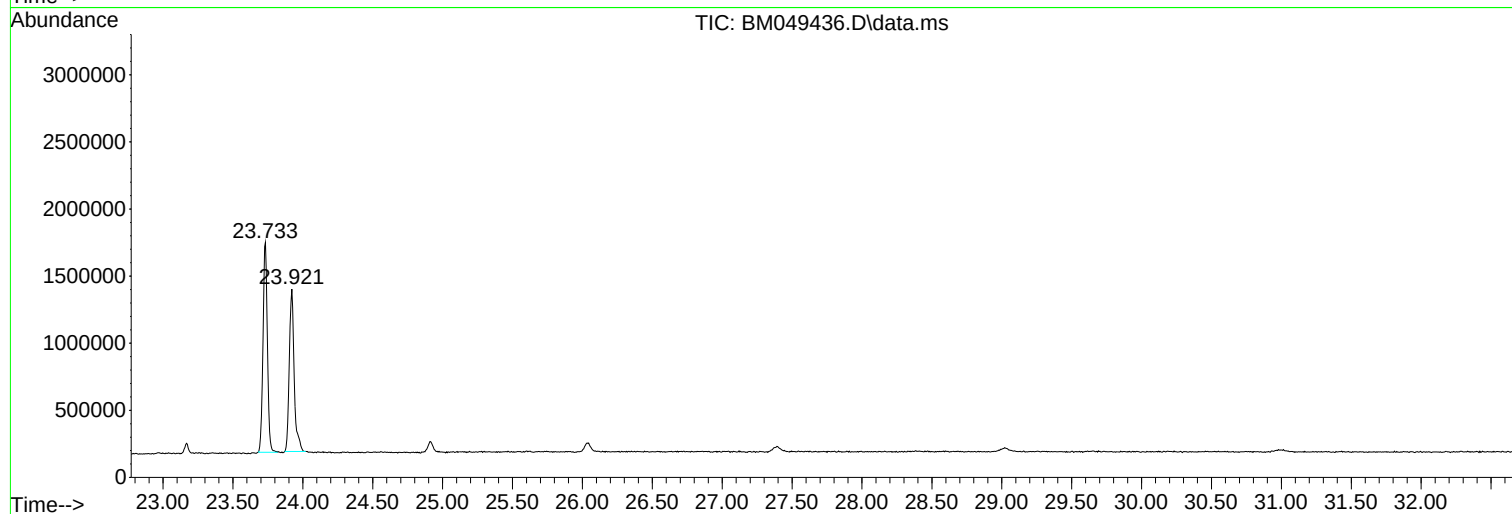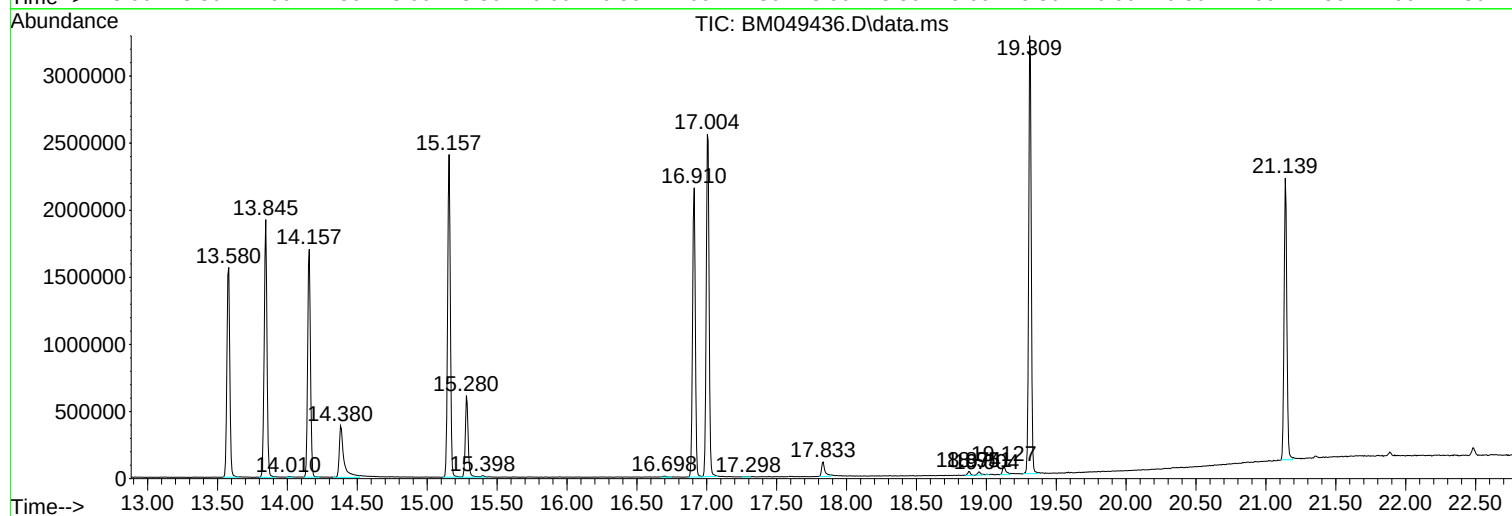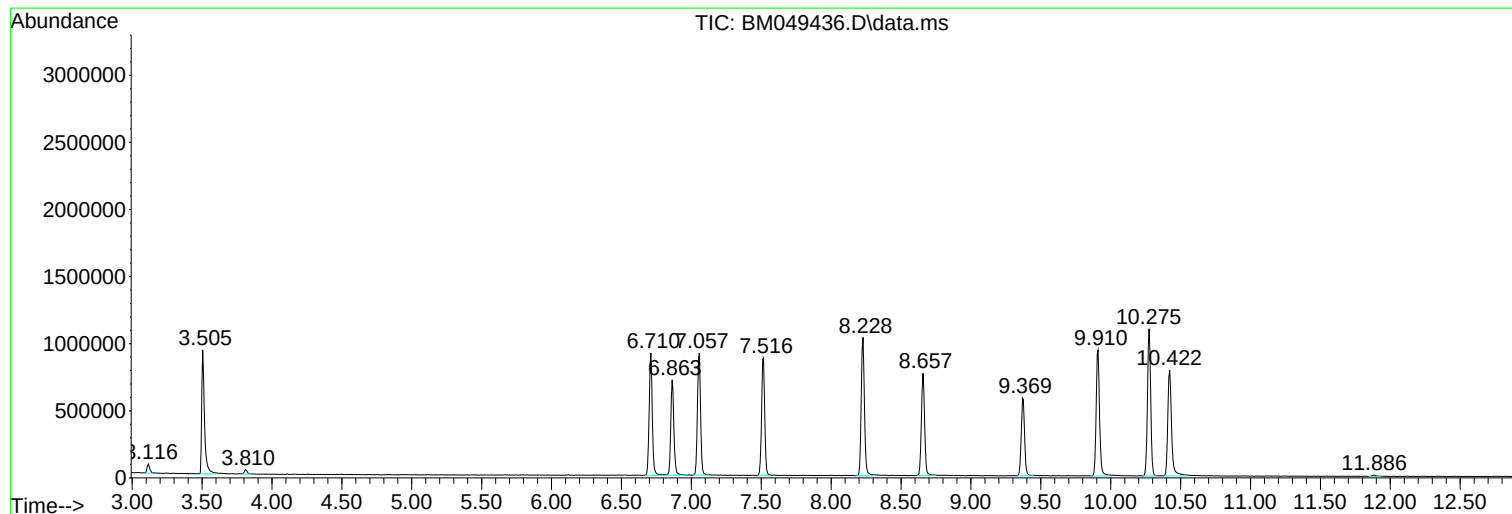

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012425\
Data File : BM049436.D
Acq On : 24 Jan 2025 15:05
Operator : RC/JU
Sample : PB166197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012425\
Data File : BM049436.D
Acq On : 24 Jan 2025 15:05
Operator : RC/JU
Sample : PB166197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc