


Data Path : Z:\HPCHEM1\BNA_M\Data\BM012516\
 Data File : BM004124.D
 Acq On : 25 Jan 2016 11:23
 Operator : SJ/IZ
 Sample : DFTPP44
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP44

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION
 Last Update : Mon Jan 25 15:41:32 2016

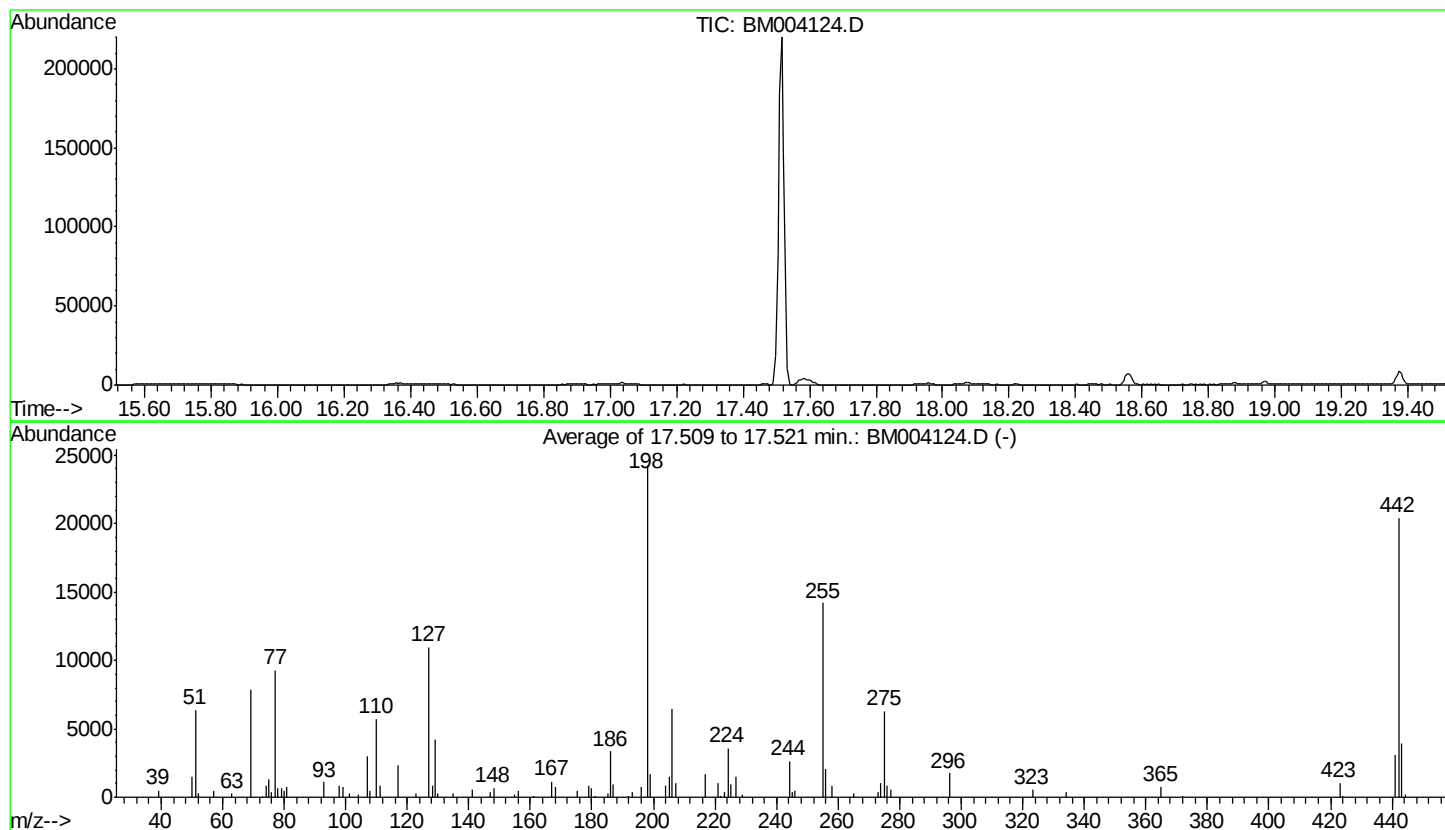

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	6380	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.3	7834	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	10946	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24232	PASS
199	198	5	9	6.8	1640	PASS
275	198	10	60	26.0	6306	PASS
365	198	1	100	3.2	781	PASS
441	443	0.01	100	78.0	3083	PASS
442	198	50	100	84.2	20409	PASS
443	442	15	24	19.4	3952	PASS

m/z	Abundance
39.00	565.0
50.10	1723.0
51.10	7460.0
52.00	364.0
57.00	580.0
63.00	361.0
69.00	8892.0
73.00	411.0
74.00	922.0
75.00	1494.0
76.00	507.0
77.10	10505.0
78.00	714.0
79.00	766.0
80.00	587.0
81.00	852.0
93.00	1199.0
98.00	851.0
99.00	789.0
101.00	477.0
104.00	301.0
107.00	3139.0
108.00	544.0
110.00	6121.0
111.00	882.0
117.00	2561.0
123.00	327.0
127.00	11829.0
128.00	953.0
129.00	4480.0
129.90	407.0
135.00	421.0
141.00	614.0
147.00	431.0
148.00	686.0
155.00	361.0
156.00	457.0
167.00	1203.0
168.00	801.0
175.00	510.0
179.00	880.0
180.00	684.0
185.10	422.0
186.10	3464.0
187.00	986.0
192.00	308.0
193.00	363.0
196.00	773.0
198.00	24600.0
199.00	1679.0
204.00	846.0
205.00	1541.0
206.10	6557.0
207.10	1042.0
217.00	1768.0
221.10	952.0
223.00	331.0
224.10	3497.0
225.10	999.0
227.00	1471.0
229.00	313.0
244.10	2508.0
245.10	369.0
246.00	450.0
255.10	13608.0
256.10	1993.0
258.00	799.0
265.00	306.0
273.00	358.0
274.00	973.0
275.10	6064.0
276.10	726.0
277.00	586.0
296.00	1704.0
323.10	532.0
334.00	301.0
365.10	671.0
423.10	767.0
441.20	2321.0
442.10	15932.0
443.10	3272.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

m/z	Abundance
39.10	576.0
50.10	1806.0
51.10	7282.0
52.00	363.0
57.00	546.0
63.00	353.0
69.00	9293.0
73.10	432.0
74.00	955.0
75.00	1482.0
76.00	534.0
77.10	10741.0
78.10	761.0
79.00	805.0
80.00	596.0
81.00	781.0
93.00	1286.0
98.00	1022.0
99.00	874.0
101.00	430.0
103.90	334.0
107.00	3568.0
108.00	566.0
110.00	6953.0
111.00	1047.0
117.00	2629.0
123.00	416.0
127.00	12914.0
128.00	1001.0
129.00	5087.0
130.00	433.0
135.00	420.0
141.00	639.0
147.00	477.0
148.00	778.0
155.00	346.0
156.10	577.0
161.00	337.0
167.00	1361.0
168.00	860.0
175.10	596.0
179.00	1016.0
180.00	843.0
181.00	351.0
185.00	475.0
186.10	3930.0
187.00	1121.0
193.00	414.0
196.00	872.0
198.00	28776.0
199.00	1973.0
204.10	1024.0
205.00	1823.0
206.10	7621.0
207.00	1060.0
217.00	2046.0
221.10	1157.0
221.90	330.0
223.00	409.0
224.10	4278.0
225.10	1032.0
227.00	1846.0
229.00	381.0
244.10	3225.0
245.10	446.0
246.00	612.0
255.10	16936.0
256.10	2345.0
258.00	946.0
265.00	416.0
273.10	527.0
274.00	1262.0
275.10	7430.0
276.10	1047.0
277.00	669.0
296.10	2128.0
323.10	650.0
334.00	425.0
365.00	937.0
372.10	300.0
423.10	1384.0
424.10	413.0
441.10	3695.0
442.10	24168.0
443.10	4694.0
444.10	399.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

m/z	Abundance
39.00	330.0
50.00	1041.0
51.10	4400.0
57.00	346.0
69.00	5319.0
73.00	406.0
74.00	565.0
75.00	890.0
77.10	6567.0
78.10	450.0
79.00	465.0
80.00	334.0
81.00	505.0
93.00	794.0
98.00	628.0
99.00	588.0
107.00	2311.0
107.90	314.0
110.00	4137.0
111.00	616.0
117.00	1706.0
127.00	8097.0
128.10	702.0
129.10	3202.0
141.00	487.0
147.00	339.0
148.00	513.0
156.00	380.0
167.00	905.0
168.00	558.0
175.00	318.0
179.00	760.0
180.00	515.0
186.10	2673.0
187.00	632.0
193.00	320.0
196.10	553.0
198.00	19320.0
199.00	1270.0
204.00	733.0
205.10	1184.0
206.10	5134.0
207.00	887.0
217.00	1304.0
221.00	851.0
223.00	315.0
224.10	2976.0
225.10	781.0
227.00	1081.0
244.10	2203.0
245.00	301.0
246.10	469.0
255.10	11983.0
256.10	1772.0
258.00	699.0
273.00	339.0
274.00	988.0
275.10	5424.0
276.00	664.0
277.00	488.0
296.00	1459.0
323.10	494.0
334.10	340.0
365.10	737.0
423.10	1083.0
441.10	3234.0
442.10	21128.0
443.10	3892.0
444.20	306.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

m/z	Abundance
73.10	405.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44