

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012517\
 Data File : BM008870.D
 Acq On : 25 Jan 2017 19:51
 Operator : SJ/MA
 Sample : I1323-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA9P8

Quant Time: Jan 26 13:06:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM010917.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 16:35:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	262	0.40	ng/ul	0.00
2) Naphthalene-d8	10.73	136	856	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.57	164	657	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.40	188	121407	0.40	ng/ul	0.09
16) Chrysene-d12	21.48	240	1276	0.40	ng/ul	0.00
20) Perylene-d12	23.69	264	93073	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.32	152	467	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.56	166	244	0.09	ng/ul#	32
17) Pyrene	19.70	202	245	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012517\
Data File : BM008870.D
Acq On : 25 Jan 2017 19:51
Operator : SJ/MA
Sample : I1323-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA9P8

Quant Time: Jan 26 13:06:16 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM010917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 16:35:23 2017
Response via : Initial Calibration




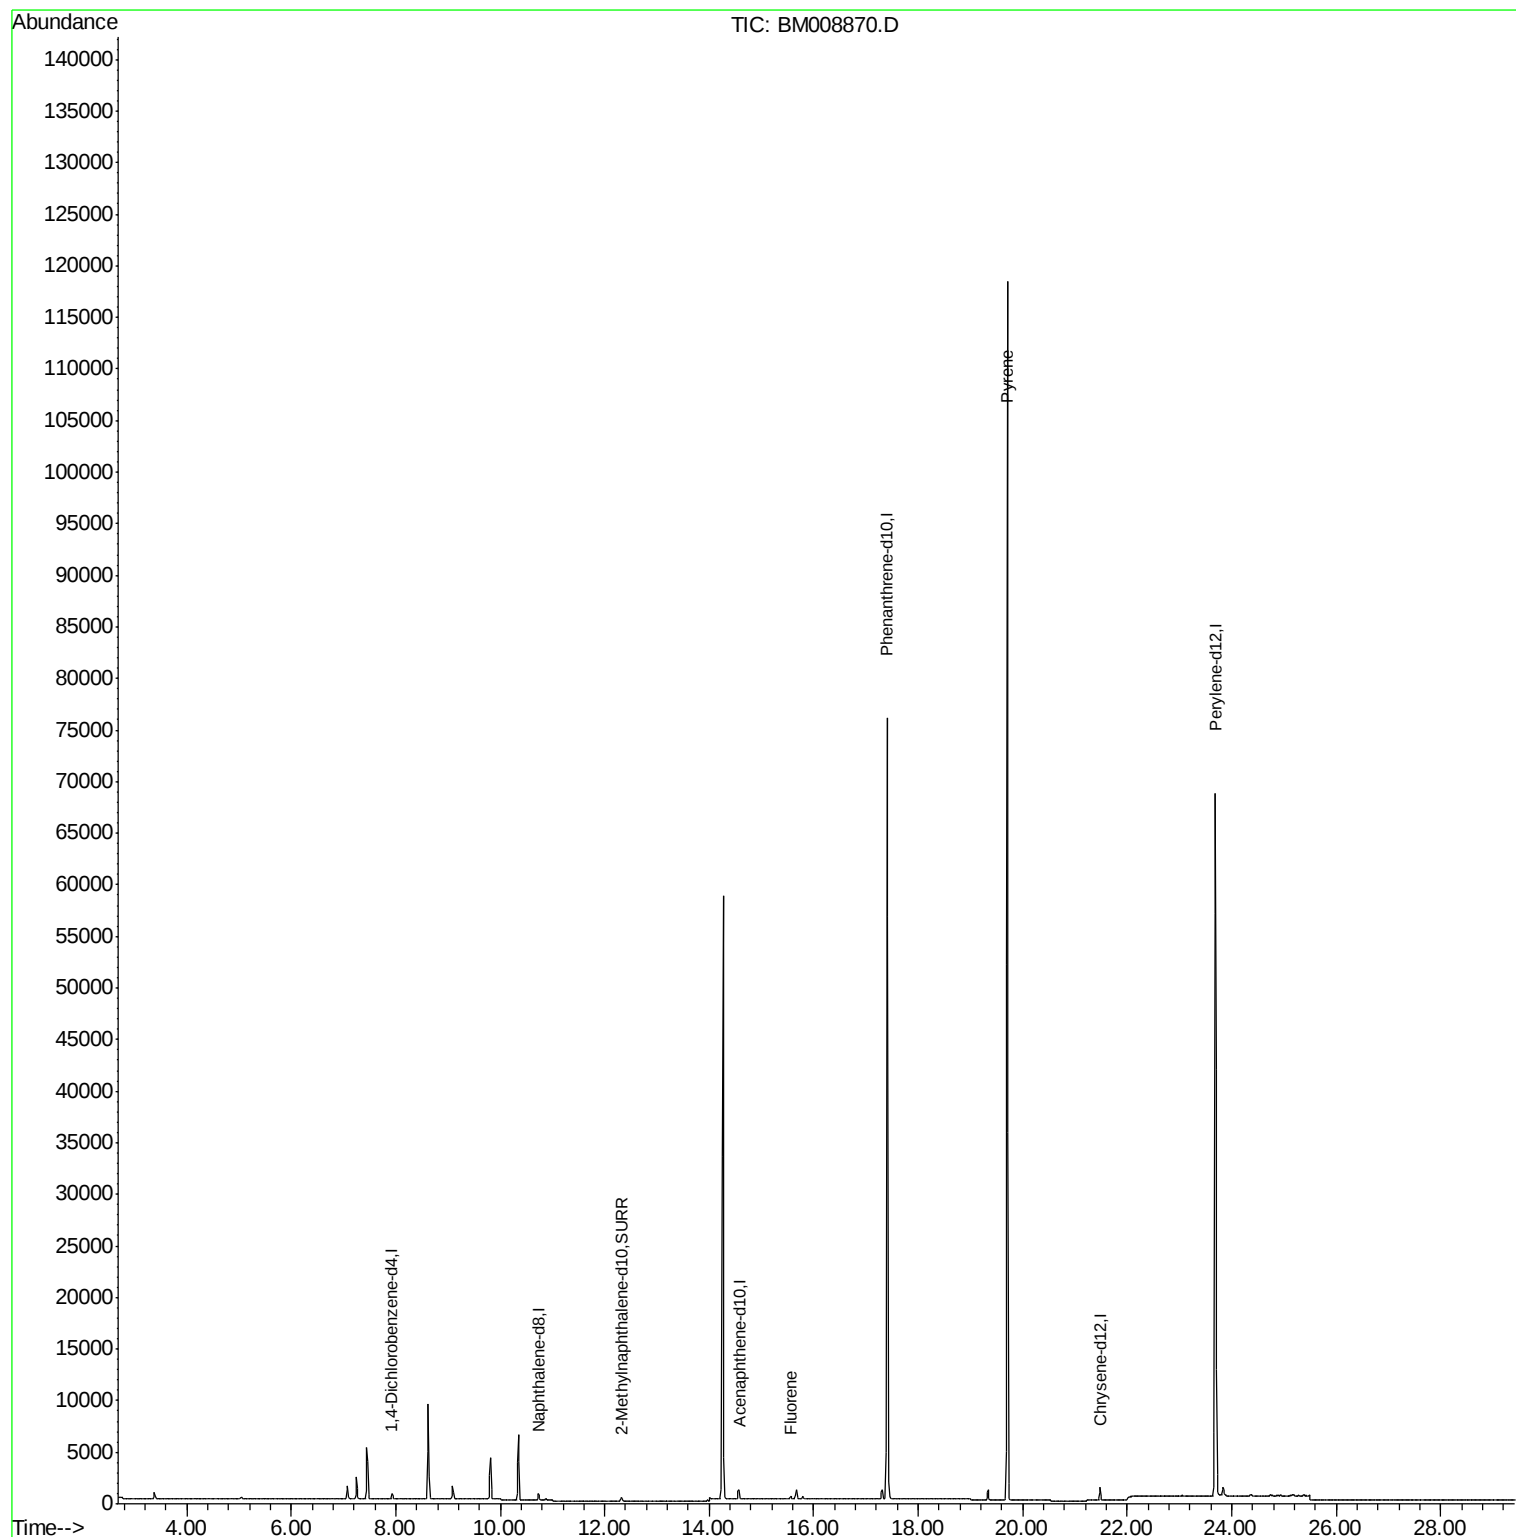


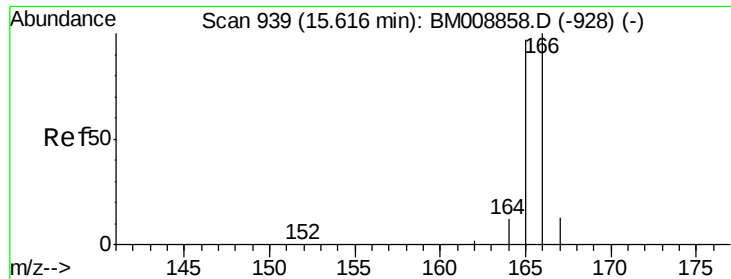

#9
Fluorene
 Concen: 0.09 ng/ul
 RT: 15.56 min Scan# 936
 Delta R.T. -0.05 min
 Lab File: BM008870.D
 Acq: 25 Jan 2017 19:51

Instrument :
 BNA_M
 ClientSampleId :
 DA9P8

Tgt Ion:166 Resp: 244
 Ion Ratio Lower Upper
 166 100
 165 28.2 73.4 110.2#
 167 51.3 14.6 22.0#

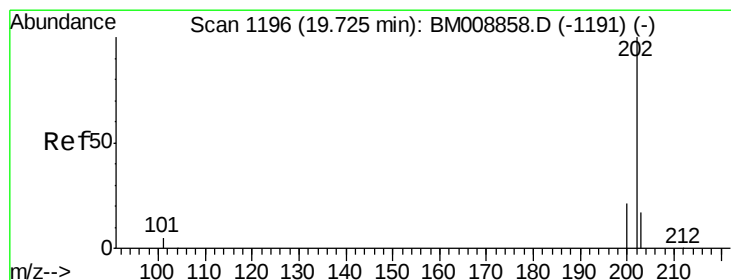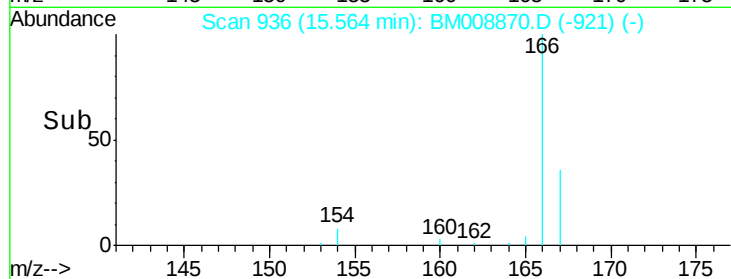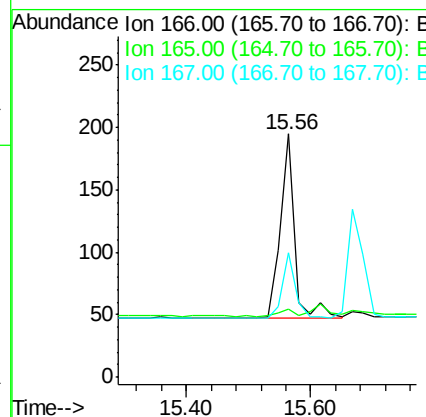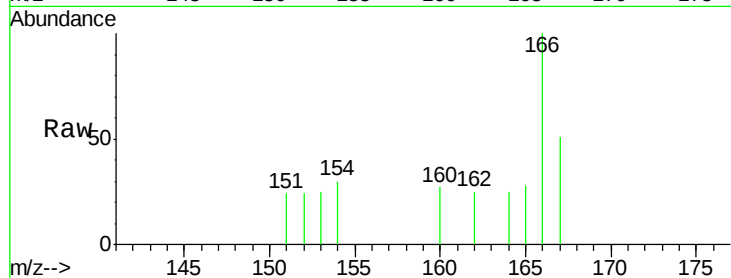

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.70 min Scan# 1194
 Delta R.T. -0.02 min
 Lab File: BM008870.D
 Acq: 25 Jan 2017 19:51

Tgt Ion:202 Resp: 245
 Ion Ratio Lower Upper
 202 100
 200 24.5 18.2 27.4
 203 177.4 15.6 23.4#

