

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012518\
 Data File : BM013813.D
 Acq On : 25 Jan 2018 19:37
 Operator : SJ/JU
 Sample : J1233-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6B10

Quant Time: Jan 26 01:47:50 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 00:22:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	107156	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	382134	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	209948	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	481017	20.00	ng/ul	0.00
75) Chrysene-d12	21.20	240	538101	20.00	ng/ul	0.00
83) Perylene-d12	23.39	264	509965	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	12229	4.51	ng/uL	0.00
5) Phenol-d5	6.78	99	230519	28.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	143468	28.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	207250	30.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	194121	30.70	ng/ul	-0.01
19) Nitrobenzene-d5	8.75	128	99542	33.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	111405	35.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	201732	33.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	238033	45.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	618699	35.76	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	756802	34.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	68114	24.22	ng/ul	0.00
57) Fluorene-d10	15.24	176	532132	34.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	77254	26.68	ng/ul	0.00
70) Anthracene-d10	17.10	188	808127	34.49	ng/ul	0.00
76) Pyrene-d10	19.40	212	875754	34.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.25	264	846109	36.10	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.80	94	22486	2.725	ng/ul 98
44) Dimethylphthalate	13.71	163	281526	16.548	ng/ul 100
55) 2,3,4,6-Tetrachlorophenol	14.89	232	20974	4.759	ng/ul# 86
68) Pentachlorophenol	16.66	266	482504	148.477	ng/ul 97
69) Phenanthrene	17.04	178	44052	1.648	ng/ul 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012518\
Data File : BM013813.D
Acq On : 25 Jan 2018 19:37
Operator : SJ/JU
Sample : J1233-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6B10

Quant Time: Jan 26 01:47:50 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 26 00:22:17 2018
Response via : Initial Calibration

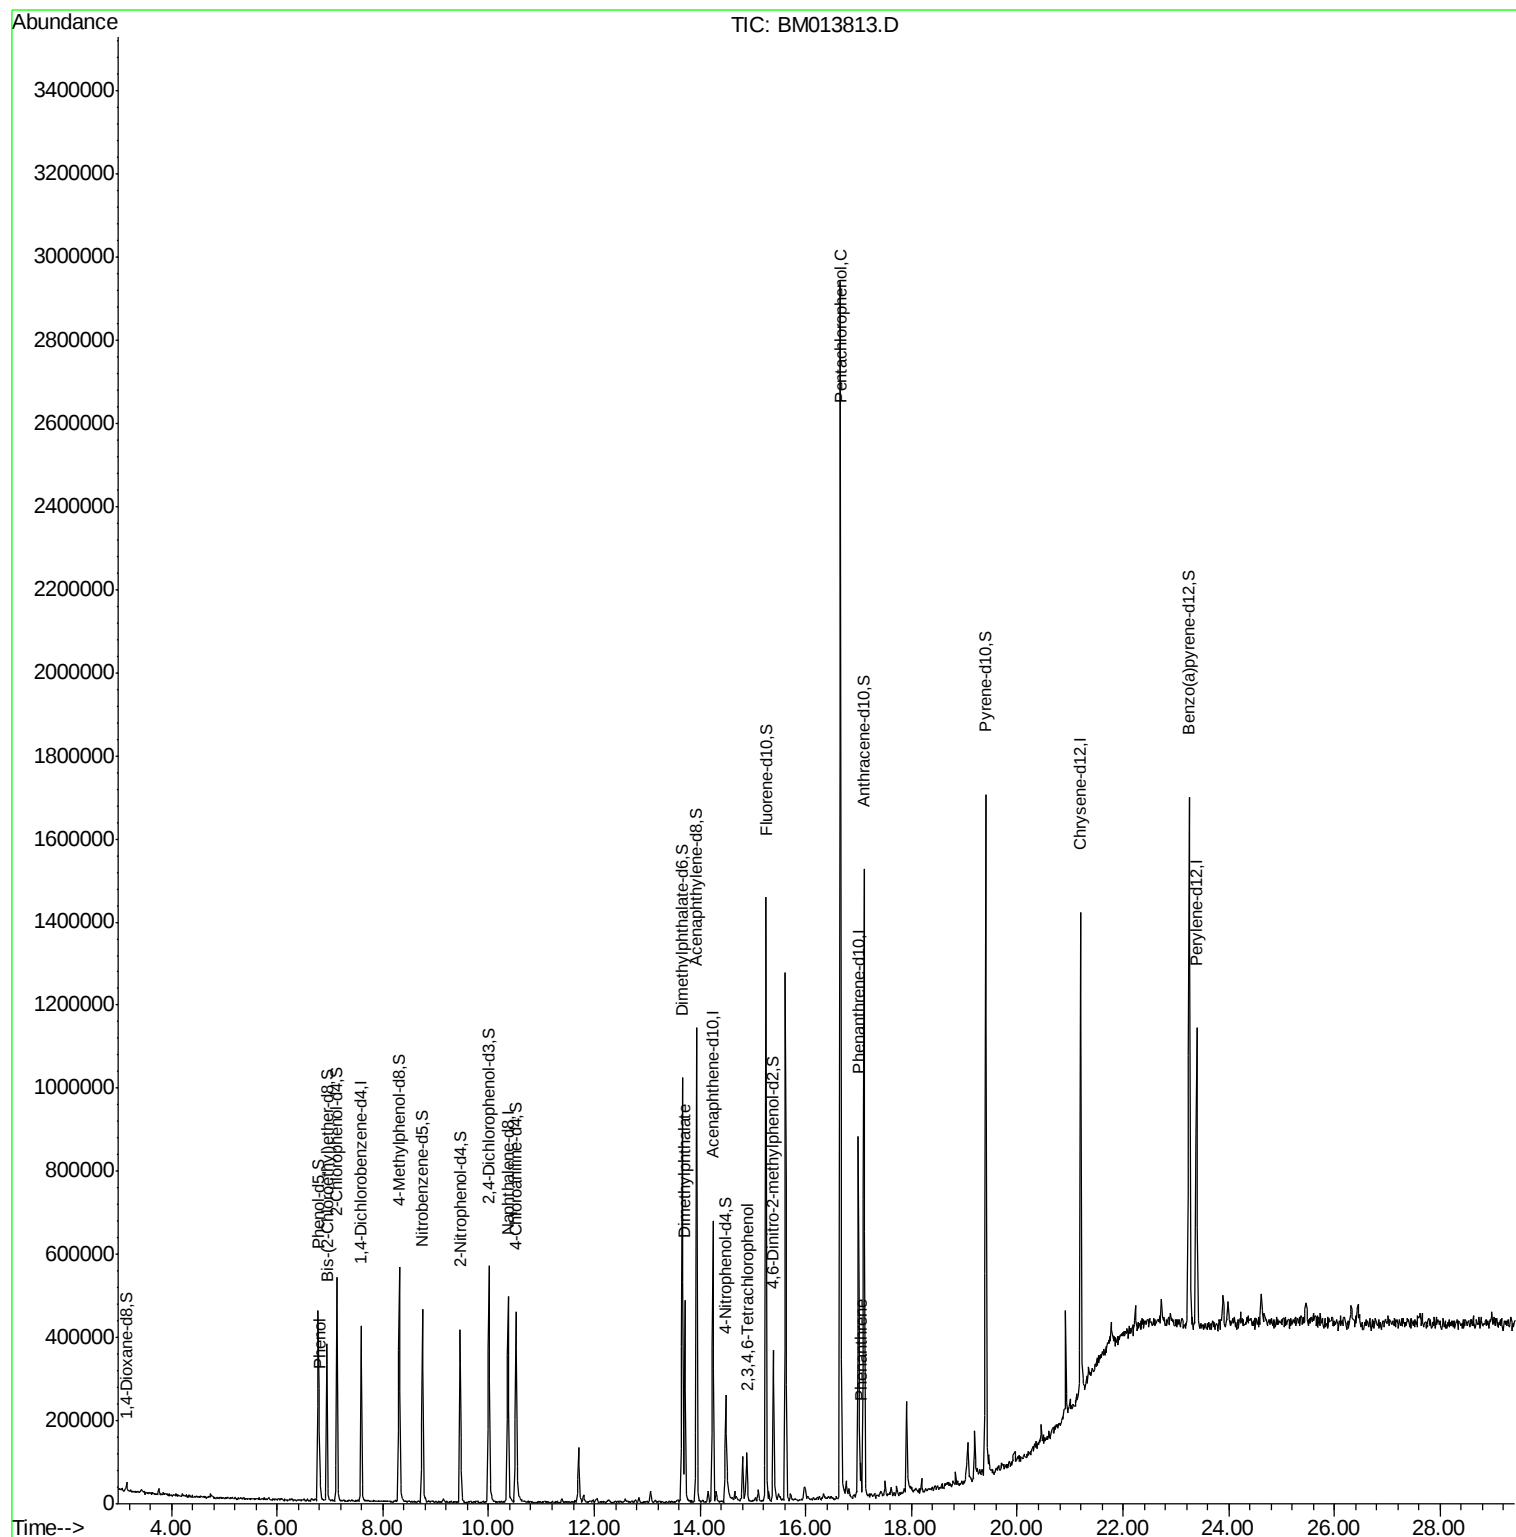

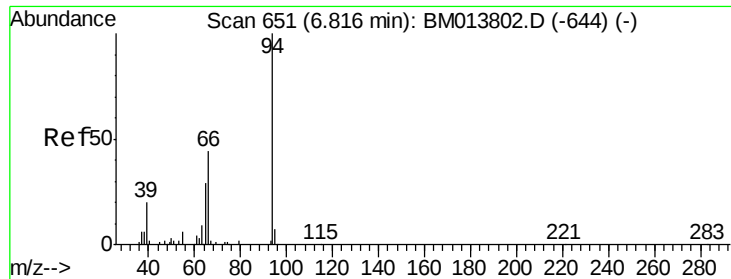

#6

Phenol

Concen: 2.725 ng/ul

RT: 6.80 min Scan# 649

Delta R.T. -0.01 min

Lab File: BM013813.D

Acq: 25 Jan 2018 19:37

Instrument :


BNA_M

ClientSampleId :

F6B10

Tot Ion: 94 Resp: 22486




Ion	Ratio	Lower	Upper
94	100		
65	34.9	28.2	42.4
66	57.2	47.2	70.8

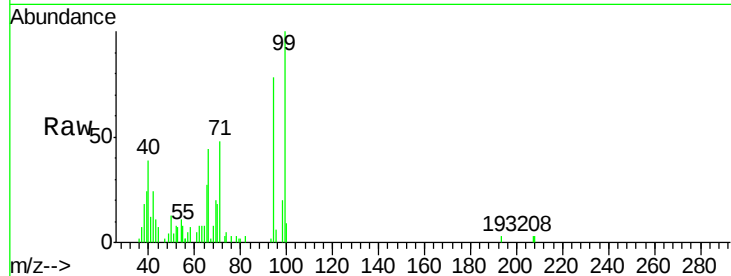

Abundance Ion 94.00 (93.70 to 94.70): BM013802.D (-644) (-)

Ion 65.00 (64.70 to 65.70): BM013802.D (-644) (-)

Ion 66.00 (65.70 to 66.70): BM013802.D (-644) (-)

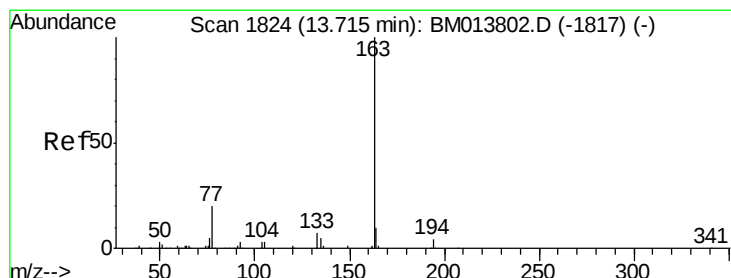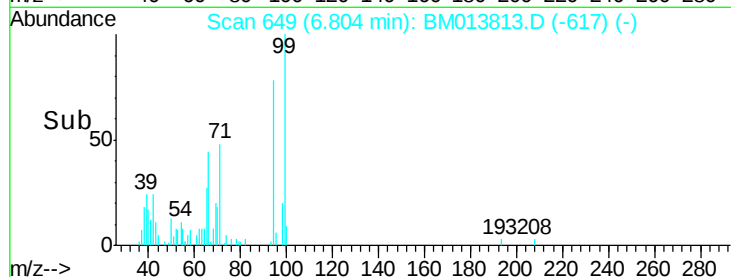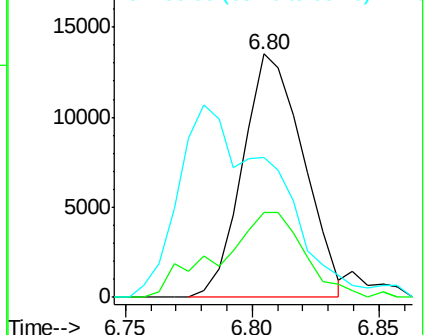

#44

Dimethylphthalate

Concen: 16.548 ng/ul

RT: 13.71 min Scan# 1823


Delta R.T. -0.01 min

Lab File: BM013813.D

Acq: 25 Jan 2018 19:37

Tgt Ion: 163 Resp: 281526



Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.5	5.3
164	10.1	8.2	12.4

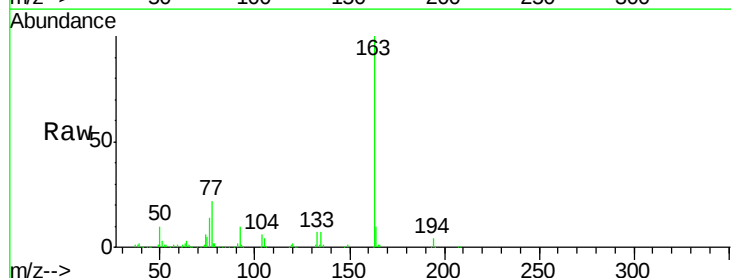


Abundance Ion 163.00 (162.70 to 163.70): BM013802.D (-1817) (-)

Ion 194.00 (193.70 to 194.70): BM013802.D (-1817) (-)

Ion 164.00 (163.70 to 164.70): BM013802.D (-1817) (-)

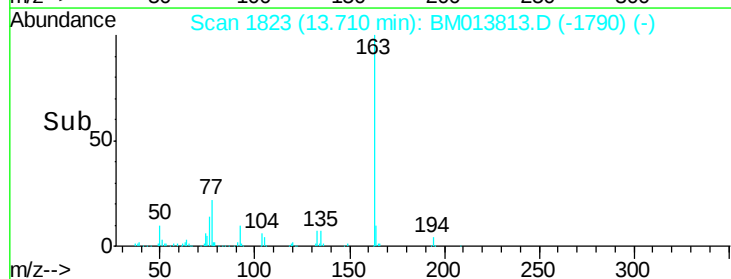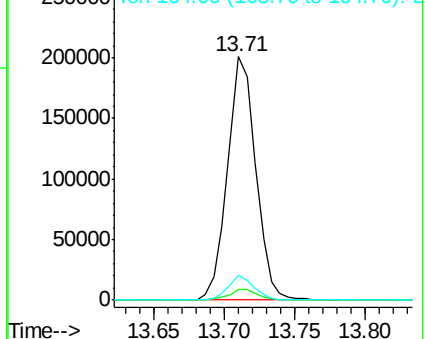


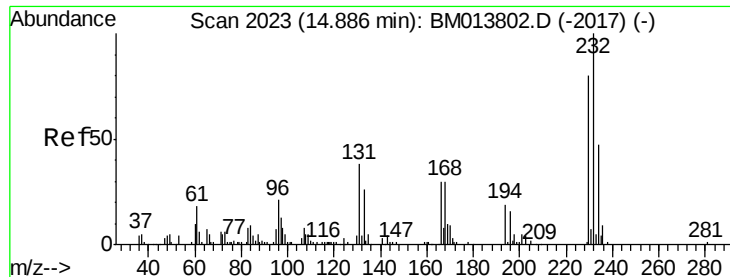




#55
 2,3,4,6-Tetrachlorophenol
 Concen: 4.759 ng/ul
 RT: 14.89 min Scan# 2024
 Delta R.T. 0.01 min
 Lab File: BM013813.D
 Acq: 25 Jan 2018 19:37

Instrument :
 BNA_M
 ClientSampleId :
 F6B10

Tot Ion:232	Resp:	20974
Ion Ratio	Lower	Upper
232	100	
131	48.1	29.0 43.4#
130	2.6	2.0 3.0
166	23.3	21.4 32.2

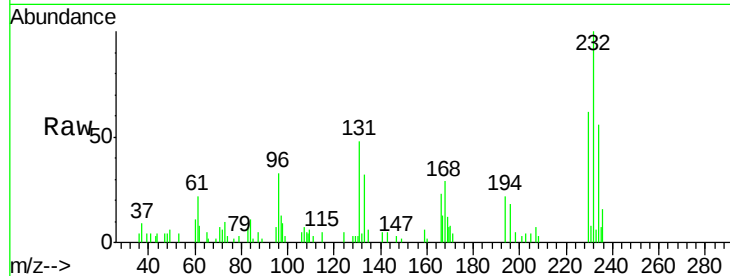


Abundance Ion 232.00 (231.70 to 232.70): E
 Ion 131.00 (130.70 to 131.70): E
 Ion 130.00 (129.70 to 130.70): E
 Ion 166.00 (165.70 to 166.70): E

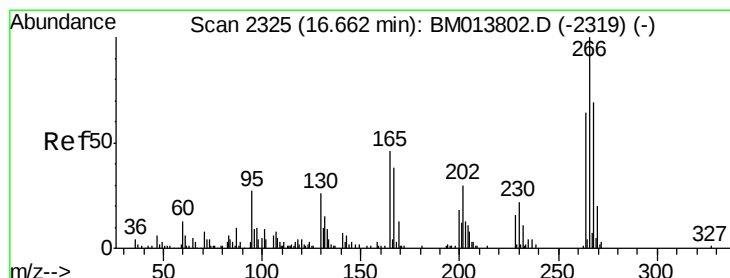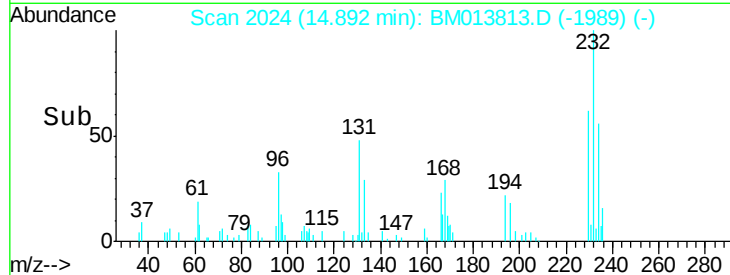
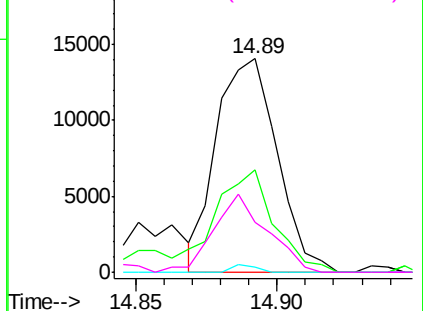



#68
 Pentachlorophenol
 Concen: 148.477 ng/ul
 RT: 16.66 min Scan# 2324
 Delta R.T. -0.01 min
 Lab File: BM013813.D
 Acq: 25 Jan 2018 19:37

Tgt Ion:266	Resp:	482504
Ion Ratio	Lower	Upper
266	100	
264	64.5	49.3 73.9
268	67.1	52.6 78.8

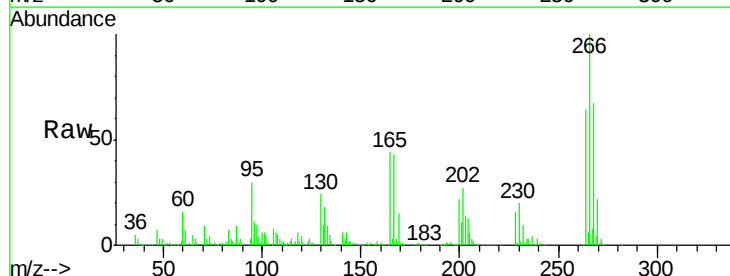

Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

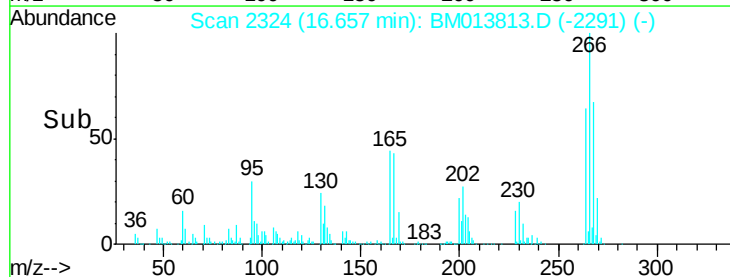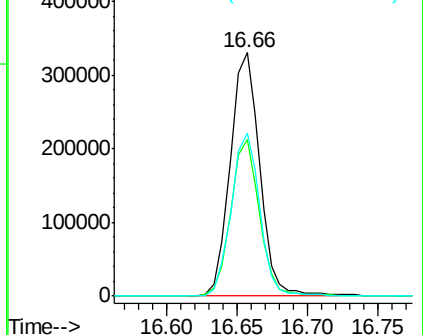

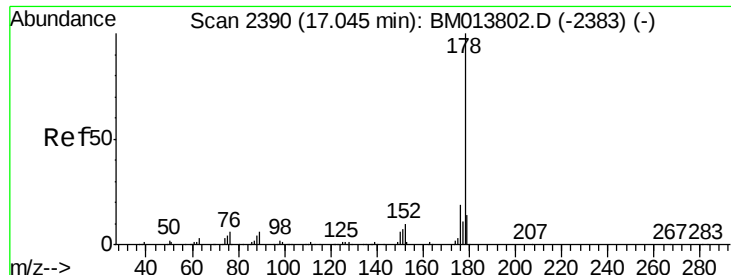

#69

Phenanthrene

Concen: 1.648 ng/ul

RT: 17.04 min Scan# 2389

Delta R.T. -0.01 min

Lab File: BM013813.D

Acq: 25 Jan 2018 19:37

Instrument :

BNA_M

ClientSampleId :

F6B10


Tot Ion:178 Resp: 44052

Ion Ratio Lower Upper

178 100

179 17.0 12.6 19.0

176 16.7 14.9 22.3

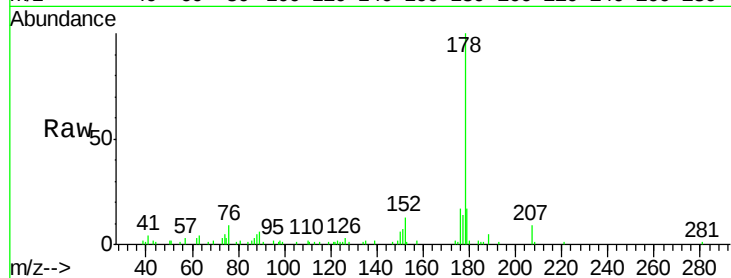

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

