

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012518\
 Data File : BM013827.D
 Acq On : 26 Jan 2018 03:55
 Operator : SJ/JU
 Sample : J1233-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6B14

Quant Time: Jan 26 07:27:58 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 02:50:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	155693	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	571246	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	328406	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	735056	20.00	ng/ul	0.00
75) Chrysene-d12	21.20	240	815490	20.00	ng/ul	0.00
83) Perylene-d12	23.39	264	786168	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	16758	4.25	ng/uL	0.00
5) Phenol-d5	6.77	99	375641	31.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	234656	32.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	326589	33.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	300894	32.75	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	164549	37.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	184847	39.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	328801	36.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	397330	50.61	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	1030936	38.09	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	1261835	36.56	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	123838	28.15	ng/ul	0.00
57) Fluorene-d10	15.24	176	857531	36.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	143568	32.45	ng/ul	0.00
70) Anthracene-d10	17.09	188	1318535	36.83	ng/ul	0.00
76) Pyrene-d10	19.40	212	1493415	39.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.25	264	1454541	40.25	ng/ul	0.00
Target Compounds						
6) Phenol	6.80	94	43927	3.664	ng/ul	98
44) Dimethylphthalate	13.71	163	370457	13.921	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012518\
Data File : BM013827.D
Acq On : 26 Jan 2018 03:55
Operator : SJ/JU
Sample : J1233-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6B14

Quant Time: Jan 26 07:27:58 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 26 02:50:24 2018
Response via : Initial Calibration

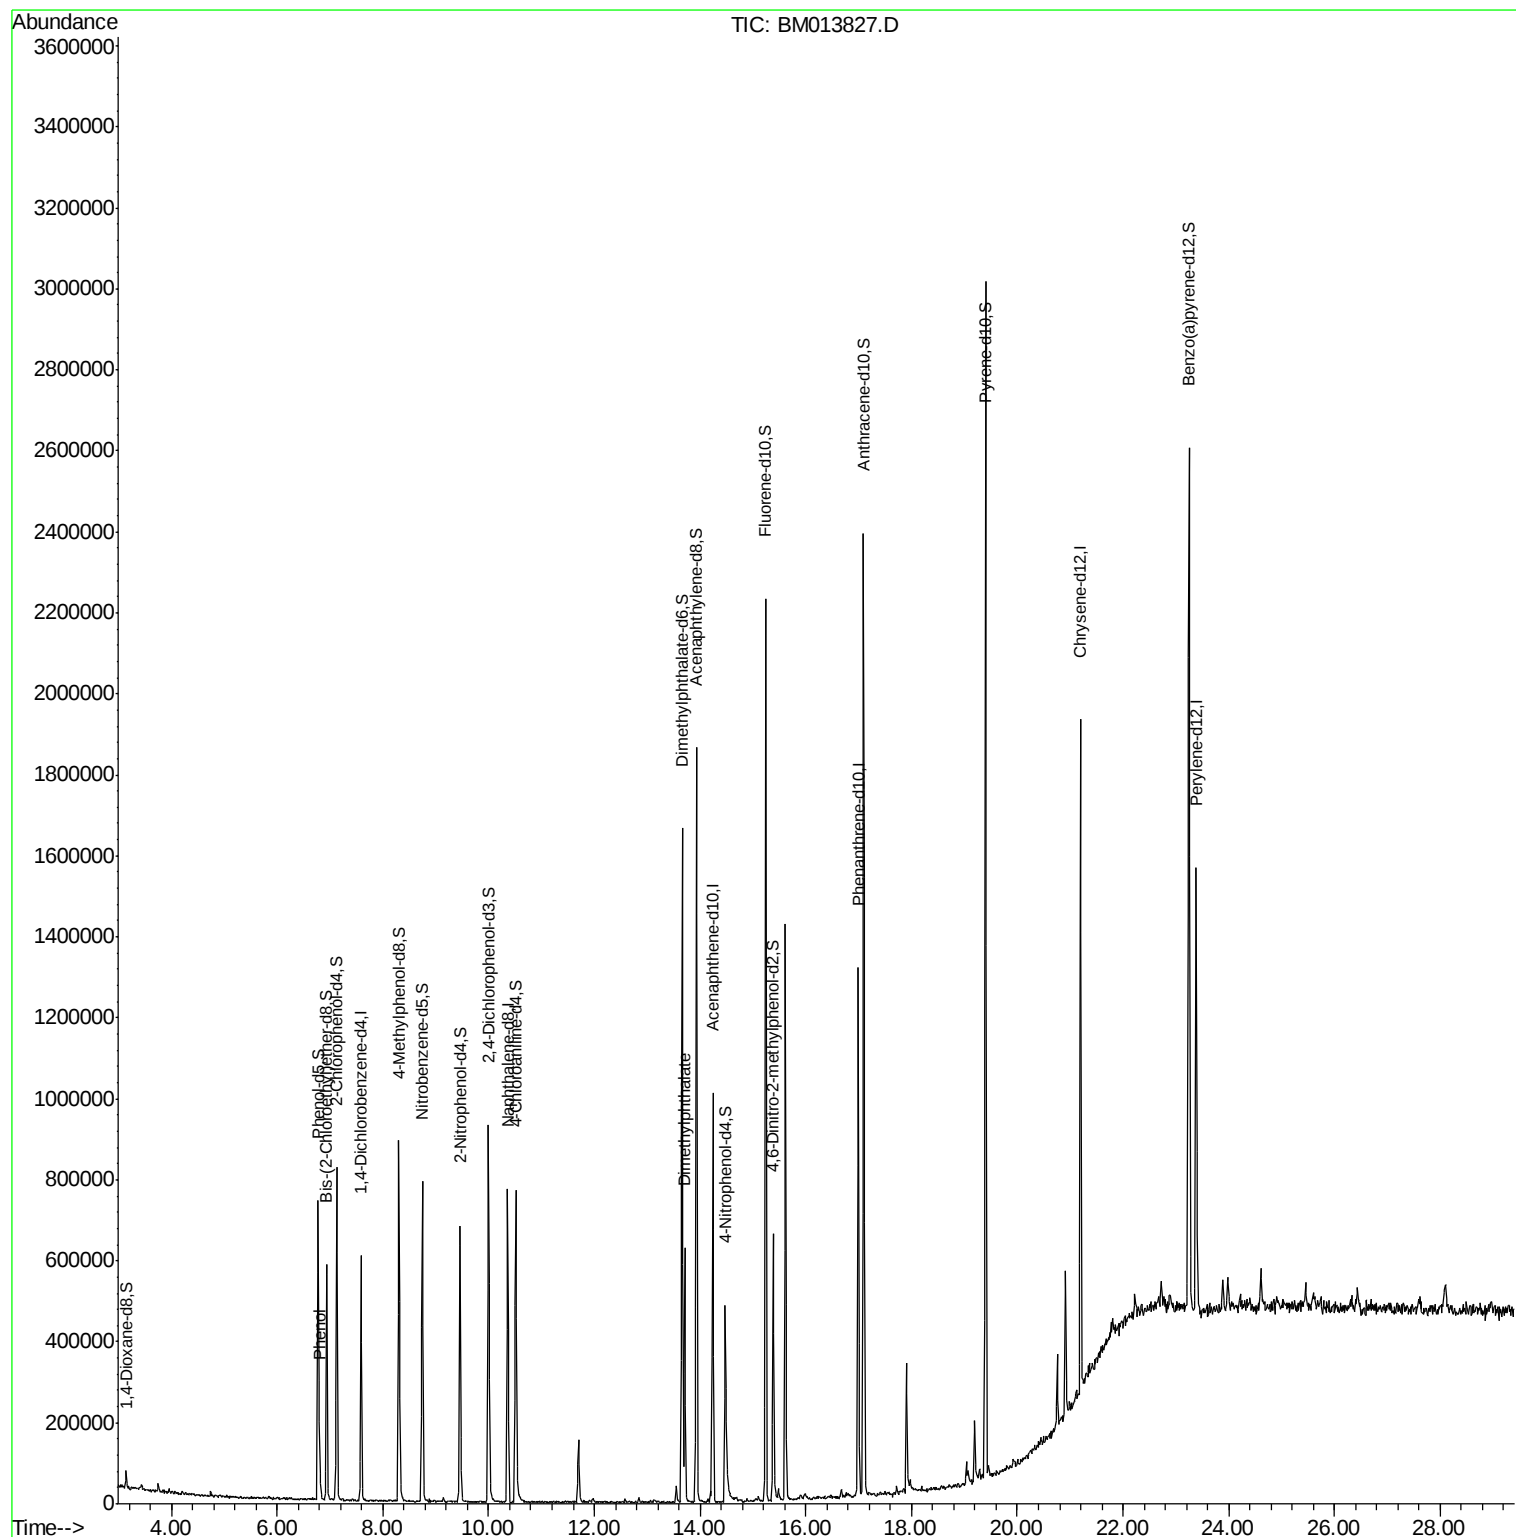

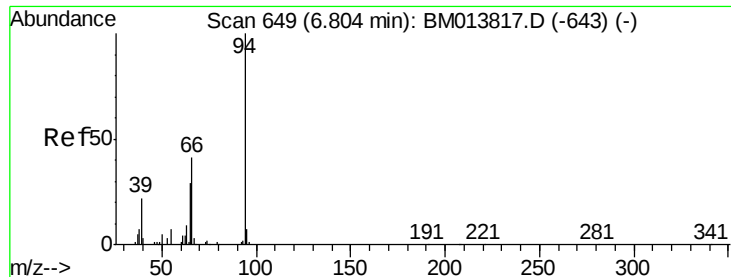

#6

Phenol

Concen: 3.664 ng/ul

RT: 6.80 min Scan# 649

Delta R.T. -0.00 min

Lab File: BM013827.D

Acq: 26 Jan 2018 03:55

Instrument :

BNA_M

ClientSampleId :

F6B14


Tot Ion: 94 Resp: 43927

Ion Ratio Lower Upper

94 100

65 37.5 28.2 42.4




66 59.5 47.2 70.8

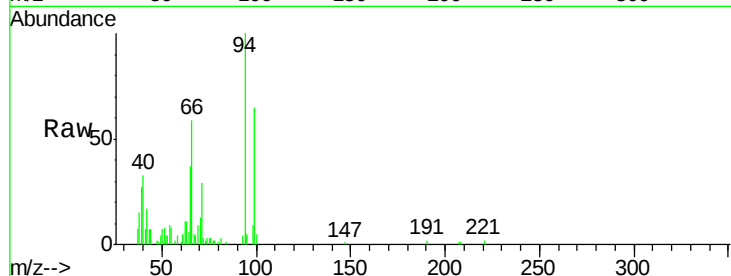

Abundance Ion 94.00 (93.70 to 94.70): BM013827.D (-615) (-)

Ion 65.00 (64.70 to 65.70): BM013827.D (-615) (-)

Ion 66.00 (65.70 to 66.70): BM013827.D (-615) (-)

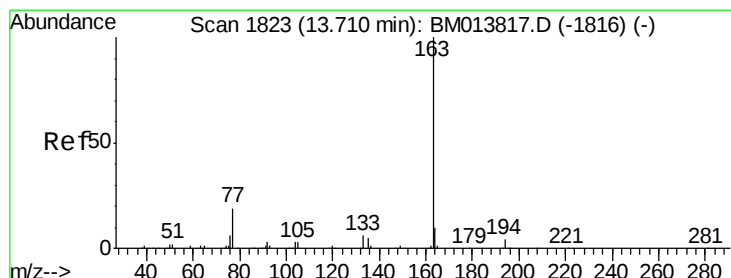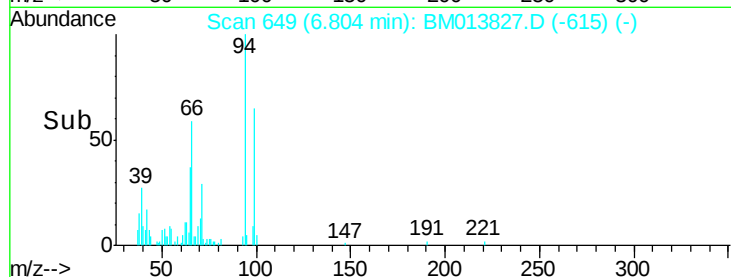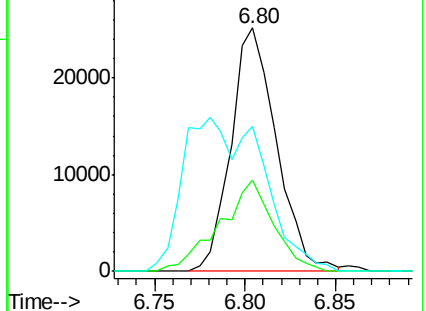

#44

Dimethylphthalate

Concen: 13.921 ng/ul

RT: 13.71 min Scan# 1823

Delta R.T. -0.00 min

Lab File: BM013827.D

Acq: 26 Jan 2018 03:55


Tgt Ion: 163 Resp: 370457

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.0 8.2 12.4

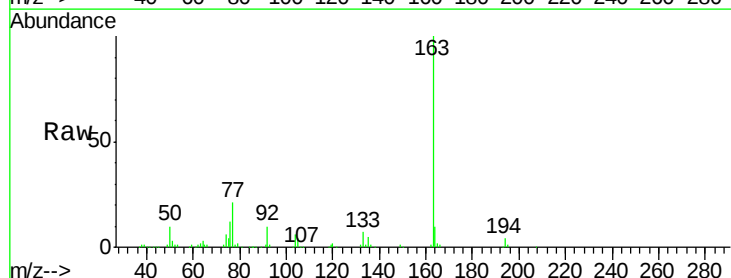

Abundance Ion 163.00 (162.70 to 163.70): BM013827.D (-1789) (-)

Ion 194.00 (193.70 to 194.70): BM013827.D (-1789) (-)

Ion 164.00 (163.70 to 164.70): BM013827.D (-1789) (-)

