
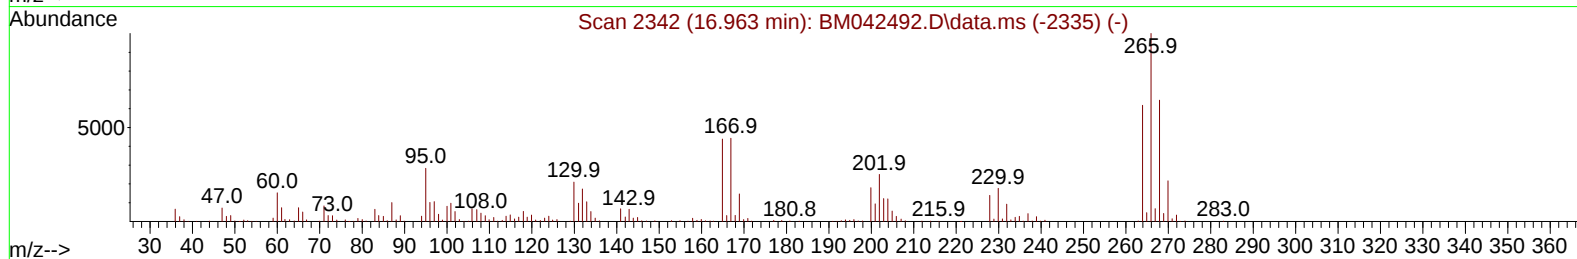
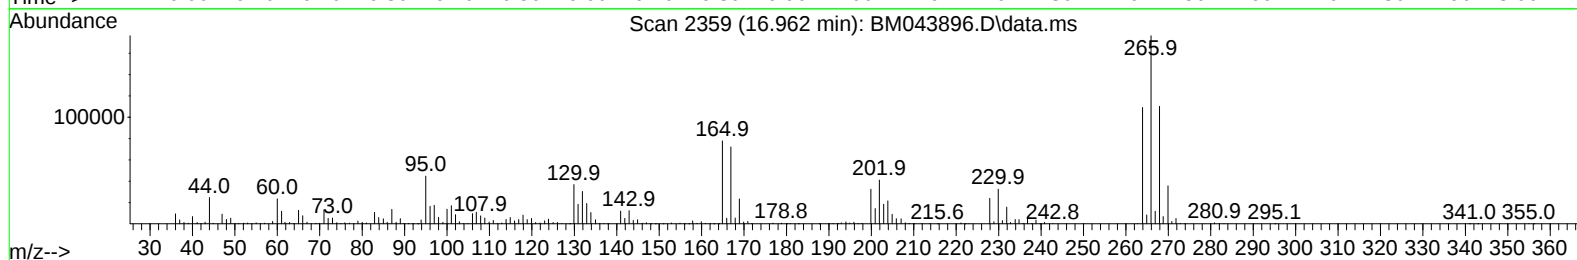


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012524\  
Data File : BM043896.D  
Acq On : 25 Jan 2024 10:31  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 12:46:34 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012524.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 09 13:21:00 2023  
Response via : Initial Calibration

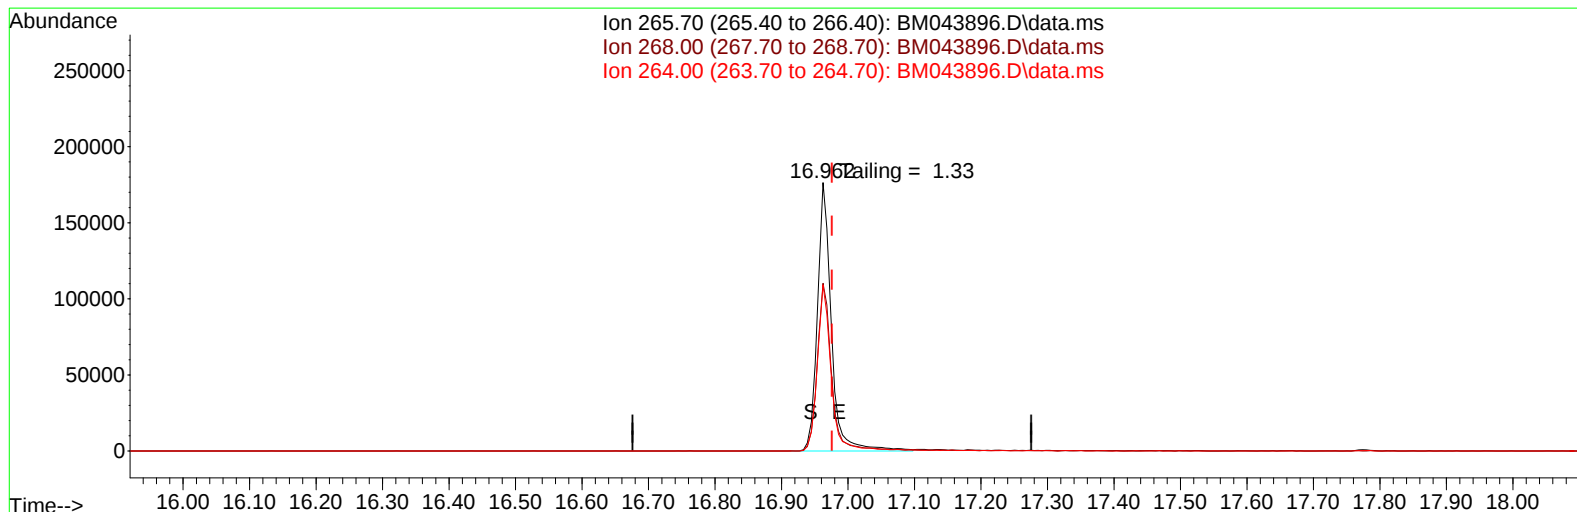

TIC: BM043896.D\data.ms

**(70) Pentachlorophenol (C)**




16.962min (-0.014) 0.00 ng m

response 258055

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.60  | 62.52  |
| 264.00 | 61.80  | 61.89  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012524\  
Data File : BM043896.D  
Acq On : 25 Jan 2024 10:31  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 12:46:34 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012524.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 09 13:21:00 2023  
Response via : Initial Calibration

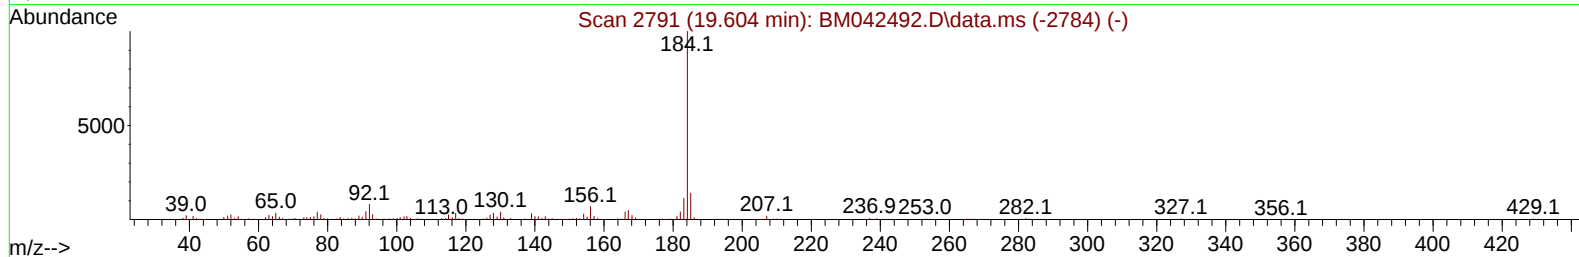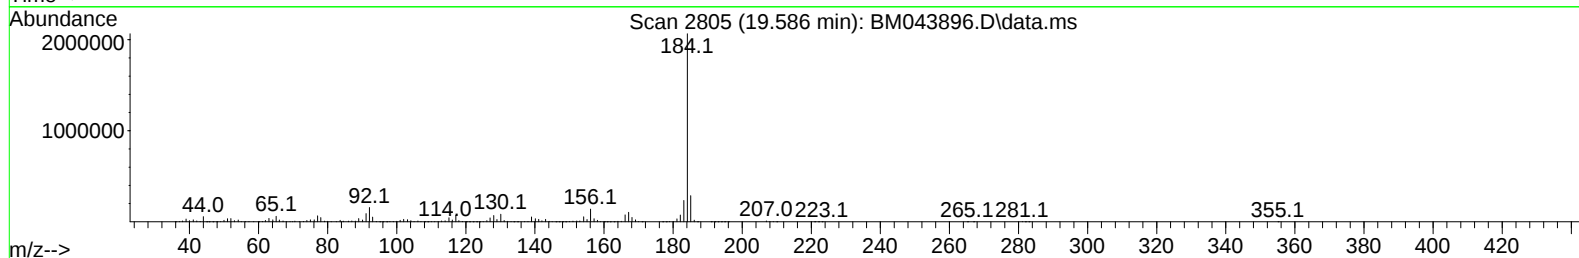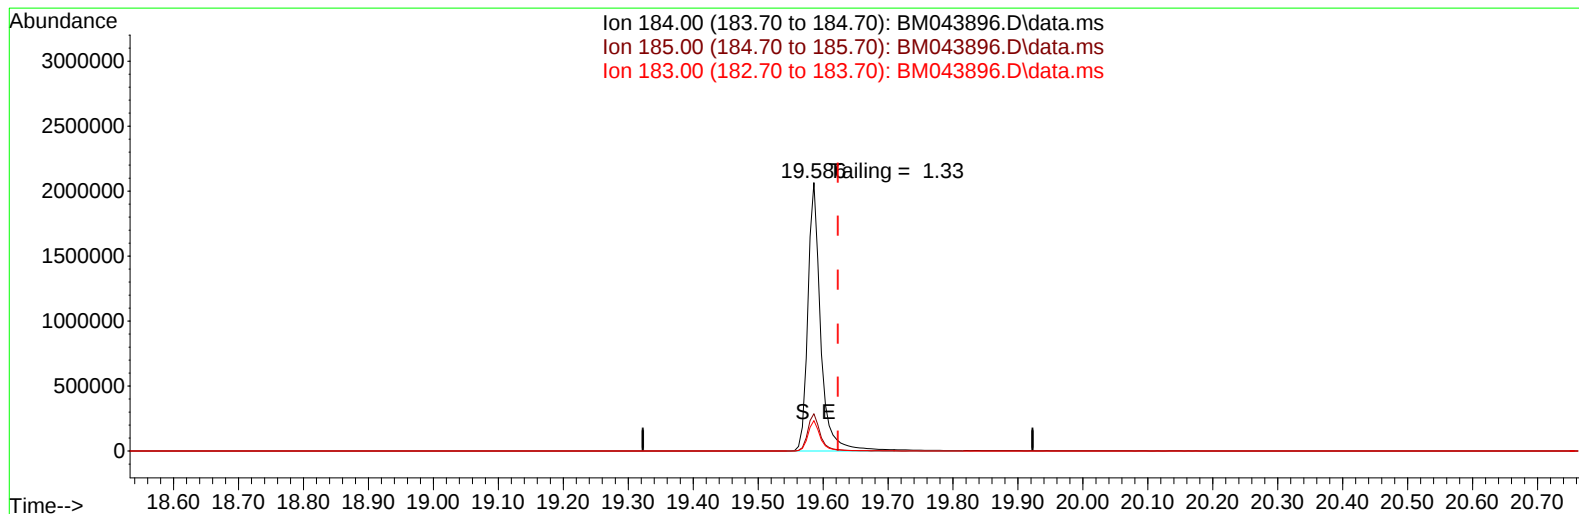

TIC: BM043896.D\data.ms

**(77) Benzidine**

19.586min (-0.037) 0.00 ng m

response 2850219

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.89  |
| 183.00 | 11.20  | 11.31  |
| 0.00   | 0.00   | 0.00   |