

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012524\
Data File : BM043906.D
Acq On : 25 Jan 2024 16:42
Operator : MA/JU
Sample : PB158578BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158578BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012524.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM043906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	402	409	425	rBV	5477656	7738848	56.63%	11.474%
2	7.087	672	680	692	rBV	5160009	7830876	57.30%	11.610%
3	7.922	815	822	829	rVB	1192700	1865163	13.65%	2.765%
4	9.093	1013	1021	1030	rBV	2934245	4762469	34.85%	7.061%
5	10.728	1291	1299	1307	rVB	1459085	2446027	17.90%	3.626%
6	13.192	1711	1718	1726	rBV	7035497	10162830	74.37%	15.067%
7	14.563	1943	1951	1958	rBV	2009645	2925717	21.41%	4.338%
8	16.057	2197	2205	2226	rBV	4508908	6334620	46.35%	9.392%
9	17.316	2412	2419	2429	rBV	2323458	3265943	23.90%	4.842%
10	19.962	2862	2869	2878	rBV	11188274	13665699	100.00%	20.261%
11	21.515	3128	3133	3142	rBV	2522811	3143595	23.00%	4.661%
12	23.927	3536	3543	3556	rVB	1613129	3307641	24.20%	4.904%




Sum of corrected areas: 67449428

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012524\
Data File : BM043906.D
Acq On : 25 Jan 2024 16:42
Operator : MA/JU
Sample : PB158578BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158578BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

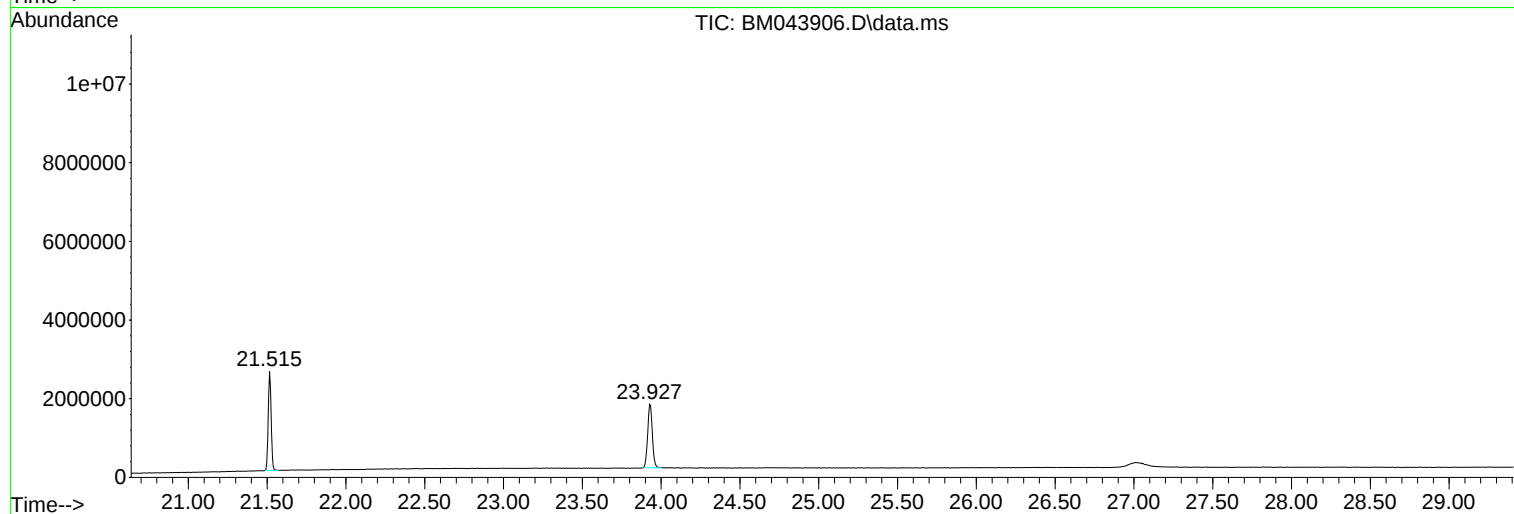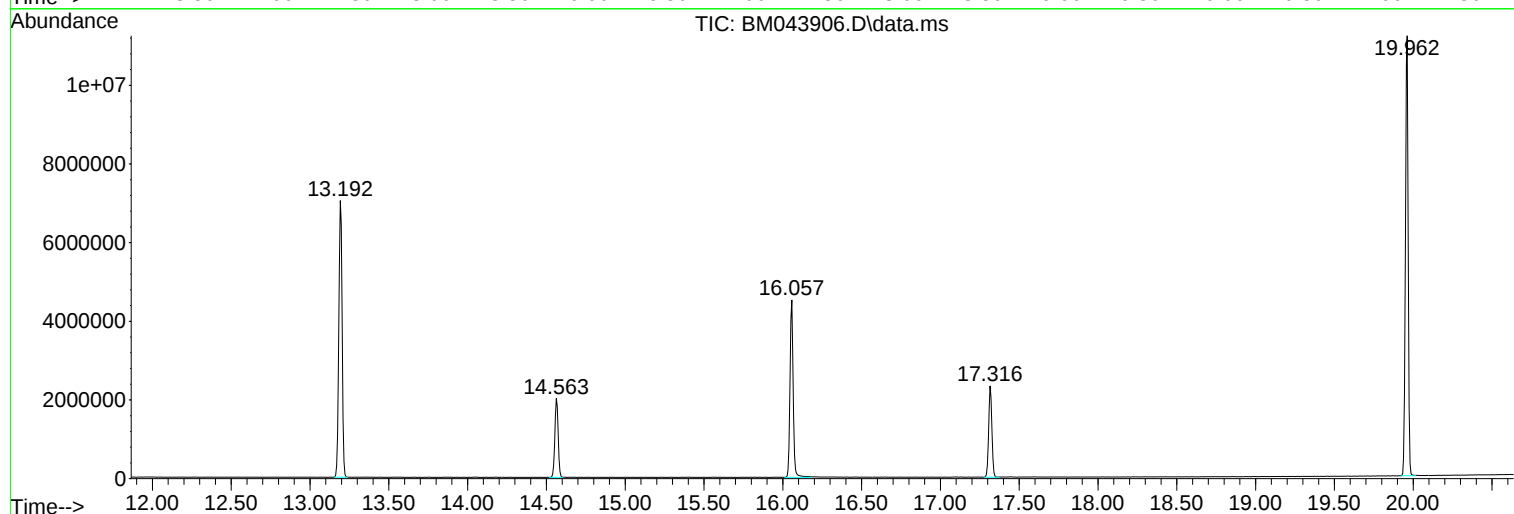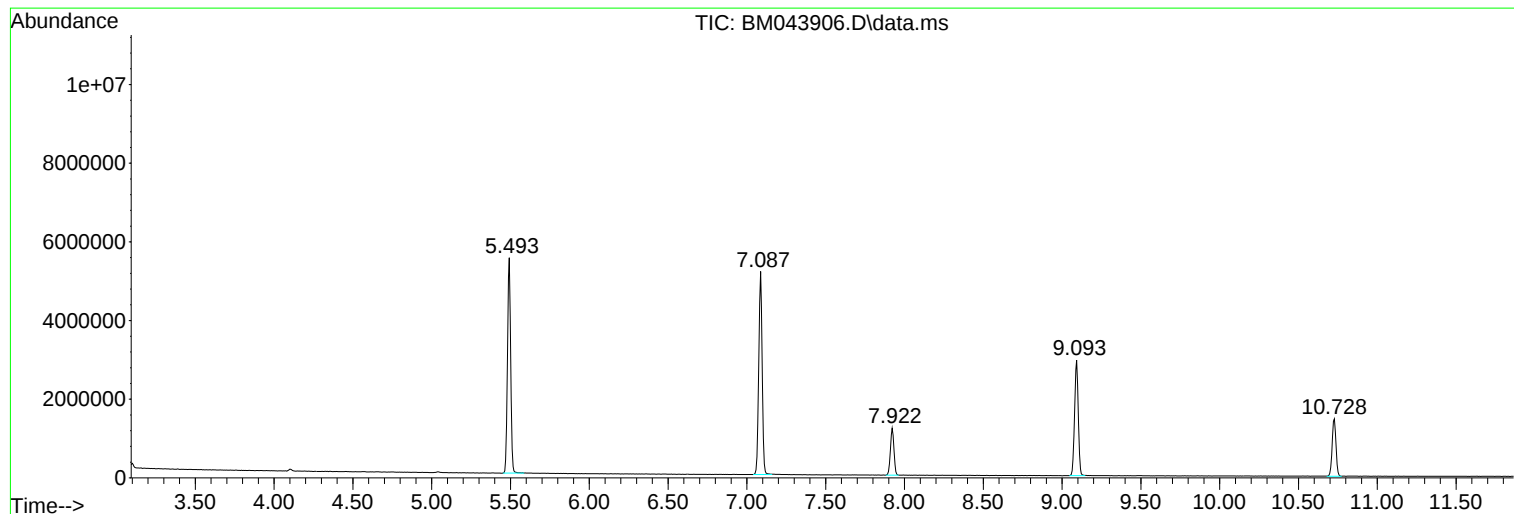

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012524\
Data File : BM043906.D
Acq On : 25 Jan 2024 16:42
Operator : MA/JU
Sample : PB158578BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158578BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012524\
Data File : BM043906.D
Acq On : 25 Jan 2024 16:42
Operator : MA/JU
Sample : PB158578BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158578BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------