


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012524\  
Data File : BM043896.D  
Acq On : 25 Jan 2024 10:31  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012524.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Jan 26 00:26:01 2024

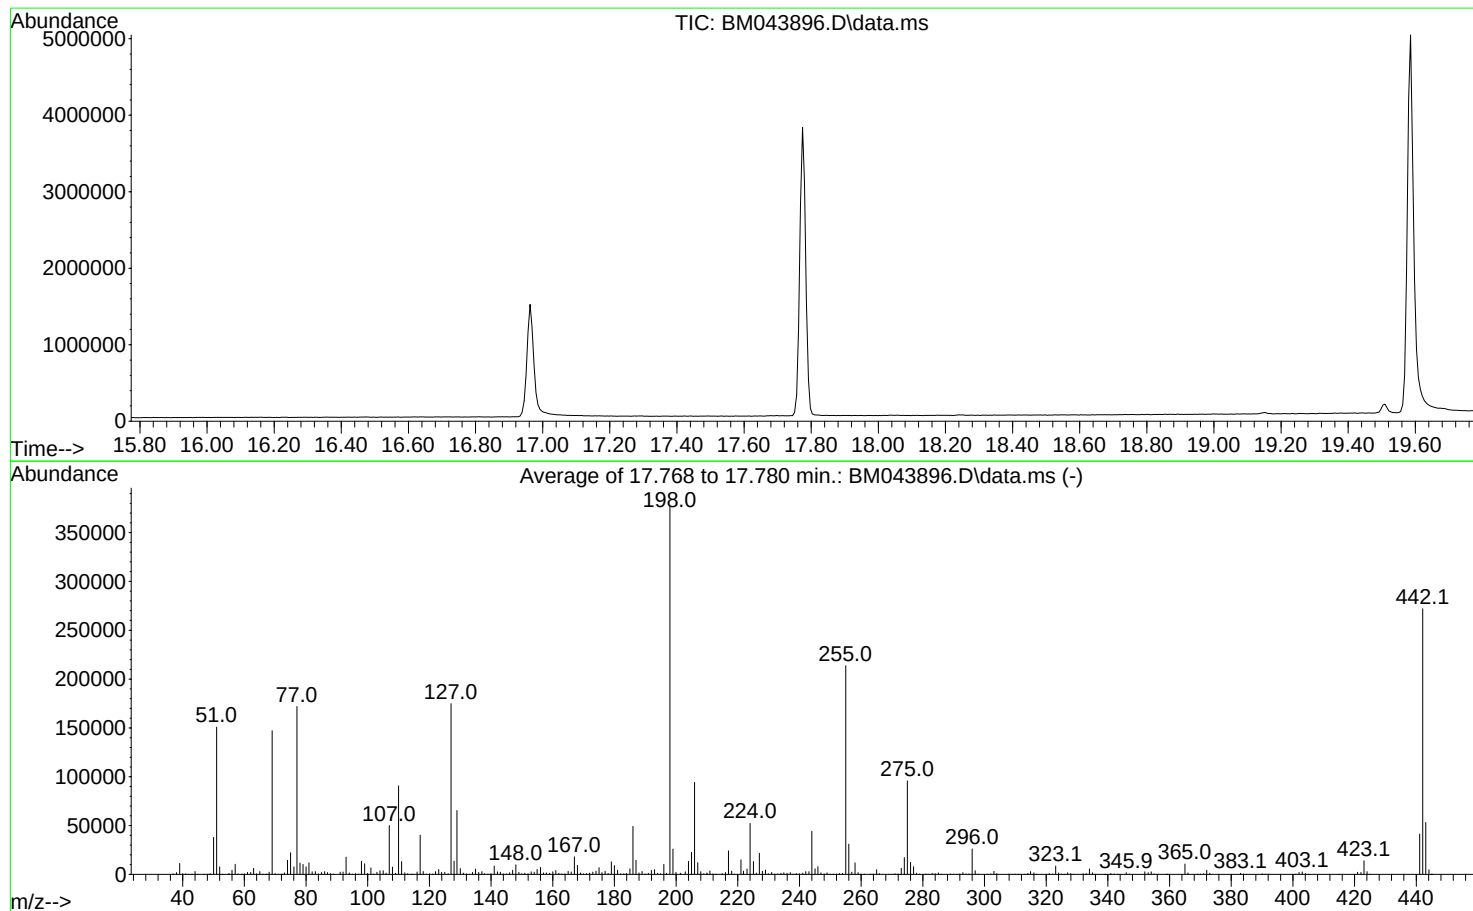




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 51     | 198     | 10     | 80     | 40.0  | 150782 | PASS      |
| 68     | 69      | 0.00   | 2      | 1.6   | 2291   | PASS      |
| 69     | 198     | 0.00   | 100    | 39.1  | 147236 | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 786    | PASS      |
| 127    | 198     | 10     | 80     | 46.4  | 174784 | PASS      |
| 197    | 198     | 0.00   | 2      | 0.3   | 1096   | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 376768 | PASS      |
| 199    | 198     | 5      | 9      | 6.9   | 25853  | PASS      |
| 275    | 198     | 10     | 60     | 25.4  | 95669  | PASS      |
| 365    | 198     | 1      | 100    | 2.8   | 10674  | PASS      |
| 441    | 198     | 0.01   | 100    | 11.0  | 41277  | PASS      |
| 442    | 442     | 50     | 100    | 100.0 | 271979 | PASS      |
| 443    | 442     | 15     | 24     | 19.5  | 53059  | PASS      |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012524\  
Data File : BM043896.D  
Acq On : 25 Jan 2024 10:31  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jan 25 12:46:34 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012524.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 09 13:21:00 2023  
Response via : Initial Calibration

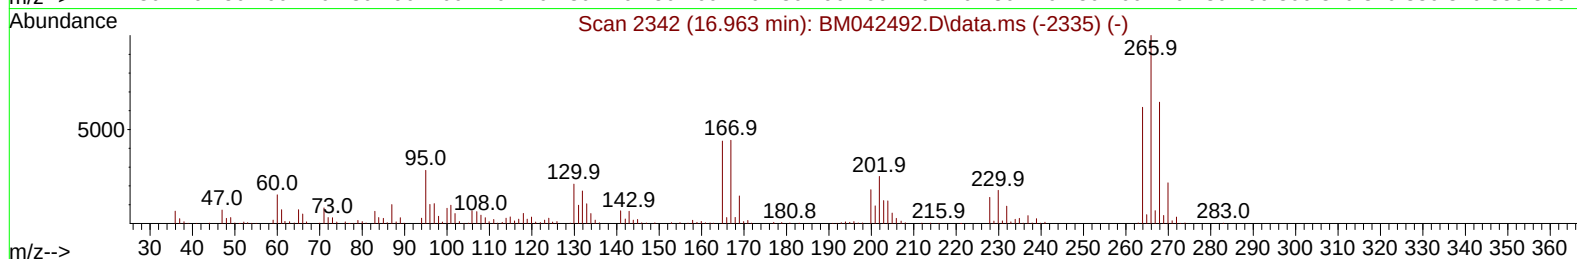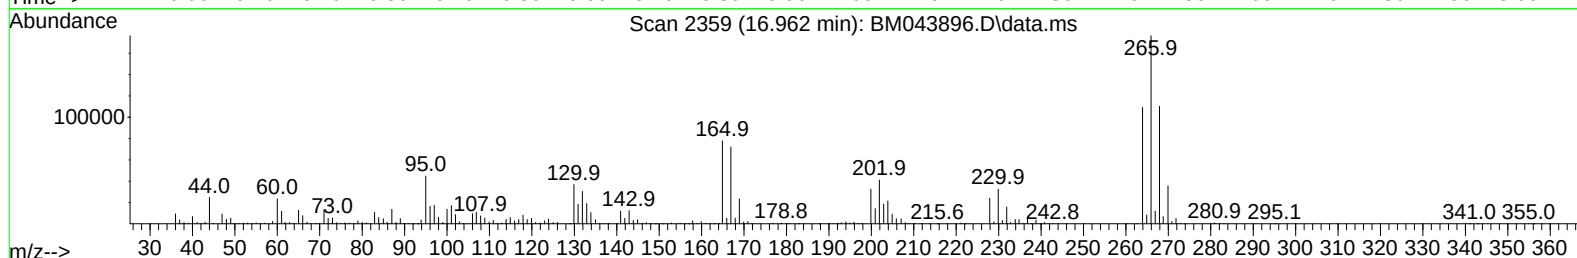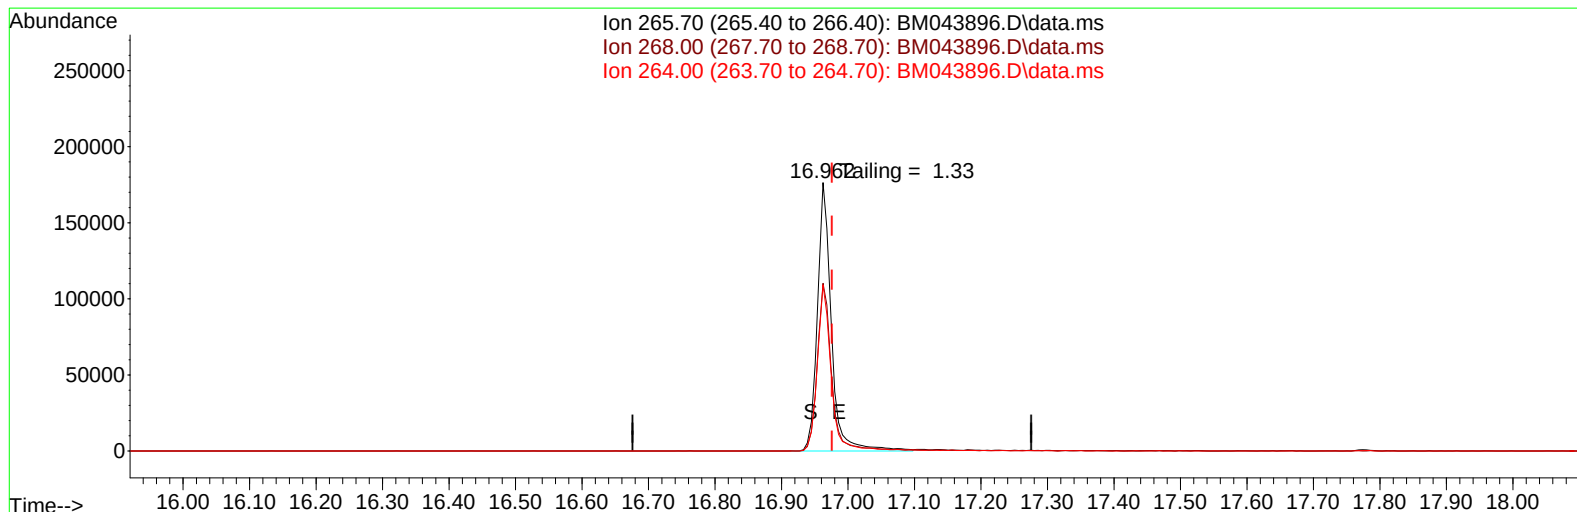

TIC: BM043896.D\data.ms

**(70) Pentachlorophenol (C)**

16.962min (-0.014) 0.00 ng m




response 258055

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.60  | 62.52  |
| 264.00 | 61.80  | 61.89  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM012524\  
 Data File : BM043896.D  
 Acq On : 25 Jan 2024 10:31  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Jan 25 12:46:34 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012524.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 09 13:21:00 2023  
 Response via : Initial Calibration

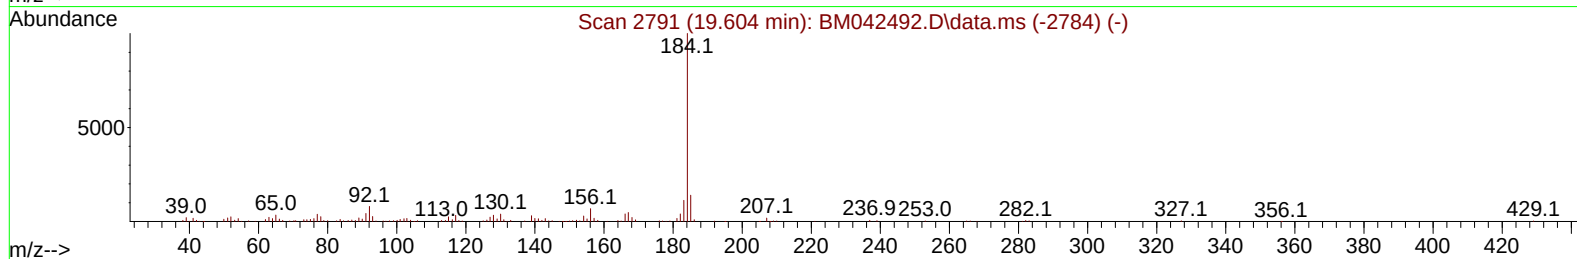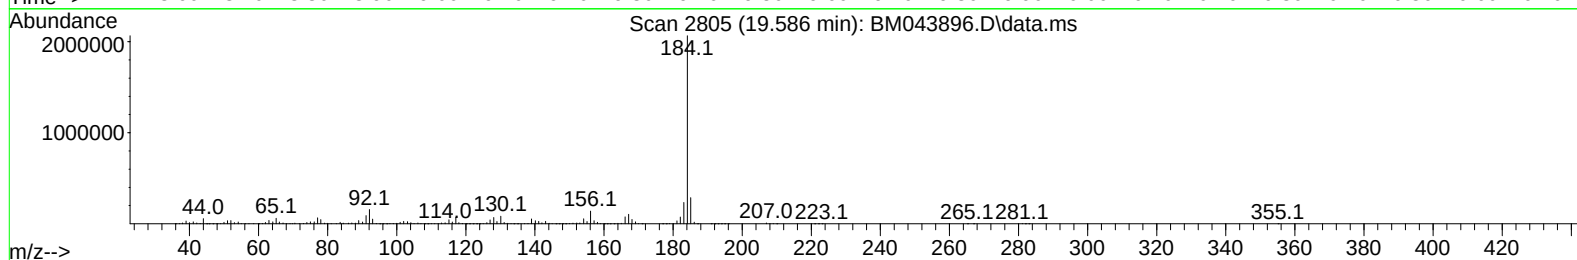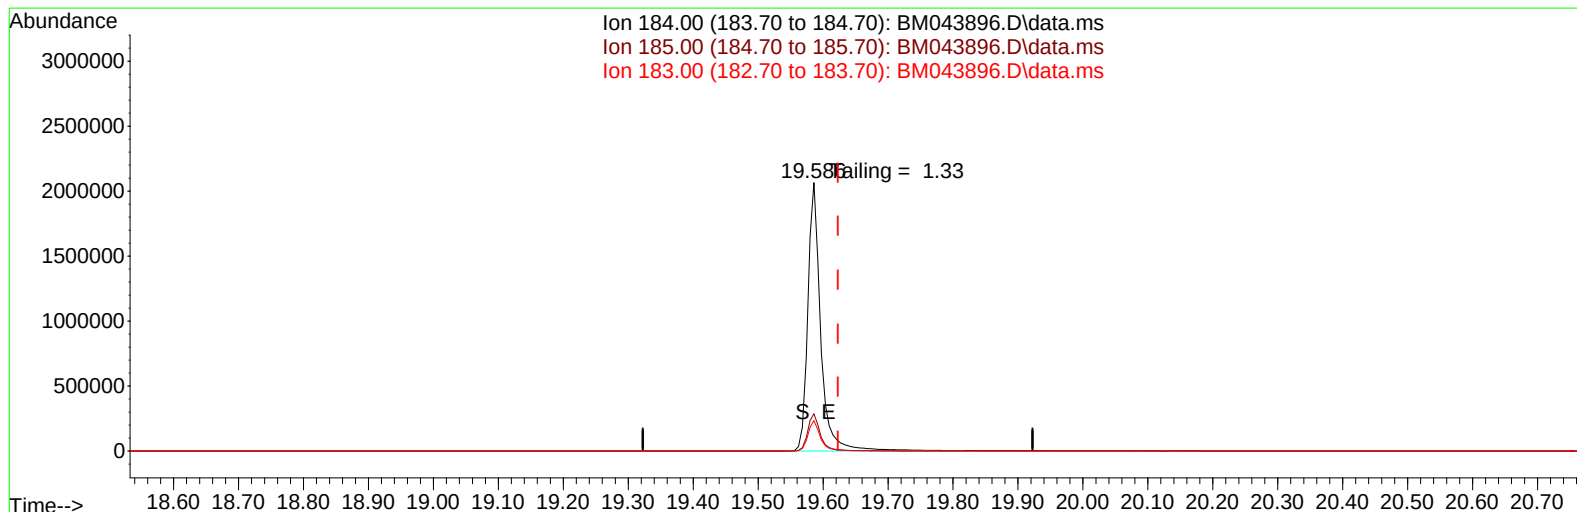

TIC: BM043896.D\data.ms

**(77) Benzidine**

19.586min (-0.037) 0.00 ng m

response 2850219

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.89  |
| 183.00 | 11.20  | 11.31  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/25/2024     | BNA_M            | <u>BM043896.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 629155           | 20.827             |
| DDD           | 6447             | 20.433             |
| DDE           | 248              | 19.515             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 6695          | 635850           | 1.05               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP