

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012615\
 Data File : BM000362.D
 Acq On : 26 Jan 2015 18:43
 Operator : TP/IZ
 Sample : G1115-03RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8RX

Quant Time: Jan 27 00:55:44 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 27 00:08:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	94052	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	354438	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	238979	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	516839	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	694821	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	748230	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	3491	1.63	ng/uL	0.00
5) Phenol-d5	6.93	99	40386	5.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	138208	25.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	111696	19.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	64769	10.55	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	77854	29.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	69710	28.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	115680	21.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	305	0.05	ng/ul	-0.12
43) Dimethylphthalate-d6	13.82	166	512400	29.86	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	667502	31.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	16973	5.98	ng/ul	0.00
57) Fluorene-d10	15.40	176	512204	33.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	76857	28.19	ng/ul	0.00
70) Anthracene-d10	17.25	188	868411	35.38	ng/ul	0.00
76) Pyrene-d10	19.55	212	1057948	34.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	1066468	31.34	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.82	165	4283	1.33	ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012615\
Data File : BM000362.D
Acq On : 26 Jan 2015 18:43
Operator : TP/IZ
Sample : G1115-03RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8RX

Quant Time: Jan 27 00:55:44 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 27 00:08:46 2015
Response via : Initial Calibration

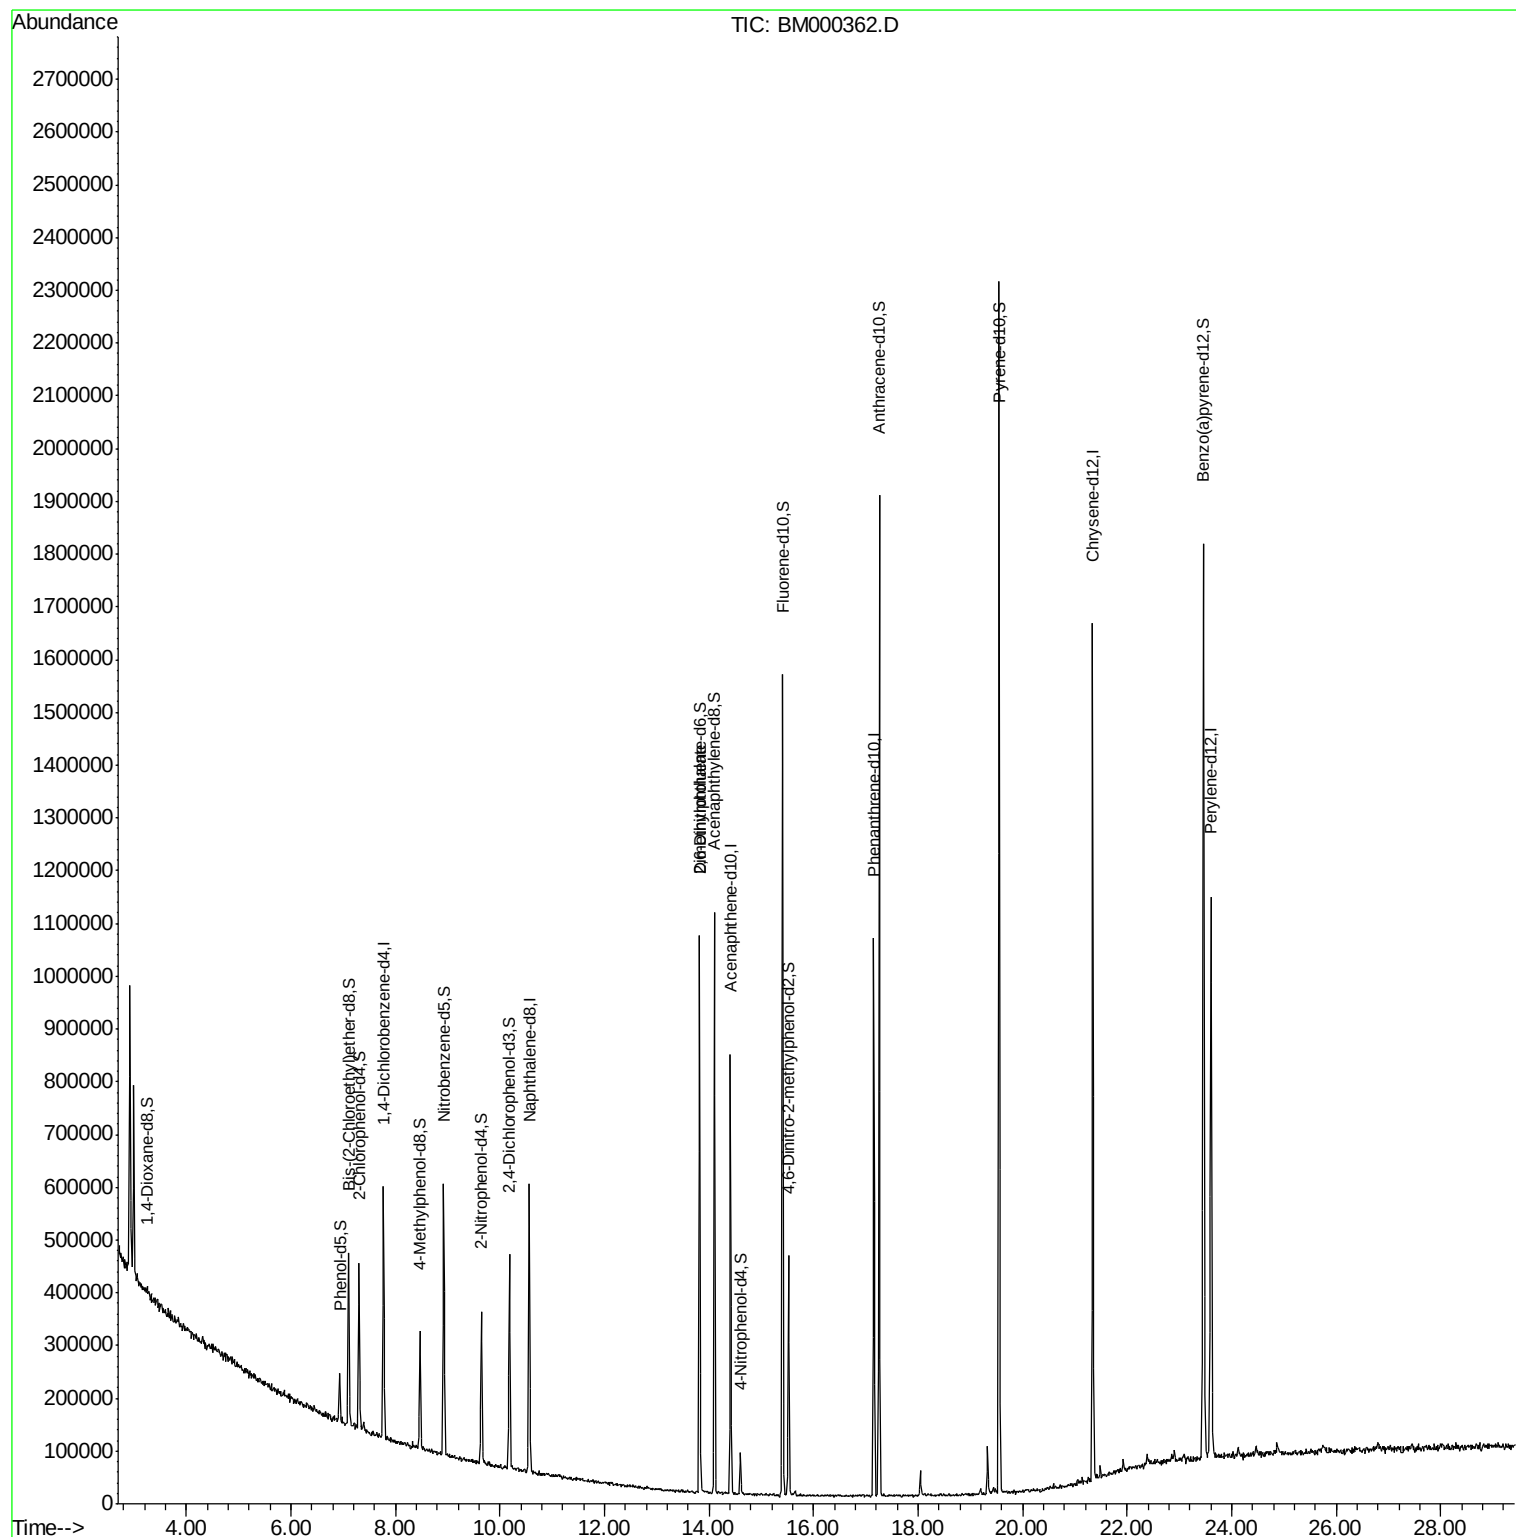

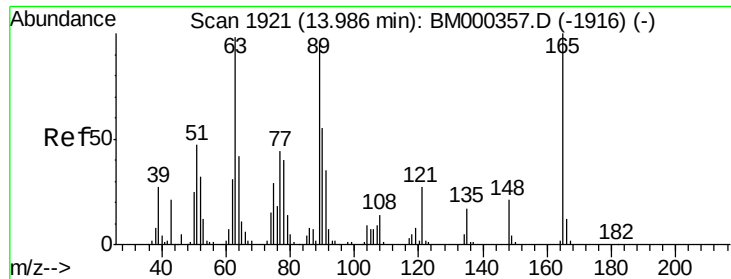

#45

2,6-Dinitrotoluene

Concen: 1.33 ng/ul

RT: 13.82 min Scan# 1893

Delta R.T. -0.16 min

Lab File: BM000362.D


Acq: 26 Jan 2015 18:43

Instrument :

BNA_M

ClientSampleId :

C0AK8RX

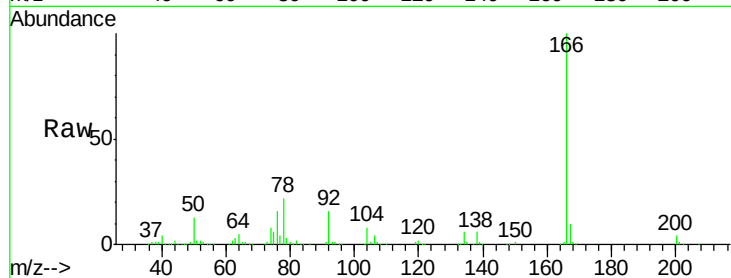

Tgt Ion:	165	Resp:	4283
Ion Ratio	Lower	Upper	
165	100		
89	0.0	69.5	104.3#
121	38.7	22.3	33.5#

