


Data Path : Z:\HPCHEM1\BNA_M\Data\BM012615\
Data File : BM000356b.D
Acq On : 26 Jan 2015 10:55
Operator : TP/IZ
Sample : DFTPP12
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP12

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM012315.M
Title : SVOA CALIBRATION
Last Update : Mon Jan 26 13:29:32 2015

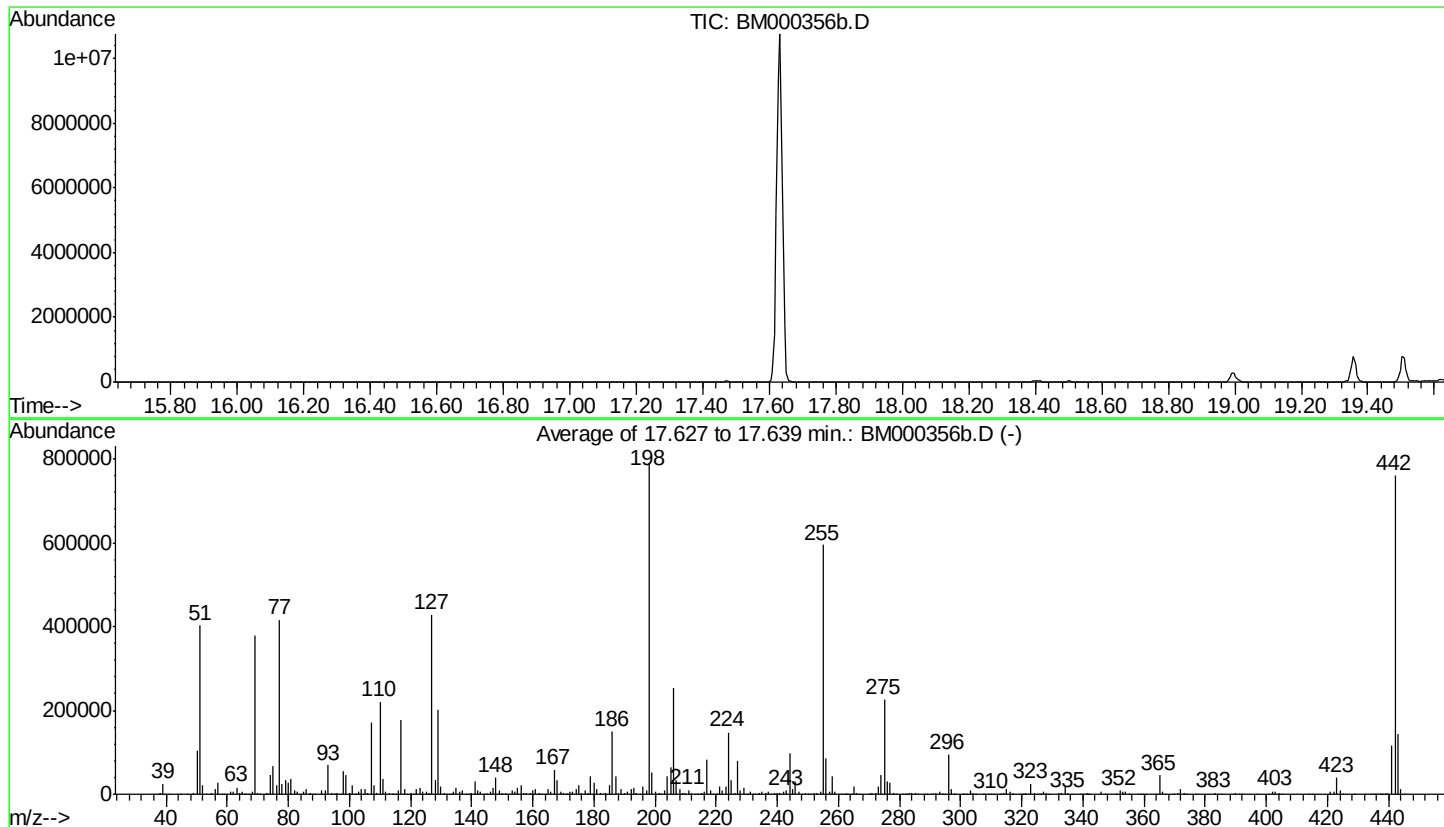

AutoFind: Scans 2540, 2541, 2542; Background Corrected with Scan 2533

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	403029	PASS
68	69	0.00	2	1.9	7159	PASS
69	198	0.00	100	47.8	378112	PASS
70	69	0.00	2	0.6	2095	PASS
127	198	10	80	54.1	428458	PASS
197	198	0.00	2	1.0	7921	PASS
198	198	100	100	100.0	791573	PASS
199	198	5	9	6.4	50978	PASS
275	198	10	60	28.4	224853	PASS
365	198	1	100	5.7	45357	PASS
441	443	0.01	100	80.0	115800	PASS
442	198	50	100	96.0	760106	PASS
443	442	15	24	19.0	144765	PASS