

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012617\
 Data File : BM008882.D
 Acq On : 26 Jan 2017 19:12
 Operator : SJ/MA
 Sample : PB96345BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	129	135	140	rBV4	28620	41835	2.17%	0.183%
2	7.075	753	763	771	rBV	492734	788953	40.83%	3.443%
3	7.257	787	794	801	rBV	310902	469085	24.28%	2.047%
4	7.457	821	828	835	rVB	481527	767195	39.71%	3.348%
5	7.928	902	908	914	rBV	369232	588753	30.47%	2.569%
6	8.622	1018	1026	1032	rBV	531316	859692	44.49%	3.752%
7	9.092	1100	1106	1117	rVB	490580	814065	42.13%	3.553%
8	9.810	1221	1228	1237	rVB	452547	729835	37.77%	3.185%
9	10.345	1311	1319	1327	rBV	555036	936169	48.45%	4.086%
10	10.733	1376	1385	1393	rVB2	421307	725032	37.52%	3.164%
11	10.869	1401	1408	1419	rVB	517042	879672	45.53%	3.839%
12	13.968	1928	1935	1941	rBV	954902	1226683	63.49%	5.353%
13	14.263	1978	1985	1993	rVB	825159	1237705	64.06%	5.401%
14	14.563	2030	2036	2043	rBV	596607	889149	46.02%	3.880%
15	14.745	2061	2067	2079	rBV	543818	791106	40.94%	3.452%
16	15.557	2198	2205	2214	rBV	1141079	1561250	80.80%	6.813%
17	15.668	2218	2224	2230	rBV	428078	573170	29.66%	2.501%
18	17.309	2497	2503	2509	rBV	768494	1059807	54.85%	4.625%
19	17.409	2512	2520	2527	rBV	1220079	1710330	88.52%	7.464%
20	19.697	2903	2909	2917	rBV	1473702	1932166	100.00%	8.432%
21	21.480	3206	3212	3218	rBV	1001157	1284481	66.48%	5.606%
22	23.074	3481	3483	3488	rVB5	51369	57224	2.96%	0.250%
23	23.685	3581	3587	3595	rVB2	937433	1831886	94.81%	7.995%
24	23.838	3606	3613	3621	rBV2	576603	1159008	59.98%	5.058%


Sum of corrected areas: 22914251

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012617\
Data File : BM008882.D
Acq On : 26 Jan 2017 19:12
Operator : SJ/MA
Sample : PB96345BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK45

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

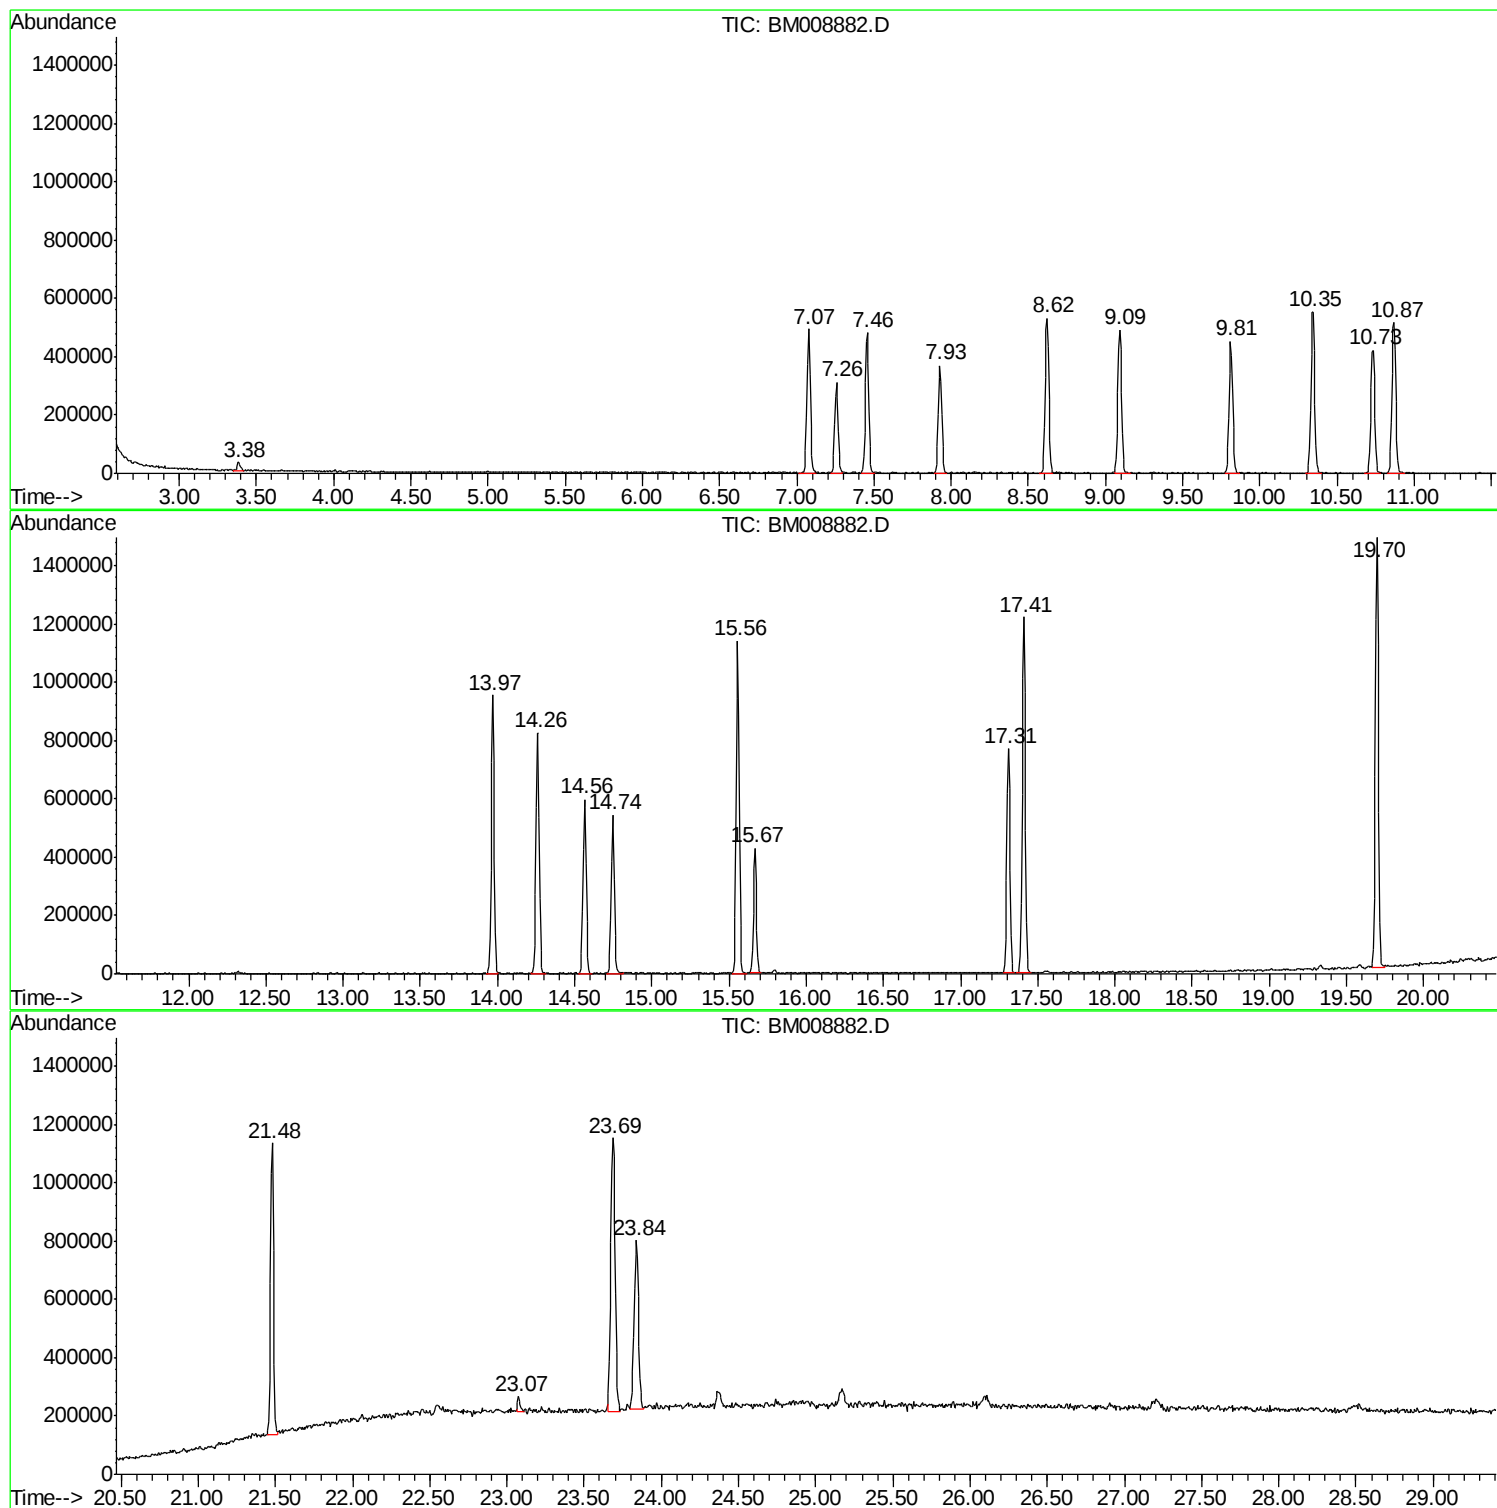

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012617\
Data File : BM008882.D
Acq On : 26 Jan 2017 19:12
Operator : SJ/MA
Sample : PB96345BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK45

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM012617\
Data File : BM008882.D
Acq On : 26 Jan 2017 19:12
Operator : SJ/MA
Sample : PB96345BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK45

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc