

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012617\
 Data File : BM008891.D
 Acq On : 27 Jan 2017 00:37
 Operator : SJ/MA
 Sample : I1426-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDMY0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	133	136	141	rVB4	15145	19071	1.14%	0.092%
2	7.075	757	763	774	rVB2	415391	729186	43.48%	3.516%
3	7.257	787	794	803	rBV	240844	395056	23.56%	1.905%
4	7.451	821	827	834	rVB	408114	637680	38.02%	3.075%
5	7.928	901	908	914	rBV	402257	645599	38.50%	3.113%
6	8.616	1019	1025	1032	rVB	422333	685760	40.89%	3.307%
7	9.092	1099	1106	1114	rBV	402418	676054	40.31%	3.260%
8	9.463	1163	1169	1173	rVB2	15456	23170	1.38%	0.112%
9	9.810	1221	1228	1239	rVB2	354943	578789	34.51%	2.791%
10	10.339	1311	1318	1326	rBV2	468711	756825	45.13%	3.649%
11	10.728	1378	1384	1391	rVB	457705	779781	46.50%	3.760%
12	10.869	1402	1408	1414	rBV3	88872	150532	8.98%	0.726%
13	13.969	1928	1935	1939	rBV	673425	923802	55.08%	4.454%
14	14.016	1939	1943	1950	rVB	223042	310088	18.49%	1.495%
15	14.257	1978	1984	1992	rVB	728855	1040638	62.05%	5.018%
16	14.439	2011	2015	2019	rBV3	16368	18724	1.12%	0.090%
17	14.563	2030	2036	2045	rVB	623317	928684	55.38%	4.478%
18	14.745	2060	2067	2073	rBV	368212	501442	29.90%	2.418%
19	15.345	2164	2169	2172	rBV	24025	27290	1.63%	0.132%
20	15.392	2174	2177	2183	rVB3	36232	43704	2.61%	0.211%
21	15.557	2198	2205	2211	rBV	894426	1297553	77.37%	6.257%
22	15.669	2218	2224	2231	rBV	261447	365262	21.78%	1.761%
23	15.792	2239	2245	2249	rBV2	20088	36762	2.19%	0.177%
24	16.251	2318	2323	2332	rBV3	45216	83701	4.99%	0.404%
25	17.045	2451	2458	2463	rBV2	44989	62469	3.72%	0.301%
26	17.092	2463	2466	2472	rVB6	12603	19974	1.19%	0.096%
27	17.310	2496	2503	2508	rBV	814417	1137234	67.81%	5.484%
28	17.404	2511	2519	2526	rBV2	1011848	1469080	87.60%	7.084%
29	17.668	2561	2564	2572	rVB6	15065	29470	1.76%	0.142%
30	17.780	2576	2583	2587	rBV2	37076	52454	3.13%	0.253%
31	18.174	2646	2650	2655	rBV4	69268	90889	5.42%	0.438%
32	18.474	2697	2701	2704	rVB2	28778	35670	2.13%	0.172%
33	19.104	2805	2808	2812	rBV6	10856	18214	1.09%	0.088%
34	19.333	2843	2847	2850	rBV6	14743	17119	1.02%	0.083%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012617\
Data File : BM008891.D
Acq On : 27 Jan 2017 00:37
Operator : SJ/MA
Sample : I1426-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDMY0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Title : SVOA CALIBRATION

35	19.451	2863	2867	2871	rBV5	40248	57960	3.46%	0.279%
36	19.698	2902	2909	2915	rBV	1172014	1677061	100.00%	8.087%
37	21.162	3155	3158	3163	rBV3	110093	131931	7.87%	0.636%
38	21.474	3206	3211	3217	rBV	1086354	1430994	85.33%	6.900%
39	22.539	3390	3392	3397	rVB5	52711	67093	4.00%	0.324%
40	23.680	3580	3586	3597	rVB2	795804	1565921	93.37%	7.551%
41	23.833	3606	3612	3620	rVB2	606316	1220172	72.76%	5.884%


Sum of corrected areas: 20738858

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012617\
Data File : BM008891.D
Acq On : 27 Jan 2017 00:37
Operator : SJ/MA
Sample : I1426-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDMY0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

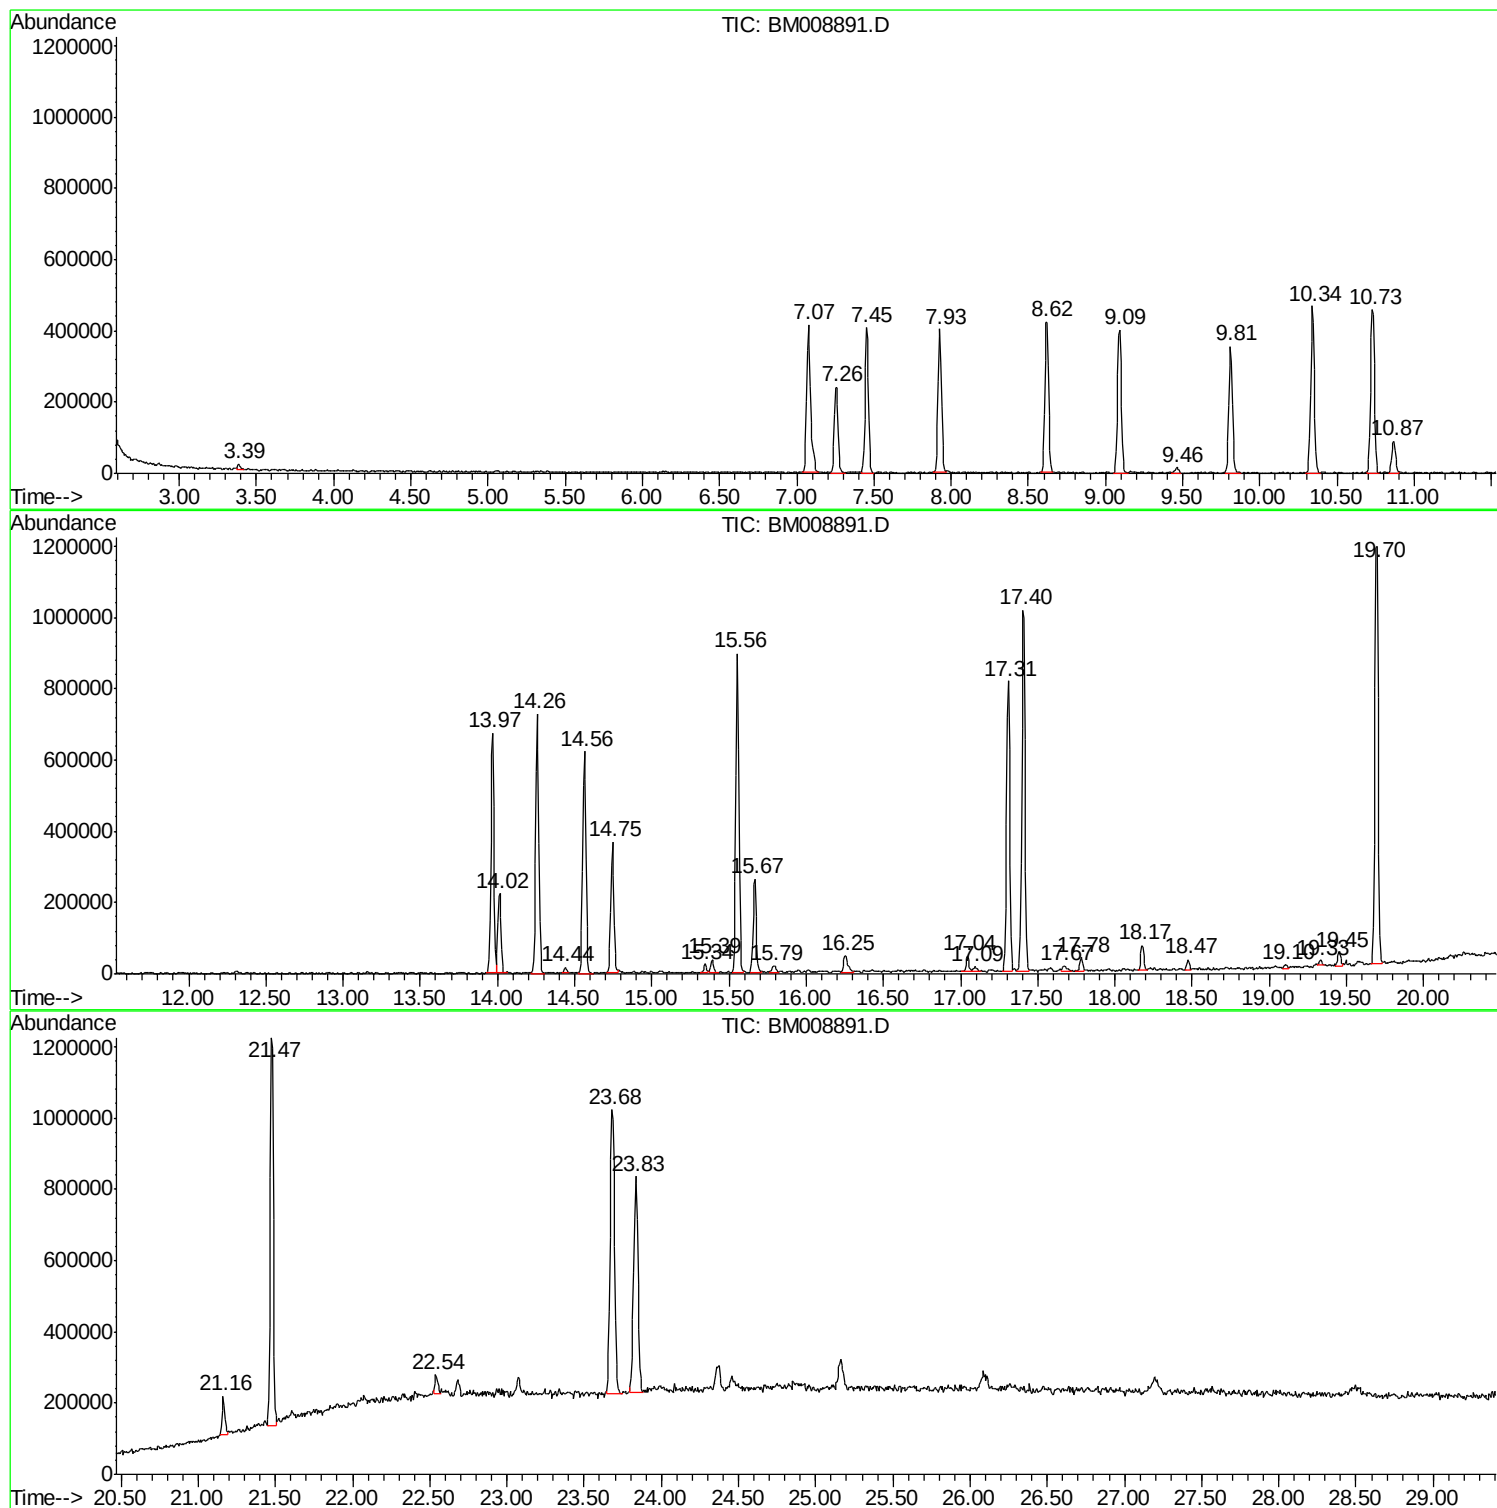

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012617\
Data File : BM008891.D
Acq On : 27 Jan 2017 00:37
Operator : SJ/MA
Sample : I1426-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDMY0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM012617\
Data File : BM008891.D
Acq On : 27 Jan 2017 00:37
Operator : SJ/MA
Sample : I1426-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDMY0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc