

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
 Data File : BM013841.D
 Acq On : 26 Jan 2018 13:31
 Operator : SJ/JU
 Sample : J1243-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 26 22:53:16 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 22:49:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	121452	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	444565	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	243396	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	530258	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	592469	20.00	ng/ul	0.00
83) Perylene-d12	23.39	264	623316	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	13562	4.41	ng/uL	0.00
5) Phenol-d5	6.78	99	61313	6.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	165106	29.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	190724	25.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	110930	15.48	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	119814	34.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	125441	34.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	204887	29.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	277	0.05	ng/ul	0.09
43) Dimethylphthalate-d6	13.66	166	672378	33.52	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	806895	31.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	6796	2.08	ng/ul	0.04
57) Fluorene-d10	15.24	176	581946	32.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	82017	25.70	ng/ul	0.00
70) Anthracene-d10	16.99	188	530258	20.53	ng/ul	-0.10
76) Pyrene-d10	19.40	212	969549	35.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	1017203	35.51	ng/ul	0.00
Target Compounds						
21) Isophorone	9.46	82	15965	1.109	ng/ul#	73
45) 2,6-Dinitrotoluene	13.66	165	3910	1.023	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
Data File : BM013841.D
Acq On : 26 Jan 2018 13:31
Operator : SJ/JU
Sample : J1243-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 26 22:53:16 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 26 22:49:32 2018
Response via : Initial Calibration

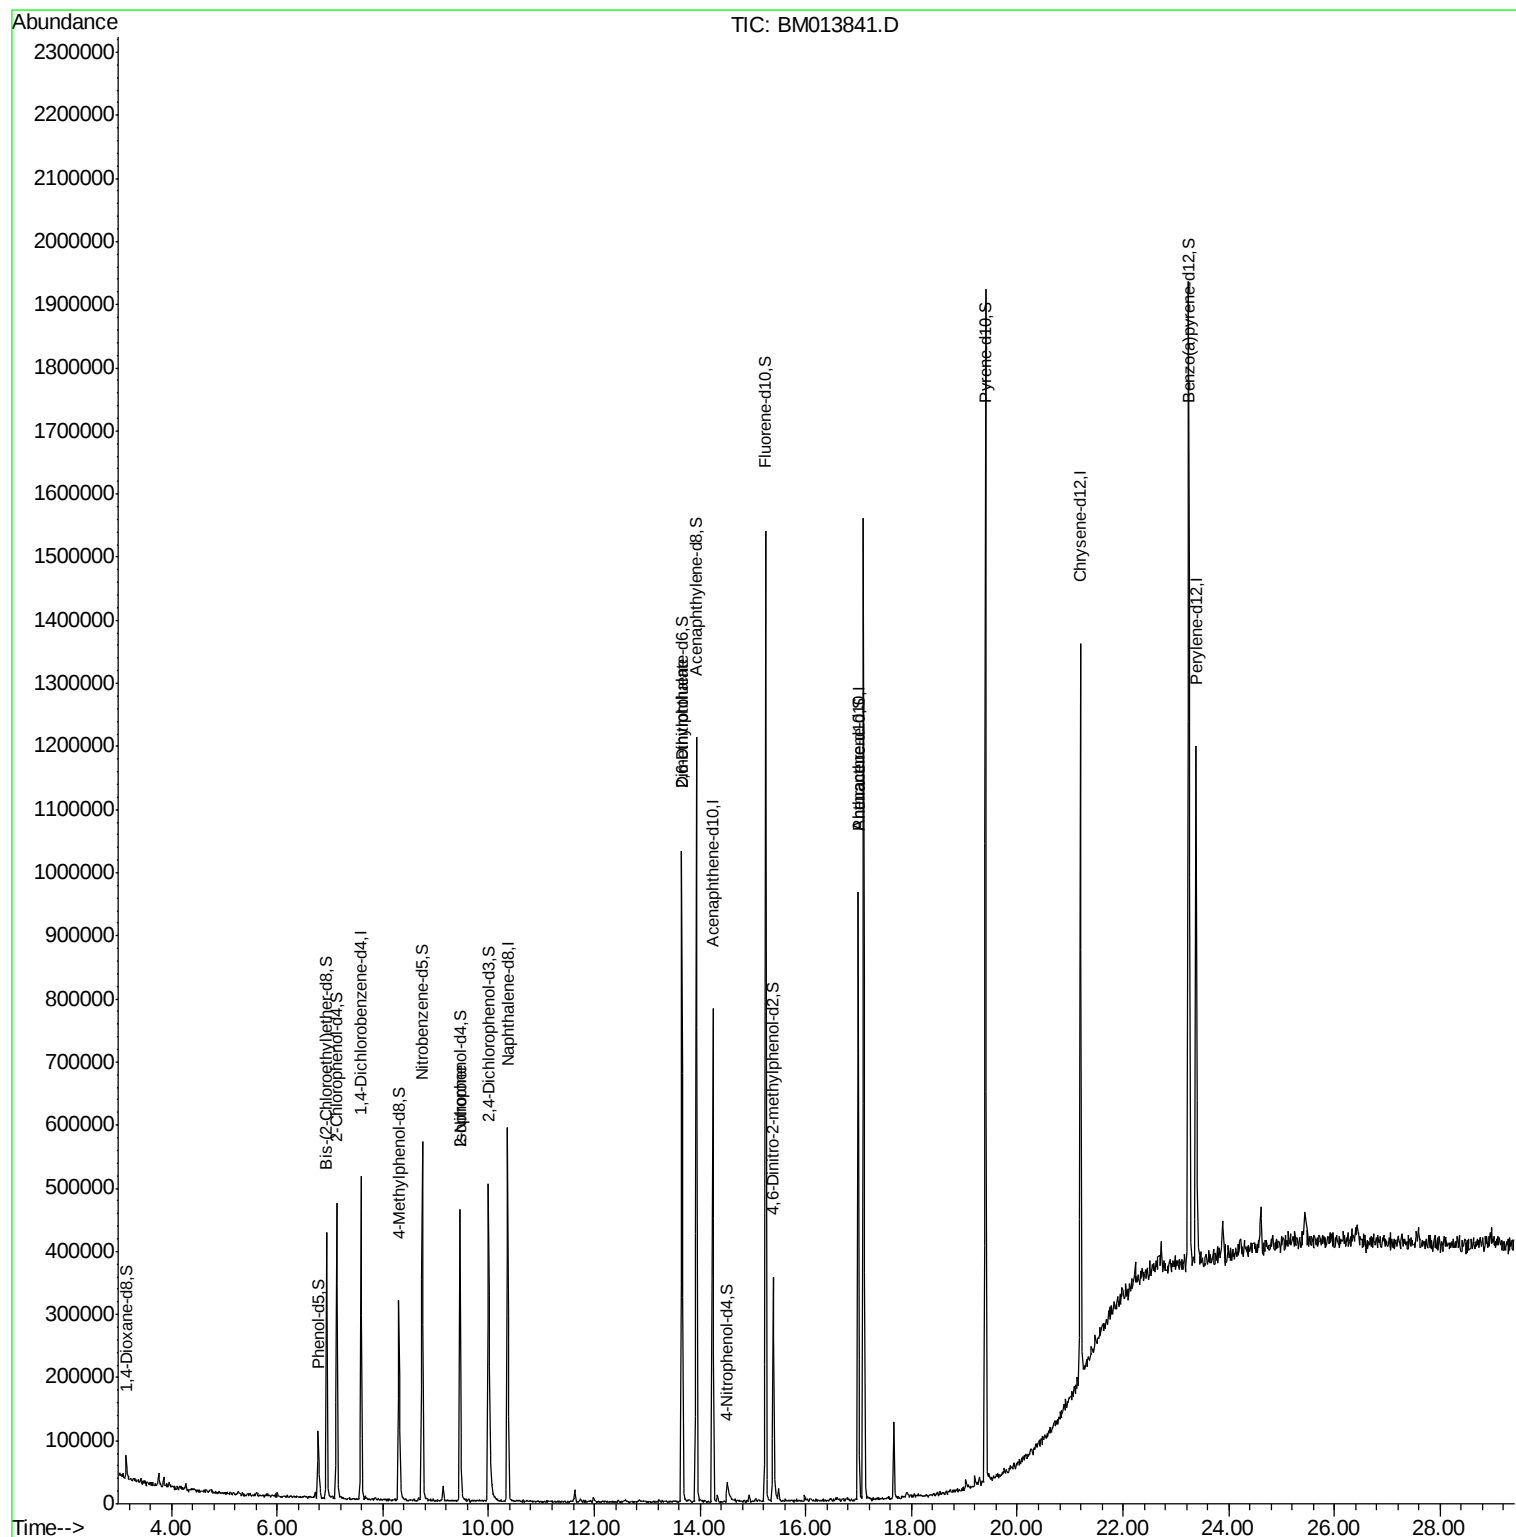

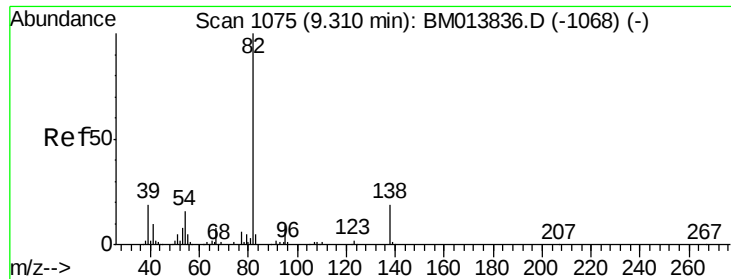

#21

Isophorone

Concen: 1.109 ng/ul

RT: 9.46 min Scan# 1101

Delta R.T. 0.15 min

Lab File: BM013841.D

Acq: 26 Jan 2018 13:31

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 82 Resp: 15965

Ion Ratio Lower Upper

82 100

95 4.5 7.8 11.8#

138 0.0 11.9 17.9#


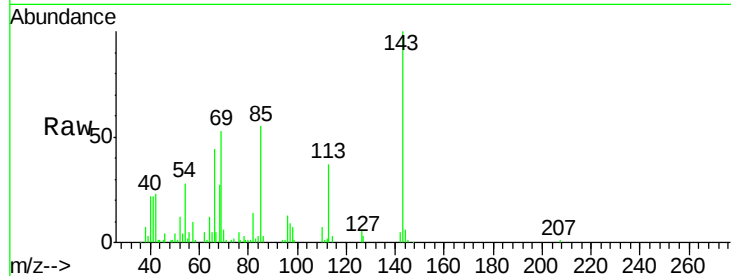


Abundance Ion 82.00 (81.70 to 82.70): BM013836.D (-1068) (-)

Ion 95.00 (94.70 to 95.70): BM013836.D (-1068) (-)

Ion 138.00 (137.70 to 138.70): BM013836.D (-1068) (-)

Time-->

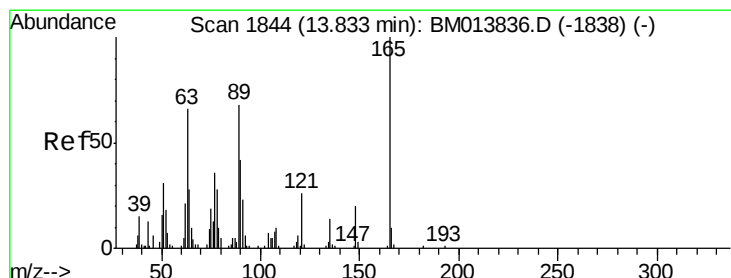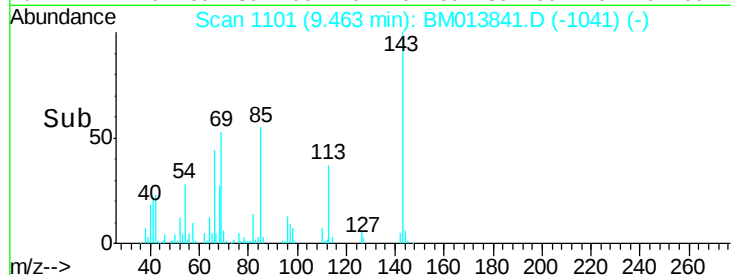

#45

2,6-Dinitrotoluene

Concen: 1.023 ng/ul

RT: 13.66 min Scan# 1815

Delta R.T. -0.17 min

Lab File: BM013841.D

Acq: 26 Jan 2018 13:31


Tgt Ion: 165 Resp: 3910

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 16.7 14.6 22.0

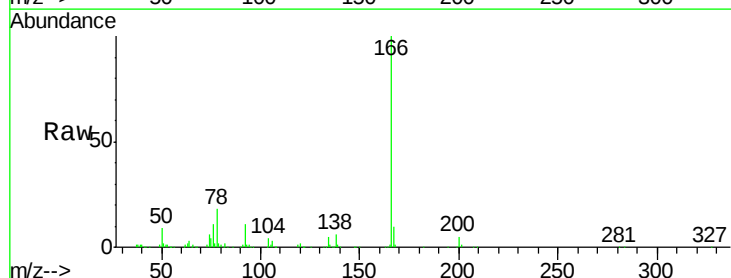

Abundance Ion 165.00 (164.70 to 165.70): BM013836.D (-1838) (-)

Ion 89.00 (88.70 to 89.70): BM013836.D (-1838) (-)

Ion 121.00 (120.70 to 121.70): BM013836.D (-1838) (-)

Time-->

