

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
 Data File : BM013844.D
 Acq On : 26 Jan 2018 15:19
 Operator : SJ/JU
 Sample : PB105940BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 26 22:53:50 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 22:49:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	114711	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	437897	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	239223	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	540881	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	615677	20.00	ng/ul	0.00
83) Perylene-d12	23.39	264	647944	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	15571	5.37	ng/uL	0.00
5) Phenol-d5	6.77	99	256119	29.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	156056	29.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	219826	30.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	208282	30.77	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	105489	31.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	108251	30.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	203734	29.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	255184	42.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	615688	31.23	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	780902	31.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	62415	19.48	ng/ul	0.00
57) Fluorene-d10	15.24	176	525934	30.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	74982	23.03	ng/ul	0.00
70) Anthracene-d10	17.09	188	792264	30.07	ng/ul	0.00
76) Pyrene-d10	19.40	212	897509	31.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	951871	31.96	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.30	70	5584	1.022 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
Data File : BM013844.D
Acq On : 26 Jan 2018 15:19
Operator : SJ/JU
Sample : PB105940BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 26 22:53:50 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 26 22:49:32 2018
Response via : Initial Calibration

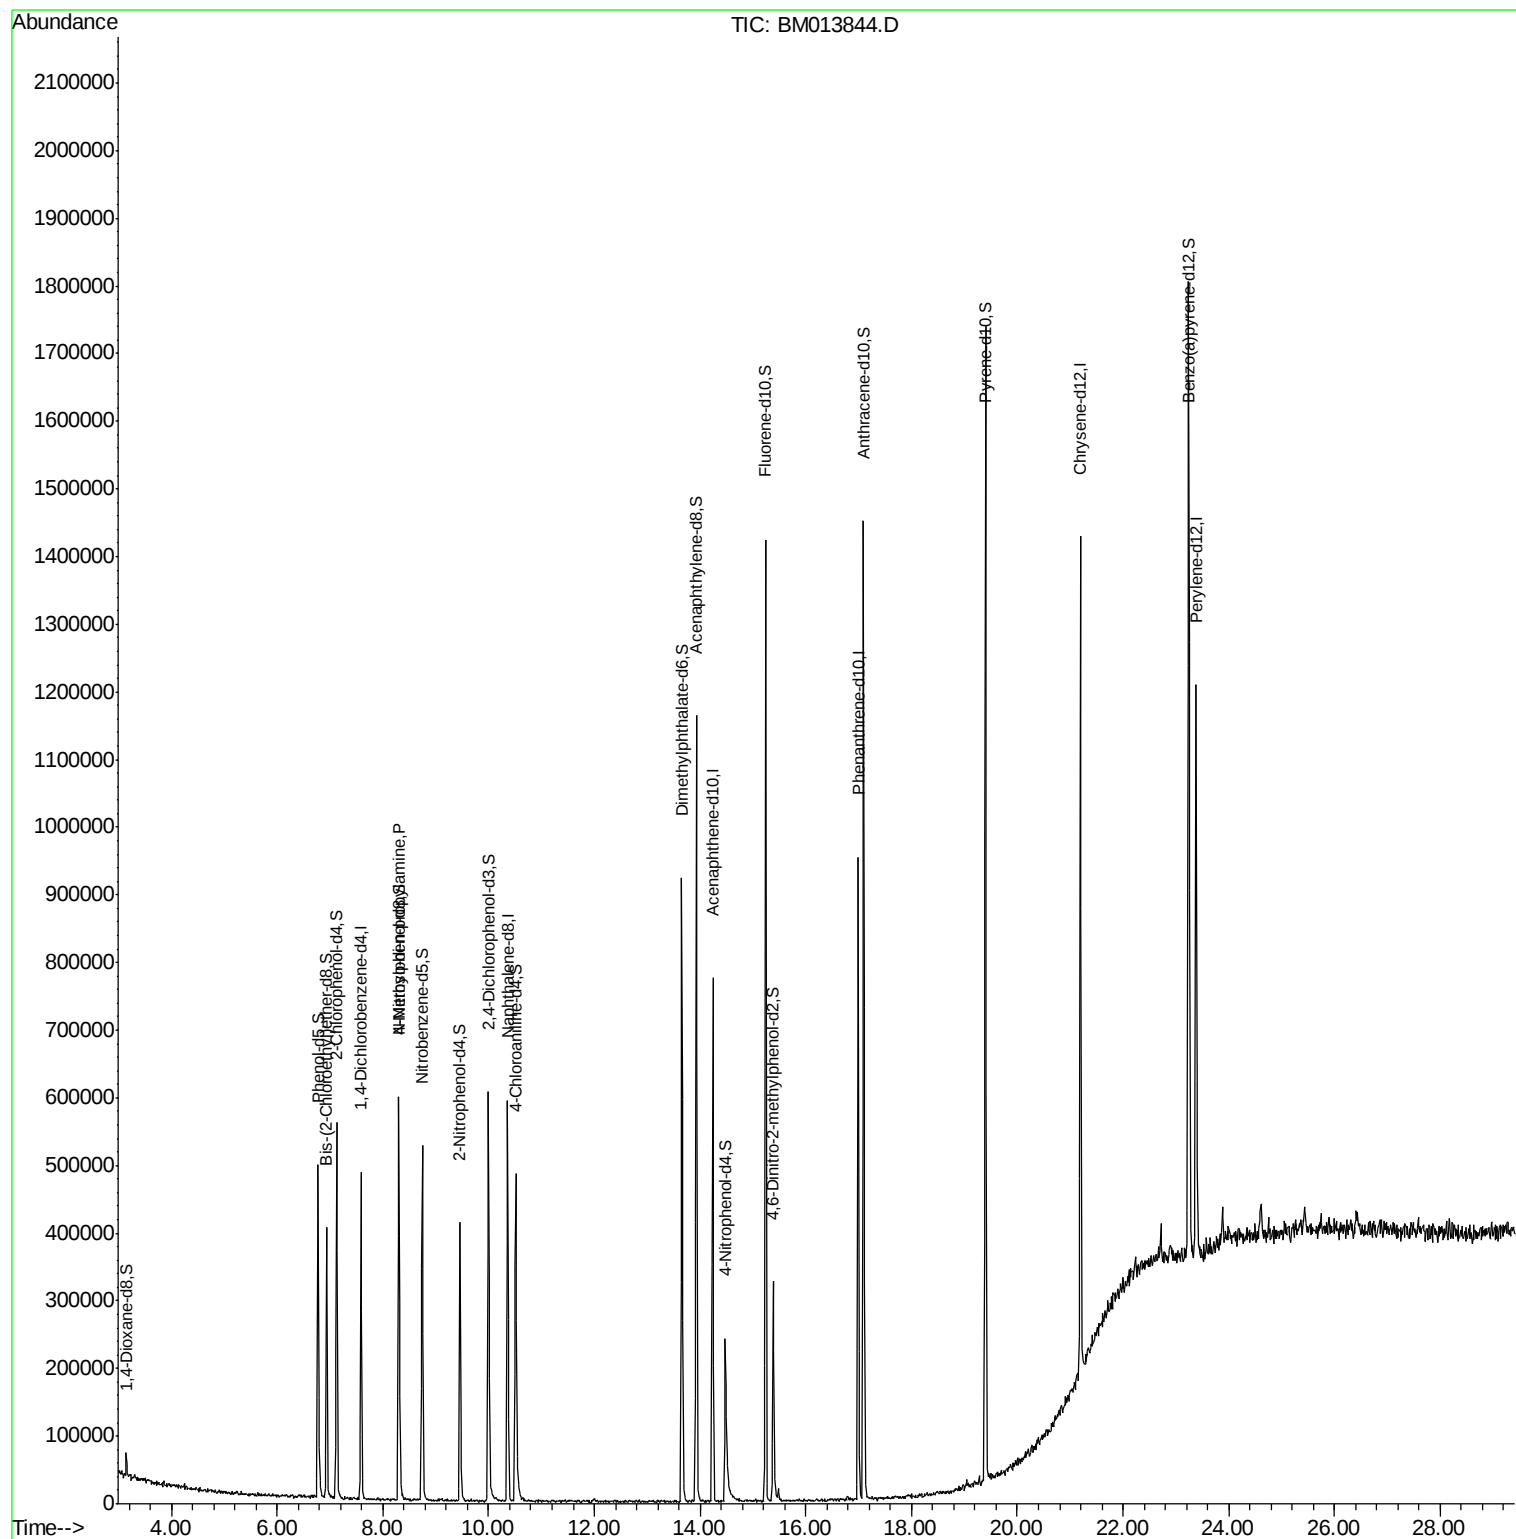

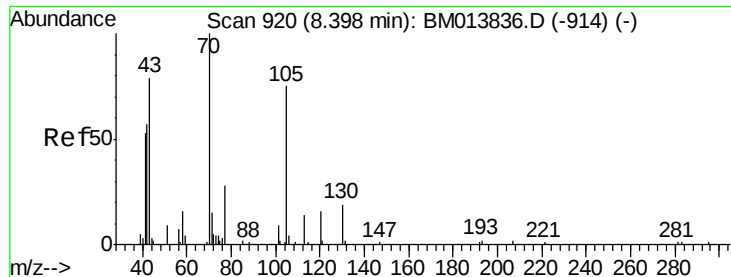

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.022 ng/ul
 RT: 8.30 min Scan# 903
 Delta R.T. -0.10 min
 Lab File: BM013844.D
 Acq: 26 Jan 2018 15:19

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 5584
 Ion Ratio Lower Upper
 70 100
 42 372.0 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

