


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
Data File : BM013851.D
Acq On : 26 Jan 2018 19:29
Operator : SJ/JU
Sample : J1245-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F6B72

Manual Integrations
APPROVED

Sohil
1/29/2018 7:20:43 PM

Quant Time: Jan 27 00:01:00 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 26 23:46:01 2018
Response via : Initial Calibration

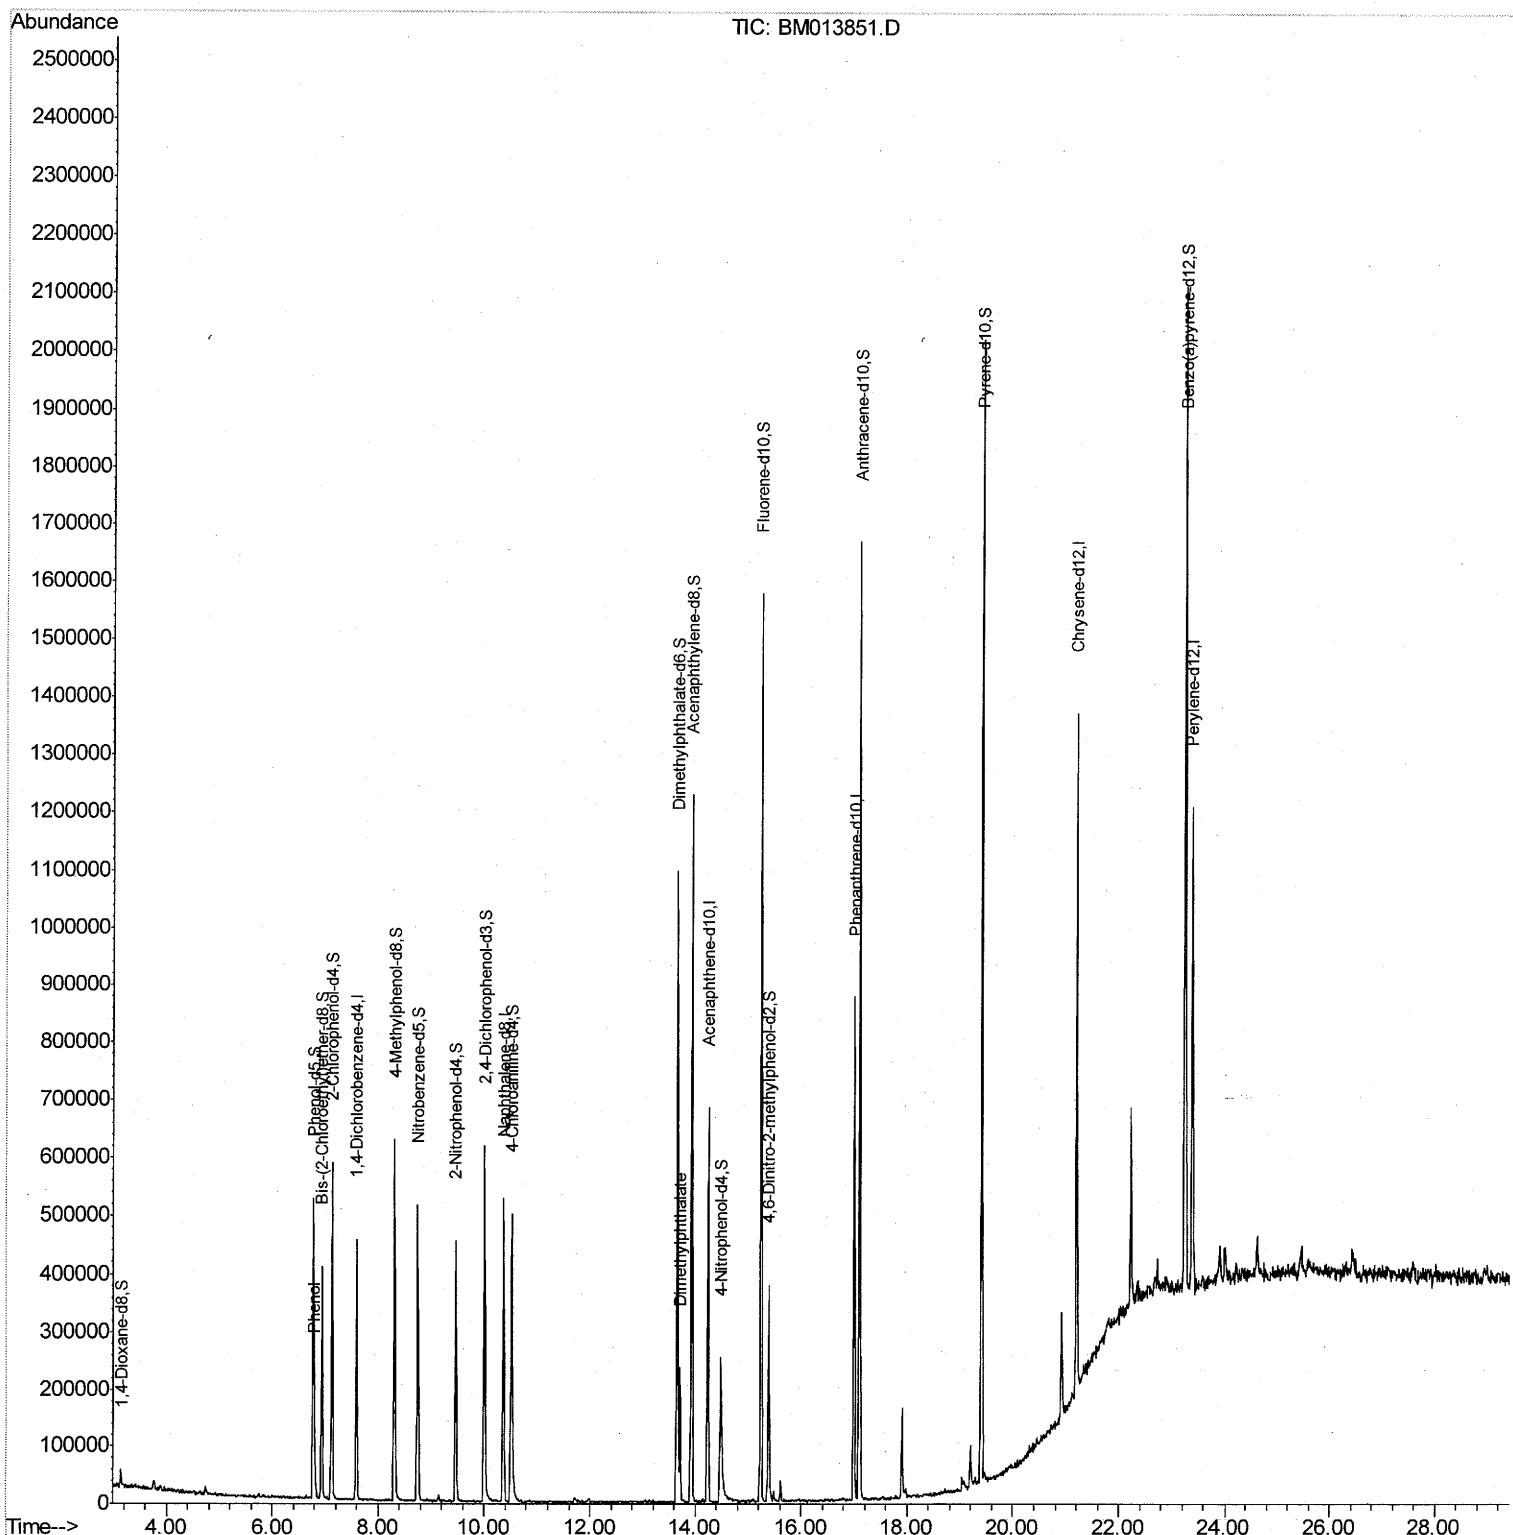




Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
 Data File : BM013851.D
 Acq On : 26 Jan 2018 19:29
 Operator : SJ/JU
 Sample : J1245-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F6B72

Manual Integrations
 APPROVED

Sohil
 1/29/2018 7:20:43 PM

Quant Time: Jan 26 23:53:14 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 23:46:01 2018
 Response via : Initial Calibration

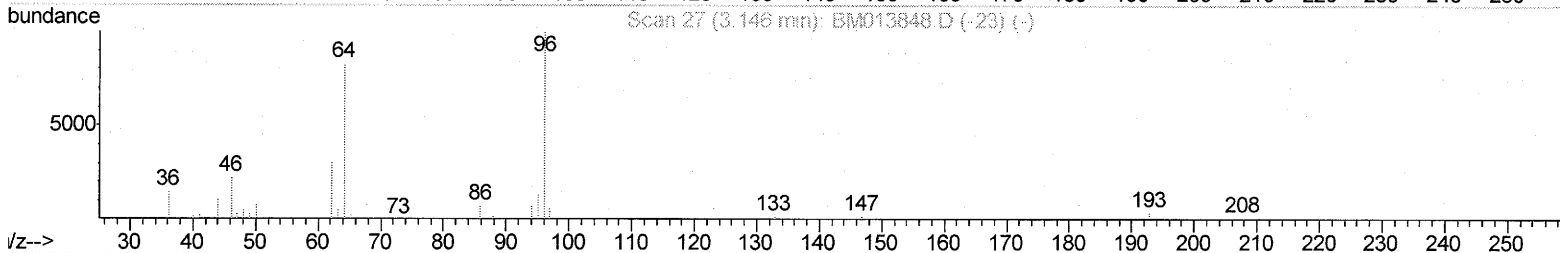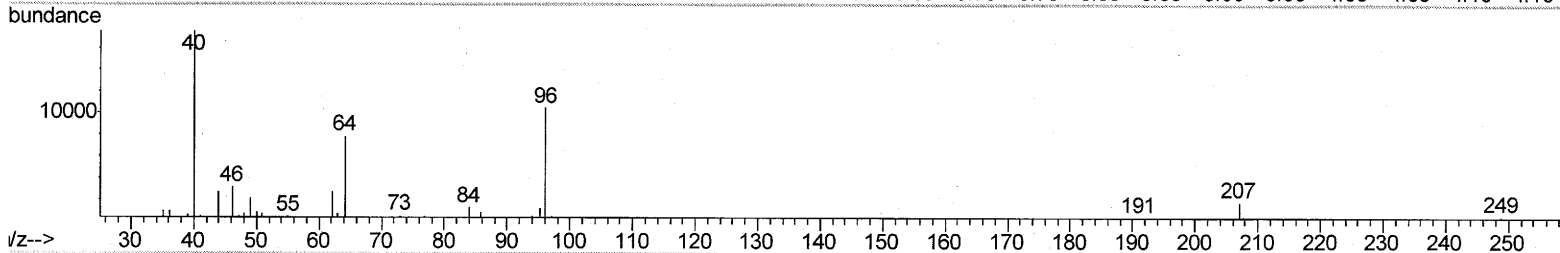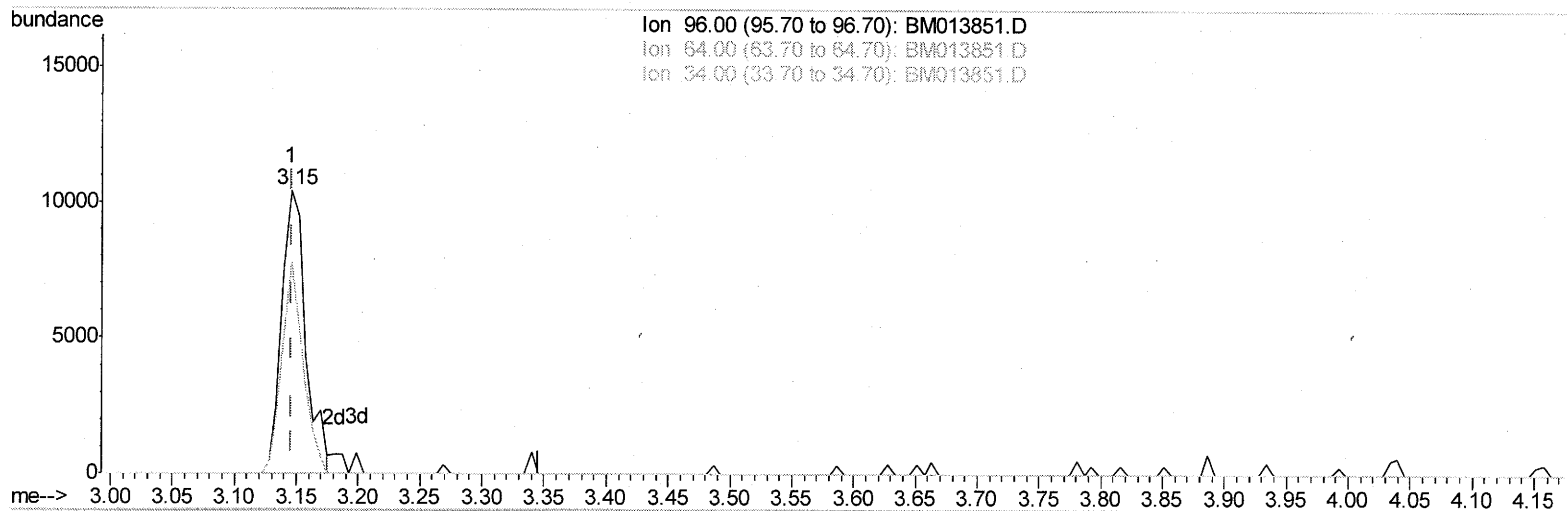

TIC: BM013851.D

(3) 1,4-Dioxane-d8 (S)

3.146min (-0.000) 5.04ng/uL

response 13988

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	65.80
34.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
 Data File : BM013851.D
 Acq On : 26 Jan 2018 19:29
 Operator : SJ/JU
 Sample : J1245-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F6B72

Manual Integrations
 APPROVED

Sohil
 1/29/2018 7:20:43 PM

Quant Time: Jan 26 23:53:14 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 23:46:01 2018
 Response via : Initial Calibration

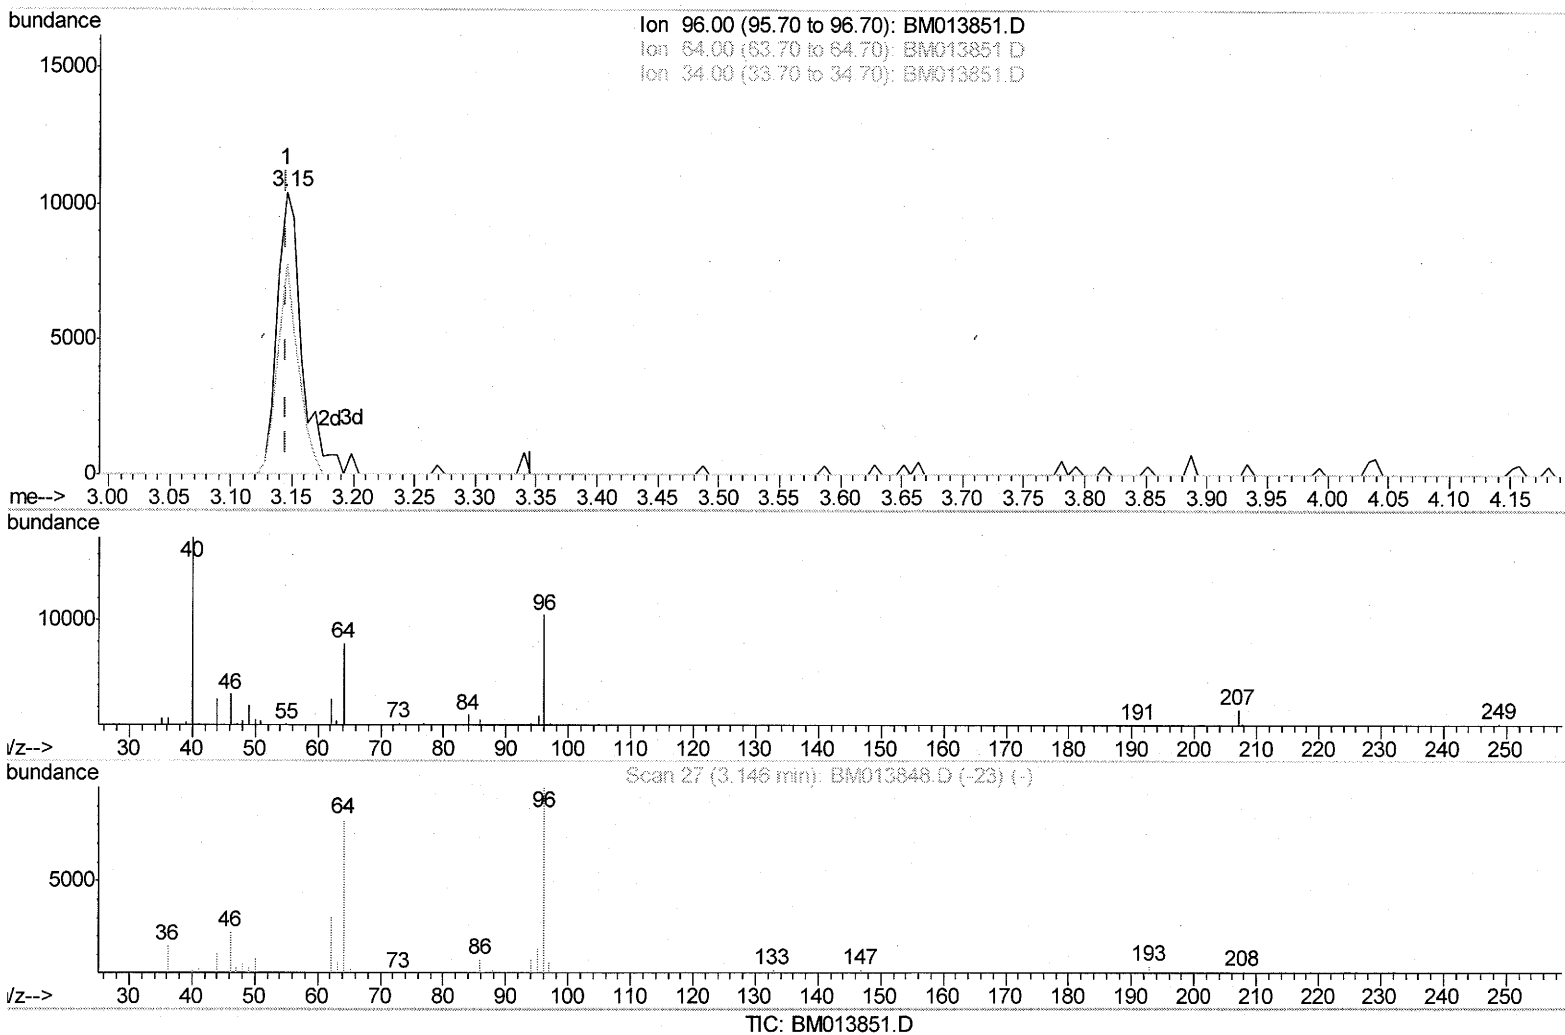

(3) 1,4-Dioxane-d8 (S)

3.146min (-0.000) 5.23ng/uL m

response 14499

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	63.48
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM012618\
 Data File : BM013851.D
 Acq On : 26 Jan 2018 19:29
 Operator : SJ/JU
 Sample : J1245-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F6B72

Manual Integrations
 APPROVED

Sohil
 1/29/2018 7:20:43 PM

Quant Time: Jan 27 00:01:00 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 23:46:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	109596	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	393156	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	217786	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	488091	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	576068	20.00	ng/ul	0.00
83) Perylene-d12	23.38	264	615409	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	14499m	5.23	ng/uL	0.00
5) Phenol-d5	6.77	99	264536	31.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	160004	31.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	218205	31.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	217563	33.64	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	107976	35.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	118945	36.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	209303	33.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	263451	48.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	663446	36.96	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	824031	36.00	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	69469	23.81	ng/ul	0.00
57) Fluorene-d10	15.24	176	575979	36.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	76555	26.06	ng/ul	0.00
70) Anthracene-d10	17.09	188	894943	37.64	ng/ul	0.00
76) Pyrene-d10	19.40	212	1036864	38.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	1140251	40.31	ng/ul	0.00

201/28/18

Target Compounds

					Ovalue	
6) Phenol	6.80	94	34114	4.043	ng/ul	96
44) Dimethylphthalate	13.70	163	140635	7.969	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed