




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012621\
 Data File : BM028542.D
 Acq On : 26 Jan 2021 13:26
 Operator : CG/JU
 Sample : PB134079BL
 Misc : PBBL-SFAM-MDL-ME-02
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK079

Manual Integrations
 APPROVED

mohammad
 1/27/2021 1:16:13 PM

Quant Time: Jan 26 14:00:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 25 12:52:04 2021
 Response via : Initial Calibration

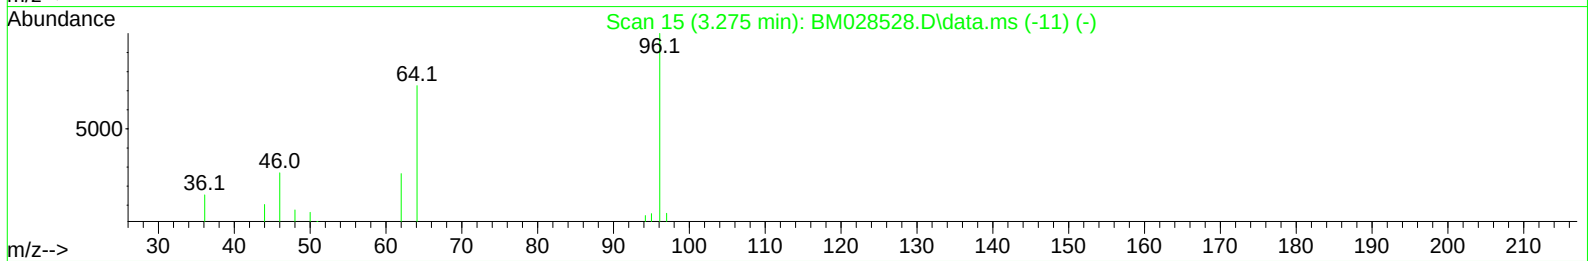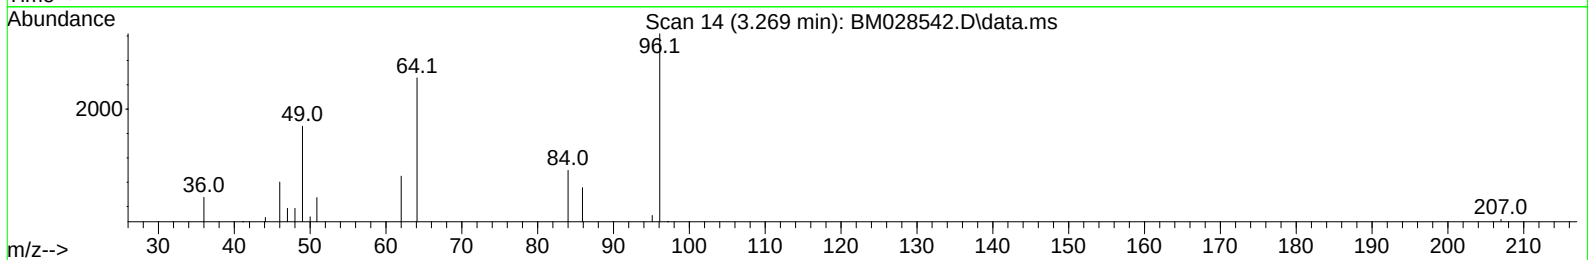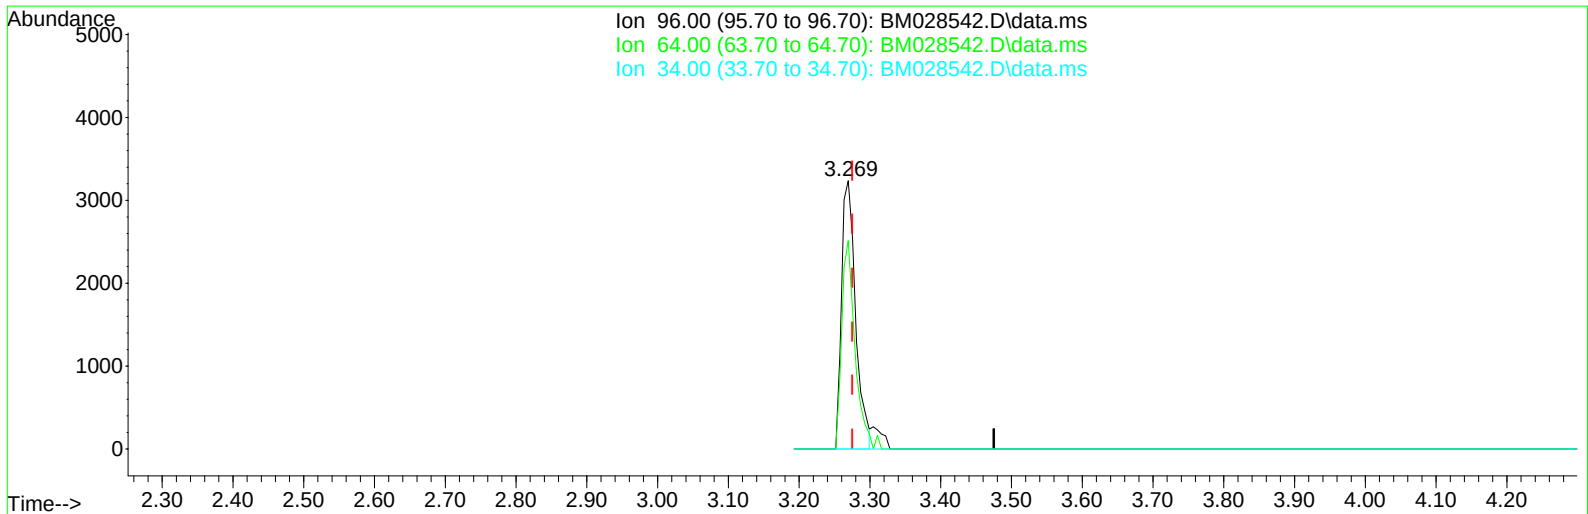

TIC: BM028542.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.269min (-0.006) 6.66 ng/uL

response 4444

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	78.00	77.61
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012621\
Data File : BM028542.D
Acq On : 26 Jan 2021 13:26
Operator : CG/JU
Sample : PB134079BL
Misc : PBBL-SFAM-MDL-ME-02
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK079

Manual Integrations
APPROVED

mohammad
1/27/2021 1:16:13 PM

Quant Time: Jan 26 14:00:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 25 12:52:04 2021
Response via : Initial Calibration

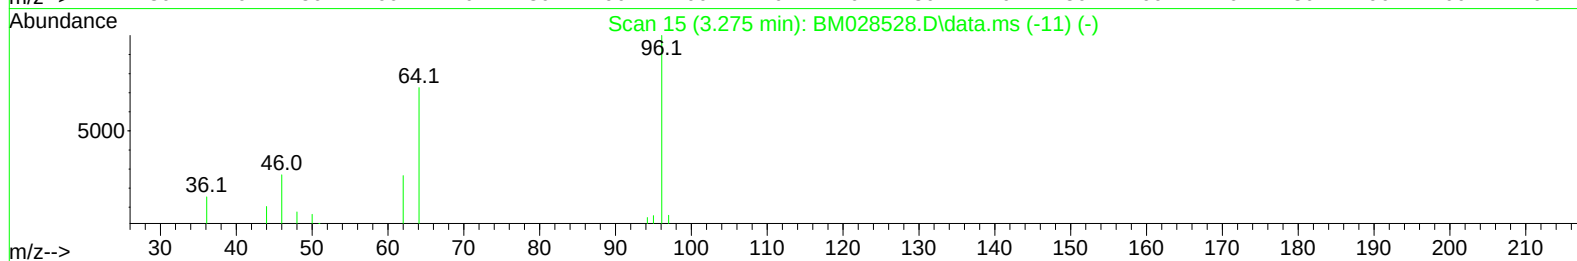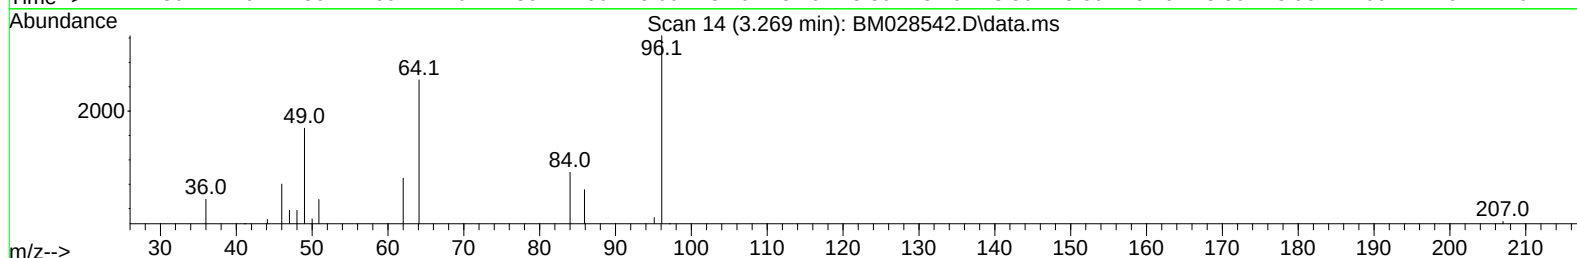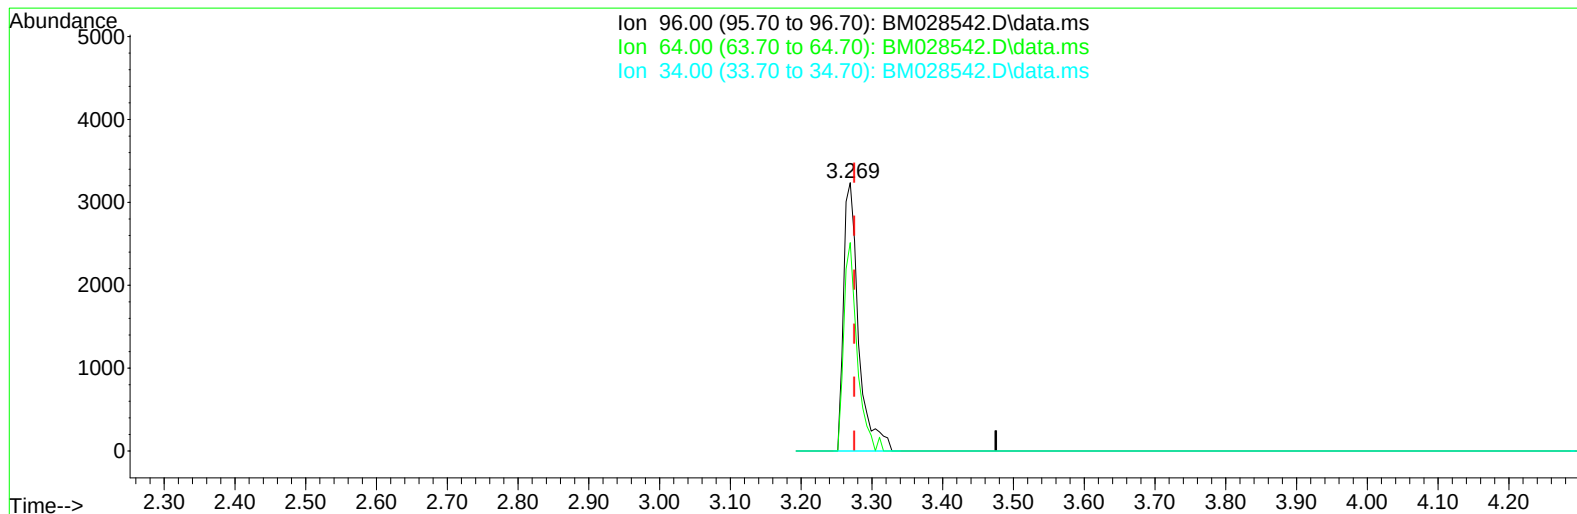

TIC: BM028542.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.269min (-0.006) 7.10 ng/uL m

response 4739

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	78.00	77.61
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012621\
 Data File : BM028542.D
 Acq On : 26 Jan 2021 13:26
 Operator : CG/JU
 Sample : PB134079BL
 Misc : PBBL-SFAM-MDL-ME-02
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK079

Manual Integrations
 APPROVED

mohammad
 1/27/2021 1:16:13 PM

Quant Time: Jan 26 14:00:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 25 12:52:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.987	152	28006	20.00	ng/ul	0.00
20) Naphthalene-d8	10.804	136	110540	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.633	164	61082	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	121789	20.00	ng/ul	0.00
79) Chrysene-d12	21.498	240	117050	20.00	ng/ul	0.00
88) Perylene-d12	23.768	264	115397	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	4739m	7.10	ng/uL	0.00
4) Pyridine-d5	3.711	84	65675	34.43	ng/ul	-0.01
7) Phenol-d5	7.146	99	88919	37.90	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	54075	36.46	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	76840	38.33	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	71080	37.28	ng/ul	-0.01
21) Nitrobenzene-d5	9.163	128	35461	39.22	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	39727	40.79	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	68107	37.22	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	95482	39.02	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	193940	39.61	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	228235	38.28	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	33664	39.17	ng/ul	0.00
60) Fluorene-d10	15.622	176	159451	38.71	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	27429	35.05	ng/ul	0.00
73) Anthracene-d10	17.463	188	238317	39.36	ng/ul	0.00
81) Pyrene-d10	19.733	212	260785	39.22	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.627	264	267852	42.26	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012621\
Data File : BM028542.D
Acq On : 26 Jan 2021 13:26
Operator : CG/JU
Sample : PB134079BL
Misc : PBBL-SFAM-MDL-ME-02
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK079

Manual Integrations
APPROVED

mohammad
1/27/2021 1:16:13 PM

Quant Time: Jan 26 14:00:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 25 12:52:04 2021
Response via : Initial Calibration

