

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012621\
 Data File : BM028539.D
 Acq On : 26 Jan 2021 11:04
 Operator : CG/JU
 Sample : L5214-02
 Misc : SFAM-MDL-W-02
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT1-2021-02

Quant Time: Jan 26 11:42:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 25 12:52:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.992	152	27759	20.00	ng/ul	0.00
20) Naphthalene-d8	10.804	136	110436	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.633	164	61697	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.362	188	120336	20.00	ng/ul	0.00
79) Chrysene-d12	21.497	240	112780	20.00	ng/ul	0.00
88) Perylene-d12	23.768	264	109586	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	2177	3.29	ng/uL	0.00
4) Pyridine-d5	3.716	84	35279	18.66	ng/ul	0.00
7) Phenol-d5	7.145	99	83271	35.81	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	52203	35.51	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	72939	36.71	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	70092	37.09	ng/ul	0.00
21) Nitrobenzene-d5	9.163	128	33974	37.61	ng/ul	0.00
24) 2-Nitrophenol-d4	9.886	143	36793	37.82	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	64333	35.19	ng/ul	0.00
31) 4-Chloroaniline-d4	10.939	131	89169	36.48	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	178446	36.08	ng/ul	0.00
49) Acenaphthylene-d8	14.327	160	233765	38.81	ng/ul	0.00
54) 4-Nitrophenol-d4	14.827	143	31955	36.81	ng/ul	0.00
60) Fluorene-d10	15.621	176	149081	35.83	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	27108	35.06	ng/ul	0.00
73) Anthracene-d10	17.462	188	219677	36.72	ng/ul	0.00
81) Pyrene-d10	19.733	212	231424	36.12	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.627	264	213185	35.42	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.304	88	819	1.16	ng/uL	97
5) Pyridine	3.746	79	7953	4.19	ng/ul	86
6) Benzaldehyde	7.122	77	5020	5.39	ng/ul	96
8) Phenol	7.175	94	9832	4.17	ng/ul	94
10) Bis(2-Chloroethyl)ether	7.410	93	8406	4.29	ng/ul	99
12) 2-Chlorophenol	7.551	128	8673	4.30	ng/ul	96
13) 2-Methylphenol	8.433	108	6920	3.86	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.522	45	12618	3.76	ng/ul#	94
16) Acetophenone	8.822	105	11700	4.04	ng/ul	95
17) N-Nitroso-di-n-propyla...	8.804	70	5488	3.83	ng/ul	94
18) 4-Methylphenol	8.769	108	7743	4.03	ng/ul	99
19) Hexachloroethane	9.075	117	3578	4.02	ng/ul	97
22) Nitrobenzene	9.204	77	9143	4.12	ng/ul	97
23) Isophorone	9.733	82	14716	3.80	ng/ul	96
25) 2-Nitrophenol	9.916	139	4509	4.28	ng/ul	97
26) 2,4-Dimethylphenol	9.975	107	8140	3.93	ng/ul	95
27) Bis(2-Chloroethoxy)met...	10.210	93	10006	3.98	ng/ul	96
29) 2,4-Dichlorophenol	10.451	162	7487	4.23	ng/ul	93
30) Naphthalene	10.857	128	25997	4.12	ng/ul	97
32) 4-Chloroaniline	10.963	127	9783	4.11	ng/ul	99
33) Hexachlorobutadiene	11.127	225	4721	3.94	ng/ul	98
34) Caprolactam	11.751	113	1778	3.42	ng/ul	91
35) 4-Chloro-3-methylphenol	12.080	107	7114	3.94	ng/ul	98
36) 2-Methylnaphthalene	12.463	142	17966	4.23	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012621\
 Data File : BM028539.D
 Acq On : 26 Jan 2021 11:04
 Operator : CG/JU
 Sample : L5214-02
 Misc : SFAM-MDL-W-02
 ALS Vial : 4 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT1-2021-02

Quant Time: Jan 26 11:42:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 25 12:52:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.680	142	16987	4.15	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.827	216	8855	4.18	ng/ul	99
40) Hexachlorocyclopentadiene	12.804	237	3943	3.62	ng/ul	99
41) 2,4,6-Trichlorophenol	13.068	196	5284	3.99	ng/ul	91
42) 2,4,5-Trichlorophenol	13.139	196	5731	4.03	ng/ul	99
43) 1,1'-Biphenyl	13.468	154	22475	4.16	ng/ul	99
44) 2-Chloronaphthalene	13.510	162	17453	4.15	ng/ul	96
45) 2-Nitroaniline	13.715	65	4158	3.58	ng/ul	96
47) Dimethylphthalate	14.086	163	20608	4.07	ng/ul	98
48) 2,6-Dinitrotoluene	14.215	165	3583	3.58	ng/ul	98
50) Acenaphthylene	14.357	152	25808	4.19	ng/ul	99
51) 3-Nitroaniline	14.539	138	3491	3.84	ng/ul#	99
52) Acenaphthene	14.698	153	18327	4.13	ng/ul	98
53) 2,4-Dinitrophenol	14.757	184	1770	3.24	ng/ul	89
55) 4-Nitrophenol	14.839	109	2804	4.05	ng/ul	88
56) Dibenzofuran	15.027	168	25349	4.26	ng/ul	97
57) 2,4-Dinitrotoluene	14.998	165	5013	3.72	ng/ul#	97
58) 2,3,4,6-Tetrachlorophenol	15.257	232	4406	3.81	ng/ul#	98
59) Diethylphthalate	15.439	149	20078	3.85	ng/ul	96
61) Fluorene	15.674	166	20701	4.18	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.668	204	9982	4.04	ng/ul	96
63) 4-Nitroaniline	15.692	138	3247	4.09	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.757	198	3231	3.89	ng/ul#	73
67) N-Nitrosodiphenylamine	15.880	169	16893	4.17	ng/ul	99
68) 4-Bromophenyl-phenylether	16.556	248	5788	3.95	ng/ul	98
69) Hexachlorobenzene	16.668	284	6742	4.06	ng/ul	96
70) Atrazine	16.821	200	5366	3.58	ng/ul	94
71) Pentachlorophenol	17.015	266	3075	3.27	ng/ul	96
72) Phenanthrene	17.403	178	30917	4.20	ng/ul	99
74) Anthracene	17.492	178	31656	4.23	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.433	216	8650	4.19	ng/uL	97
76) Pentachlorobenzene	14.951	250	8169	4.05	ng/uL	95
77) Carbazole	17.762	167	26572	4.19	ng/ul	99
78) Di-n-butylphthalate	18.309	149	32067	3.67	ng/ul	99
80) Fluoranthene	19.397	202	33639	3.97	ng/ul	98
82) Pyrene	19.756	202	35291	4.06	ng/ul	98
83) Butylbenzylphthalate	20.639	149	14374	3.65	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.409	252	11186	4.82	ng/ul	95
85) Benzo(a)anthracene	21.480	228	32400	4.20	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.397	149	21488	3.52	ng/ul	99
87) Chrysene	21.533	228	31124	4.15	ng/ul	98
89) Di-n-octyl phthalate	22.280	149	36157	3.51	ng/ul	100
90) Benzo(b)fluoranthene	23.080	252	32837	4.37	ng/ul	98
91) Benzo(k)fluoranthene	23.127	252	30871	4.22	ng/ul	98
93) Benzo(a)pyrene	23.668	252	29854	4.39	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.073	276	34961	4.35	ng/ul	99
95) Dibenzo(a,h)anthracene	26.079	278	29320	4.30	ng/ul	96
96) Benzo(g,h,i)perylene	26.779	276	29246	4.32	ng/ul	96





(#) = qualifier out of range (m) = manual integration (+) = signals summed

Abundance Scan 20 (3.304 min): BM028537.D\data.ms (-16)

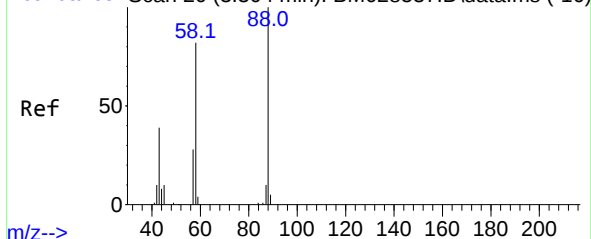


#2
1,4-Dioxane
Concen: 1.16 ng/uL
RT: 3.304 min Scan# 20
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	88	Resp:	819
Ion	Ratio	Lower	Upper
88	100		
43	35.5	30.7	46.1
58	80.2	66.0	99.0

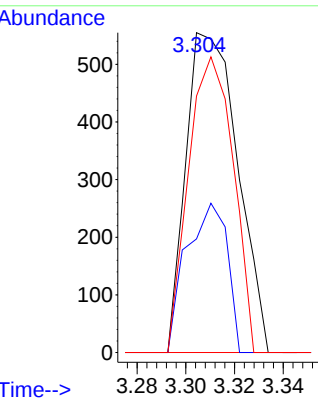


#5
Pyridine
Concen: 4.19 ng/uL
RT: 3.746 min Scan# 95
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	79	Resp:	7953
Ion	Ratio	Lower	Upper
79	100		
52	110.0	74.5	111.7
51	42.8	37.5	56.3

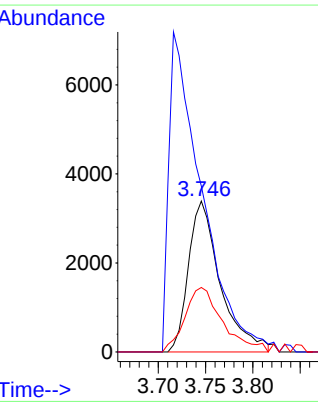





Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02



#6
Benzaldehyde
Concen: 5.39 ng/ul
RT: 7.122 min Scan# 669
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	77	Resp:	5020
Ion	Ratio	Lower	Upper
77	100		
105	102.8	77.2	115.8
106	93.5	73.8	110.6

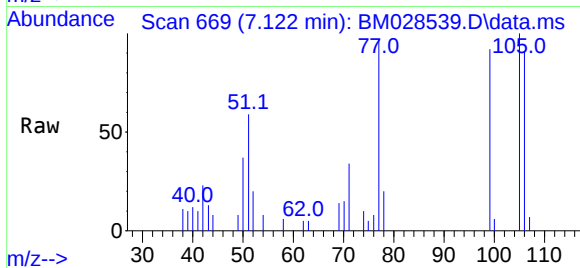

#8
Phenol
Concen: 4.17 ng/ul
RT: 7.175 min Scan# 678
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	94	Resp:	9832
Ion	Ratio	Lower	Upper
94	100		
65	31.6	24.1	36.1
66	35.8	32.6	49.0




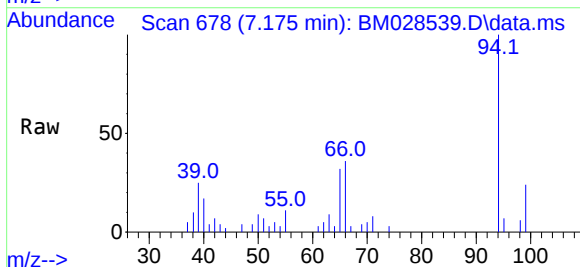




#10
Bis(2-Chloroethyl)ether
Concen: 4.29 ng/ul
RT: 7.410 min Scan# 718
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	93	Resp:	8406
Ion	Ratio	Lower	Upper
93	100		
63	81.1	64.8	97.2
95	29.8	25.7	38.5



#12
2-Chlorophenol
Concen: 4.30 ng/ul
RT: 7.551 min Scan# 742
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	128	Resp:	8673
Ion	Ratio	Lower	Upper
128	100		
64	44.5	38.0	57.0
130	32.7	27.2	40.8









#13
2-Methylphenol
Concen: 3.86 ng/ul
RT: 8.433 min Scan# 892
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:108 Resp: 6920
Ion Ratio Lower Upper
108 100
107 85.4 69.6 104.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 3.76 ng/ul
RT: 8.522 min Scan# 907
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion: 45 Resp: 12618
Ion Ratio Lower Upper
45 100
77 15.3 9.7 14.5#
79 9.9 6.8 10.2









#16
Acetophenone
Concen: 4.04 ng/ul
RT: 8.822 min Scan# 958
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	105	Resp:	11700
Ion	Ratio	Lower	Upper
105	100		
77	83.1	61.5	92.3
51	33.2	26.4	39.6

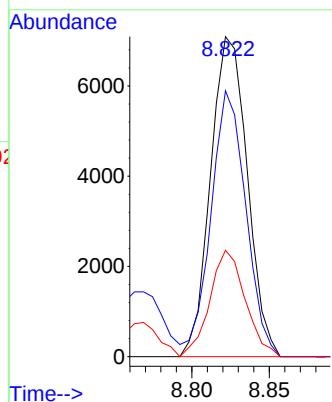

#17
N-Nitroso-di-n-propylamine
Concen: 3.83 ng/ul
RT: 8.804 min Scan# 955
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	70	Resp:	5488
Ion	Ratio	Lower	Upper
70	100		
42	69.9	60.4	90.6
101	8.9	8.4	12.6
130	24.1	17.0	25.6









#18
4-Methylphenol
Concen: 4.03 ng/ul
RT: 8.769 min Scan# 949
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:108 Resp: 7743
Ion Ratio Lower Upper
108 100
107 111.8 90.1 135.1

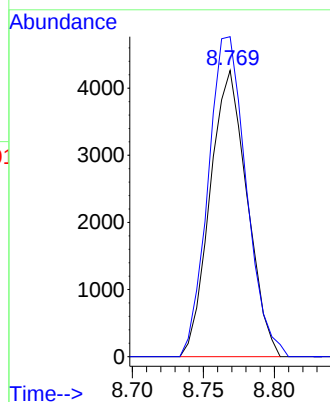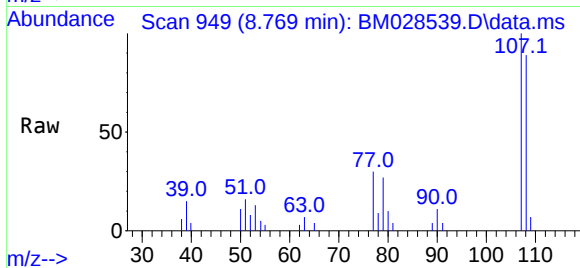

#19
Hexachloroethane
Concen: 4.02 ng/ul
RT: 9.075 min Scan# 1001
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:117 Resp: 3578
Ion Ratio Lower Upper
117 100
201 95.5 76.9 115.3
199 63.5 46.9 70.3



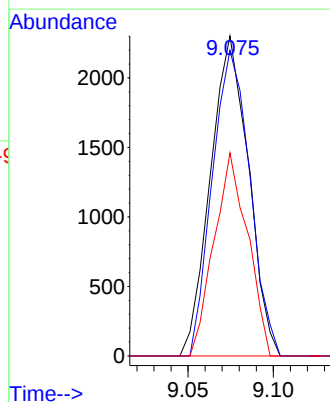
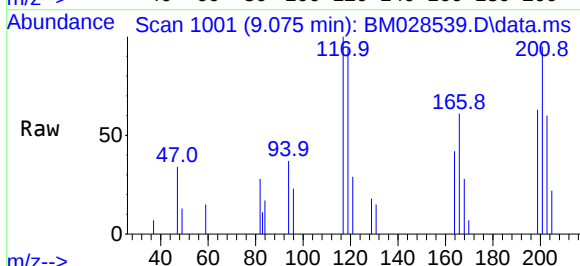


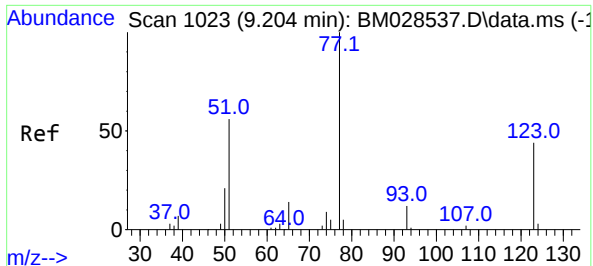

#22
Nitrobenzene
Concen: 4.12 ng/ul
RT: 9.204 min Scan# 1023
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion: 77 Resp: 9143
Ion Ratio Lower Upper
77 100
123 48.3 37.0 55.6
65 15.9 11.4 17.0

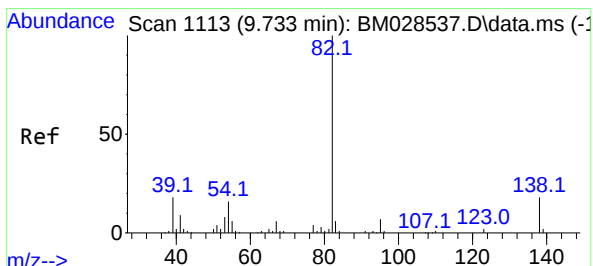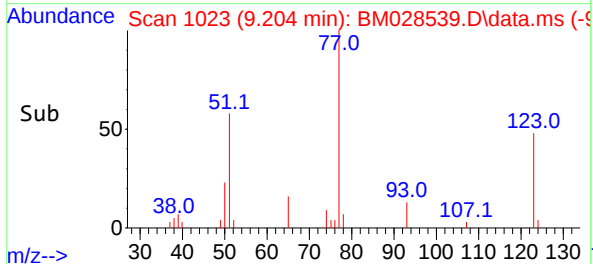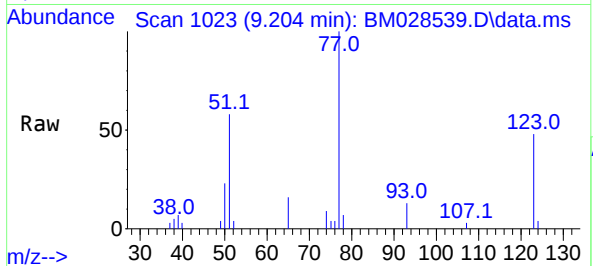

#23
Isophorone
Concen: 3.80 ng/ul
RT: 9.733 min Scan# 1113
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion: 82 Resp: 14716
Ion Ratio Lower Upper
82 100
95 7.5 5.8 8.8
138 21.4 15.2 22.8


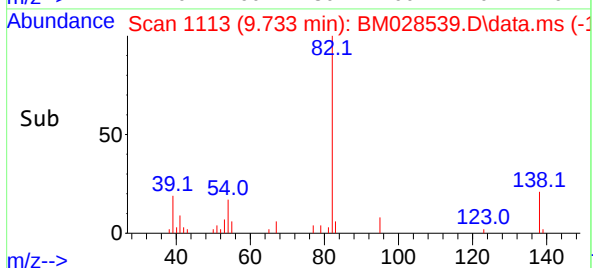
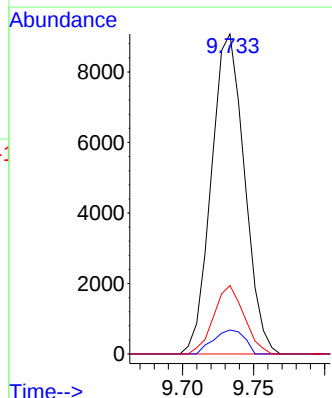
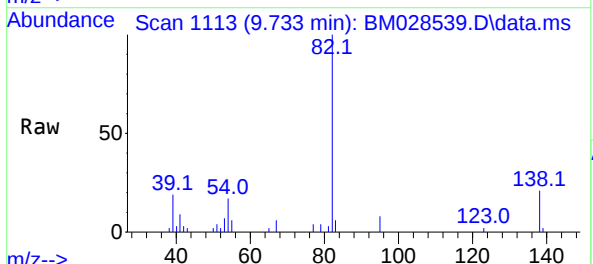




#25
2-Nitrophenol
Concen: 4.28 ng/ul
RT: 9.916 min Scan# 1144
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	139	Resp:	4509
Ion	Ratio	Lower	Upper
139	100		
65	59.0	45.2	67.8
109	31.4	24.4	36.6



#26
2,4-Dimethylphenol
Concen: 3.93 ng/ul
RT: 9.975 min Scan# 1154
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	107	Resp:	8140
Ion	Ratio	Lower	Upper
107	100		
121	52.7	40.6	60.8
122	88.9	66.3	99.5









#27
Bis(2-Chloroethoxy)methane
Concen: 3.98 ng/ul
RT: 10.210 min Scan# 1194
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02

Tgt Ion: 93 Resp: 10006




Ion	Ratio	Lower	Upper
93	100		
95	29.7	26.1	39.1
123	11.9	9.3	13.9

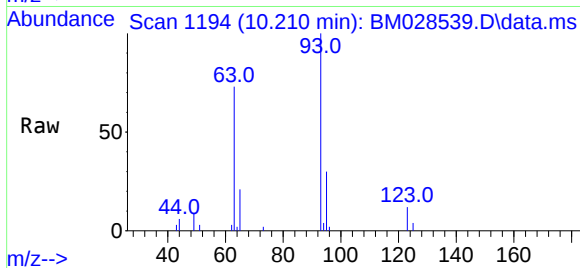


#29
2,4-Dichlorophenol
Concen: 4.23 ng/ul
RT: 10.451 min Scan# 1235
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion: 162 Resp: 7487


Ion	Ratio	Lower	Upper
162	100		
164	71.7	51.9	77.9
98	35.0	30.1	45.1

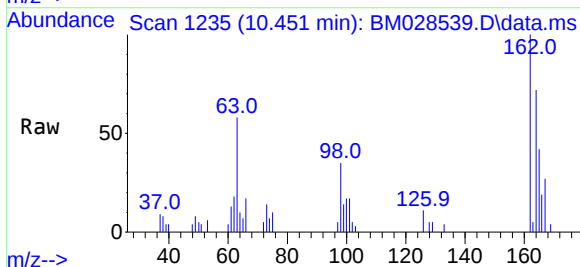






#30
Naphthalene
Concen: 4.12 ng/ul
RT: 10.857 min Scan# 1304
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02





Tgt Ion:	128	Resp:	25997
Ion	Ratio	Lower	Upper
128	100		
129	9.2	9.0	13.6
127	12.8	10.5	15.7

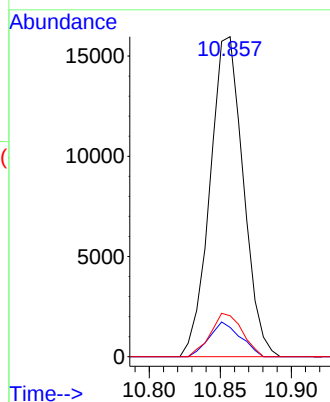


#32
4-Chloroaniline
Concen: 4.11 ng/ul
RT: 10.963 min Scan# 1322
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04



Tgt Ion:	127	Resp:	9783
Ion	Ratio	Lower	Upper
127	100		
129	32.9	26.1	39.1




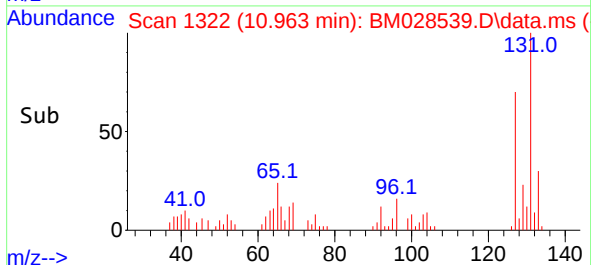




#33
Hexachlorobutadiene
Concen: 3.94 ng/ul
RT: 11.127 min Scan# 1350
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:225 Resp: 4721
Ion Ratio Lower Upper
225 100
223 65.6 50.9 76.3
227 65.3 50.7 76.1

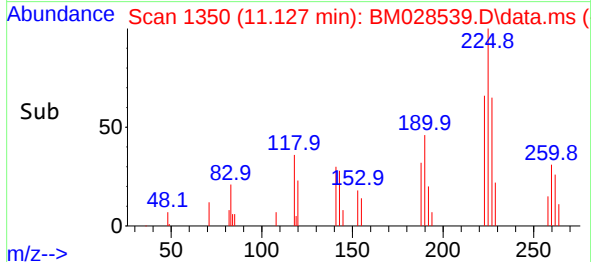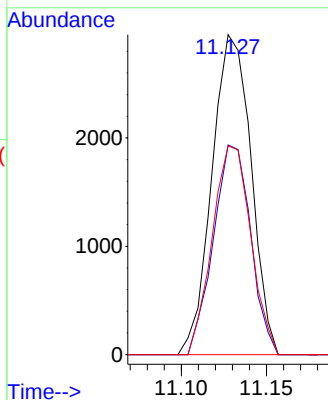

#34
Caprolactam
Concen: 3.42 ng/ul
RT: 11.751 min Scan# 1456
Delta R.T. 0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:113 Resp: 1778
Ion Ratio Lower Upper
113 100
55 162.4 146.2 219.2
56 135.8 110.6 165.8



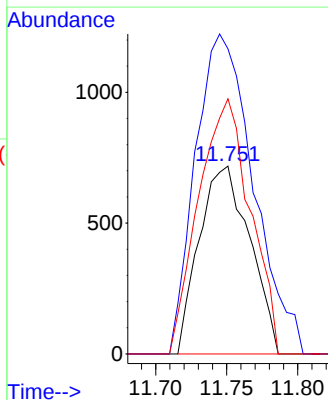
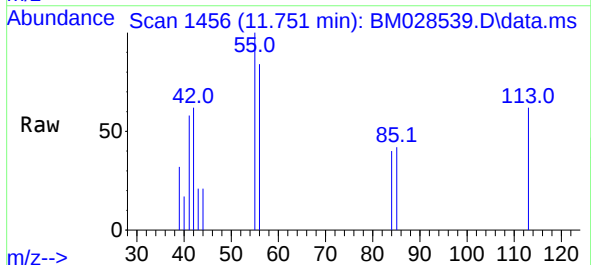




#35
4-Chloro-3-methylphenol
Concen: 3.94 ng/ul
RT: 12.080 min Scan# 1512
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:107	Resp:	7114
Ion	Ratio	Lower Upper
107	100	
144	26.6	21.0 31.6
142	82.4	64.1 96.1

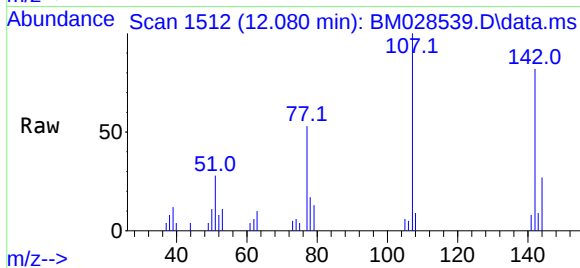

#36
2-Methylnaphthalene
Concen: 4.23 ng/ul
RT: 12.463 min Scan# 1577
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:142	Resp:	17966
Ion	Ratio	Lower Upper
142	100	
141	85.9	71.3 106.9

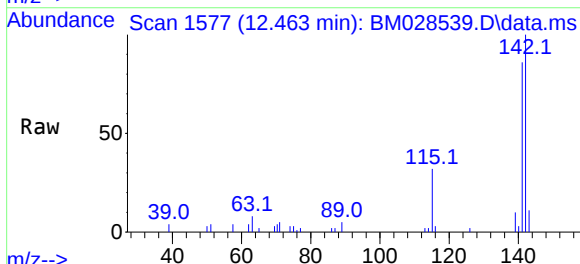



#37

1-Methylnaphthalene

Concen: 4.15 ng/ul

RT: 12.680 min Scan# 1614

Delta R.T. -0.006 min

Lab File: BM028539.D





Acq: 26 Jan 2021 11:04

Tgt Ion:142 Resp: 16987

Ion Ratio Lower Upper

142 100

141 92.7 74.2 111.4

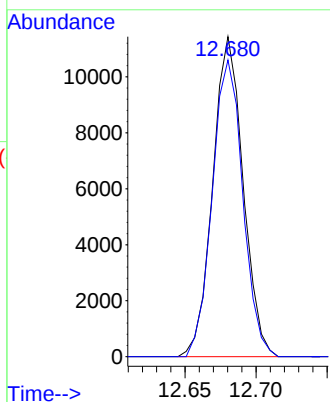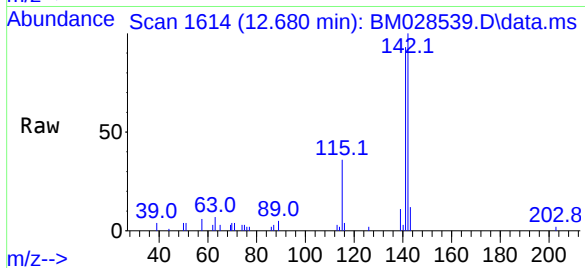

#39

1,2,4,5-Tetrachlorobenzene

Concen: 4.18 ng/ul

RT: 12.827 min Scan# 1639

Delta R.T. -0.006 min

Lab File: BM028539.D

Acq: 26 Jan 2021 11:04

Tgt Ion:216 Resp: 8855




Ion Ratio Lower Upper


216 100

214 79.5 64.1 96.1

179 21.8 17.8 26.6

108 16.7 14.6 21.8




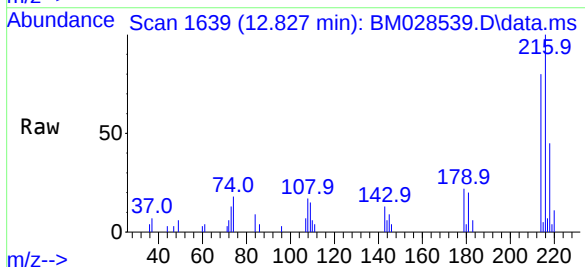




#40
Hexachlorocyclopentadiene
Concen: 3.62 ng/ul
RT: 12.804 min Scan# 1635
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	237	Resp:	3943
Ion	Ratio	Lower	Upper
237	100		
235	63.2	50.9	76.3
272	11.1	10.5	15.7

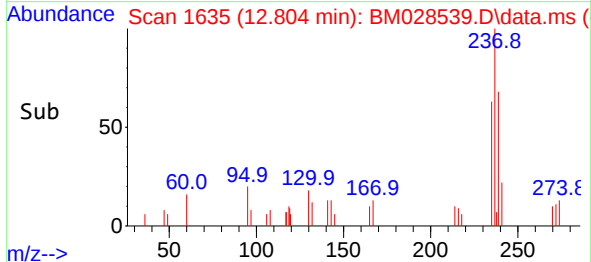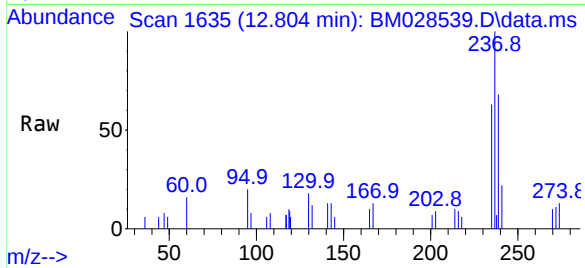

#41
2,4,6-Trichlorophenol
Concen: 3.99 ng/ul
RT: 13.068 min Scan# 1680
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	196	Resp:	5284
Ion	Ratio	Lower	Upper
196	100		
198	104.1	75.8	113.8
200	34.7	24.7	37.1




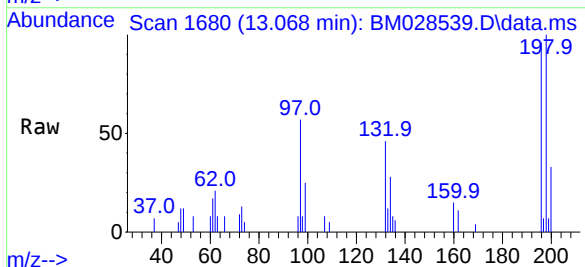




#42
2,4,5-Trichlorophenol
Concen: 4.03 ng/ul
RT: 13.139 min Scan# 1692
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:196 Resp: 5731
Ion Ratio Lower Upper
196 100
198 92.1 74.2 111.4
200 30.0 24.8 37.2

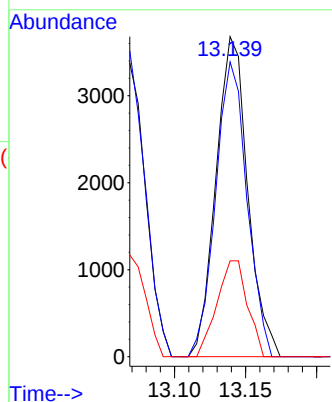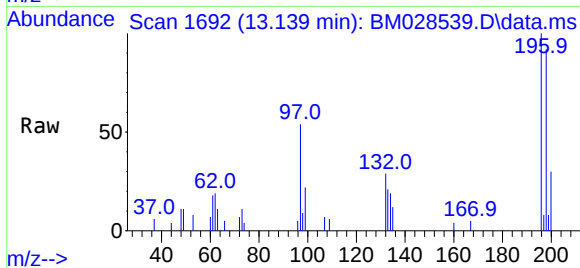

#43
1,1'-Biphenyl
Concen: 4.16 ng/ul
RT: 13.468 min Scan# 1748
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:154 Resp: 22475
Ion Ratio Lower Upper
154 100
153 40.5 32.7 49.1
76 12.8 10.2 15.4

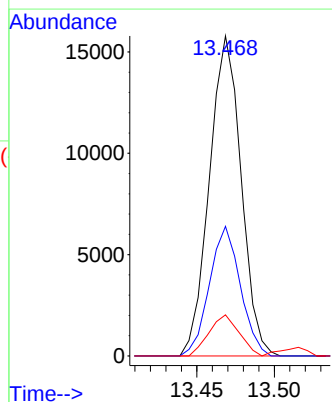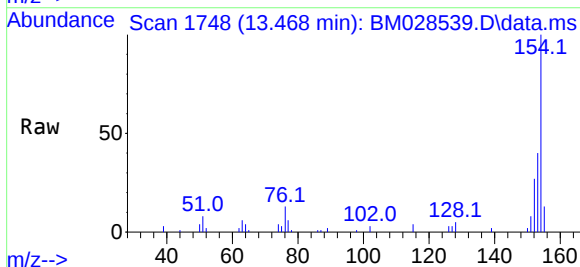







#44
2-Chloronaphthalene
Concen: 4.15 ng/ul
RT: 13.510 min Scan# 1755
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02

Tgt Ion:162 Resp: 17453




Ion	Ratio	Lower	Upper
162	100		
164	33.4	26.1	39.1
127	36.2	31.8	47.6

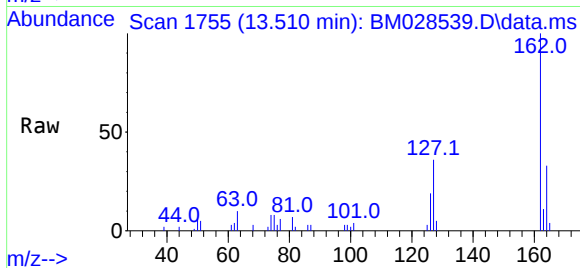


#45
2-Nitroaniline
Concen: 3.58 ng/ul
RT: 13.715 min Scan# 1790
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion: 65 Resp: 4158

Ion	Ratio	Lower	Upper
65	100		
92	68.2	51.2	76.8
138	97.2	80.2	120.2


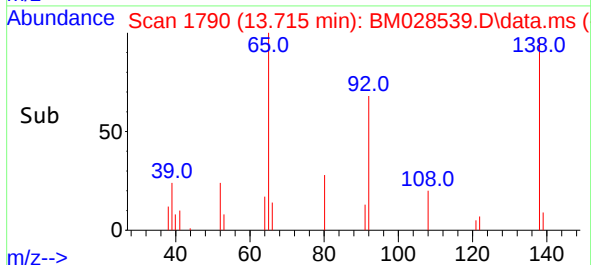
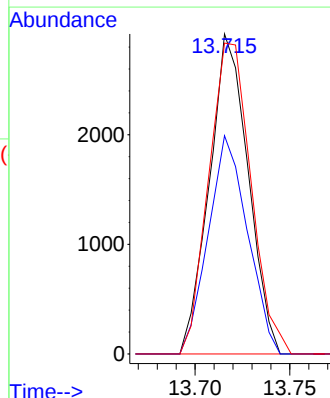
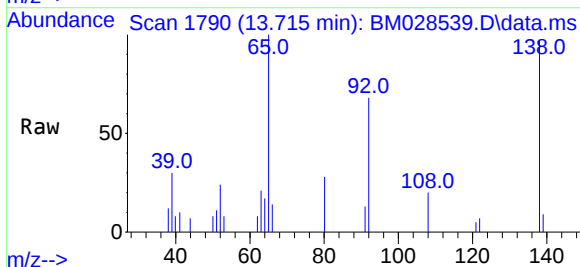




#47
Dimethylphthalate
Concen: 4.07 ng/ul
RT: 14.086 min Scan# 1853
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:163	Resp:	20608
Ion Ratio	Lower	Upper
163	100	
194	3.7	3.3 4.9
164	10.0	8.7 13.1

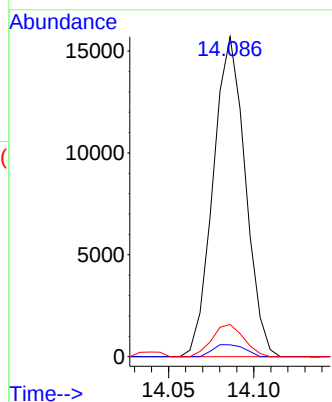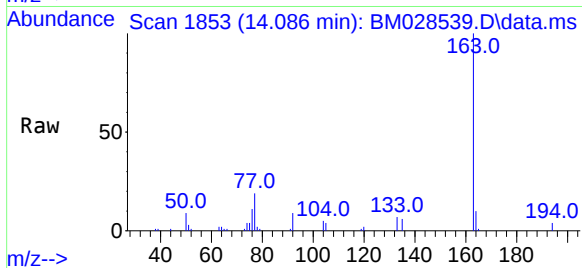

#48
2,6-Dinitrotoluene
Concen: 3.58 ng/ul
RT: 14.215 min Scan# 1875
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:165	Resp:	3583
Ion Ratio	Lower	Upper
165	100	
89	57.4	46.3 69.5
121	24.4	17.4 26.2


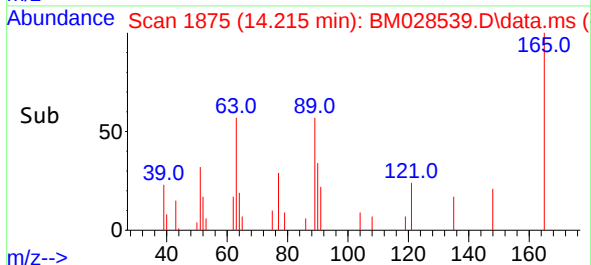

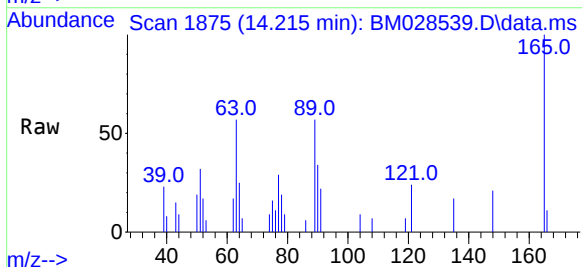




#50
Acenaphthylene
Concen: 4.19 ng/ul
RT: 14.357 min Scan# 1899
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:152	Resp:	25808
Ion Ratio	Lower	Upper
152	100	
151	18.9	15.4 23.2
153	12.8	10.2 15.4

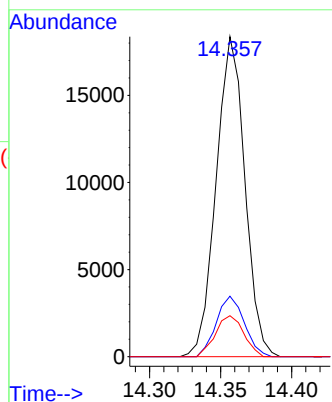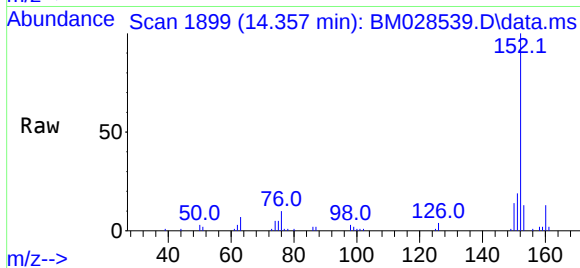

#51
3-Nitroaniline
Concen: 3.84 ng/ul
RT: 14.539 min Scan# 1930
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:138	Resp:	3491
Ion Ratio	Lower	Upper
138	100	
108	8.0	8.2 12.4#
92	115.0	92.8 139.2



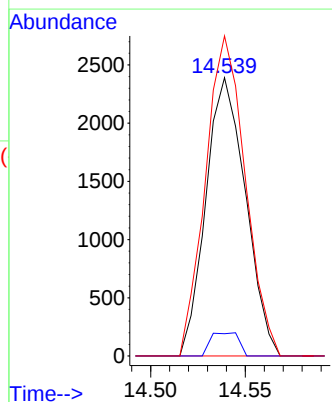
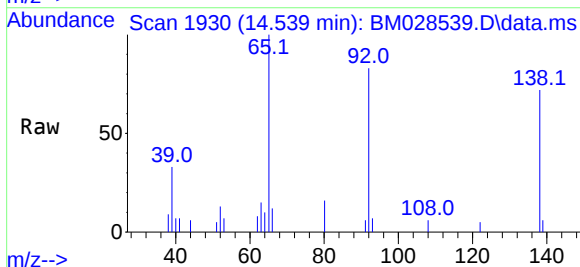




#52
Acenaphthene
Concen: 4.13 ng/ul
RT: 14.698 min Scan# 1957
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:153 Resp: 18327
Ion Ratio Lower Upper
153 100
152 46.3 37.5 56.3
154 89.4 69.1 103.7

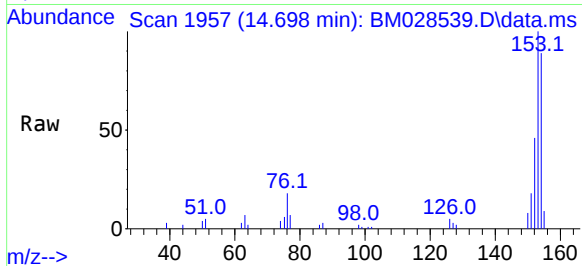

#53
2,4-Dinitrophenol
Concen: 3.24 ng/ul
RT: 14.757 min Scan# 1967
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:184 Resp: 1770
Ion Ratio Lower Upper
184 100
63 69.0 61.0 91.4
154 50.6 49.2 73.8



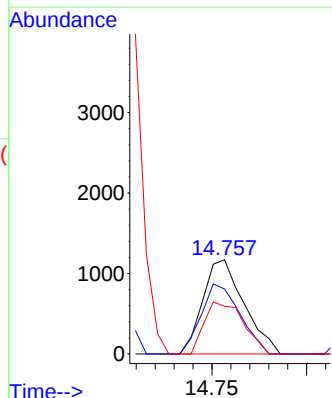
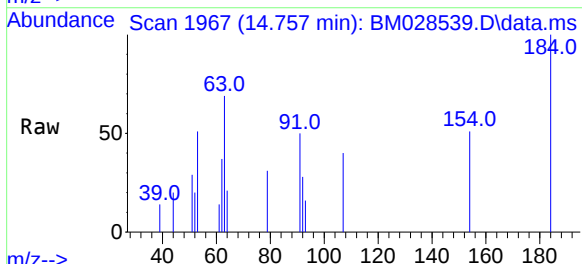




#55
4-Nitrophenol
Concen: 4.05 ng/ul
RT: 14.839 min Scan# 1981
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:109 Resp: 2804
Ion Ratio Lower Upper
109 100
139 135.8 103.4 155.2
65 152.3 104.9 157.3

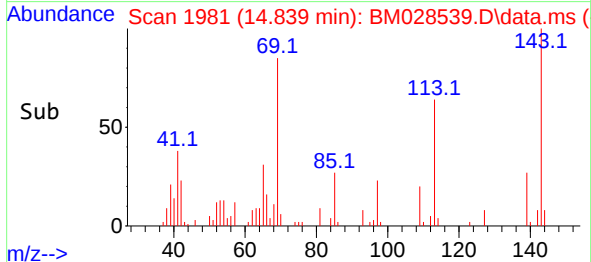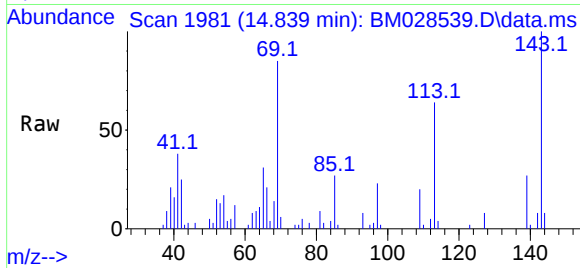

#56
Dibenzofuran
Concen: 4.26 ng/ul
RT: 15.027 min Scan# 2013
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:168 Resp: 25349
Ion Ratio Lower Upper
168 100
139 35.2 29.8 44.6




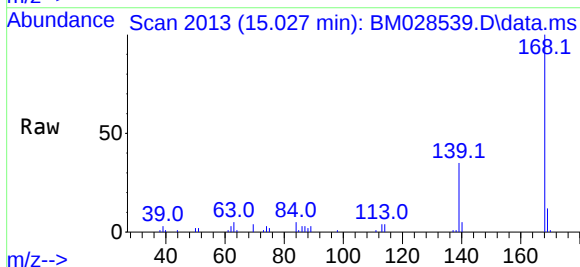




#57
2,4-Dinitrotoluene
Concen: 3.72 ng/ul
RT: 14.998 min Scan# 2008
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:165 Resp: 5013
Ion Ratio Lower Upper
165 100
63 50.6 39.3 58.9
182 0.0 2.2 3.4#

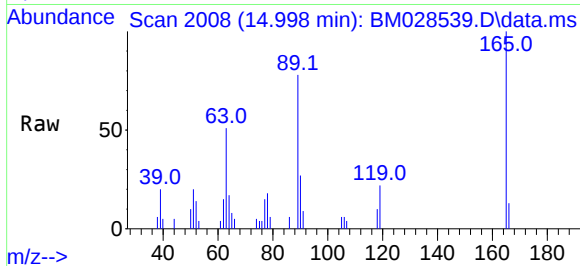

#58
2,3,4,6-Tetrachlorophenol
Concen: 3.81 ng/ul
RT: 15.257 min Scan# 2052
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:232 Resp: 4406
Ion Ratio Lower Upper
232 100
131 48.0 38.6 57.8
130 0.0 2.1 3.1#
166 32.2 24.2 36.4


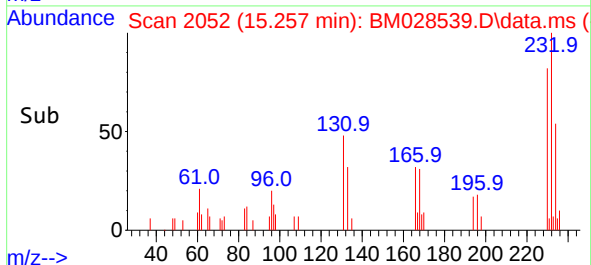
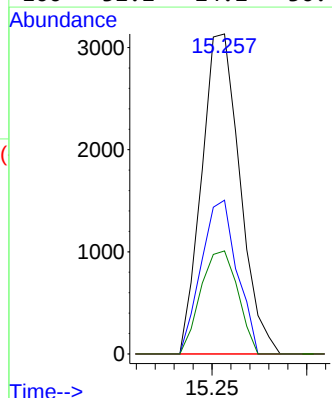
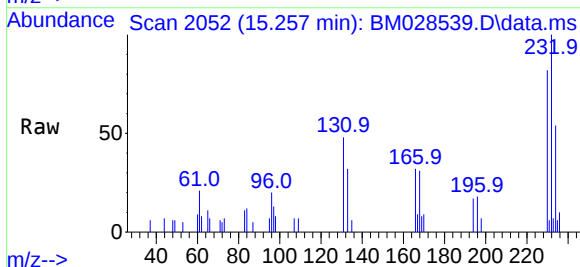




#59
Diethylphthalate
Concen: 3.85 ng/ul
RT: 15.439 min Scan# 2083
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:149 Resp: 20078
Ion Ratio Lower Upper
149 100
177 23.7 16.9 25.3
150 12.9 9.9 14.9

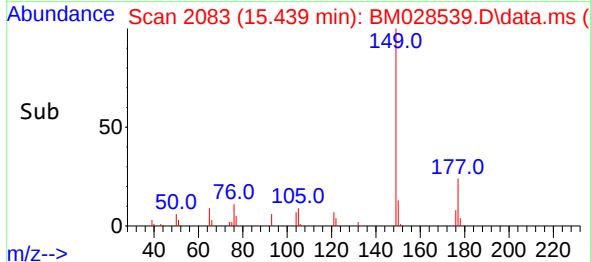

#61
Fluorene
Concen: 4.18 ng/ul
RT: 15.674 min Scan# 2123
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:166 Resp: 20701
Ion Ratio Lower Upper
166 100
165 94.4 77.0 115.4
167 13.6 10.6 16.0


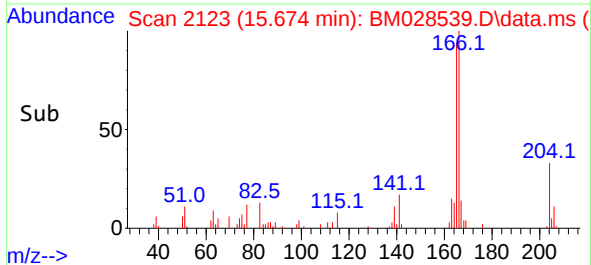






#62
4-Chlorophenyl-phenylether
Concen: 4.04 ng/ul
RT: 15.668 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:204 Resp: 9982
Ion Ratio Lower Upper
204 100
206 33.0 25.9 38.9
141 56.8 49.0 73.4

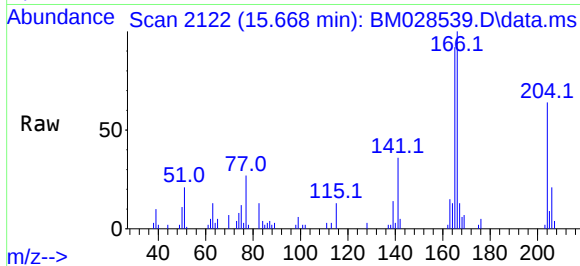

#63
4-Nitroaniline
Concen: 4.09 ng/ul
RT: 15.692 min Scan# 2126
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:138 Resp: 3247
Ion Ratio Lower Upper
138 100
92 52.0 39.8 59.8
108 68.8 60.6 91.0




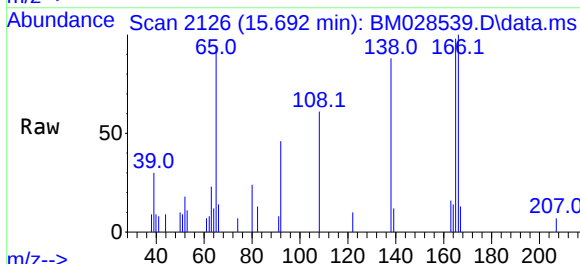




#66
4,6-Dinitro-2-methylphenol
Concen: 3.89 ng/ul
RT: 15.757 min Scan# 2137
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:198 Resp: 3231
Ion Ratio Lower Upper
198 100
182 9.8 3.3 4.9#
77 40.6 20.6 31.0#

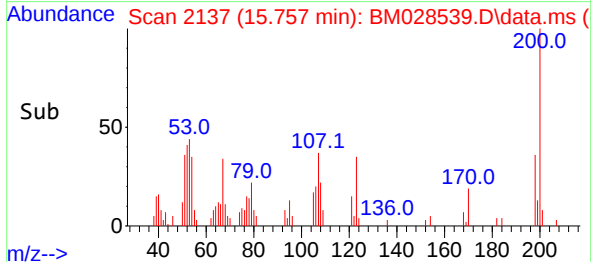

#67
N-Nitrosodiphenylamine
Concen: 4.17 ng/ul
RT: 15.880 min Scan# 2158
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:169 Resp: 16893
Ion Ratio Lower Upper
169 100
168 65.7 53.5 80.3
167 34.7 28.2 42.2


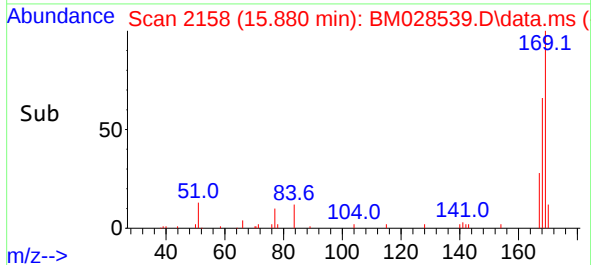






#68
4-Bromophenyl-phenylether
Concen: 3.95 ng/ul
RT: 16.556 min Scan# 2273
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:248 Resp: 5788
Ion Ratio Lower Upper
248 100
250 96.0 77.9 116.9
141 73.7 60.6 90.8

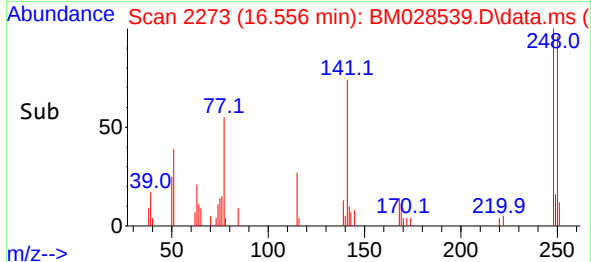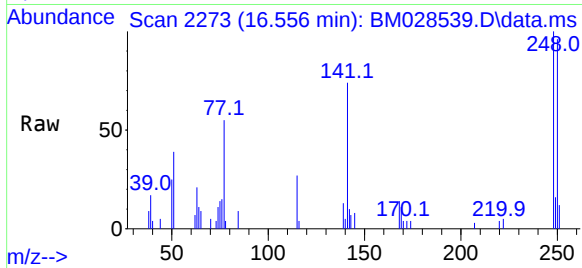

#69
Hexachlorobenzene
Concen: 4.06 ng/ul
RT: 16.668 min Scan# 2292
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:284 Resp: 6742
Ion Ratio Lower Upper
284 100
142 32.5 28.1 42.1
249 27.8 23.4 35.2




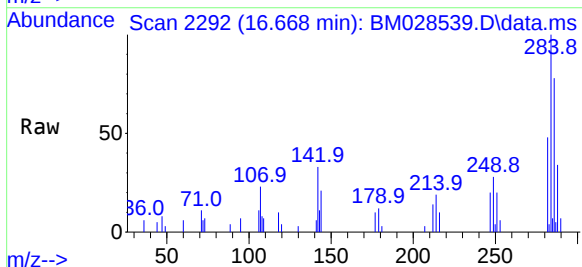




#70
Atrazine
Concen: 3.58 ng/ul
RT: 16.821 min Scan# 2318
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	200	Resp:	5366
Ion Ratio	Lower	Upper	
200	100		
173	29.9	21.5	32.3
215	51.3	37.9	56.9

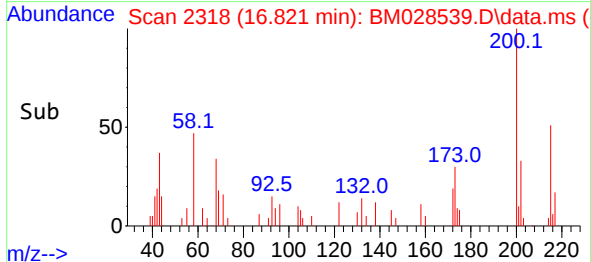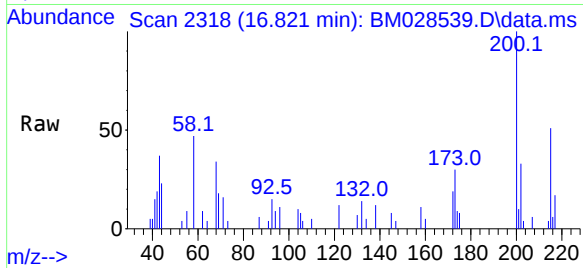

#71
Pentachlorophenol
Concen: 3.27 ng/ul
RT: 17.015 min Scan# 2351
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	266	Resp:	3075
Ion Ratio	Lower	Upper	
266	100		
264	56.4	49.5	74.3
268	63.3	50.6	76.0




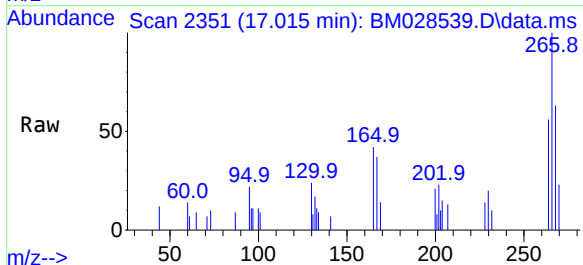




#72
Phenanthrene
Concen: 4.20 ng/ul
RT: 17.403 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:178	Resp:	30917
Ion Ratio	Lower	Upper
178	100	
179	15.3	12.3 18.5
176	18.0	14.8 22.2

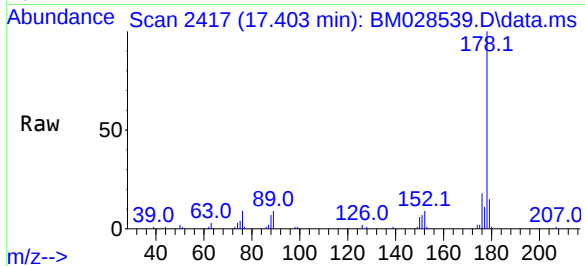

#74
Anthracene
Concen: 4.23 ng/ul
RT: 17.492 min Scan# 2432
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:178	Resp:	31656
Ion Ratio	Lower	Upper
178	100	
179	15.4	12.2 18.4
176	18.5	14.3 21.5




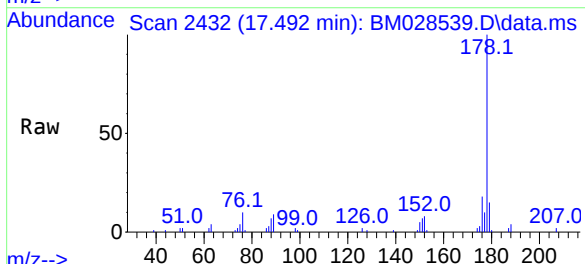




#75
1,2,3,4-Tetrachlorobenzene
Concen: 4.19 ng/uL
RT: 13.433 min Scan# 1742
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	216	Resp:	8650
Ion Ratio	Lower	Upper	
216	100		
214	82.8	62.6	93.8
218	48.2	38.7	58.1

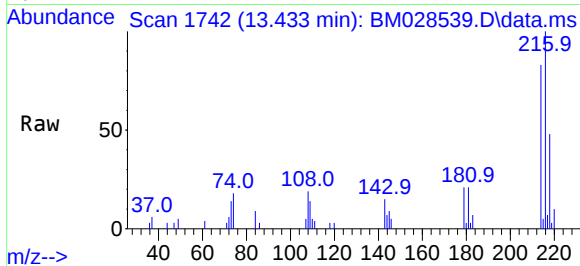

#76
Pentachlorobenzene
Concen: 4.05 ng/uL
RT: 14.951 min Scan# 2000
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04


Tgt Ion:	250	Resp:	8169
Ion Ratio	Lower	Upper	
250	100		
248	65.2	51.2	76.8
252	67.9	49.6	74.4

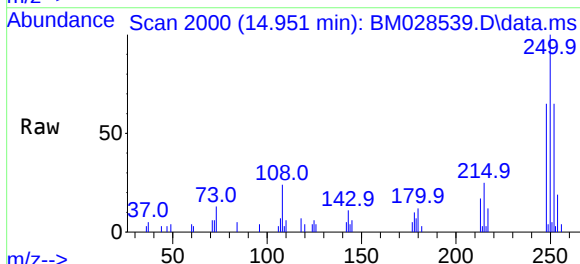






#77
 Carbazole
 Concen: 4.19 ng/ul
 RT: 17.762 min Scan# 2478
 Delta R.T. -0.006 min
 Lab File: BM028539.D
 Acq: 26 Jan 2021 11:04

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT1-2021-02

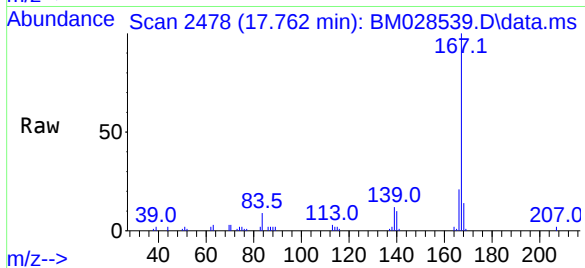


Tgt Ion:167 Resp: 26572

Ion	Ratio	Lower	Upper
167	100		
166	21.3	17.1	25.7
139	11.7	10.1	15.1


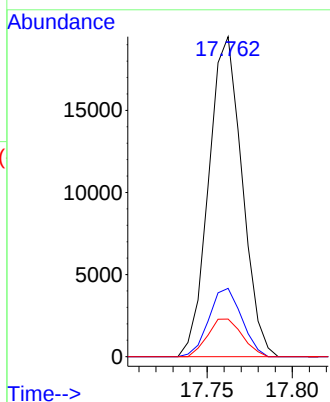



#78
 Di-n-butylphthalate
 Concen: 3.67 ng/ul
 RT: 18.309 min Scan# 2571
 Delta R.T. -0.006 min
 Lab File: BM028539.D
 Acq: 26 Jan 2021 11:04

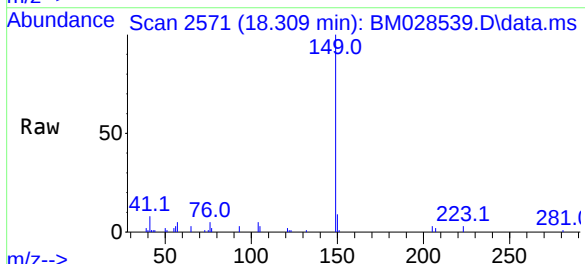

Tgt Ion:149 Resp: 32067

Ion	Ratio	Lower	Upper
149	100		
150	8.7	7.2	10.8
104	5.0	4.2	6.2




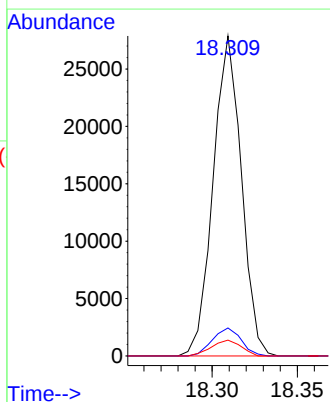




#80
Fluoranthene
Concen: 3.97 ng/ul
RT: 19.397 min Scan# 2756
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	202	Resp:	33639
Ion	Ratio	Lower	Upper
202	100		
101	12.6	9.3	13.9
100	8.6	7.4	11.2

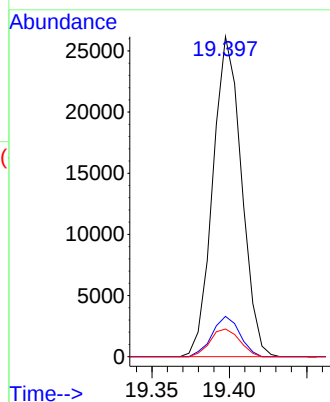

#82
Pyrene
Concen: 4.06 ng/ul
RT: 19.756 min Scan# 2817
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	202	Resp:	35291
Ion	Ratio	Lower	Upper
202	100		
101	14.3	10.9	16.3
100	12.4	9.4	14.2









#83
Butylbenzylphthalate
Concen: 3.65 ng/ul
RT: 20.639 min Scan# 2967
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	149	Resp:	14374
Ion	Ratio	Lower	Upper
149	100		
91	69.0	58.8	88.2
206	20.7	16.1	24.1



#84
3,3'-Dichlorobenzidine
Concen: 4.82 ng/ul
RT: 21.409 min Scan# 3098
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	252	Resp:	11186
Ion	Ratio	Lower	Upper
252	100		
254	62.2	52.9	79.3
126	12.7	9.4	14.2



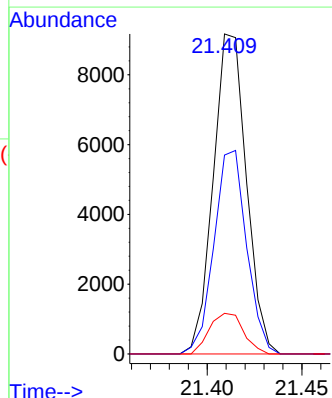





#85
Benzo(a)anthracene
Concen: 4.20 ng/ul
RT: 21.480 min Scan# 3110
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	228	Resp:	32400
Ion Ratio	Lower	Upper	
228	100		
229	20.0	15.4	23.2
226	26.0	21.7	32.5

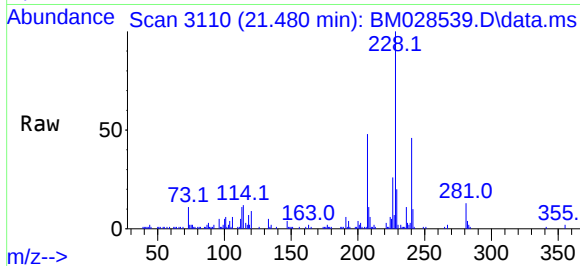

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.52 ng/ul
RT: 21.397 min Scan# 3096
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	149	Resp:	21488
Ion Ratio	Lower	Upper	
149	100		
167	27.2	21.4	32.0
279	4.2	3.3	4.9




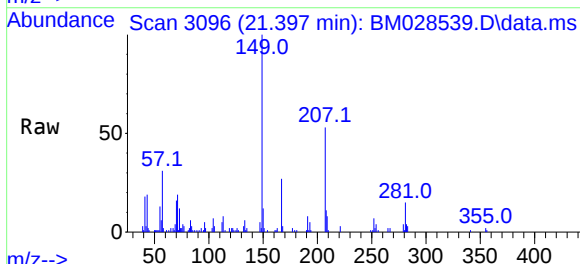




#87
Chrysene
Concen: 4.15 ng/ul
RT: 21.533 min Scan# 3119
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:228 Resp: 31124
Ion Ratio Lower Upper
228 100
226 29.8 23.2 34.8
229 18.7 15.8 23.6



#89
Di-n-octyl phthalate
Concen: 3.51 ng/ul
RT: 22.280 min Scan# 3246
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:149 Resp: 36157









#90
Benzo(b)fluoranthene
Concen: 4.37 ng/ul
RT: 23.080 min Scan# 3382
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:252 Resp: 32837
Ion Ratio Lower Upper
252 100
253 22.6 17.5 26.3
125 12.1 8.7 13.1



#91
Benzo(k)fluoranthene
Concen: 4.22 ng/ul
RT: 23.127 min Scan# 3390
Delta R.T. -0.006 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:252 Resp: 30871
Ion Ratio Lower Upper
252 100
253 23.9 17.8 26.6
125 11.2 9.0 13.6









#93
Benzo(a)pyrene
Concen: 4.39 ng/u1
RT: 23.668 min Scan# 3482
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02


Tgt Ion:	252	Resp:	29854
Ion Ratio	Lower	Upper	
252	100		
253	20.9	17.4	26.2
125	12.5	10.6	15.8



#94
Indeno(1,2,3-cd)pyrene
Concen: 4.35 ng/u1
RT: 26.073 min Scan# 3891
Delta R.T. -0.012 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	276	Resp:	34961
Ion Ratio	Lower	Upper	
276	100		
138	27.5	22.0	33.0
277	24.8	20.4	30.6



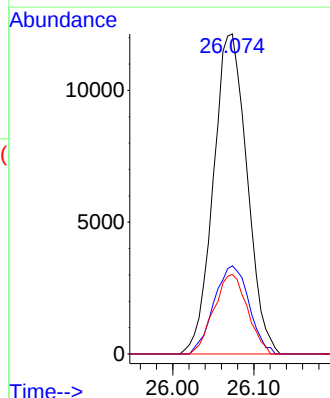





#95
Dibenzo(a,h)anthracene
Concen: 4.30 ng/ul
RT: 26.079 min Scan# 3892
Delta R.T. -0.018 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-02

Tgt Ion:	278	Resp:	29320
Ion	Ratio	Lower	Upper
278	100		
139	19.9	13.8	20.8
279	24.1	18.2	27.4

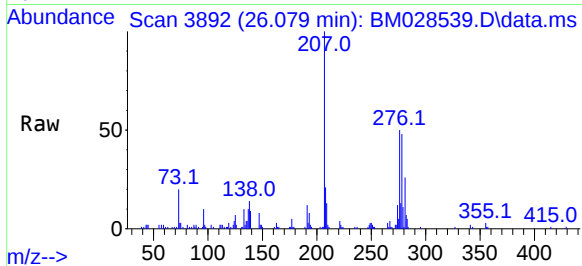

#96
Benzo(g,h,i)perylene
Concen: 4.32 ng/ul
RT: 26.779 min Scan# 4011
Delta R.T. -0.024 min
Lab File: BM028539.D
Acq: 26 Jan 2021 11:04

Tgt Ion:	276	Resp:	29246
Ion	Ratio	Lower	Upper
276	100		
138	22.4	18.9	28.3
277	25.5	18.3	27.5

