

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
 Data File : BM038544.D
 Acq On : 26 Jan 2023 11:56
 Operator : CG/JU
 Sample : PB150439BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK439

Quant Time: Jan 27 00:43:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 27 00:18:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	1505	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	3830	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	2530	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	5154	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	6331	0.400	ng/ul	0.00
23) Perylene-d12	23.933	264	7712	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	12627	6.389	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	1417	0.238	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	5049	0.279	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.729	202	911	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.769	252	1989	0.076	ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012623\
Data File : BM038544.D
Acq On : 26 Jan 2023 11:56
Operator : CG/JU
Sample : PB150439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK439

Quant Time: Jan 27 00:43:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 00:18:15 2023
Response via : Initial Calibration




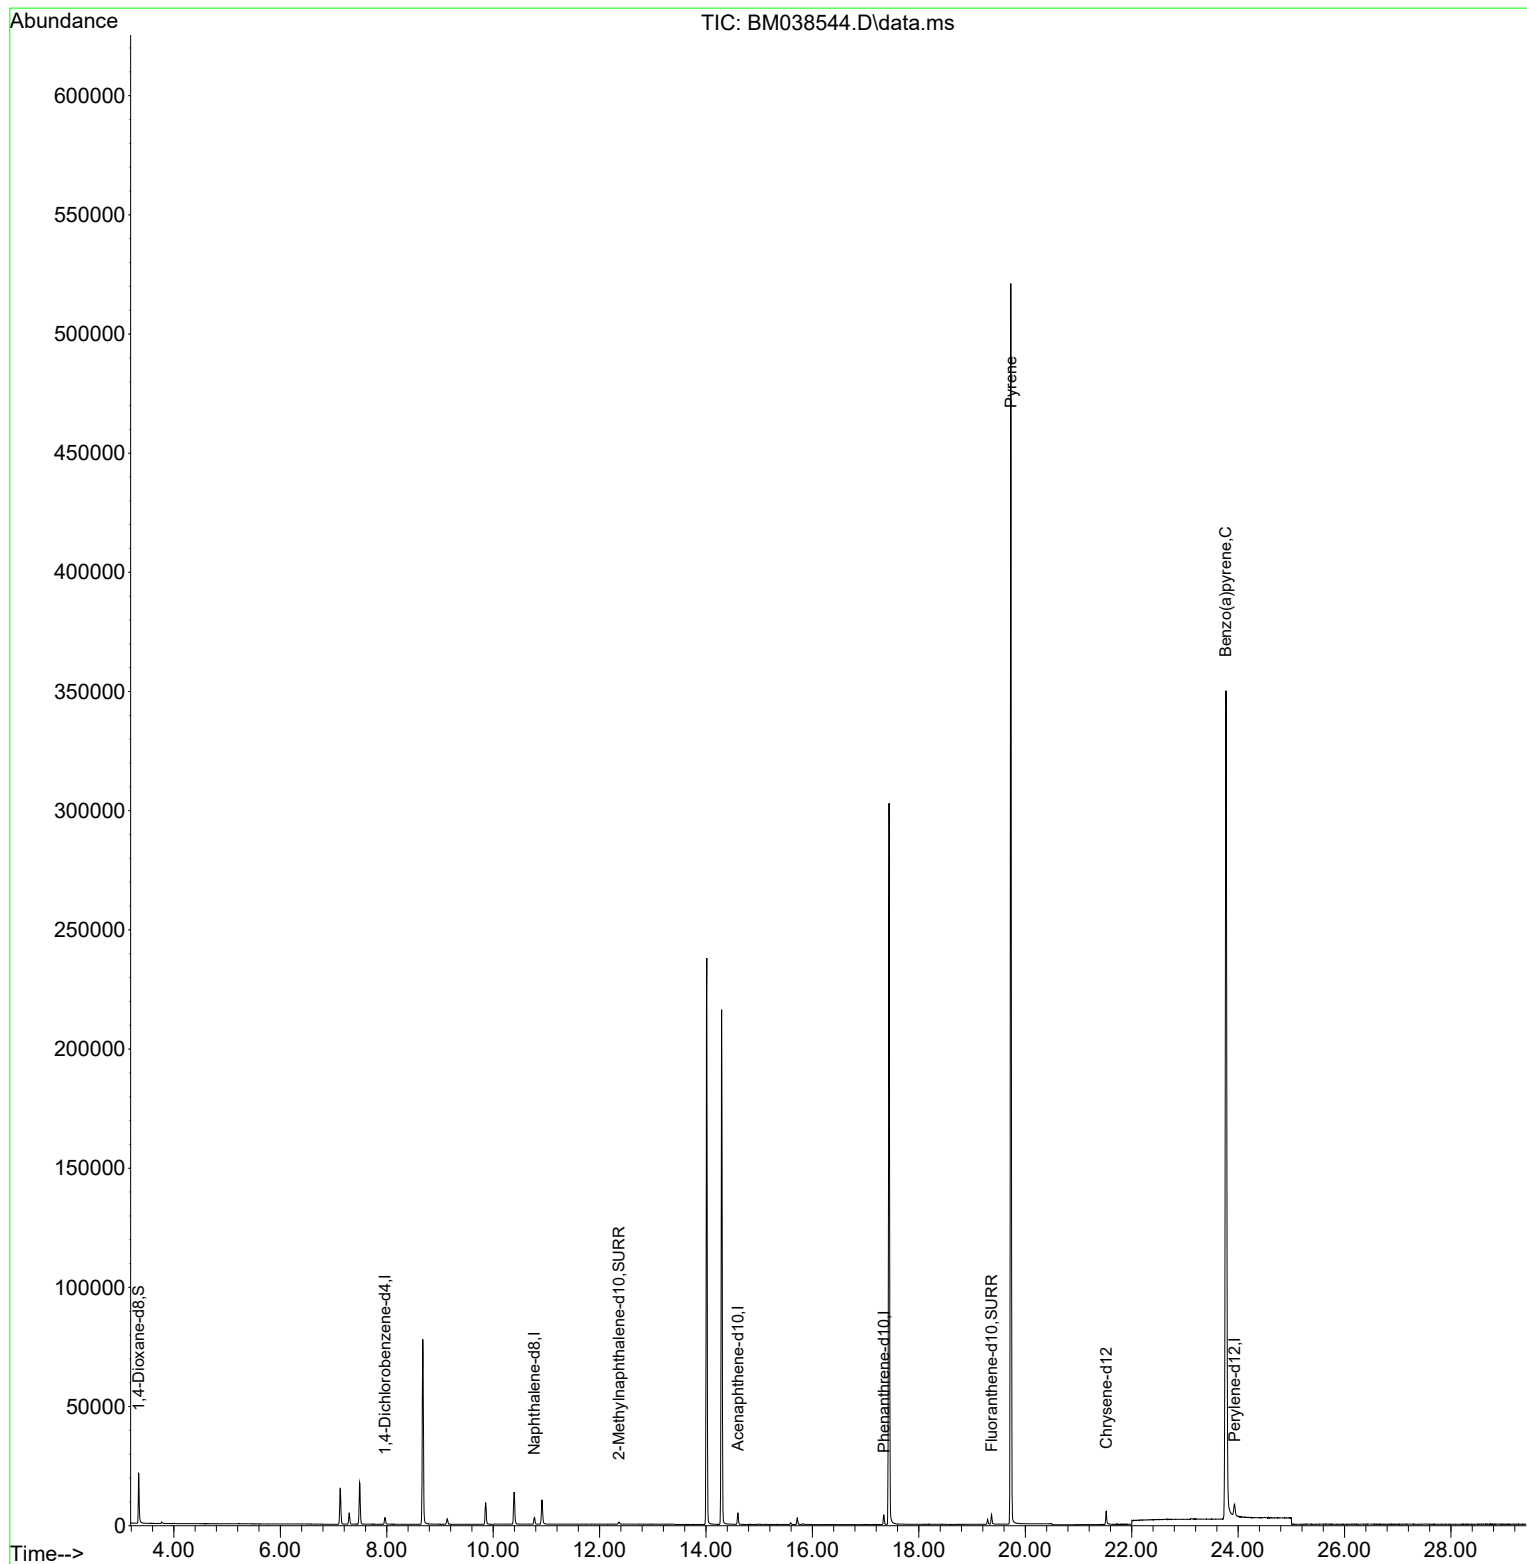


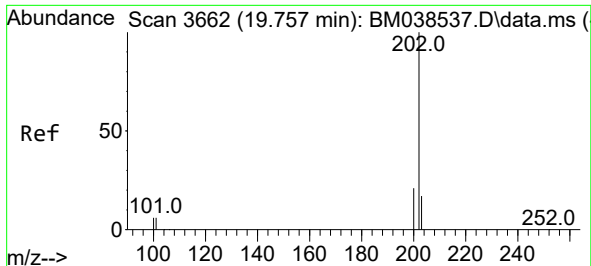

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.729 min Scan# 30
Delta R.T. -0.028 min
Lab File: BM038544.D
Acq: 26 Jan 2023 11:56

Instrument :
BNA_M
ClientSampleId :
SBLK439

Tgt Ion:202 Resp: 911
Ion Ratio Lower Upper
202 100
101 135.9 5.9 8.9#
100 1022.3 5.2 7.8#

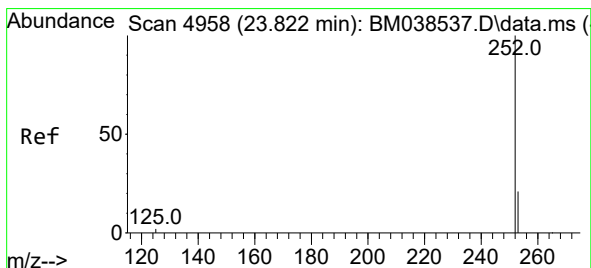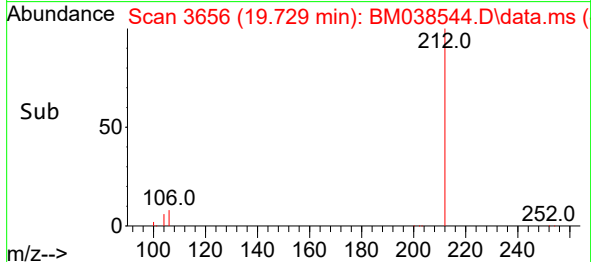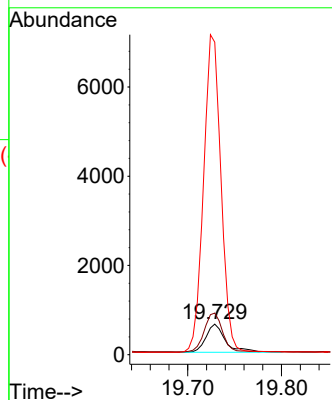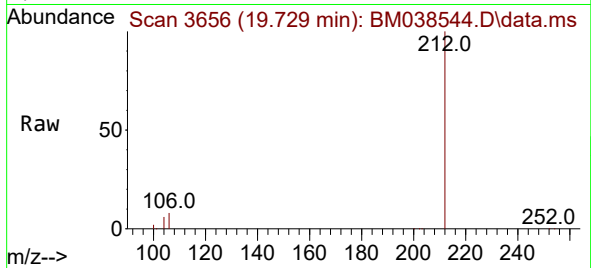

#26
Benzo(a)pyrene
Concen: 0.076 ng/ul
RT: 23.769 min Scan# 4940
Delta R.T. -0.053 min
Lab File: BM038544.D
Acq: 26 Jan 2023 11:56

Tgt Ion:252 Resp: 1989
Ion Ratio Lower Upper
252 100
253 64.6 25.1 37.7#
125 42.0 10.0 15.0#

